

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD041923\
 Data File : VD075755.D
 Acq On : 19 Apr 2023 18:13
 Operator : KP/SY
 Sample : 02270-22
 Misc : 4.98G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-15-0-2-20230412

Quant Time: Apr 20 06:01:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D041323S.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 13 14:16:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	183625	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	366349	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	325218	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	122799	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	110850	63.599	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	127.200%
35) Dibromofluoromethane	7.804	113	137206	55.683	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	111.360%
50) Toluene-d8	10.269	98	483150	48.964	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.920%
62) 4-Bromofluorobenzene	12.575	95	115762	44.137	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	88.280%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD041923\
Data File : VD075755.D
Acq On : 19 Apr 2023 18:13
Operator : KP/SY
Sample : 02270-22
Misc : 4.98G/5.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-15-0-2-20230412

Quant Time: Apr 20 06:01:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D041323S.M
Quant Title : SW846 8260
QLast Update : Thu Apr 13 14:16:29 2023
Response via : Initial Calibration




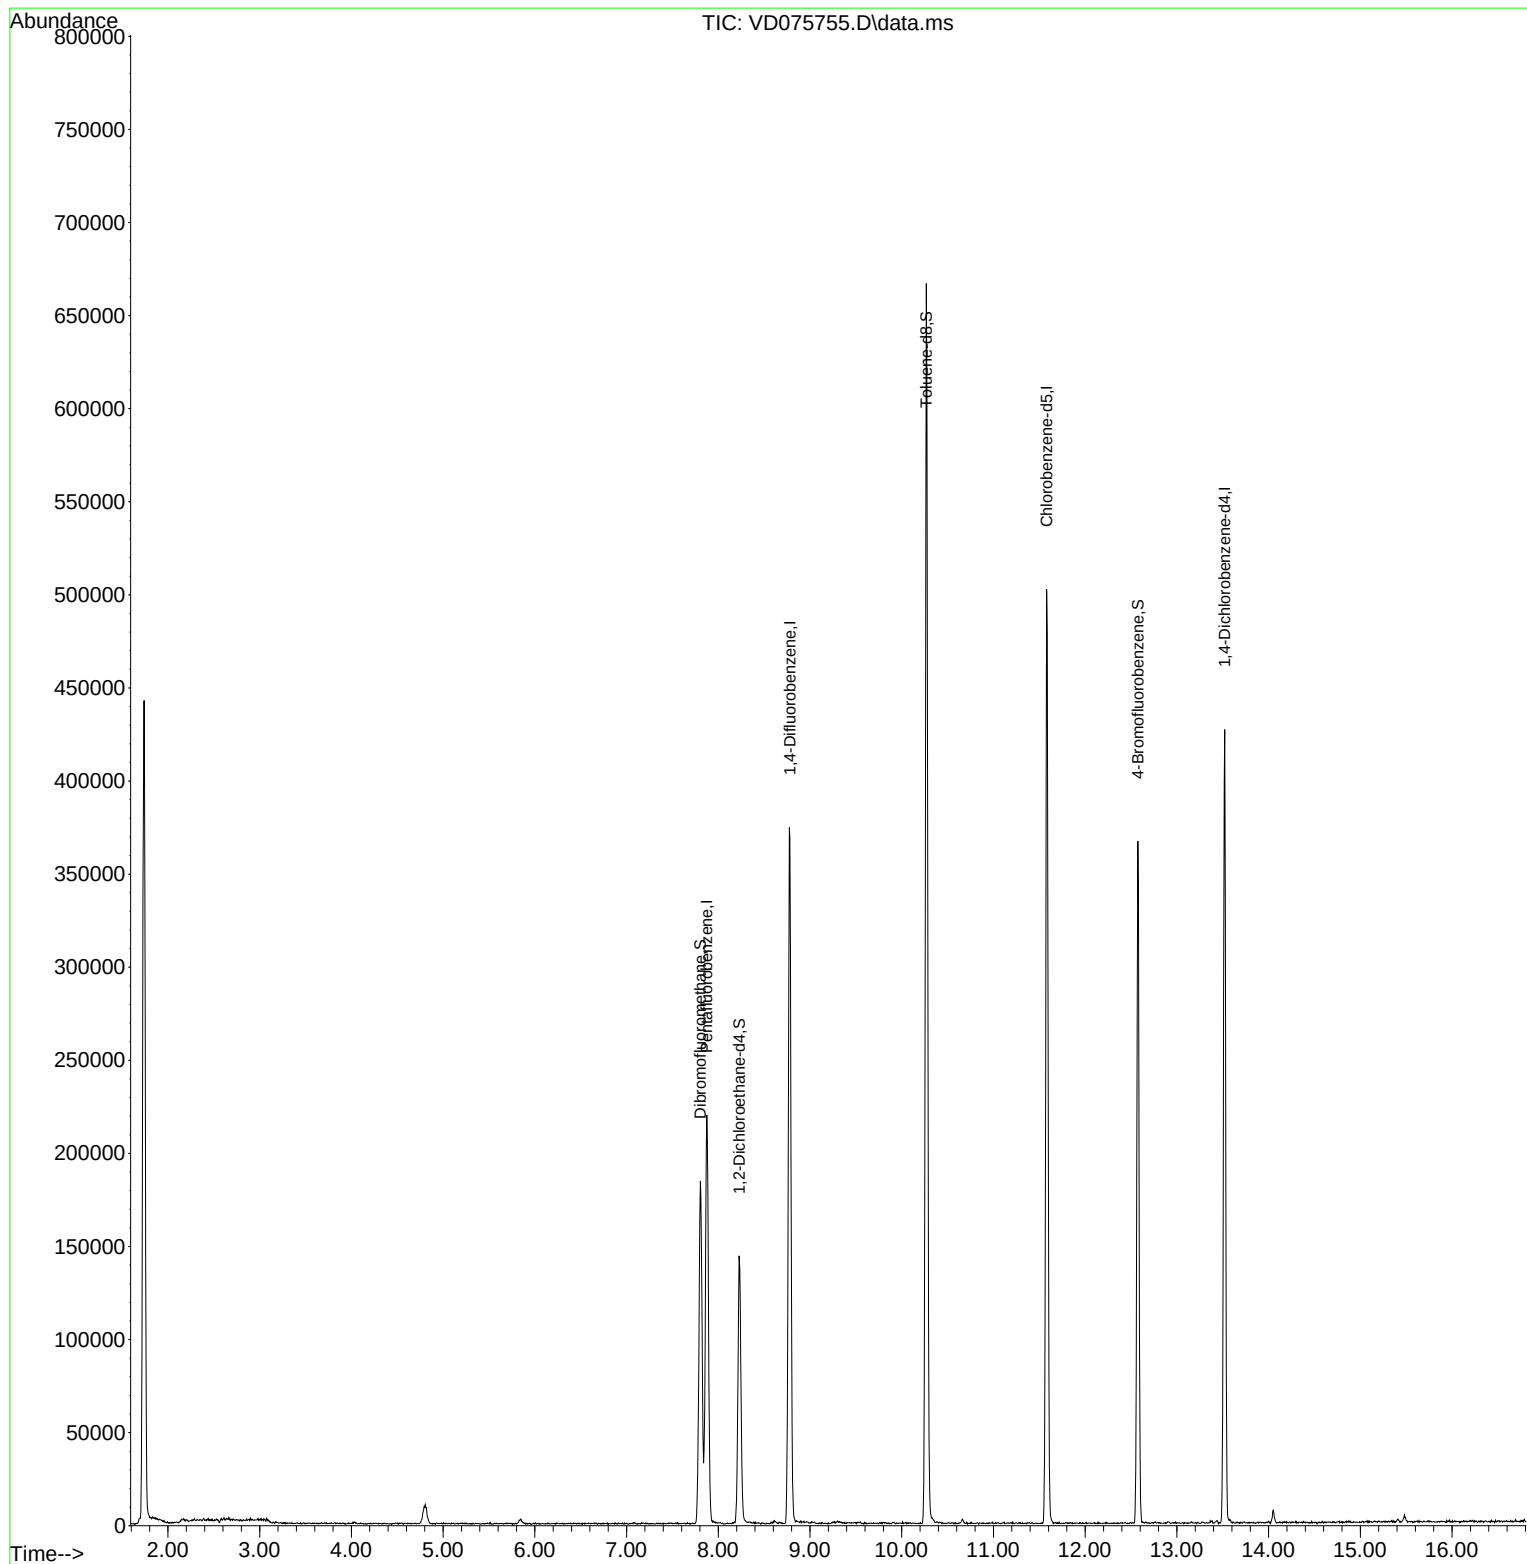


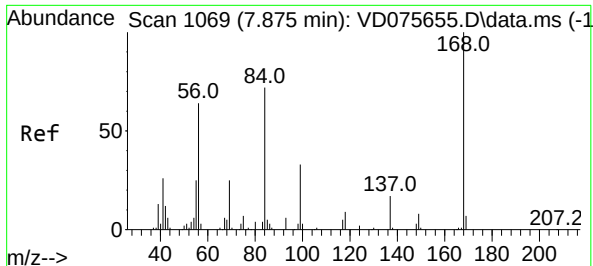

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1109
Delta R.T. -0.000 min
Lab File: VD075755.D
Acq: 19 Apr 2023 18:13




Instrument :
MSVOA_D
ClientSampleId :
SB-15-0-2-20230412


Tgt Ion:168 Resp: 183625
Ion Ratio Lower Upper
168 100
99 50.3 43.8 65.6

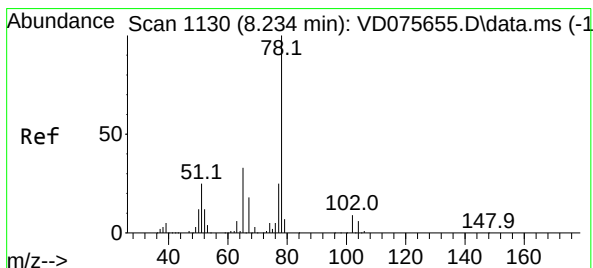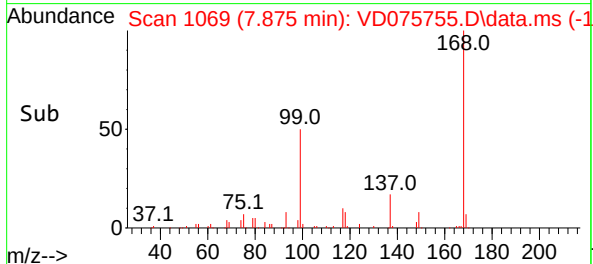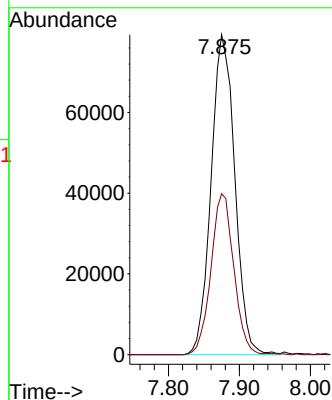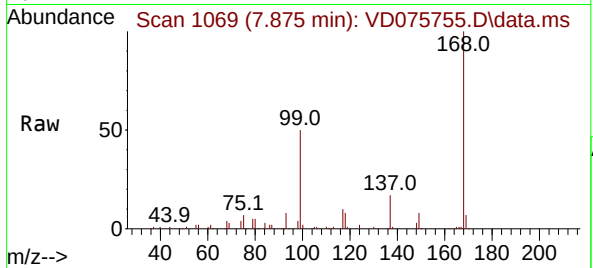

#33
1,2-Dichloroethane-d4
Concen: 63.599 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.006 min
Lab File: VD075755.D
Acq: 19 Apr 2023 18:13

Tgt Ion: 65 Resp: 110850
Ion Ratio Lower Upper
65 100
67 53.8 0.0 102.2

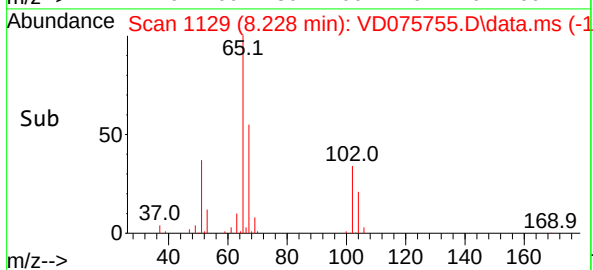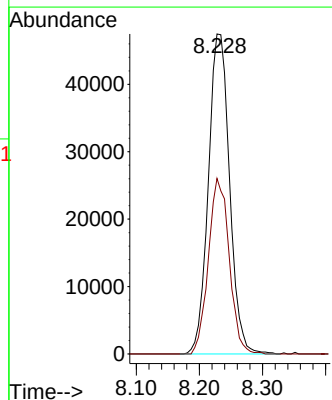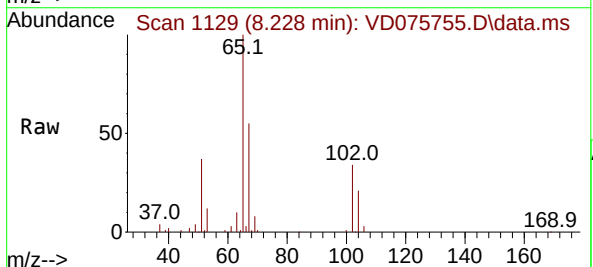

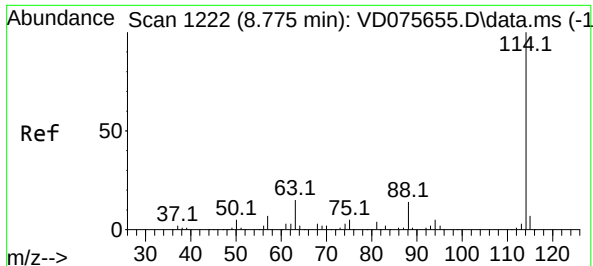

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD075755.D

Acq: 19 Apr 2023 18:13

Instrument :

MSVOA_D

ClientSampleId :

SB-15-0-2-20230412





Tgt Ion:114 Resp: 366349

Ion Ratio Lower Upper

114 100

63 16.1 0.0 41.6

88 14.2 0.0 30.6

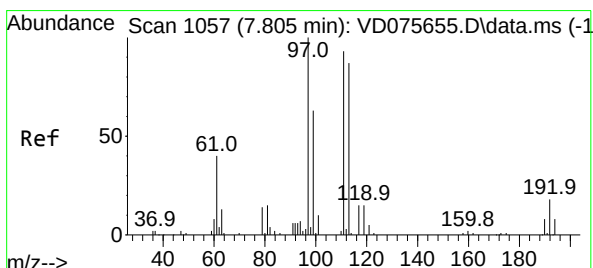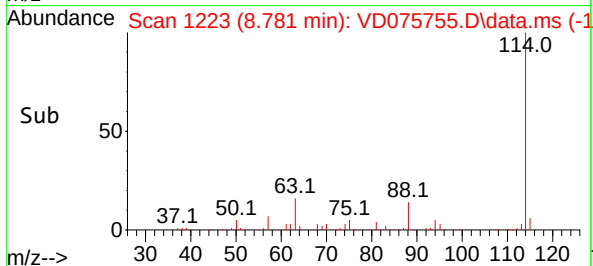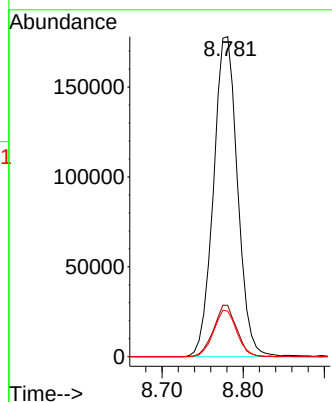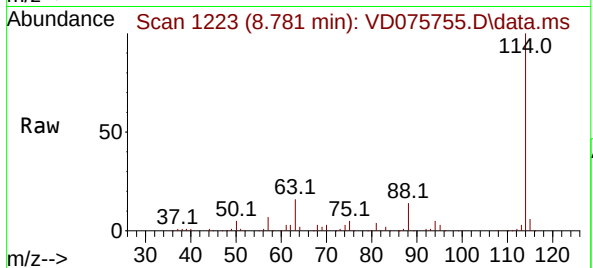

#35

Dibromofluoromethane

Concen: 55.683 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. -0.001 min

Lab File: VD075755.D

Acq: 19 Apr 2023 18:13




Tgt Ion:113 Resp: 137206


Ion Ratio Lower Upper

113 100

111 103.7 81.4 122.0

192 19.2 15.2 22.8


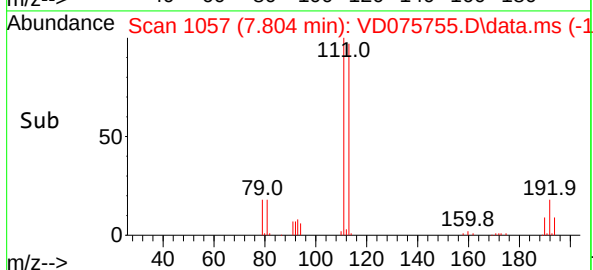
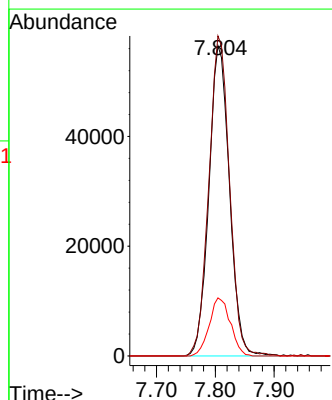
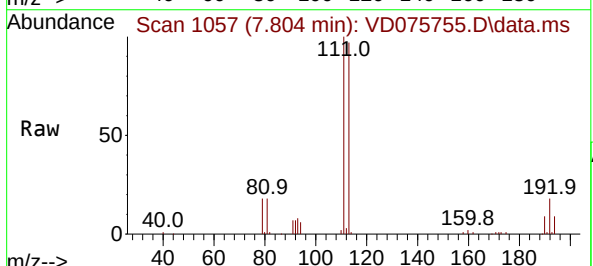


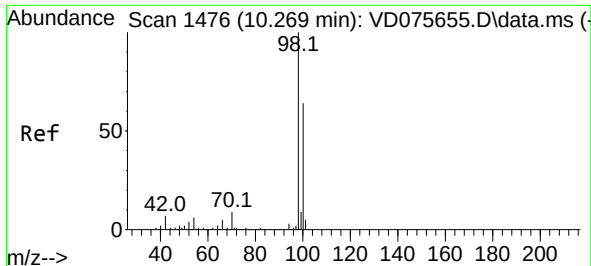

#50
Toluene-d8
Concen: 48.964 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD075755.D
Acq: 19 Apr 2023 18:13




Instrument :
MSVOA_D
ClientSampleId :
SB-15-0-2-20230412


Tgt Ion: 98 Resp: 483150
Ion Ratio Lower Upper
98 100
100 62.7 52.1 78.1

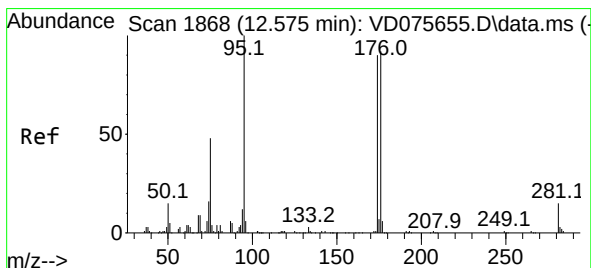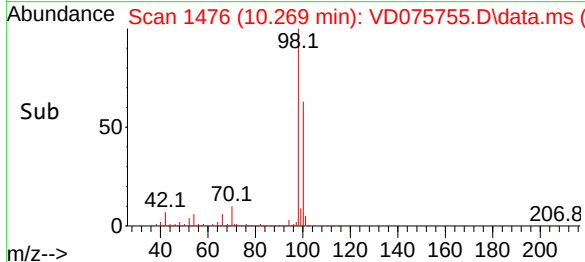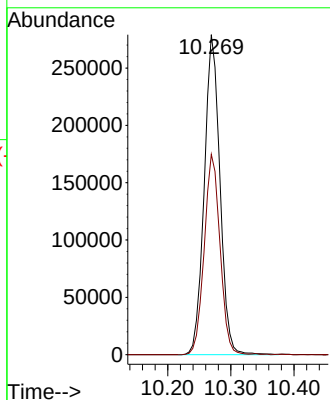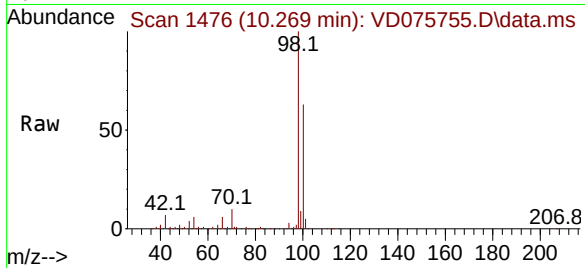

#62
4-Bromofluorobenzene
Concen: 44.137 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD075755.D
Acq: 19 Apr 2023 18:13

Tgt Ion: 95 Resp: 115762
Ion Ratio Lower Upper
95 100
174 90.0 0.0 164.0
176 87.5 0.0 156.8


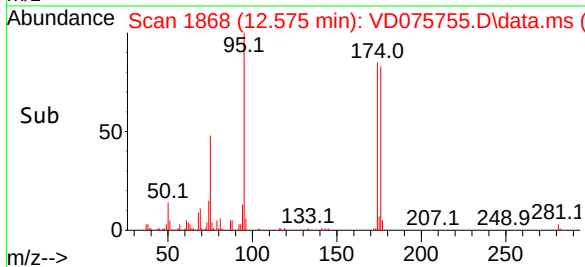
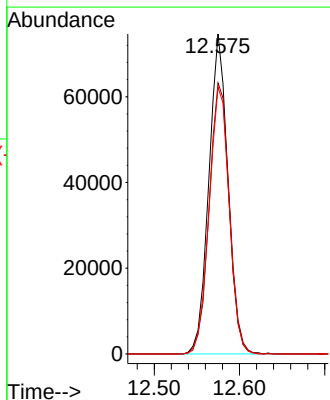
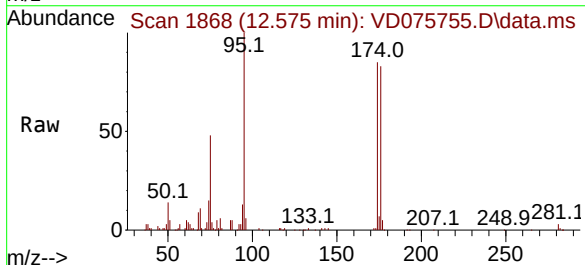


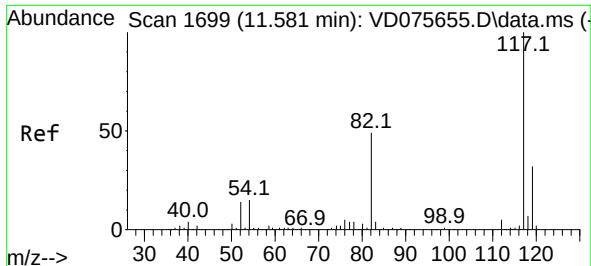

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD075755.D
Acq: 19 Apr 2023 18:13

Instrument :
MSVOA_D
ClientSampleId :
SB-15-0-2-20230412

Tgt Ion:117 Resp: 325218
Ion Ratio Lower Upper
117 100
82 49.1 44.0 66.0
119 32.7 25.1 37.7

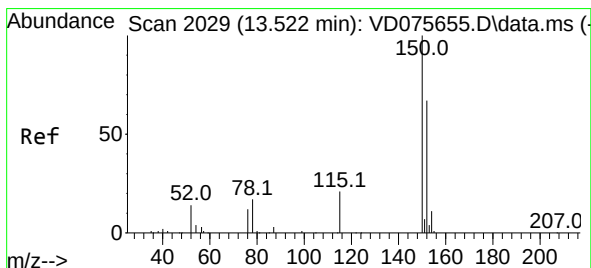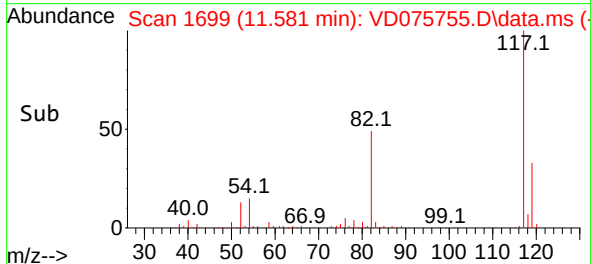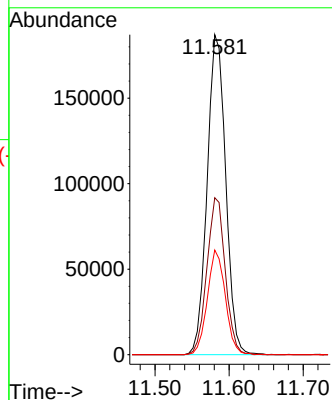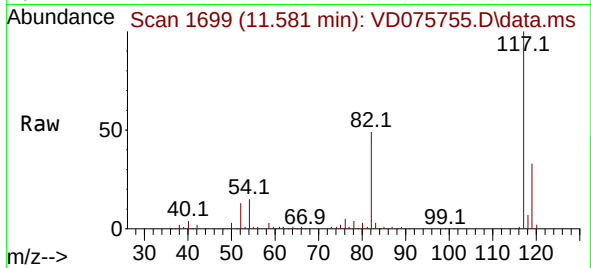

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. -0.000 min
Lab File: VD075755.D
Acq: 19 Apr 2023 18:13

Tgt Ion:152 Resp: 122799
Ion Ratio Lower Upper
152 100
115 54.7 30.1 90.3
150 159.7 0.0 364.8

