
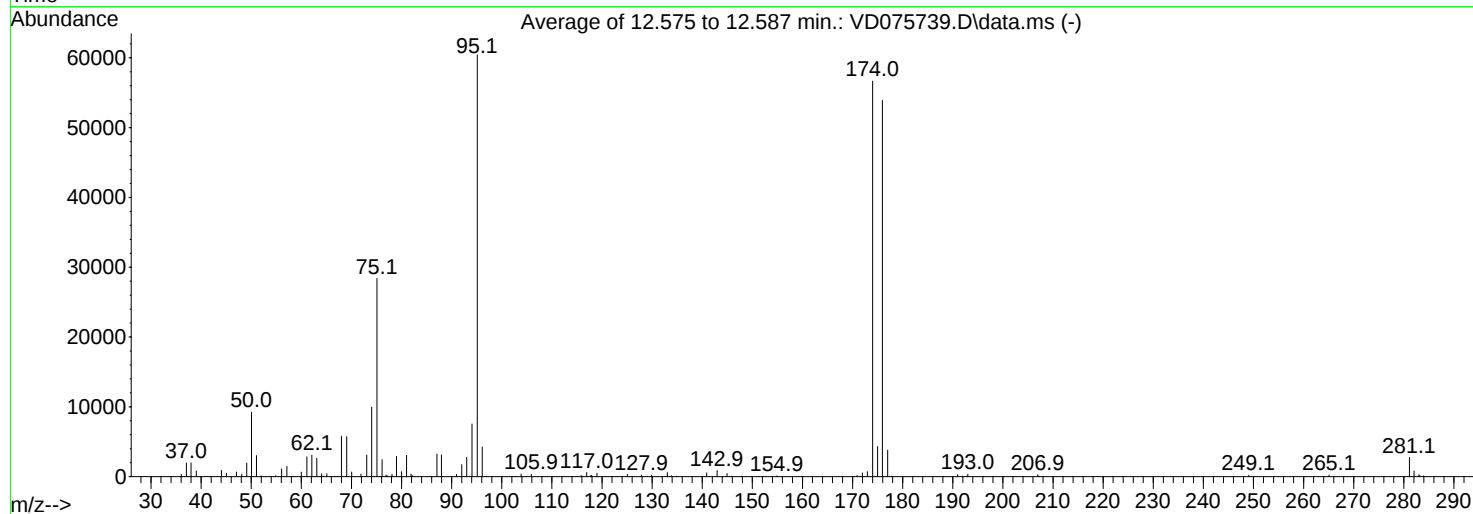


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD041923\
Data File : VD075739.D
Acq On : 19 Apr 2023 09:57
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D041323S.M
Title : SW846 8260
Last Update : Thu Apr 13 14:16:29 2023

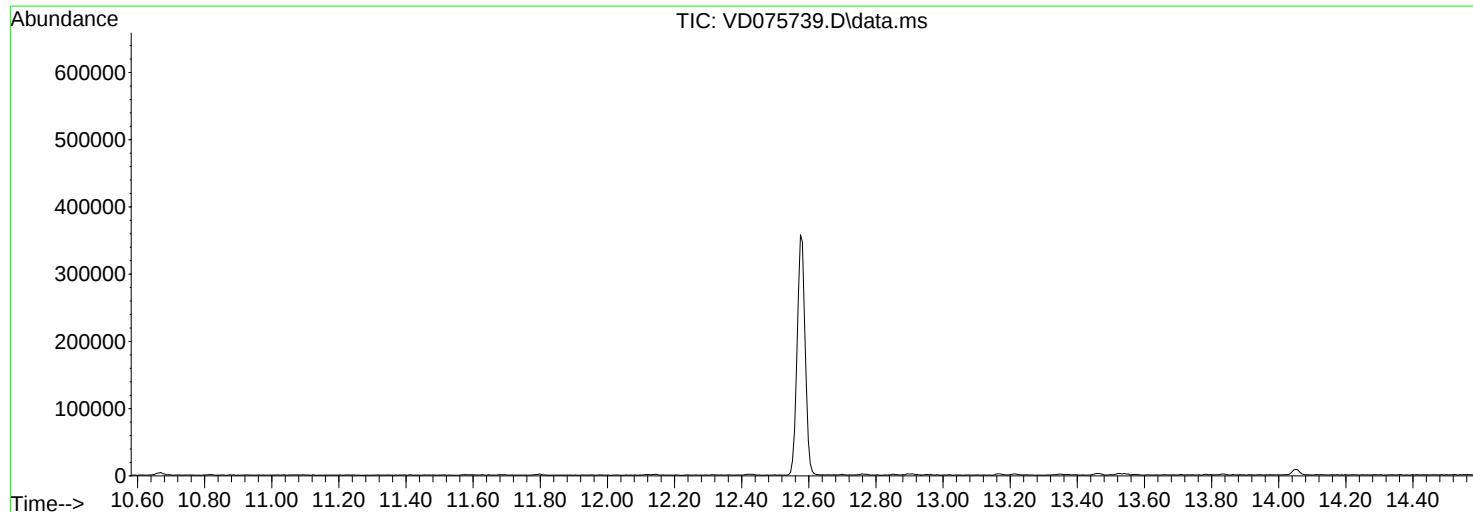

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	9242	PASS
75	95	30	60	47.0	28395	PASS
95	95	100	100	100.0	60424	PASS
96	95	5	9	7.1	4269	PASS
173	174	0.00	2	1.3	717	PASS
174	95	50	100	93.8	56659	PASS
175	174	5	9	7.6	4318	PASS
176	174	95	101	95.1	53877	PASS
177	176	5	9	7.1	3805	PASS