


Bromomethane

Response Ratio

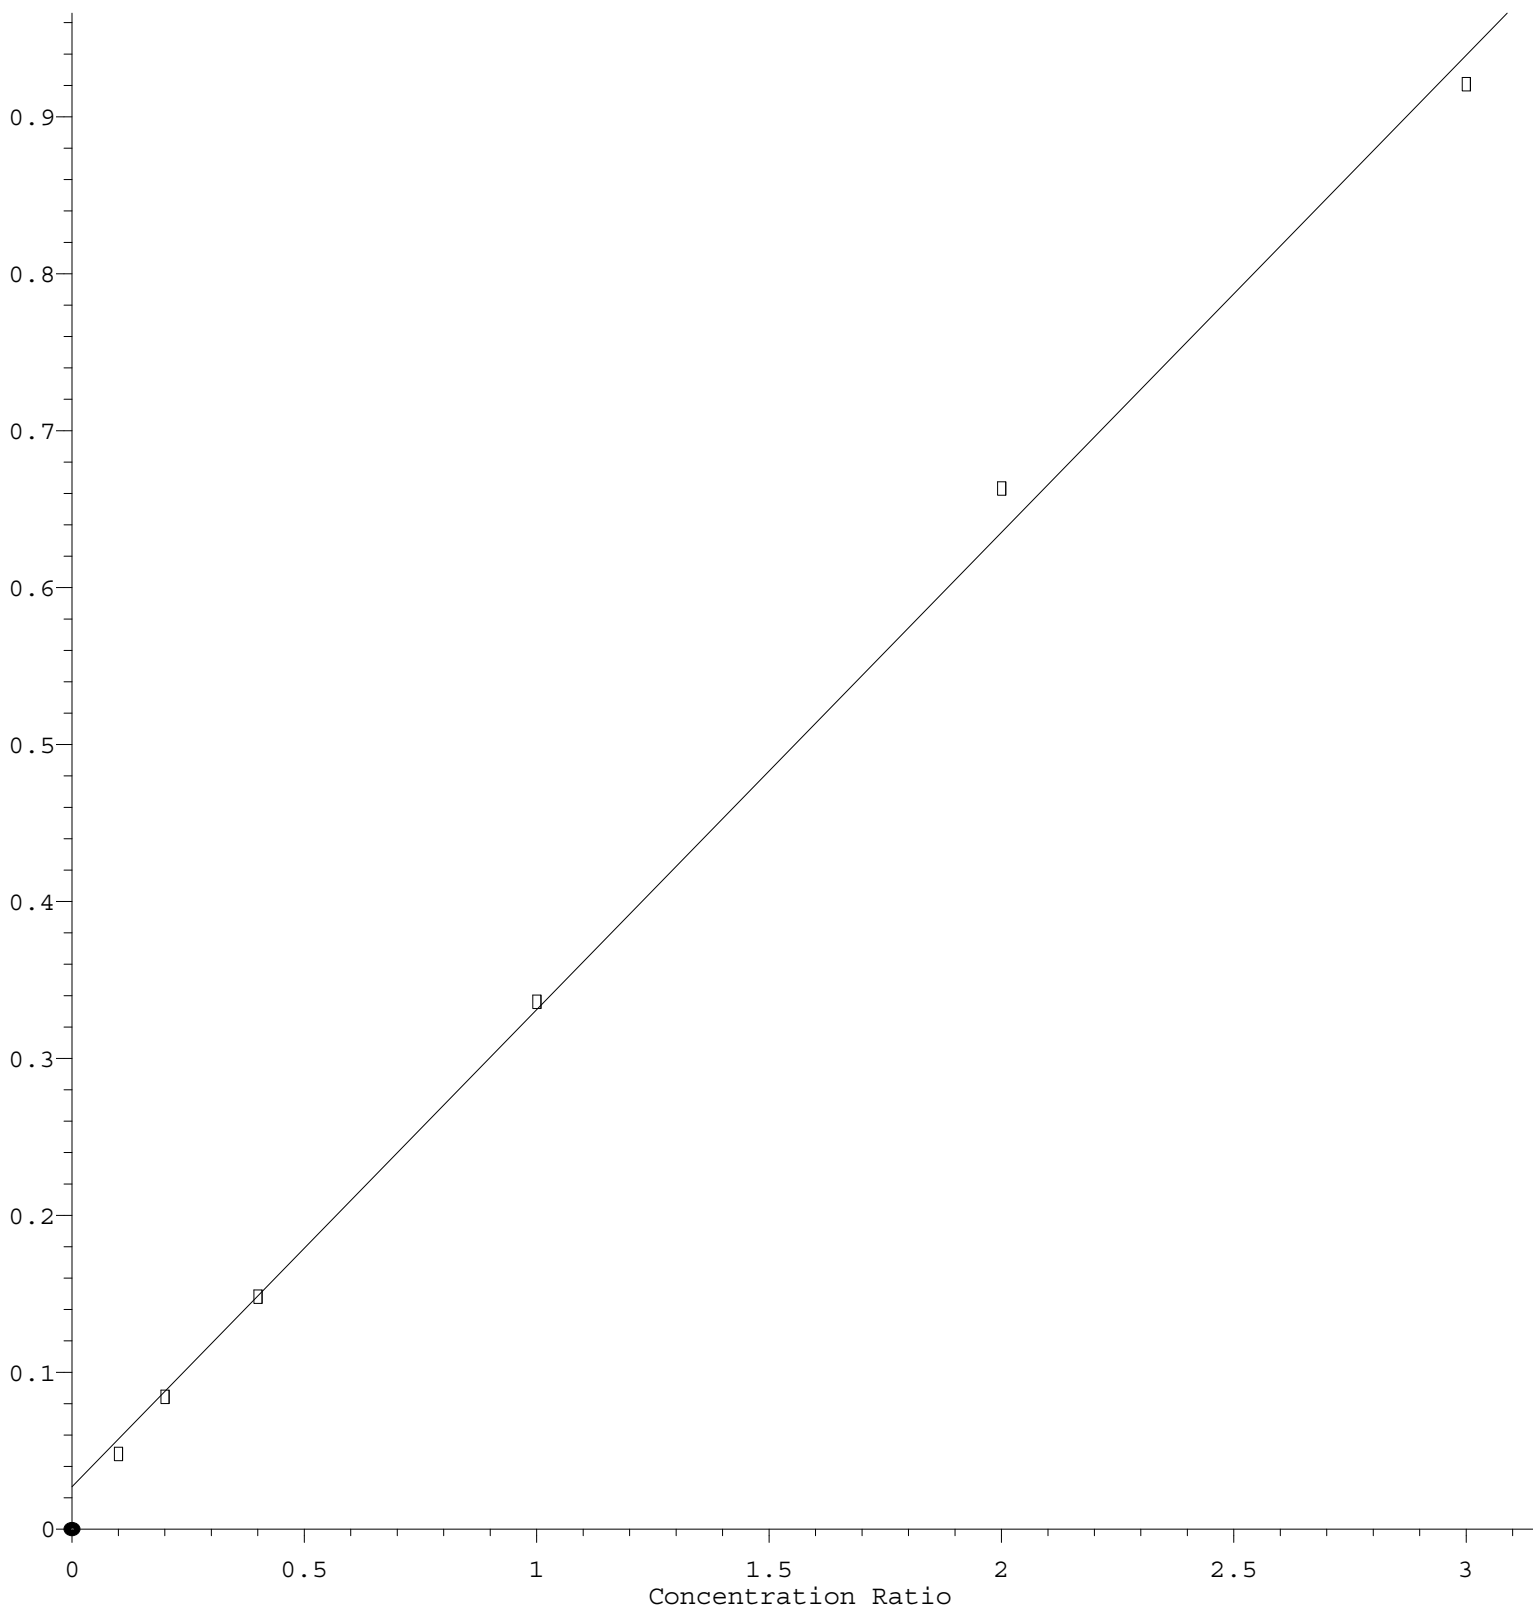


$$\text{Response} = 3.045\text{e-}001 * \text{Amt} + 2.673\text{e-}002$$

Coef of Det (r^2) = 0.997999 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D051922S.M

Calibration Table Last Updated: Thu May 19 15:13:42 2022


Acrolein

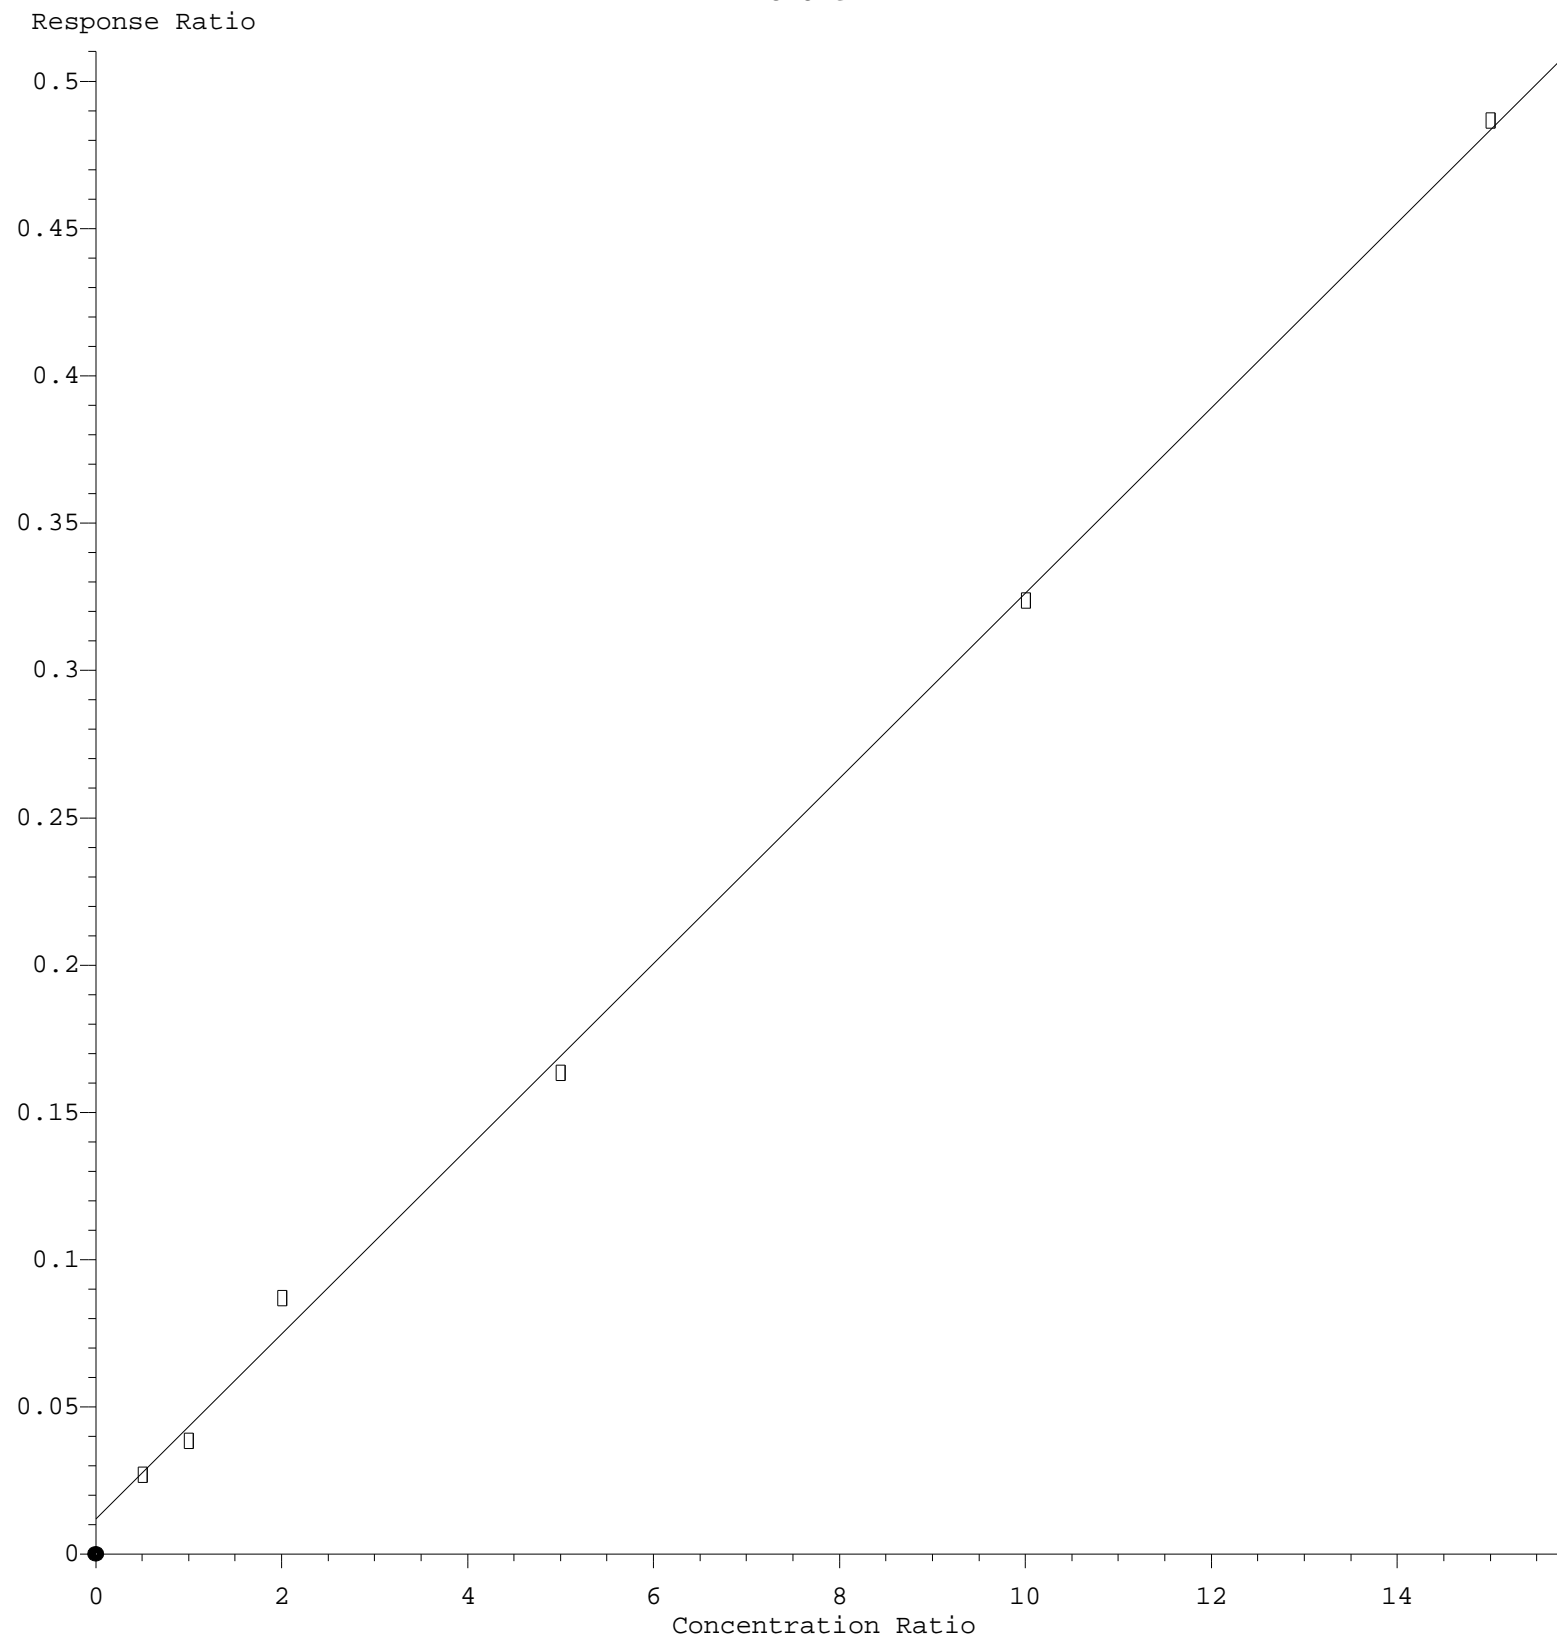

Response = $3.145 \times 10^{-2} \times \text{Amt} + 1.202 \times 10^{-2}$
 Coef of Det (r^2) = 0.998677 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M
 Calibration Table Last Updated: Thu May 19 15:13:42 2022

Methylene Chloride

Response Ratio

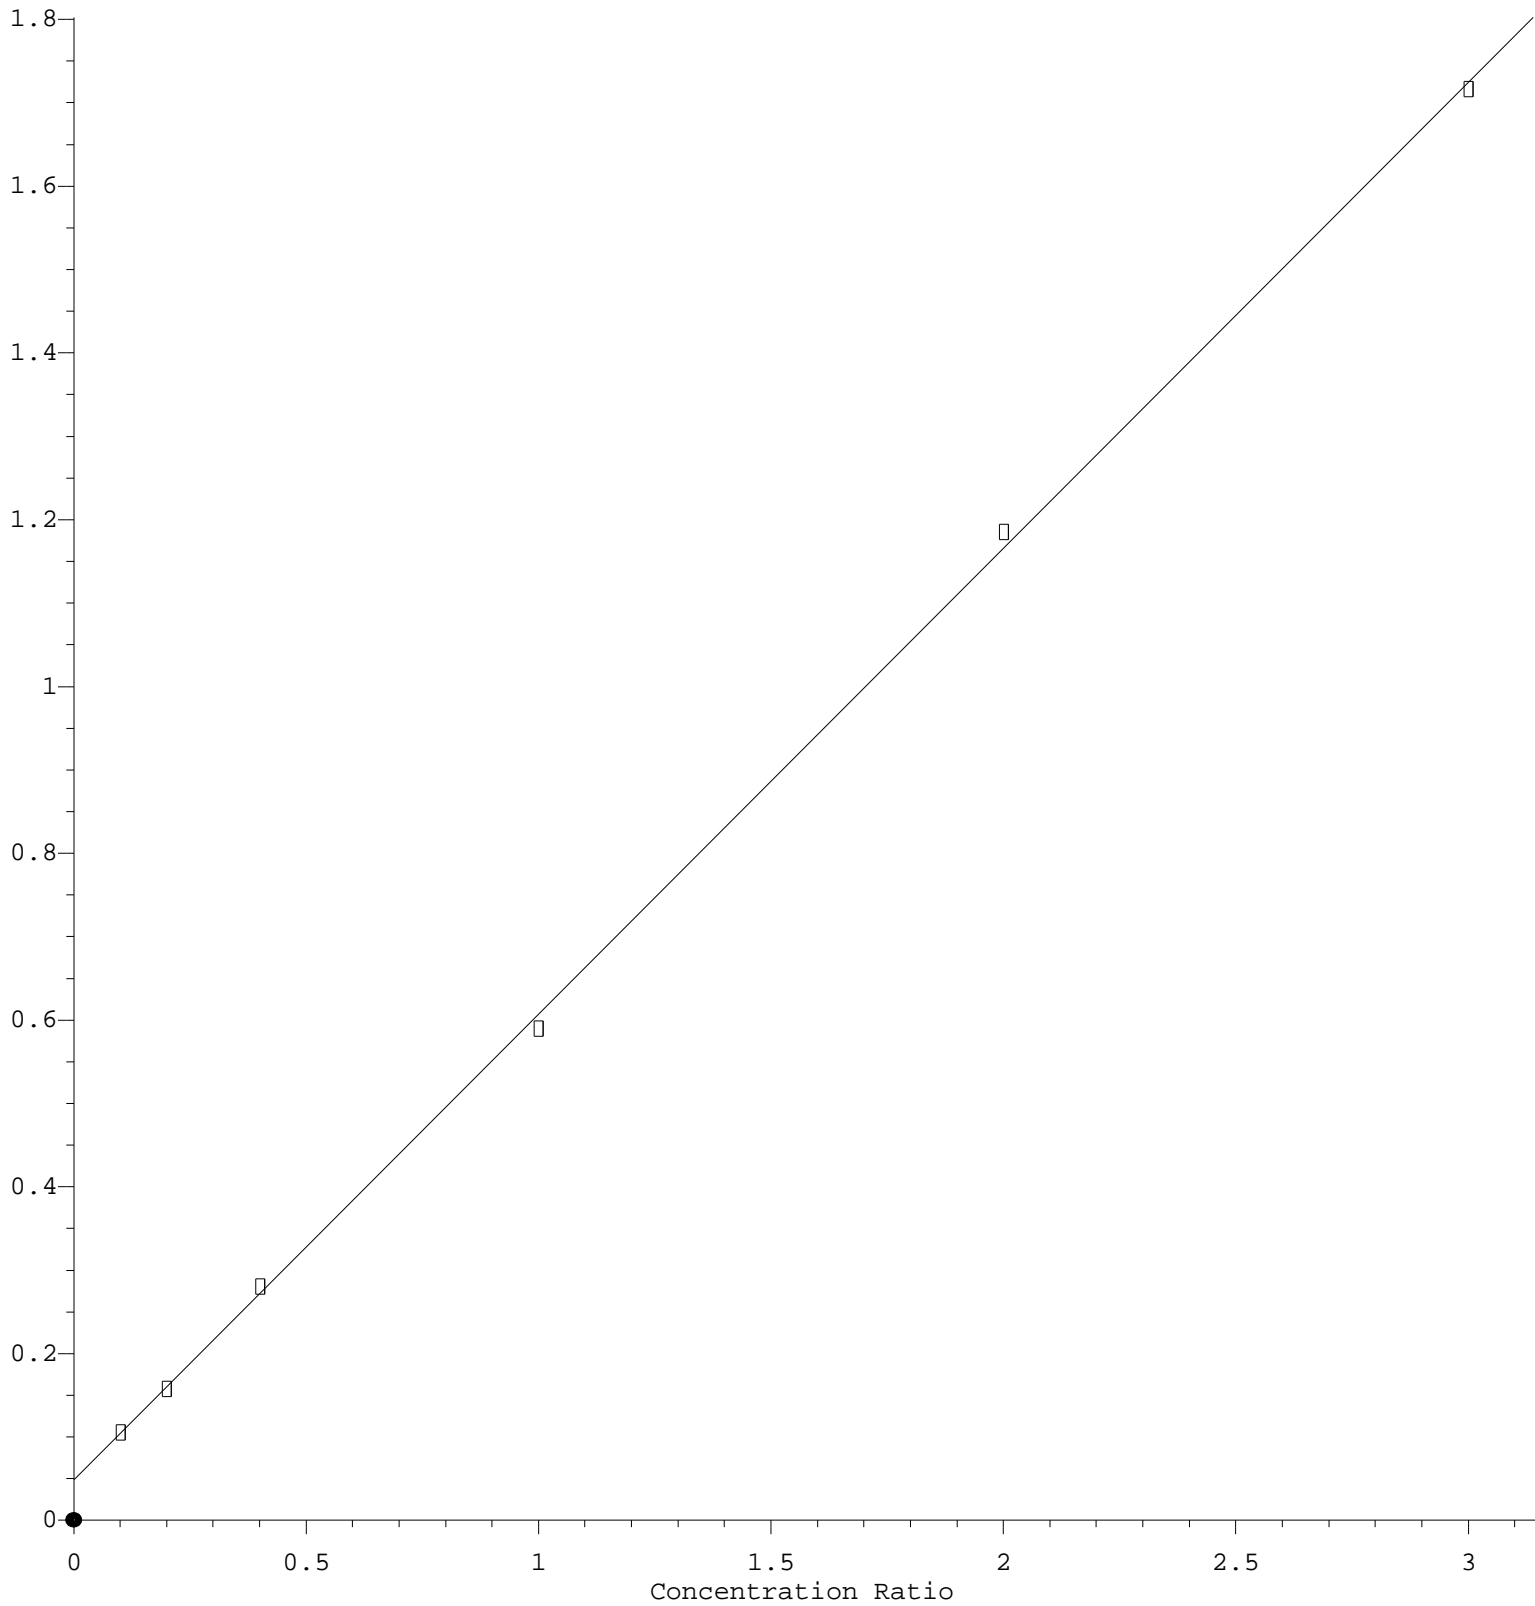

$$\text{Response} = 5.586\text{e-}001 * \text{Amt} + 4.848\text{e-}002$$


Coef of Det (r^2) = 0.999604 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M

Calibration Table Last Updated: Thu May 19 15:13:42 2022

2-Chloroethyl Vinyl ether

Response Ratio

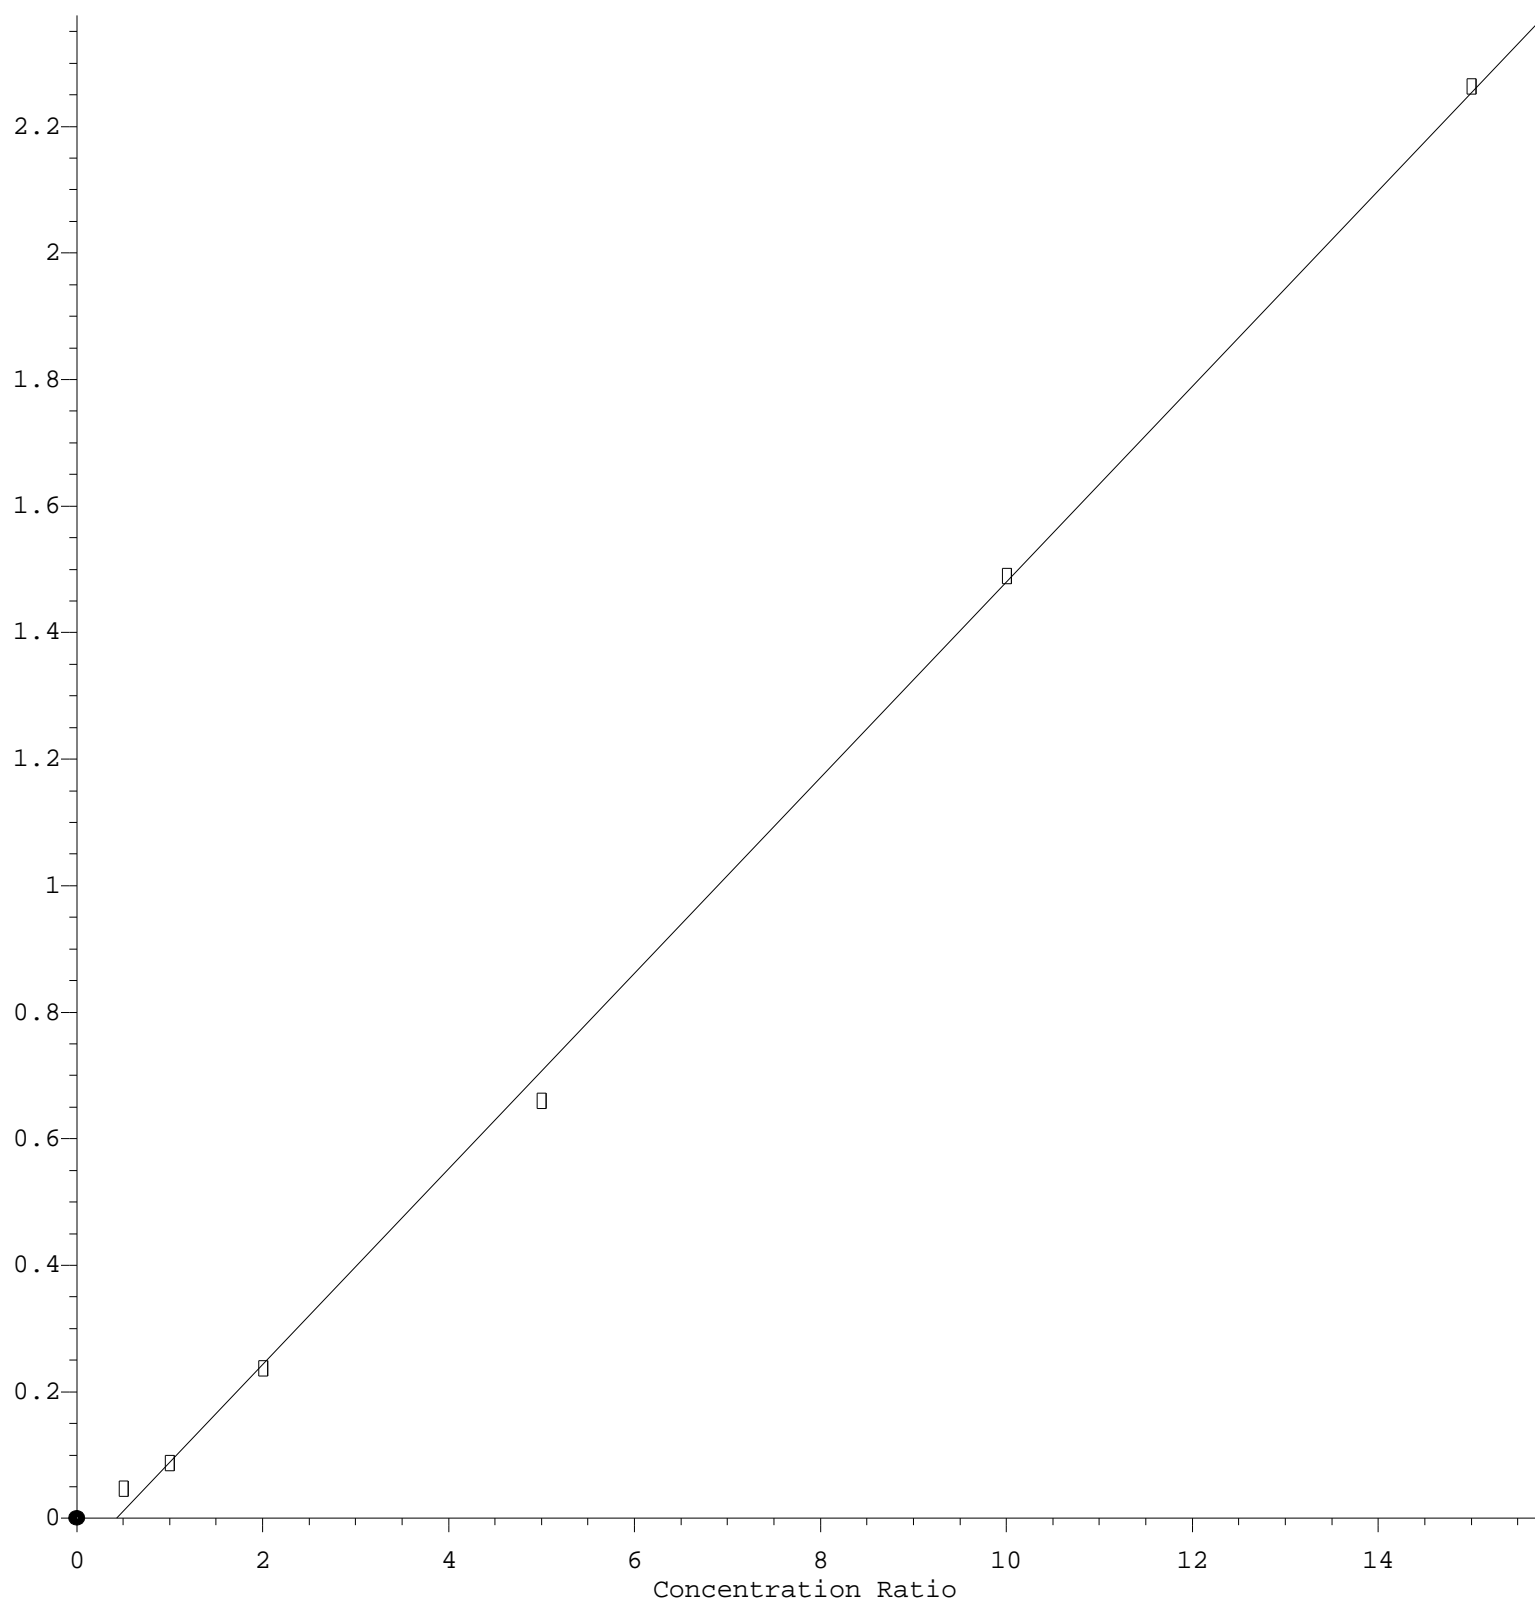

$$\text{Response} = 1.547\text{e-}001 * \text{Amt} - 6.688\text{e-}002$$


Coef of Det (r^2) = 0.999073 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M

Calibration Table Last Updated: Thu May 19 15:13:42 2022

Naphthalene

Response Ratio

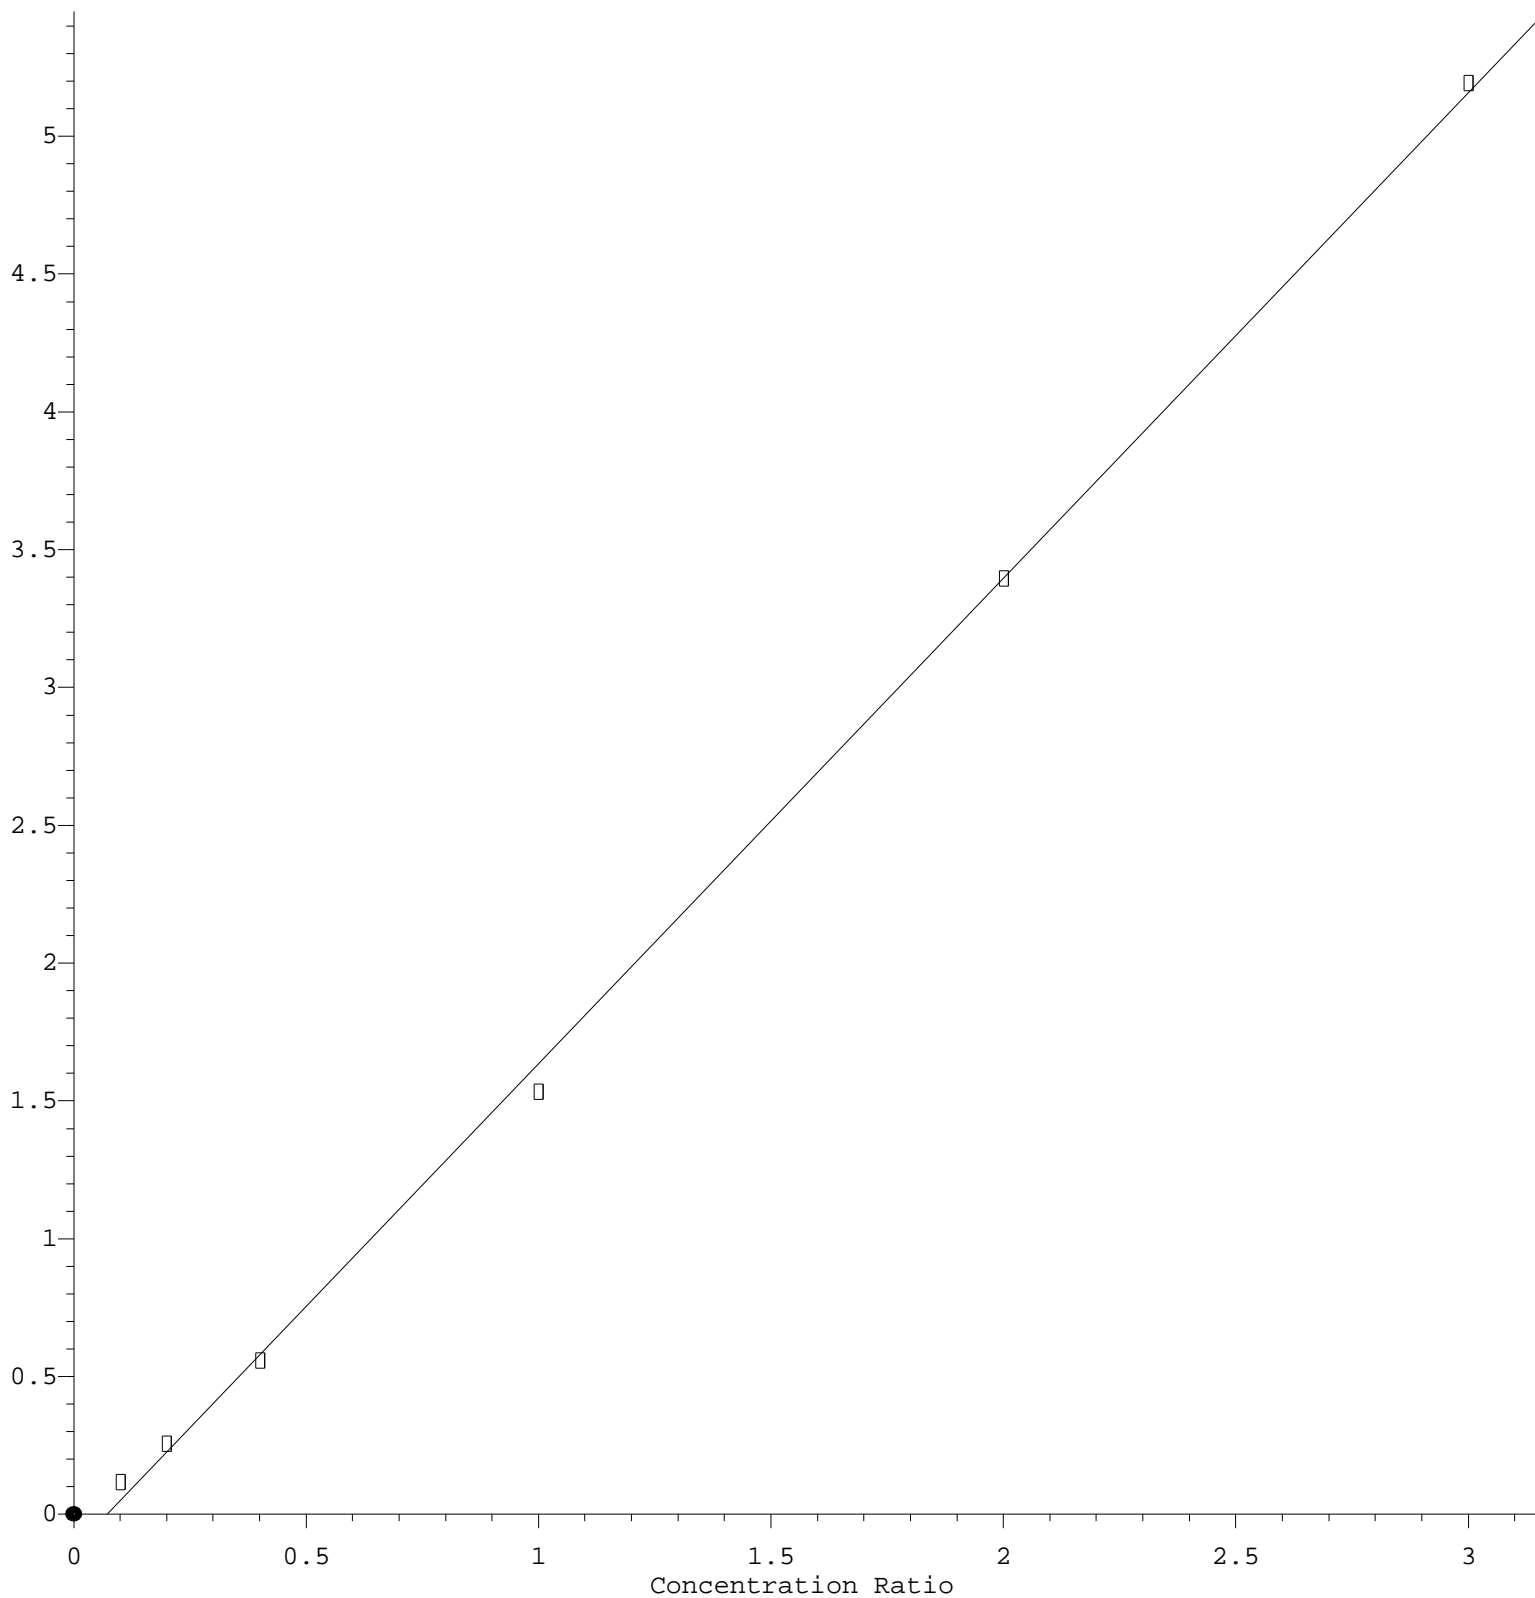

$$\text{Response} = 1.761\text{e}+000 * \text{Amt} - 1.247\text{e}-001$$

Coef of Det (r^2) = 0.999159 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M

Calibration Table Last Updated: Thu May 19 15:13:42 2022