

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD051922\  
 Data File : VD073167.D  
 Acq On : 20 May 2022 06:18  
 Operator : VA/SY  
 Sample : VD0519SBL02  
 Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
 ALS Vial : 41 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 VD0519SBL02

Quant Time: May 20 07:53:53 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D051922S.M  
 Quant Title : SW846 8260  
 QLast Update : Thu May 19 15:13:42 2022  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.973  | 168  | 306356   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.855  | 114  | 550327   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.638 | 117  | 573875   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.561 | 152  | 259753   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.320  | 65    | 168753   | 49.843   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 99.680%  |
| 35) Dibromofluoromethane    | 7.908  | 113   | 186625   | 51.392   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 102.780% |
| 50) Toluene-d8              | 10.332 | 98    | 676240   | 50.517   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 49 - 140 | Recovery | =    | 101.040% |
| 62) 4-Bromofluorobenzene    | 12.620 | 95    | 247780   | 52.744   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 25 - 144 | Recovery | =    | 105.480% |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD051922\  
Data File : VD073167.D  
Acq On : 20 May 2022 06:18  
Operator : VA/SY  
Sample : VD0519SBL02  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
VD0519SBL02

Quant Time: May 20 07:53:53 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D051922S.M  
Quant Title : SW846 8260  
QLast Update : Thu May 19 15:13:42 2022  
Response via : Initial Calibration

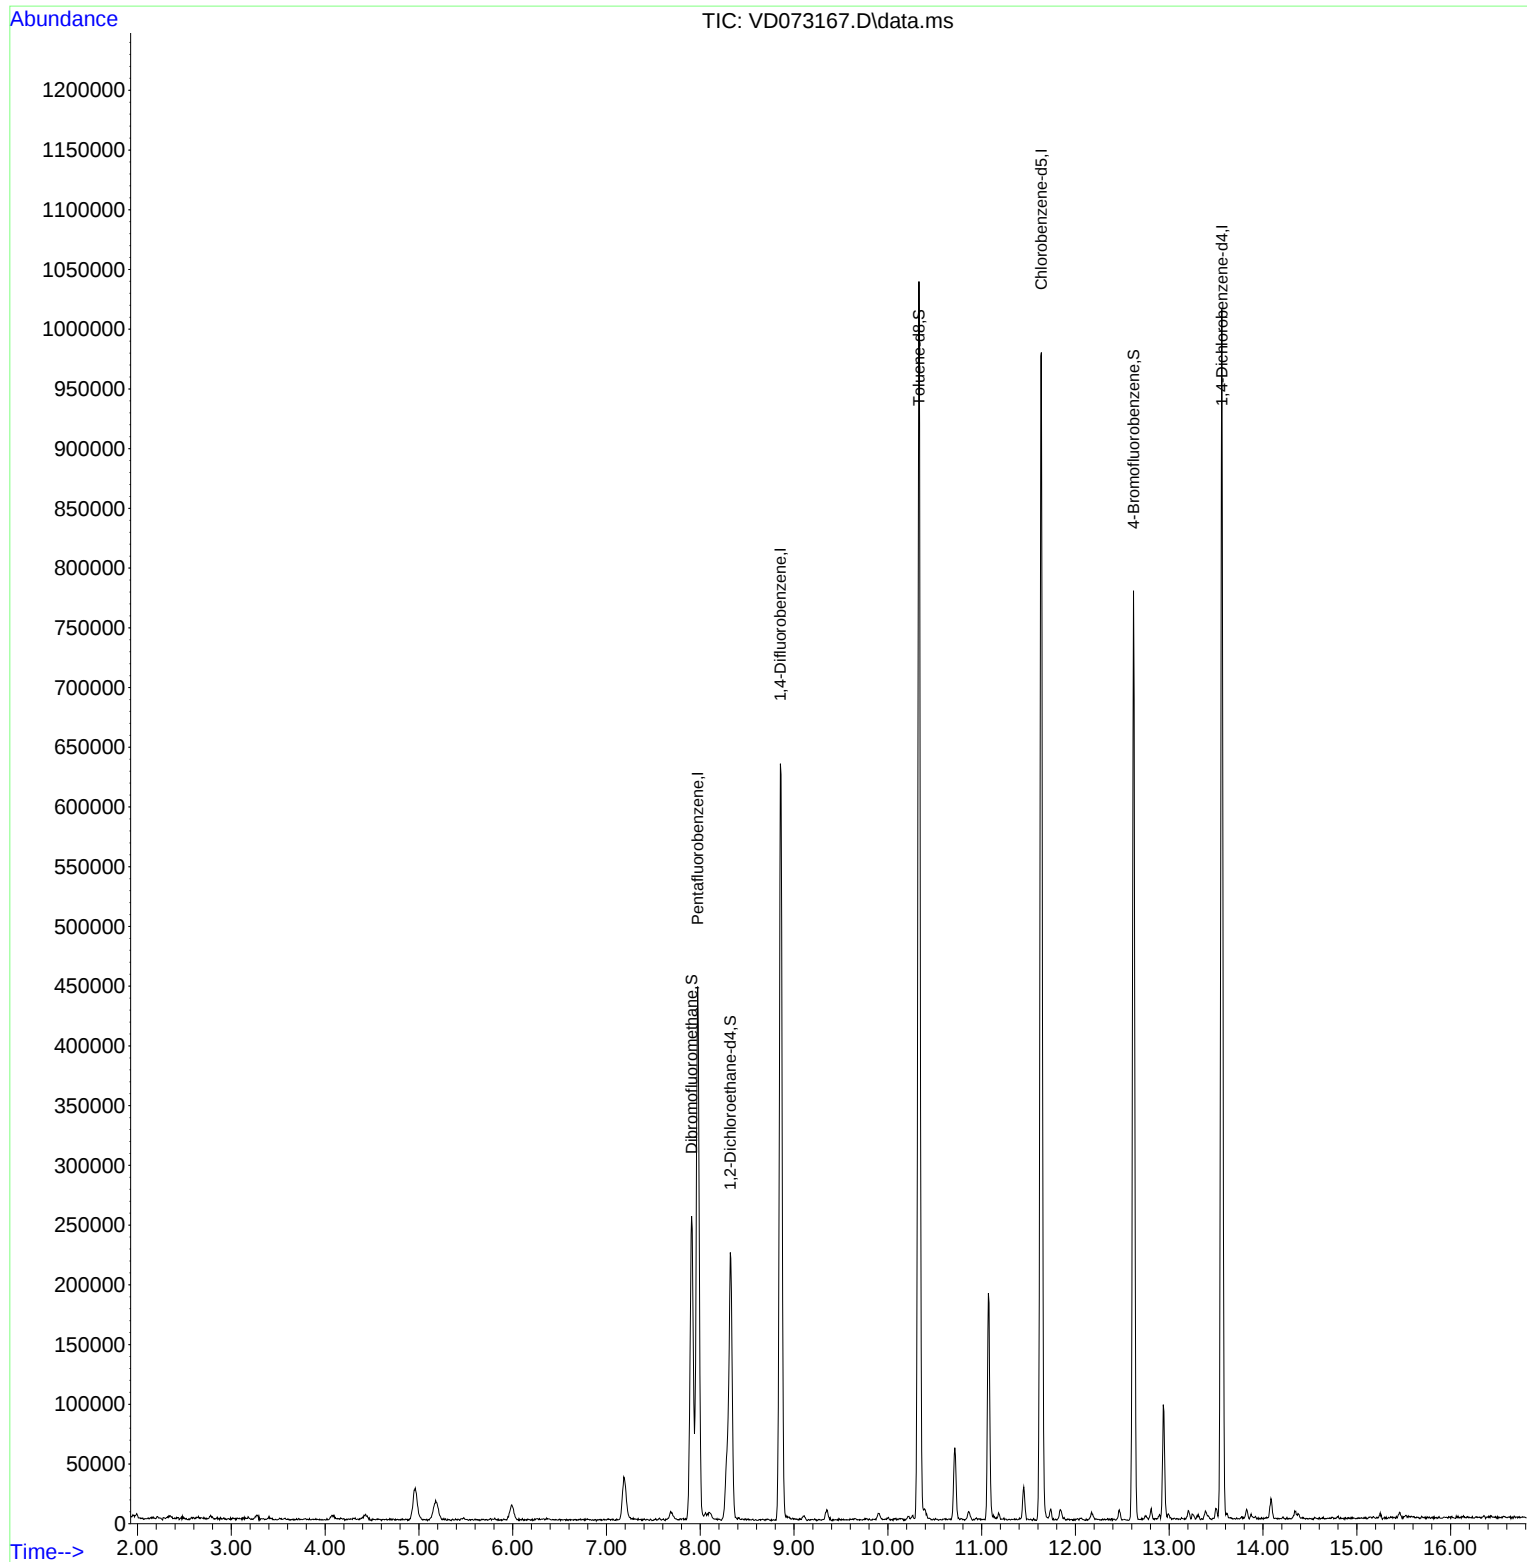

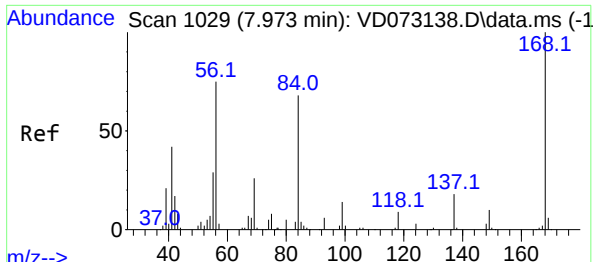

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.973 min Scan# 1029

Delta R.T. 0.000 min

Lab File: VD073167.D

Acq: 20 May 2022 06:18

Instrument :

MSVOA\_D

ClientSampleId :





VD0519SBL02

Tgt Ion:168 Resp: 306356

Ion Ratio Lower Upper

168 100

99 62.2 49.8 74.6

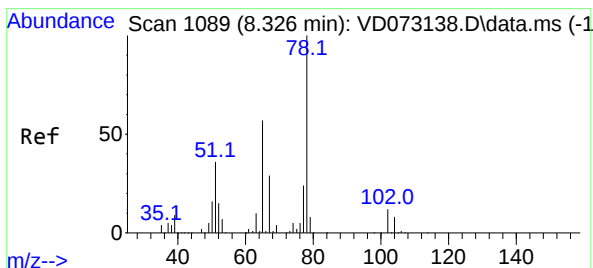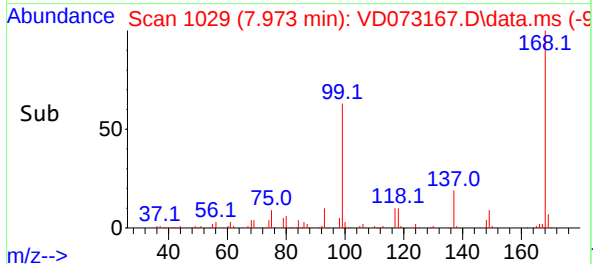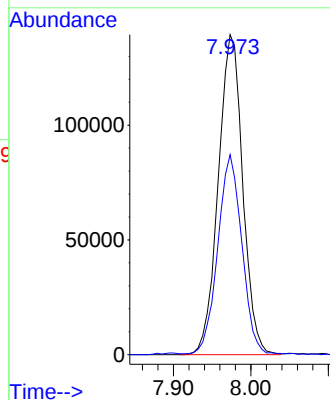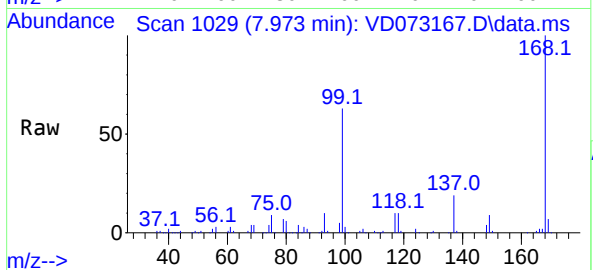

1,2-Dichloroethane-d4

Concen: 49.843 ug/l

RT: 8.320 min Scan# 1088

Delta R.T. -0.006 min

Lab File: VD073167.D




Acq: 20 May 2022 06:18


Tgt Ion: 65 Resp: 168753

Ion Ratio Lower Upper

65 100

67 53.6 0.0 101.4

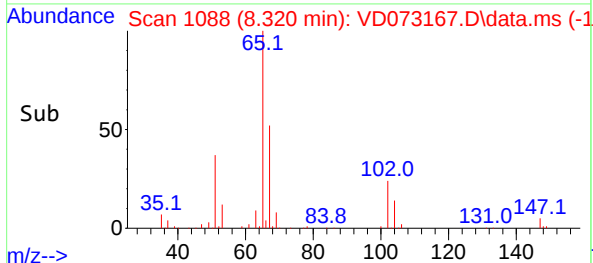
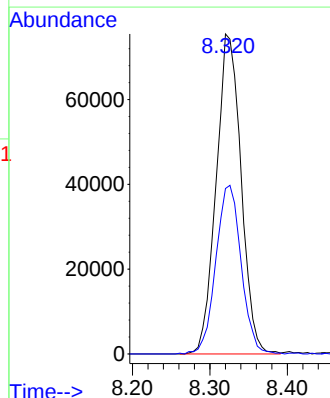
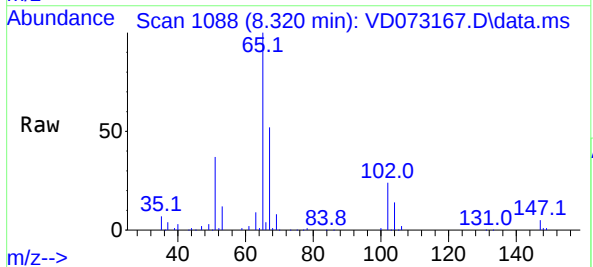


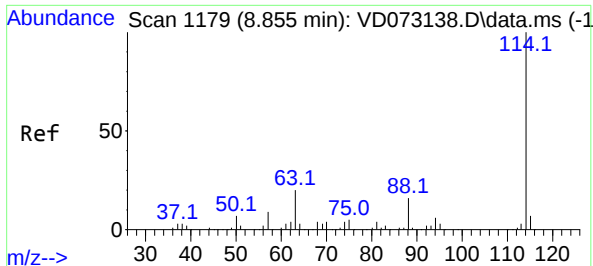

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 8.855 min Scan# 1179  
Delta R.T. 0.000 min  
Lab File: VD073167.D  
Acq: 20 May 2022 06:18




Instrument :  
MSVOA\_D  
ClientSampleId :  
VD0519SBL02


Tgt Ion:114 Resp: 550327  
Ion Ratio Lower Upper  
114 100  
63 20.4 0.0 46.6  
88 16.7 0.0 33.2

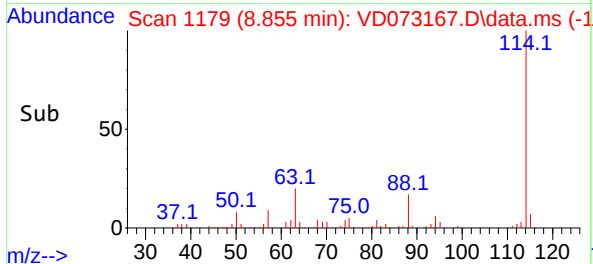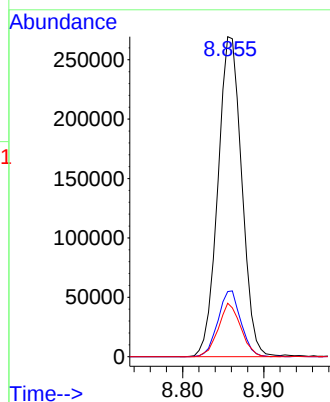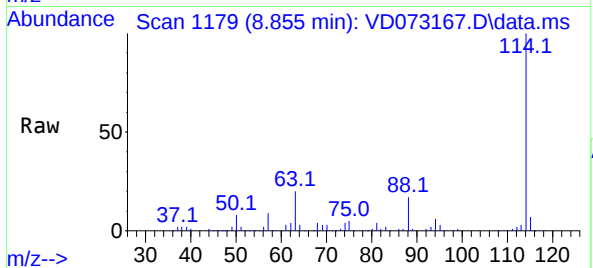

#35  
Dibromofluoromethane  
Concen: 51.392 ug/l  
RT: 7.908 min Scan# 1018  
Delta R.T. -0.006 min  
Lab File: VD073167.D  
Acq: 20 May 2022 06:18

Tgt Ion:113 Resp: 186625  
Ion Ratio Lower Upper  
113 100  
111 101.6 83.8 125.6  
192 17.6 14.6 21.8


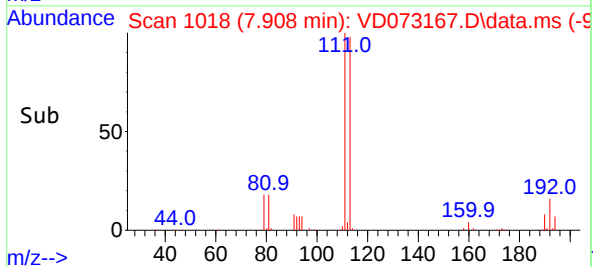
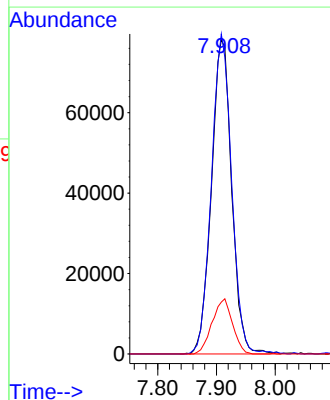
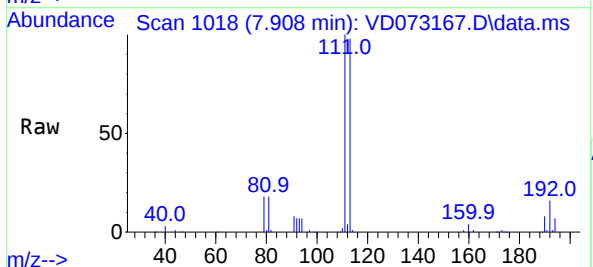


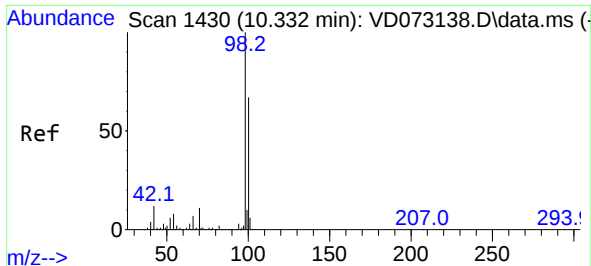

#50  
Toluene-d8  
Concen: 50.517 ug/l  
RT: 10.332 min Scan# 1430  
Delta R.T. -0.000 min  
Lab File: VD073167.D  
Acq: 20 May 2022 06:18




Instrument :  
MSVOA\_D  
ClientSampleId :  
VD0519SBL02


Tgt Ion: 98 Resp: 676240  
Ion Ratio Lower Upper  
98 100  
100 66.6 52.4 78.6

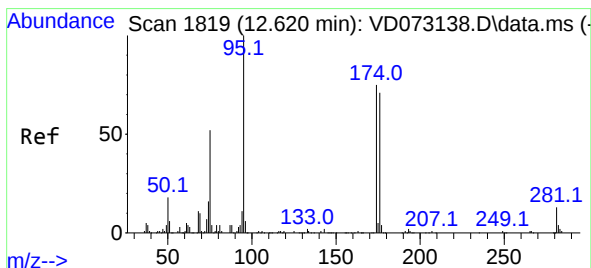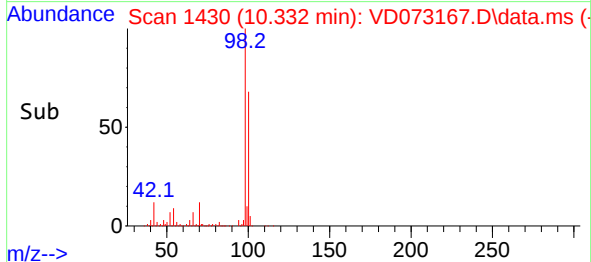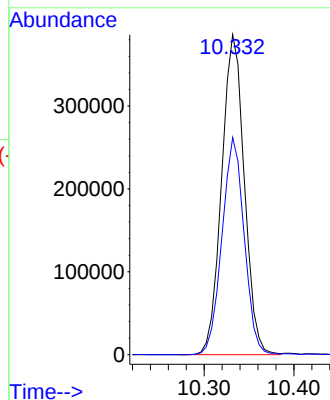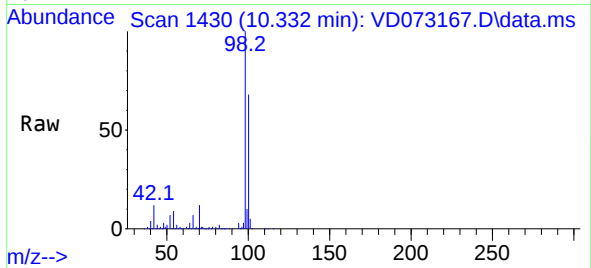

#62  
4-Bromofluorobenzene  
Concen: 52.744 ug/l  
RT: 12.620 min Scan# 1819  
Delta R.T. -0.000 min  
Lab File: VD073167.D  
Acq: 20 May 2022 06:18

Tgt Ion: 95 Resp: 247780  
Ion Ratio Lower Upper  
95 100  
174 75.7 0.0 152.8  
176 73.1 0.0 145.4


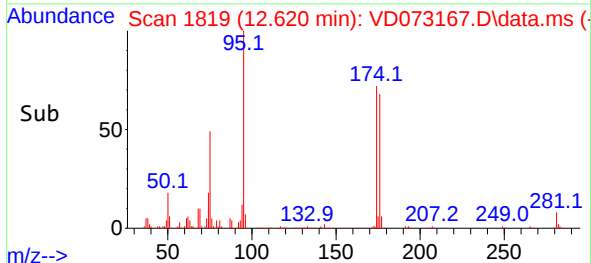
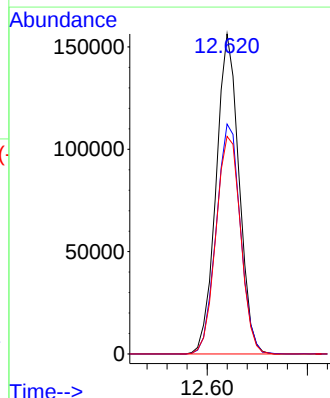
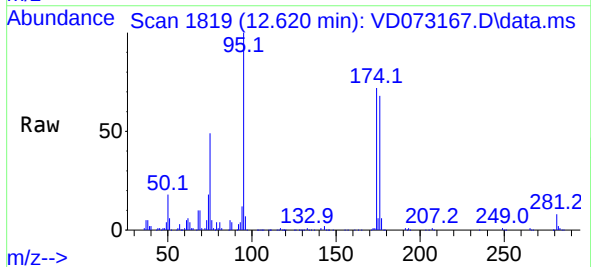


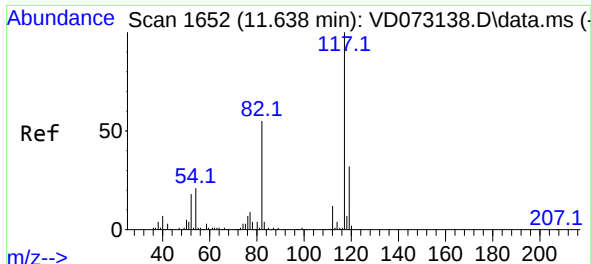

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.638 min Scan# 117  
Delta R.T. -0.000 min  
Lab File: VD073167.D  
Acq: 20 May 2022 06:18

Instrument :  
MSVOA\_D  
ClientSampleId :  
VD0519SBL02

Tgt Ion:117 Resp: 573875  
Ion Ratio Lower Upper  
117 100  
82 55.3 45.3 67.9  
119 31.7 26.6 40.0

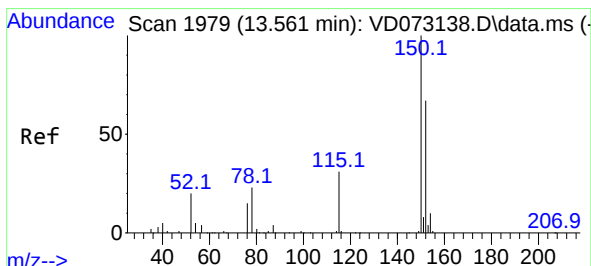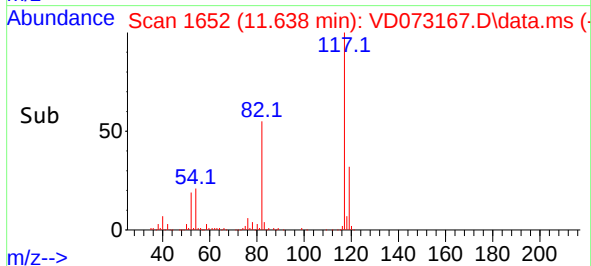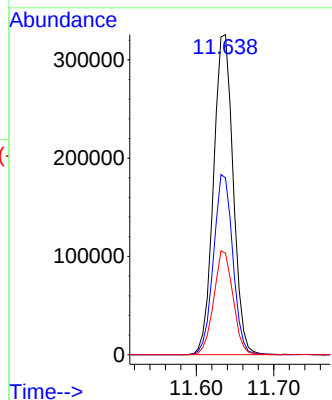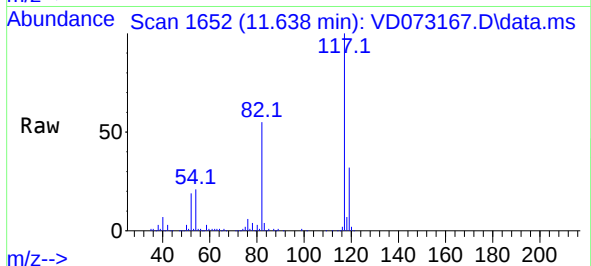

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.561 min Scan# 1979  
Delta R.T. -0.000 min  
Lab File: VD073167.D  
Acq: 20 May 2022 06:18

Tgt Ion:152 Resp: 259753  
Ion Ratio Lower Upper  
152 100  
115 60.0 31.3 93.8  
150 157.2 0.0 348.6

