
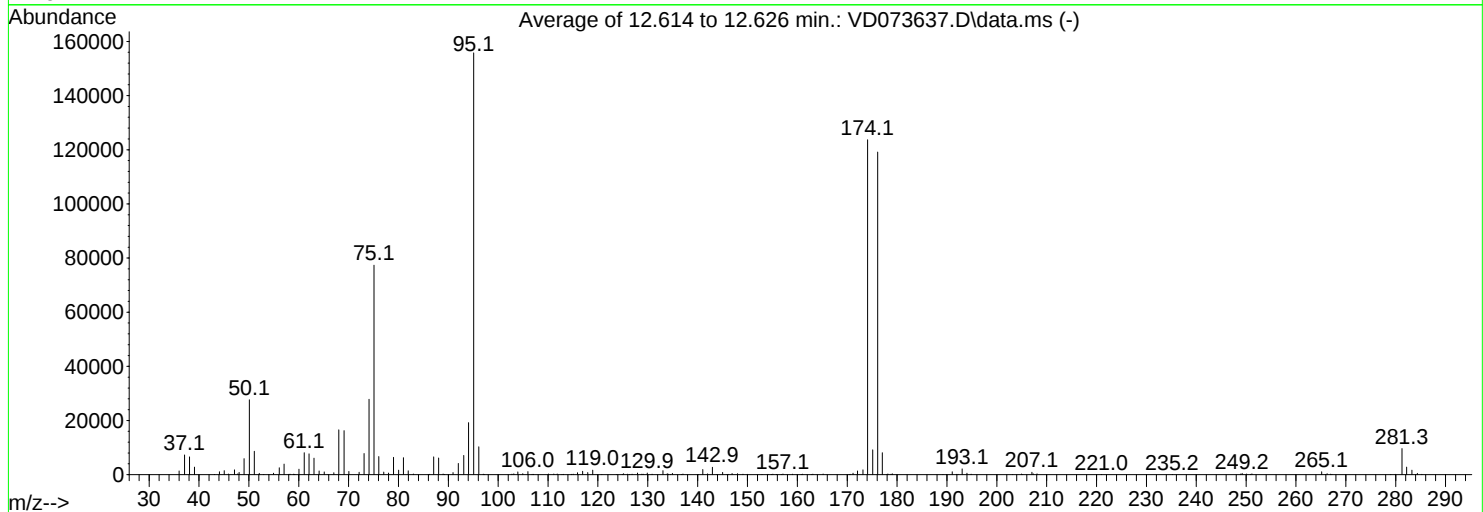


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062122\
Data File : VD073637.D
Acq On : 21 Jun 2022 08:56
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062022S.M
Title : SW846 8260
Last Update : Tue Jun 21 05:24:45 2022

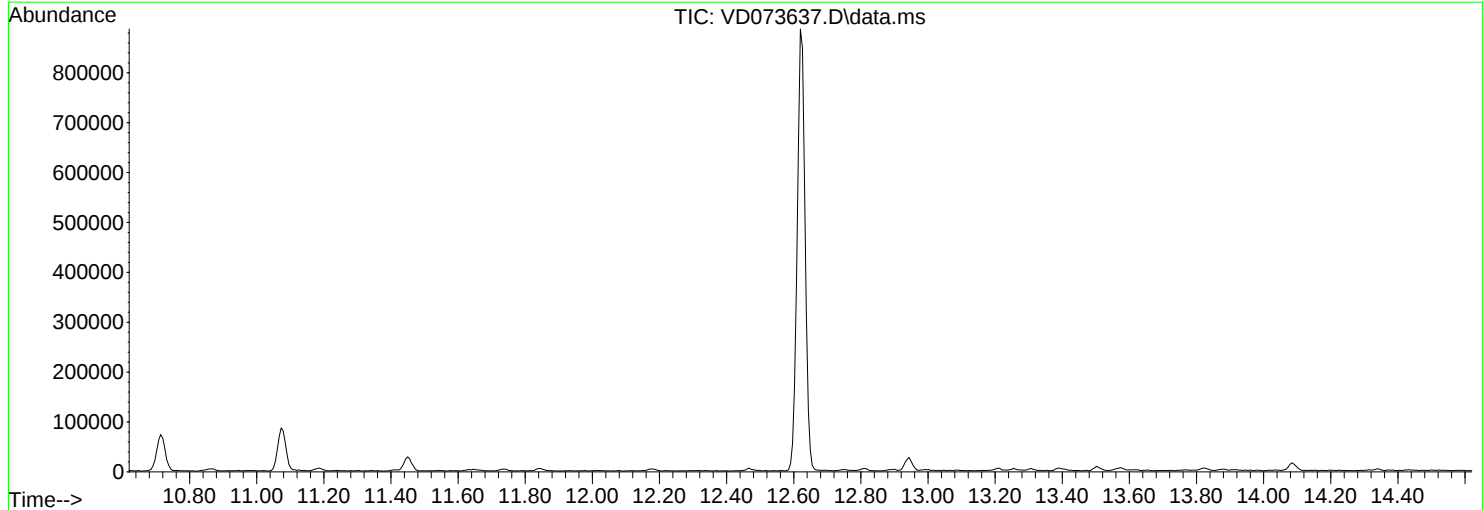

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	27685	PASS
75	95	30	60	49.7	77363	PASS
95	95	100	100	100.0	155800	PASS
96	95	5	9	6.6	10284	PASS
173	174	0.00	2	1.5	1799	PASS
174	95	50	100	79.4	123696	PASS
175	174	5	9	7.4	9136	PASS
176	174	95	101	96.3	119147	PASS
177	176	5	9	6.8	8108	PASS