

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070124\
 Data File : VD079303.D
 Acq On : 01 Jul 2024 18:30
 Operator : RP/MD
 Sample : P3141-01
 Misc : 7.62G/5.0ml/MSVOA_D/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1


Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Jul 02 06:00:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062824S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 29 06:28:31 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.875	168	94623	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.775	114	186755	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.575	117	160665	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	51606	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	55218	60.536	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	121.080%
35) Dibromofluoromethane	7.810	113	68640	55.994	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	111.980%
50) Toluene-d8	10.269	98	189460	42.961	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	85.920%
62) 4-Bromofluorobenzene	12.569	95	61827	43.720	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	87.440%
Target Compounds						
					Qvalue	
5) Bromomethane	2.699	94	248	Below Cal	#	24
10) Methyl Iodide	4.169	142	64	6.182	ug/l #	41
16) Acetone	4.022	43	5645	25.136	ug/l	95
17) Carbon Disulfide	4.269	76	4560	1.043	ug/l #	82
18) Methyl Acetate	4.563	43	787	1.206	ug/l #	56
20) Methylene Chloride	4.805	84	32504	17.414	ug/l	90
25) 2-Butanone	7.075	43	400	1.278	ug/l #	42
31) Cyclohexane	7.875	56	2426	1.206	ug/l #	1
38) Carbon Tetrachloride	7.875	117	10848	5.609	ug/l #	18
48) Methyl methacrylate	9.275	41	857	1.358	ug/l #	34
55) 1,1,2-Trichloroethane	10.704	97	2624	2.479	ug/l #	15
56) Ethyl methacrylate	10.610	69	711	4.183	ug/l #	51
64) Tetrachloroethene	10.810	164	1040	1.039	ug/l #	85
68) m/p-Xylenes	11.798	106	3296	1.370	ug/l #	59
74) N-amyl acetate	12.210	43	9467	11.243	ug/l #	77
76) 1,2,3-Trichloropropane	12.569	75	31977	61.917	ug/l #	100
78) n-propylbenzene	12.757	91	7626	1.553	ug/l	91
79) 2-Chlorotoluene	12.840	91	4618	1.682	ug/l	70
80) 1,3,5-Trimethylbenzene	12.898	105	5647	1.739	ug/l	88
81) trans-1,4-Dichloro-2-b...	12.569	75	31977	114.894	ug/l #	19
82) 4-Chlorotoluene	12.940	91	5873	2.036	ug/l	88
84) 1,2,4-Trimethylbenzene	13.216	105	4663	1.434	ug/l	94
85) sec-Butylbenzene	13.339	105	5165	1.234	ug/l	96
87) 1,3-Dichlorobenzene	13.457	146	2717	1.481	ug/l #	59
88) 1,4-Dichlorobenzene	13.534	146	2852	1.564	ug/l #	38
89) n-Butylbenzene	13.781	91	9292	2.740	ug/l	96
91) 1,2-Dichlorobenzene	13.822	146	1606	1.017	ug/l #	1
93) 1,2,4-Trichlorobenzene	15.092	180	3001	3.564	ug/l #	61
94) Hexachlorobutadiene	15.198	225	1585	3.385	ug/l	85
95) Naphthalene	15.334	128	3506	2.133	ug/l #	84
96) 1,2,3-Trichlorobenzene	15.510	180	5037	6.765	ug/l	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1
Delta R.T. 0.000 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30

Instrument :
MSVOA_D
ClientSampleId :



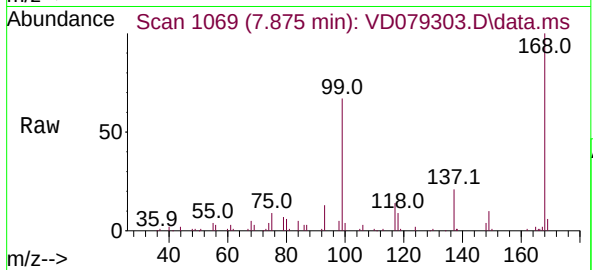



Tgt Ion:168 Resp: 94623
Ion Ratio Lower Upper
168 100
99 66.6 41.1 61.7#

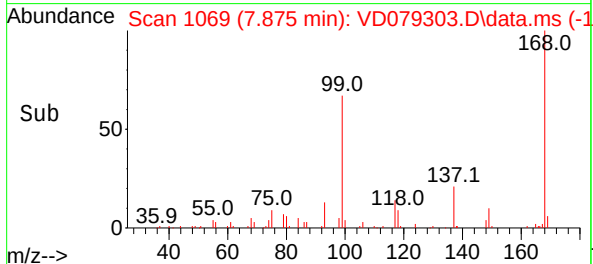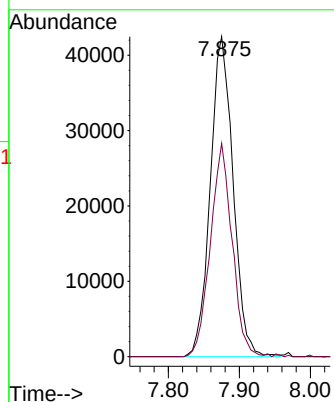

#5
Bromomethane
Concen: Below Cal
RT: 2.699 min Scan# 189
Delta R.T. 0.041 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30

Tgt Ion: 94 Resp: 248
Ion Ratio Lower Upper
94 100
96 22.2 76.9 115.3#

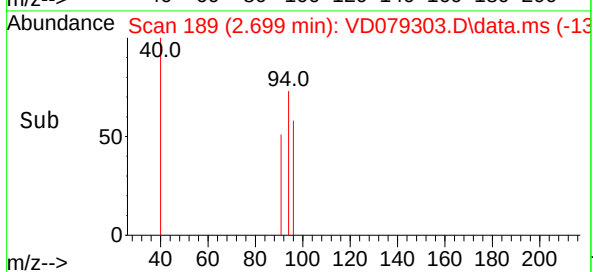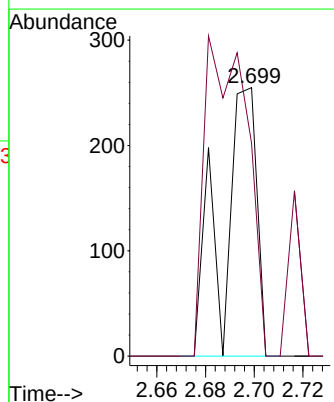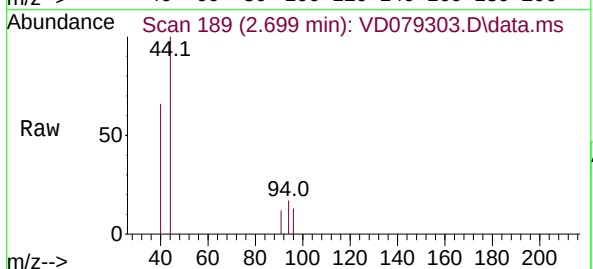

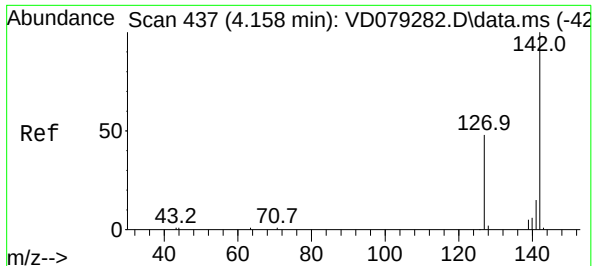

#10

Methyl Iodide

Concen: 6.182 ug/l

RT: 4.169 min Scan# 41

Delta R.T. 0.011 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Instrument :

MSVOA_D

ClientSampleId :





Tgt Ion:142 Resp: 64

Ion Ratio Lower Upper

142 100

127 0.0 34.2 51.4#

141 0.0 11.7 17.5#

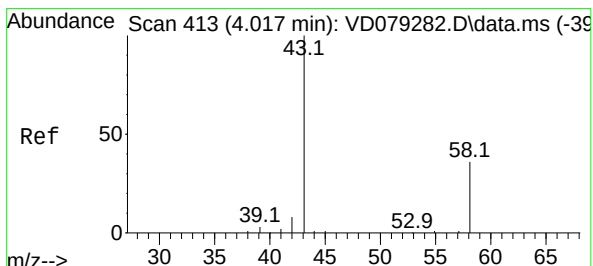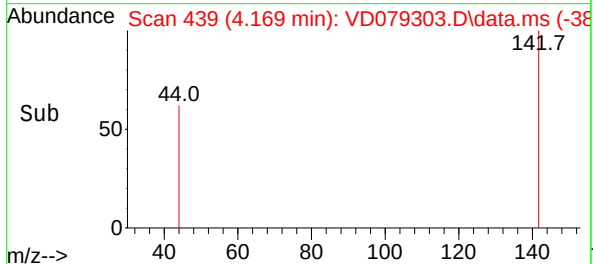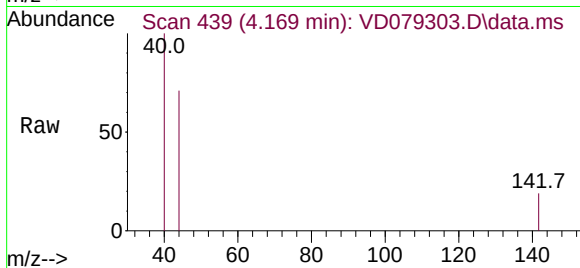

#16

Acetone

Concen: 25.136 ug/l

RT: 4.022 min Scan# 414

Delta R.T. 0.006 min

Lab File: VD079303.D




Acq: 01 Jul 2024 18:30


Tgt Ion: 43 Resp: 5645

Ion Ratio Lower Upper

43 100

58 40.9 30.4 45.6




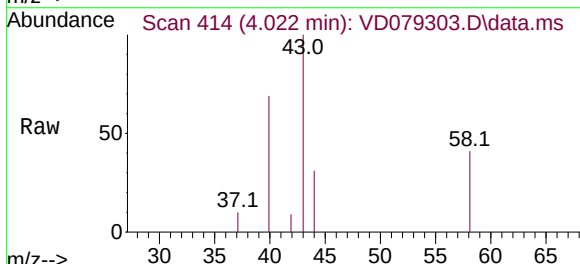




#17
Carbon Disulfide
Concen: 1.043 ug/l
RT: 4.269 min Scan# 455
Delta R.T. 0.006 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 76 Resp: 4560
Ion Ratio Lower Upper
76 100
78 14.9 6.9 10.3#

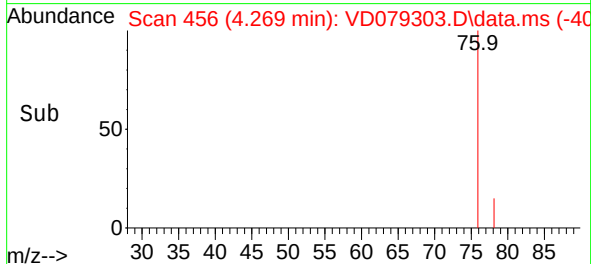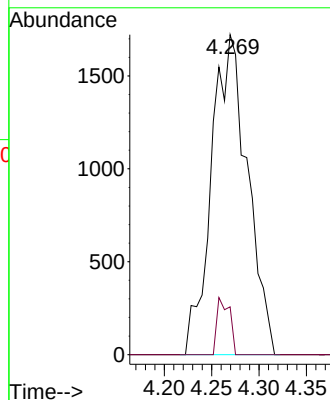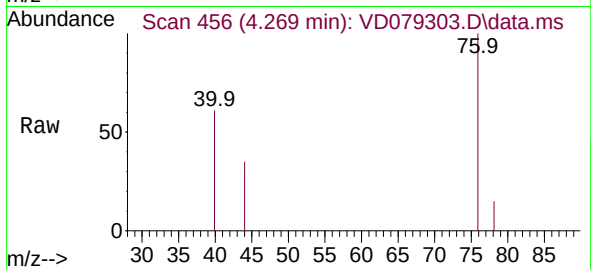

#18
Methyl Acetate
Concen: 1.206 ug/l
RT: 4.563 min Scan# 506
Delta R.T. 0.006 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30


Tgt Ion: 43 Resp: 787
Ion Ratio Lower Upper
43 100
74 9.5 28.1 42.1#

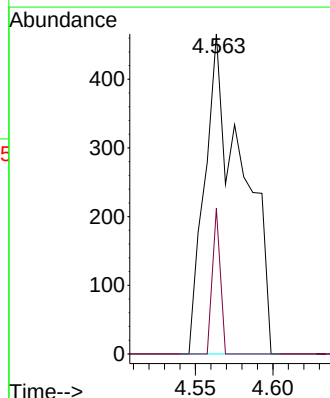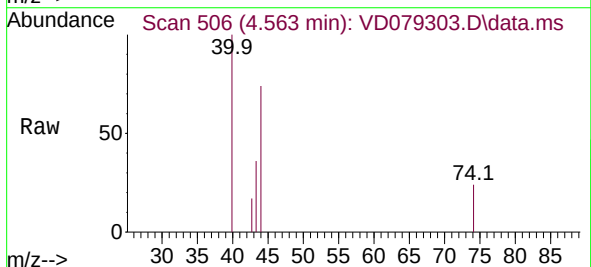






#20
Methylene Chloride
Concen: 17.414 ug/l
RT: 4.805 min Scan# 545
Delta R.T. 0.012 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30

Instrument :
MSVOA_D
ClientSampleId :







Tgt Ion: 84	Resp: 32504
Ion Ratio	Lower Upper
84 100	
49 108.8	75.6 113.4
51 30.9	24.2 36.2
86 65.7	49.2 73.8

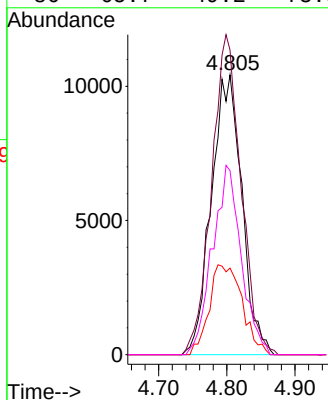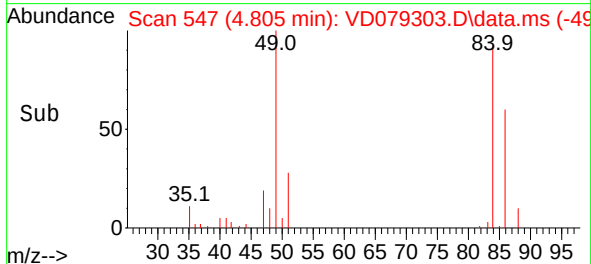

#25
2-Butanone
Concen: 1.278 ug/l
RT: 7.075 min Scan# 933
Delta R.T. -0.000 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30


Tgt Ion: 43	Resp: 400
Ion Ratio	Lower Upper
43 100	
72 0.0	26.4 39.6#

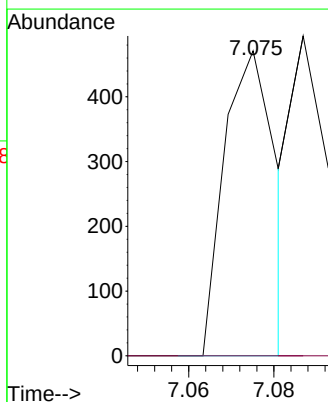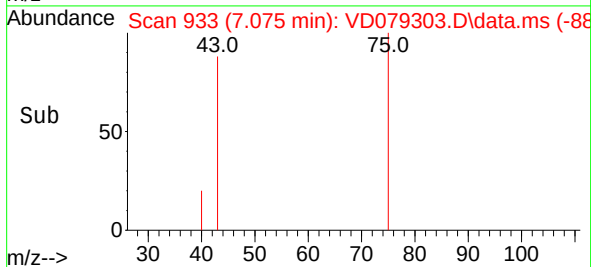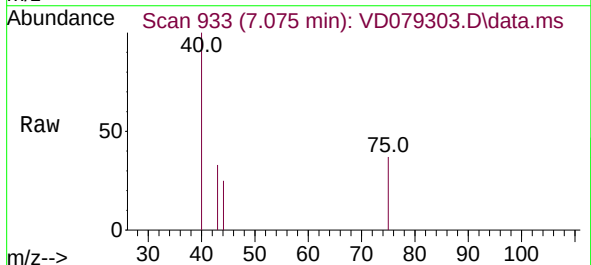






#31
Cyclohexane
Concen: 1.206 ug/l
RT: 7.875 min Scan# 1109
Delta R.T. -0.000 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30

Instrument :
MSVOA_D
ClientSampleId :



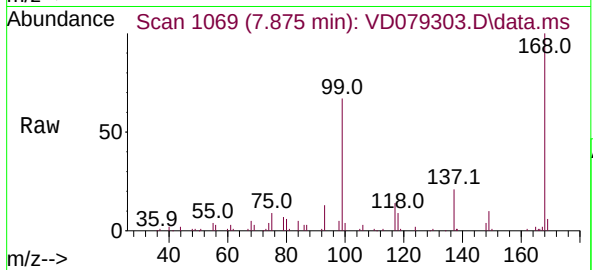



Tgt Ion: 56 Resp: 2426
Ion Ratio Lower Upper
56 100
69 137.9 28.0 42.0#
84 188.0 87.4 131.0#

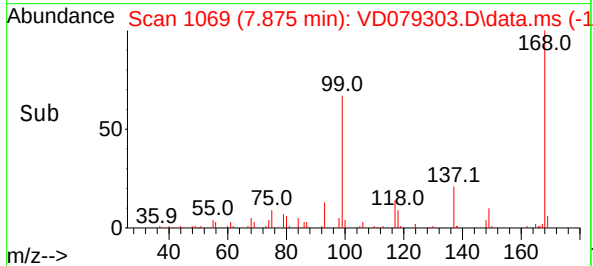

#33
1,2-Dichloroethane-d4
Concen: 60.536 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30

Tgt Ion: 65 Resp: 55218
Ion Ratio Lower Upper
65 100
67 55.5 0.0 111.0

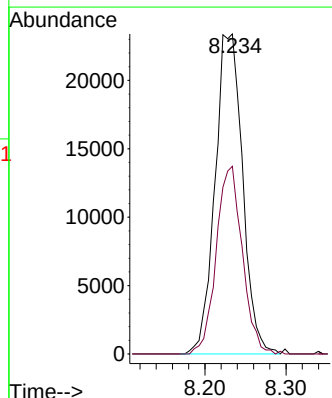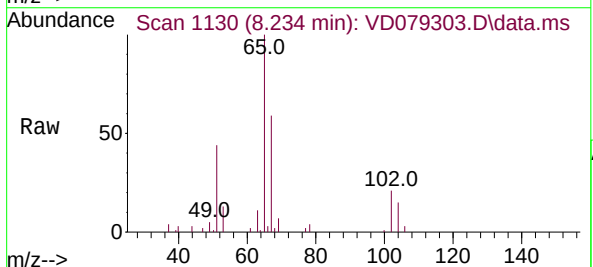

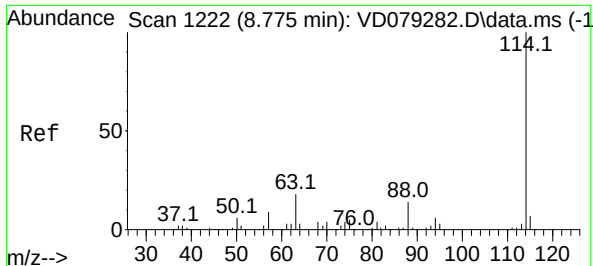

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 11

Delta R.T. -0.000 min MSVOA_D

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Instrument :

MSVOA_D

ClientSampleId :





Tgt Ion:114 Resp: 186755

Ion Ratio Lower Upper

114 100

63 20.9 0.0 34.0

88 17.1 0.0 27.2

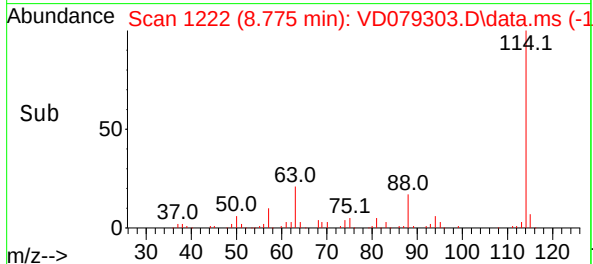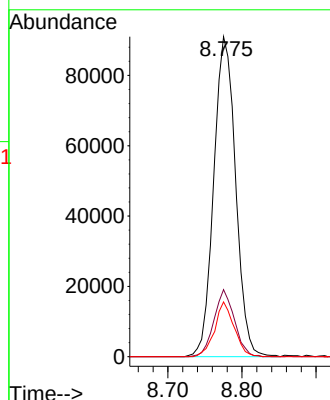

#35

Dibromofluoromethane

Concen: 55.994 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30




Tgt Ion:113 Resp: 68640


Ion Ratio Lower Upper

113 100

111 103.5 84.0 126.0

192 16.3 15.4 23.0

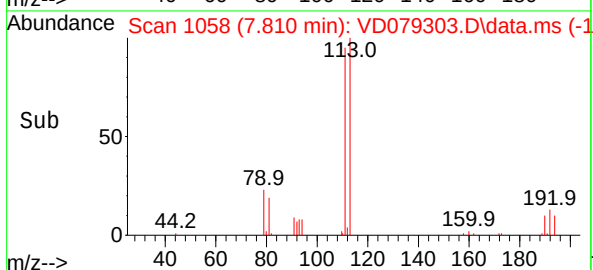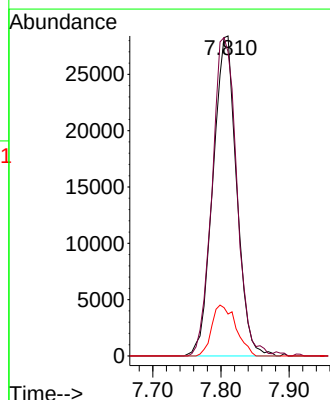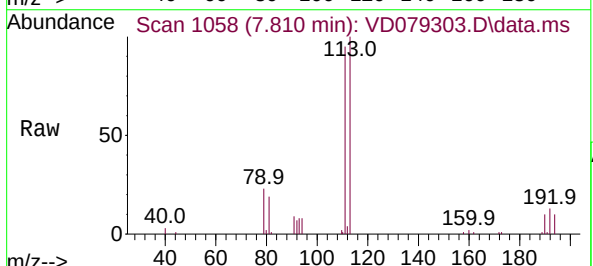



#38

Carbon Tetrachloride

Concen: 5.609 ug/l

RT: 7.875 min Scan# 1

Delta R.T. -0.112 min


Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Instrument :

MSVOA_D

ClientSampleId :

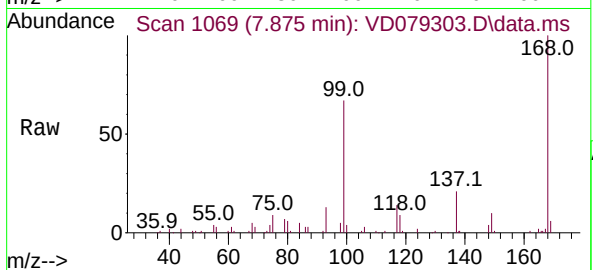




Tgt Ion:117 Resp: 10848

Ion Ratio Lower Upper

117 100

119 7.0 75.4 113.0#

121 0.0 25.0 37.4#

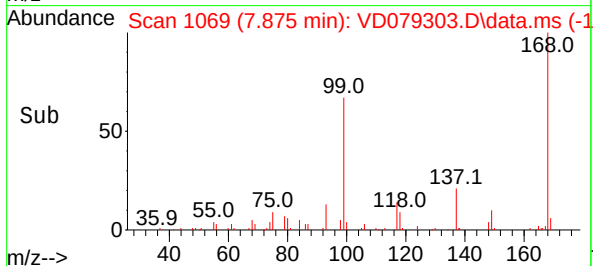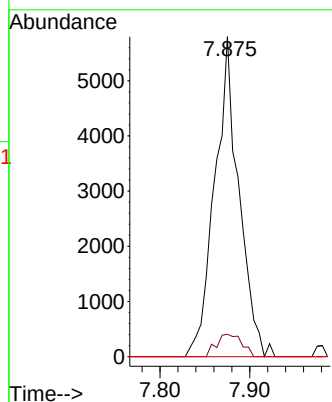

#48

Methyl methacrylate

Concen: 1.358 ug/l

RT: 9.275 min Scan# 1307

Delta R.T. -0.100 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30




Tgt Ion: 41 Resp: 857


Ion Ratio Lower Upper

41 100

69 19.5 96.7 145.1#

39 47.7 43.8 65.6


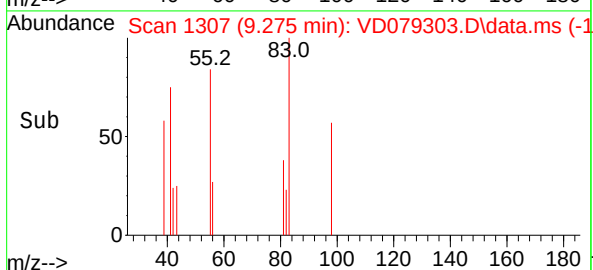

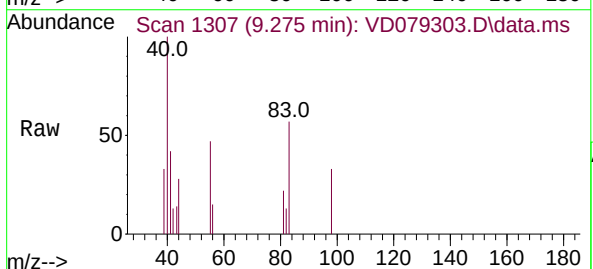


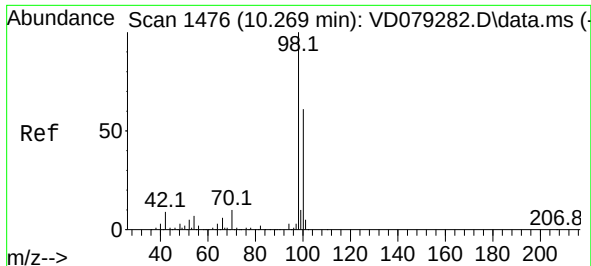

#50
Toluene-d8
Concen: 42.961 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 98 Resp: 189460
Ion Ratio Lower Upper
98 100
100 61.4 51.6 77.4

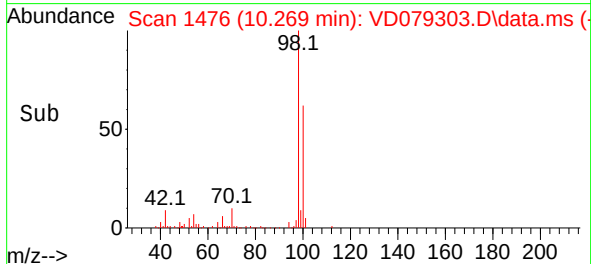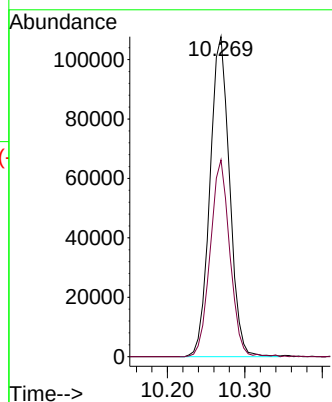

#55
1,1,2-Trichloroethane
Concen: 2.479 ug/l
RT: 10.704 min Scan# 1550
Delta R.T. -0.024 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30

Tgt Ion: 97 Resp: 2624
Ion Ratio Lower Upper
97 100
83 0.0 65.8 98.8#
85 0.0 43.8 65.8#
99 0.0 55.4 83.0#

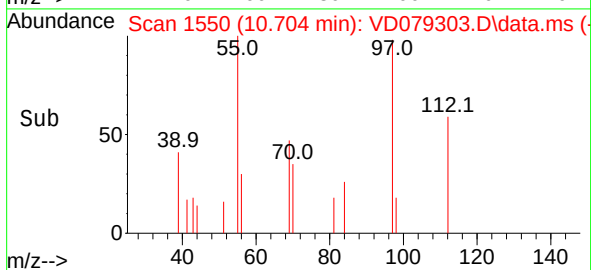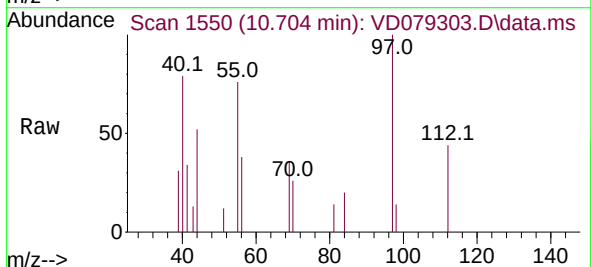



#56

Ethyl methacrylate

Concen: 4.183 ug/l

RT: 10.610 min Scan# 1534

Delta R.T. 0.017 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Instrument :

MSVOA_D

ClientSampleId :





Tgt Ion: 69 Resp: 711

Ion Ratio Lower Upper

69 100

41 96.6 39.8 59.6#

39 19.0 20.2 30.4#

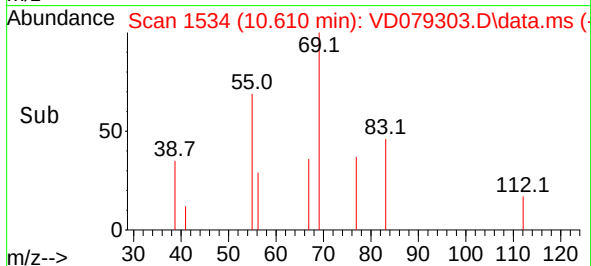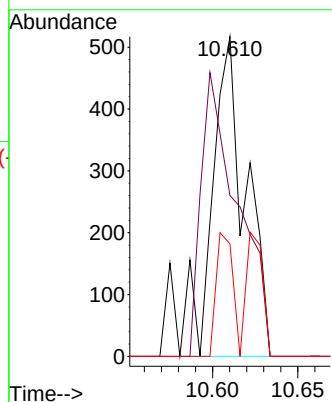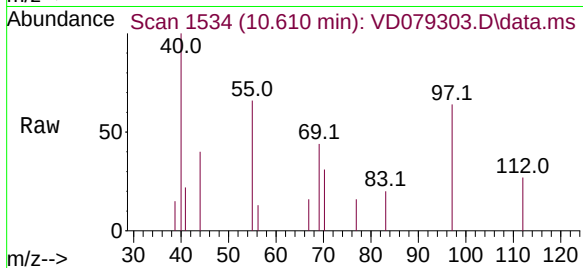

#62

4-Bromofluorobenzene

Concen: 43.720 ug/l

RT: 12.569 min Scan# 1867

Delta R.T. -0.000 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30




Tgt Ion: 95 Resp: 61827


Ion Ratio Lower Upper

95 100

174 74.5 0.0 195.4

176 70.6 0.0 192.6

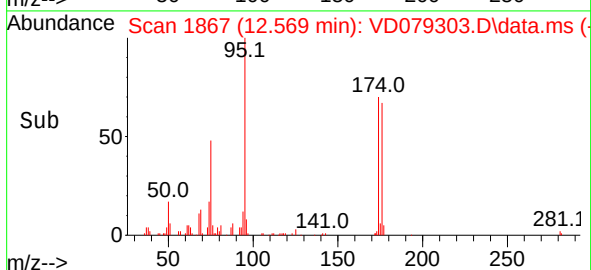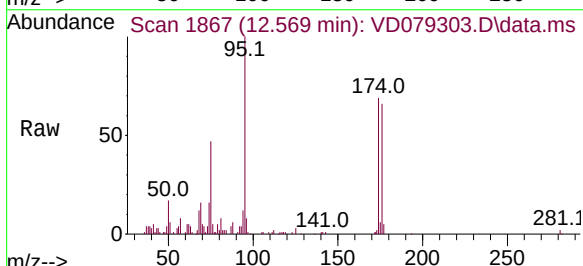

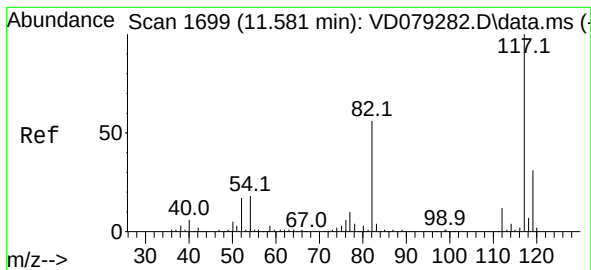

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.575 min Scan# 1

Delta R.T. -0.006 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Instrument :

MSVOA_D

ClientSampleId :





Tgt Ion:117 Resp: 160665

Ion Ratio Lower Upper

117 100

82 53.6 39.8 59.6

119 30.5 25.7 38.5

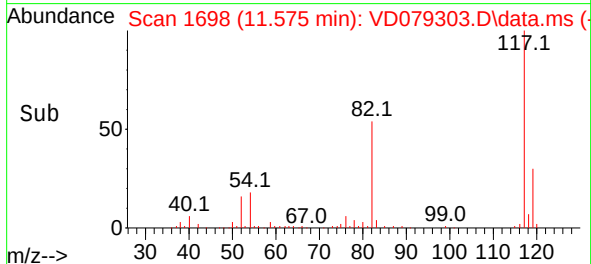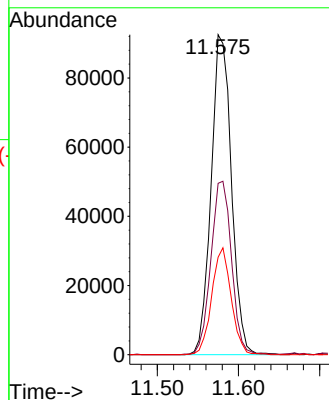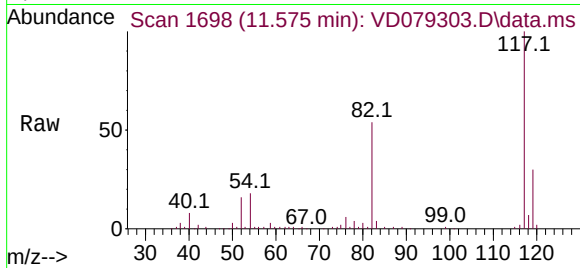

#64

Tetrachloroethene

Concen: 1.039 ug/l

RT: 10.810 min Scan# 1568

Delta R.T. 0.006 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Tgt Ion:164 Resp: 1040




Ion Ratio Lower Upper


164 100

166 136.2 108.6 163.0

129 60.4 74.6 112.0#

131 69.3 68.6 103.0

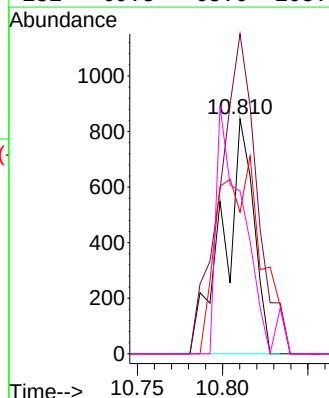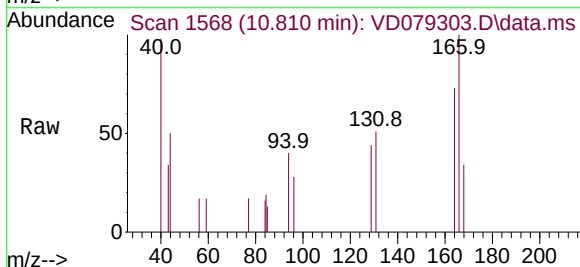



#68

m/p-Xylenes

Concen: 1.370 ug/l

RT: 11.798 min Scan# 1

Delta R.T. 0.006 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Instrument :

MSVOA_D





ClientSampleId :

Tgt Ion:106 Resp: 3296

Ion Ratio Lower Upper

106 100

91 244.5 148.5 222.7#

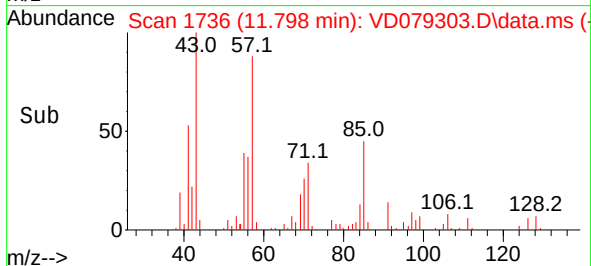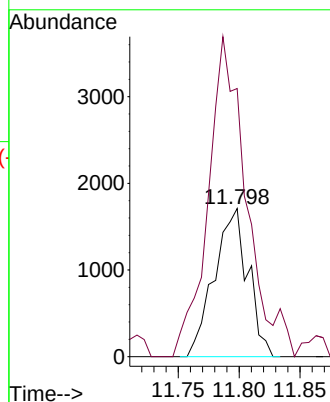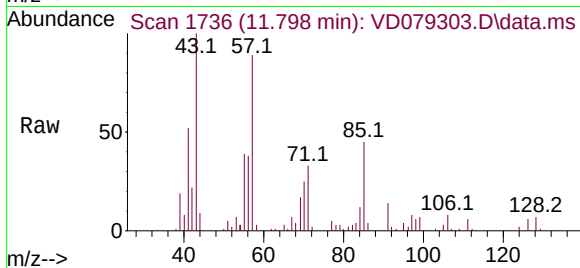

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.516 min Scan# 2028

Delta R.T. -0.000 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30




Tgt Ion:152 Resp: 51606


Ion Ratio Lower Upper

152 100

115 62.2 26.5 79.5


150 154.4 0.0 341.6

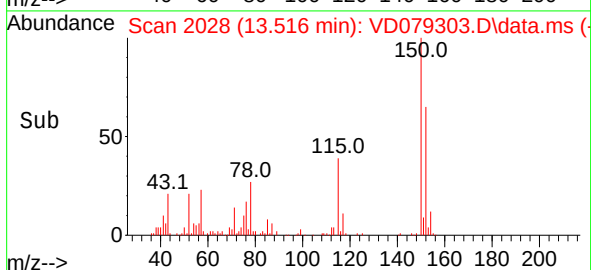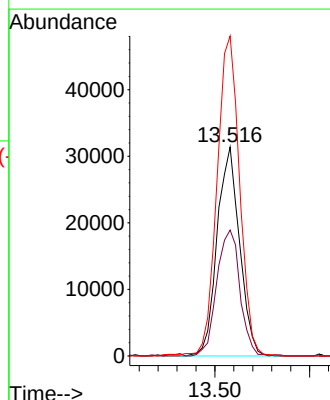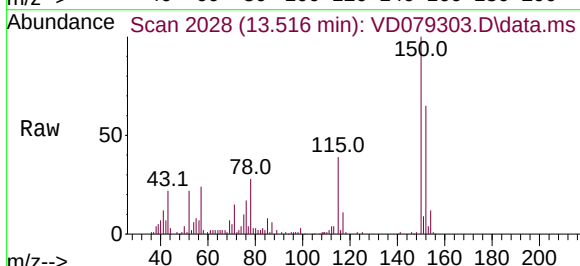



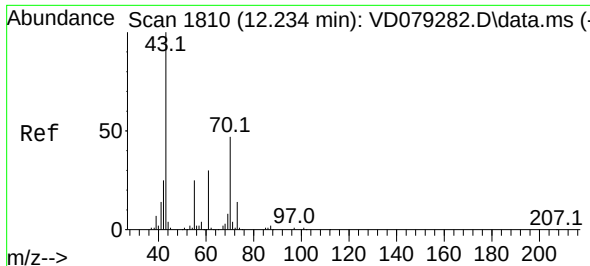


#74
N-ethyl acetate
Concen: 11.243 ug/l
RT: 12.210 min Scan# 1806
Delta R.T. -0.018 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30

Instrument :
MSVOA_D
ClientSampleId :



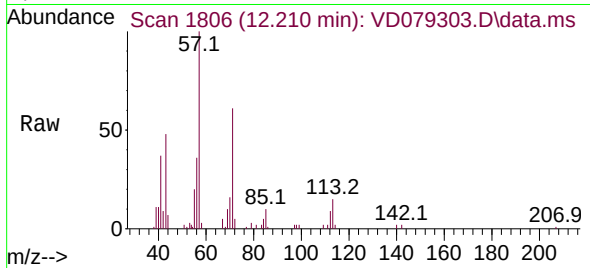



Tgt Ion: 43 Resp: 9467
Ion Ratio Lower Upper
43 100
70 49.5 44.3 66.5
55 19.3 23.2 34.8#
61 0.0 24.2 36.4#

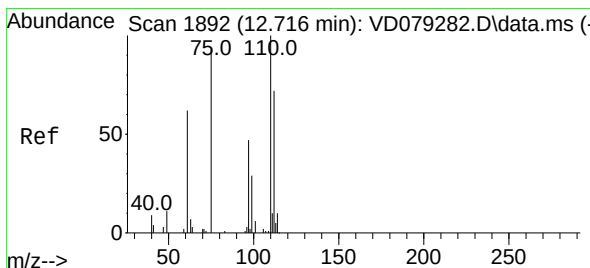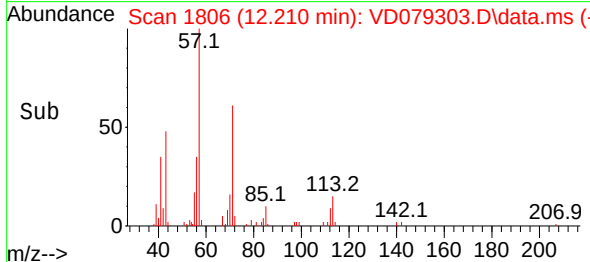

#76
1,2,3-Trichloropropane
Concen: 61.917 ug/l
RT: 12.569 min Scan# 1867
Delta R.T. -0.153 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30

Tgt Ion: 75 Resp: 31977
Ion Ratio Lower Upper
75 100
77 2.7 0.0 0.0#


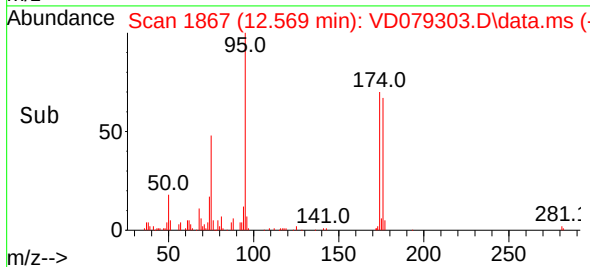

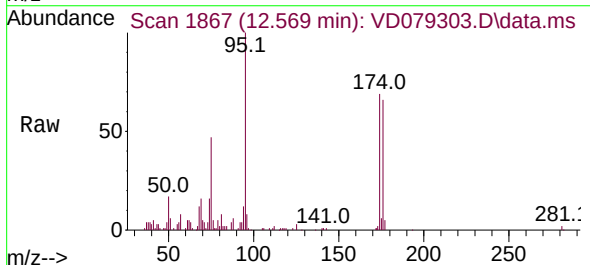


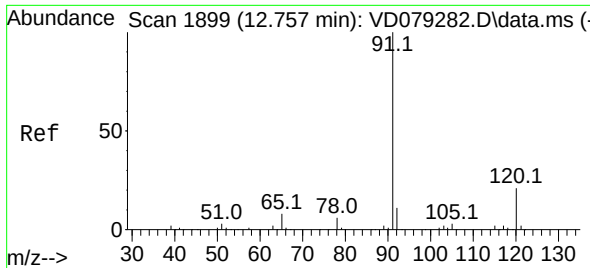

#78
n-propylbenzene
Concen: 1.553 ug/l
RT: 12.757 min Scan# 1899
Delta R.T. -0.006 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 91 Resp: 7626
Ion Ratio Lower Upper
91 100
120 20.1 12.3 36.8

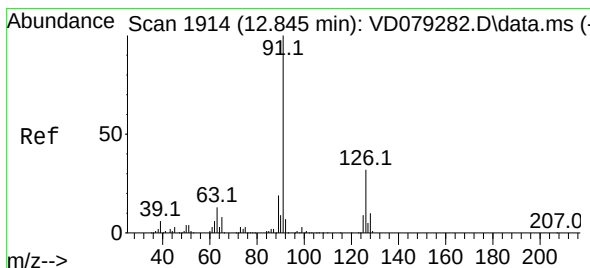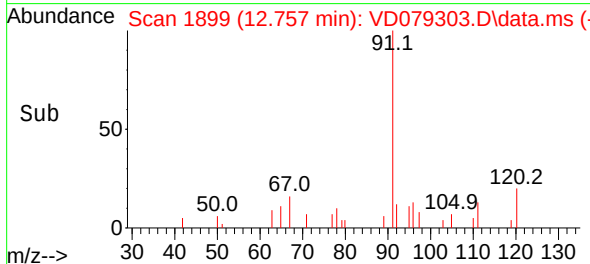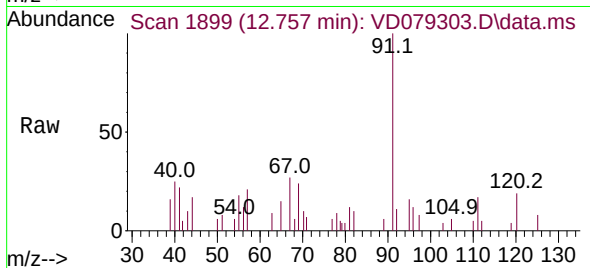

#79
2-Chlorotoluene
Concen: 1.682 ug/l
RT: 12.840 min Scan# 1913
Delta R.T. -0.006 min
Lab File: VD079303.D
Acq: 01 Jul 2024 18:30

Tgt Ion: 91 Resp: 4618
Ion Ratio Lower Upper
91 100
126 20.4 19.3 57.8

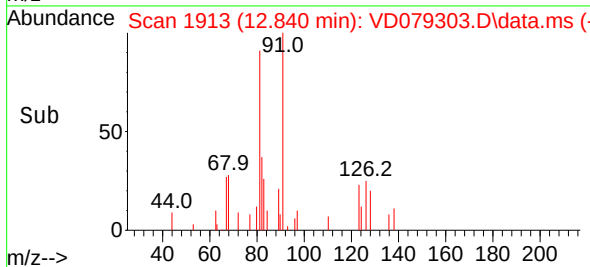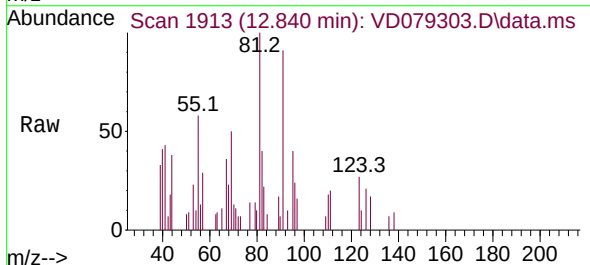

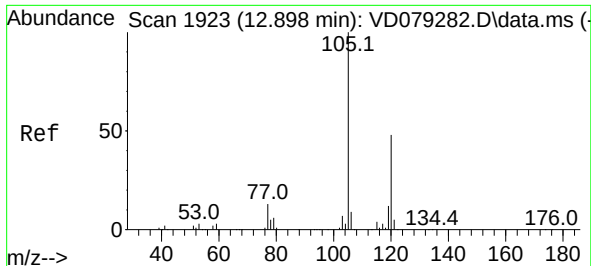

#80

1,3,5-Trimethylbenzene

Concen: 1.739 ug/l

RT: 12.898 min Scan# 1923

Delta R.T. -0.000 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Instrument :

MSVOA_D





ClientSampleId :

Tgt Ion:105 Resp: 5647

Ion Ratio Lower Upper

105 100

120 43.1 25.7 77.1

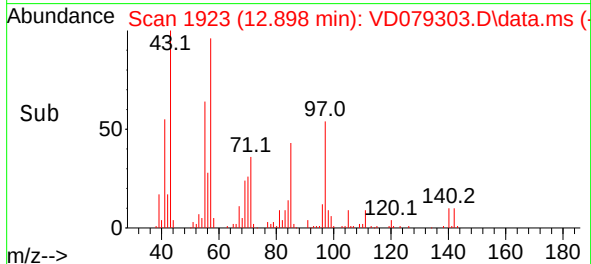

#81

trans-1,4-Dichloro-2-butene

Concen: 114.894 ug/l

RT: 12.569 min Scan# 1867

Delta R.T. 0.100 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30




Tgt Ion: 75 Resp: 31977


Ion Ratio Lower Upper

75 100

53 0.0 61.4 92.2#

89 0.2 35.4 53.0#

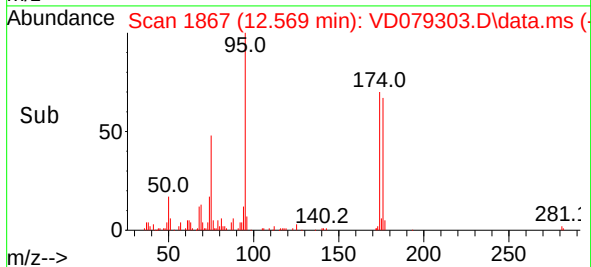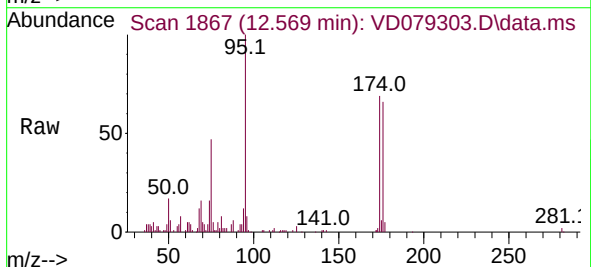

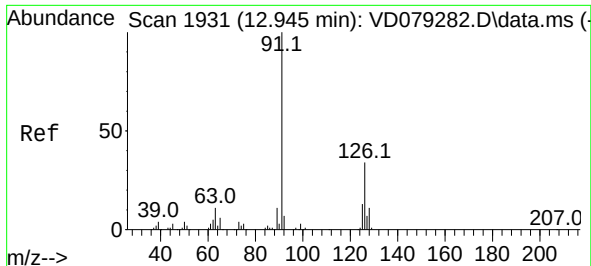

#82

4-Chlorotoluene

Concen: 2.036 ug/l

RT: 12.940 min Scan# 1931

Delta R.T. -0.006 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Instrument :

MSVOA_D





ClientSampleId :

Tgt Ion: 91 Resp: 5873

Ion Ratio Lower Upper

91 100

126 30.4 18.9 56.9

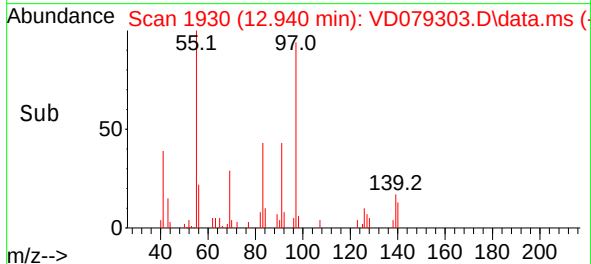

#84

1,2,4-Trimethylbenzene

Concen: 1.434 ug/l

RT: 13.216 min Scan# 1977

Delta R.T. 0.006 min

Lab File: VD079303.D




Acq: 01 Jul 2024 18:30


Tgt Ion:105 Resp: 4663

Ion Ratio Lower Upper

105 100

120 43.2 23.6 71.0


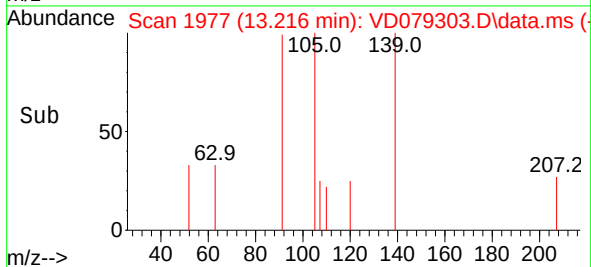

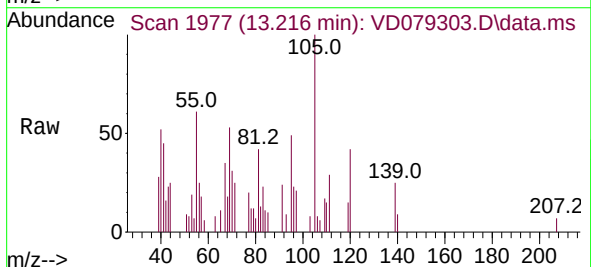


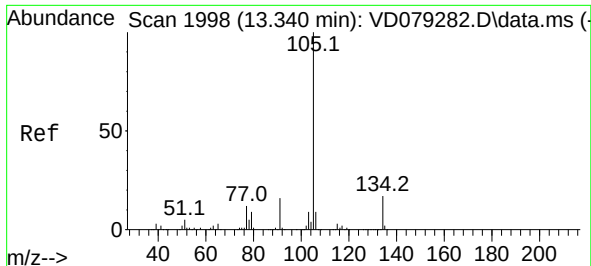

#85
 sec-Butylbenzene
 Concen: 1.234 ug/l
 RT: 13.339 min Scan# 1998
 Delta R.T. -0.000 min
 Lab File: VD079303.D
 Acq: 01 Jul 2024 18:30




Instrument :
 MSVOA_D
 ClientSampleId :


Tgt Ion:105 Resp: 5165
 Ion Ratio Lower Upper
 105 100
 134 18.5 10.3 30.8

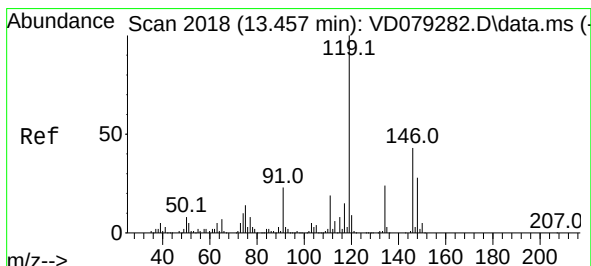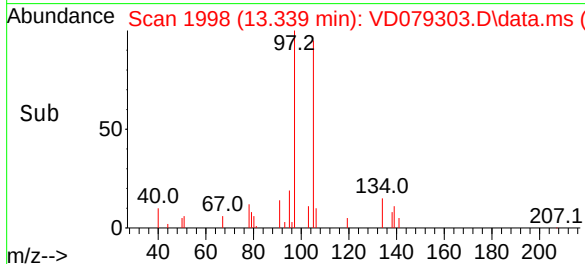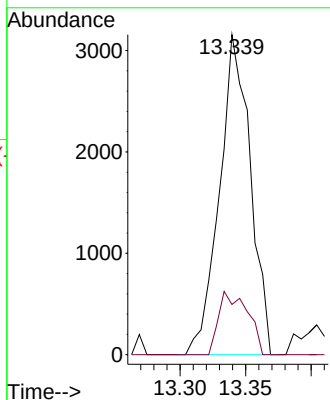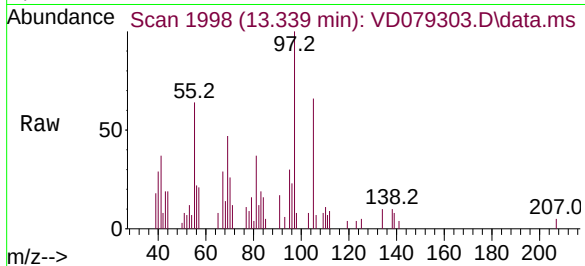

#87
 1,3-Dichlorobenzene
 Concen: 1.481 ug/l
 RT: 13.457 min Scan# 2018
 Delta R.T. -0.000 min
 Lab File: VD079303.D
 Acq: 01 Jul 2024 18:30

Tgt Ion:146 Resp: 2717
 Ion Ratio Lower Upper
 146 100
 111 87.7 18.5 55.5#
 148 72.7 30.9 92.8

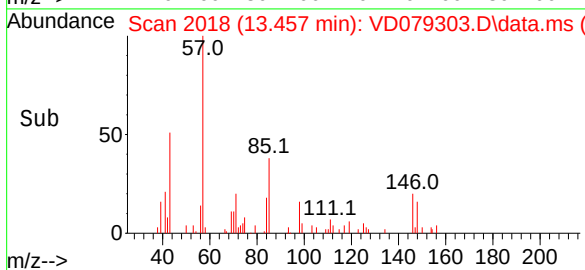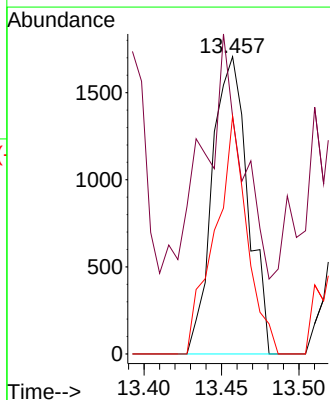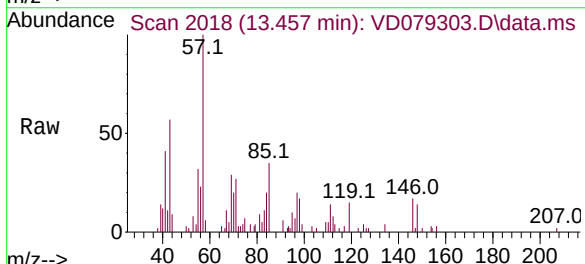

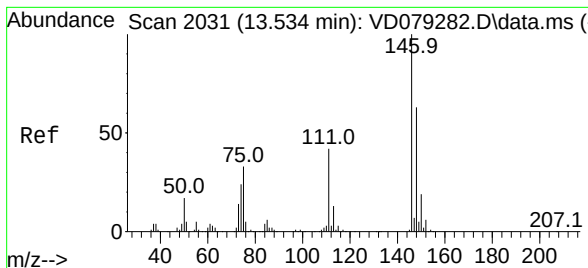

#88

1,4-Dichlorobenzene

Concen: 1.564 ug/l

RT: 13.534 min Scan# 2031

Delta R.T. -0.000 min

Lab File: VD079303.D





Acq: 01 Jul 2024 18:30

Instrument :

MSVOA_D

ClientSampleId :

Tgt Ion:	146	Resp:	2852
Ion	Ratio	Lower	Upper
146	100		
111	129.0	17.5	52.6#
148	67.5	31.4	94.2

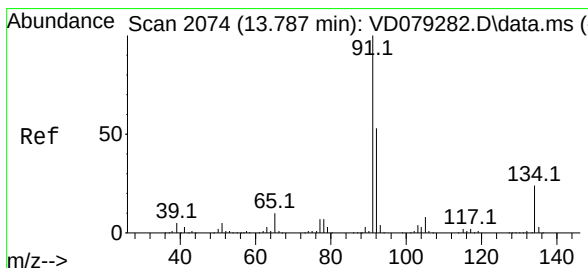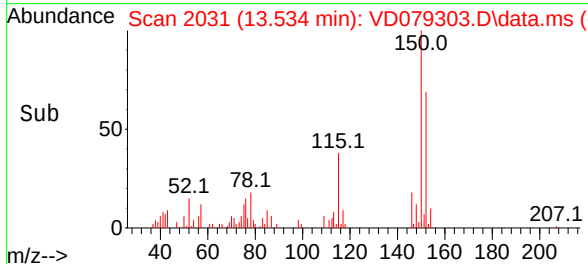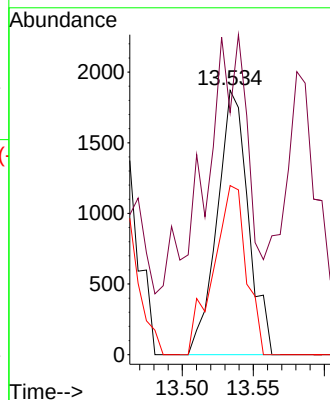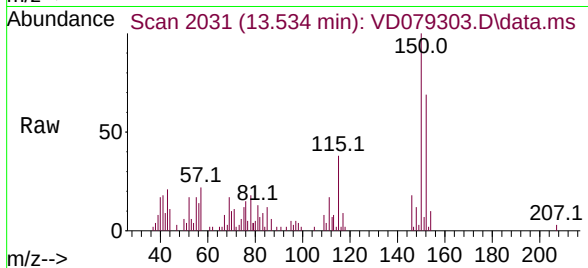

#89

n-Butylbenzene

Concen: 2.740 ug/l




RT: 13.781 min Scan# 2073


Delta R.T. -0.000 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Tgt Ion:	91	Resp:	9292
Ion	Ratio	Lower	Upper
91	100		
92	50.7	25.7	77.0
134	21.3	13.6	40.8

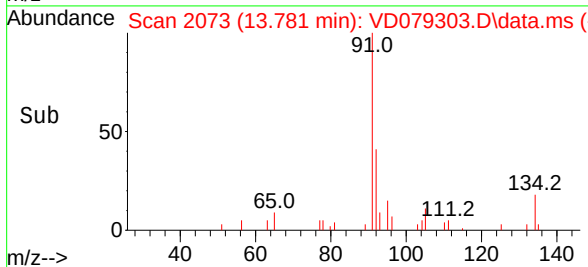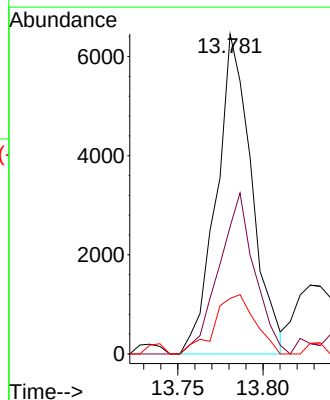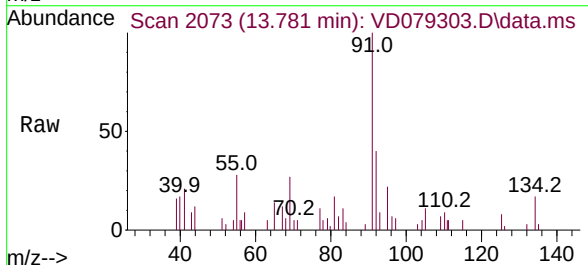

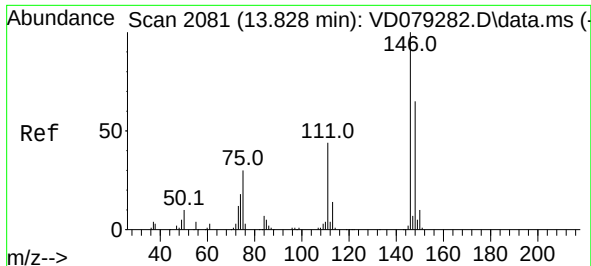

#91

1,2-Dichlorobenzene

Concen: 1.017 ug/l

RT: 13.822 min Scan# 2081

Delta R.T. -0.006 min

Lab File: VD079303.D





Acq: 01 Jul 2024 18:30

Instrument :

MSVOA_D

ClientSampleId :

Tgt Ion:146	Resp:	1606
Ion Ratio	Lower	Upper
146	100	
111	252.0	19.1 57.1#
148	71.5	31.1 93.5

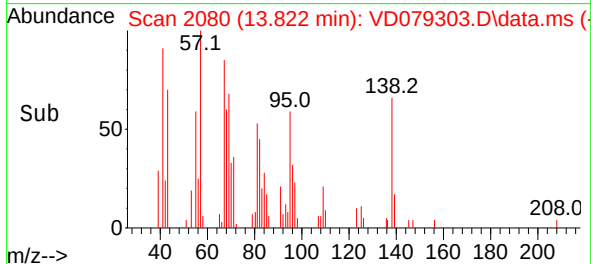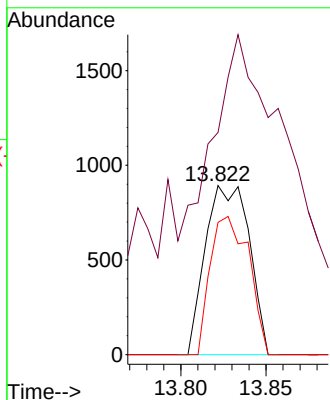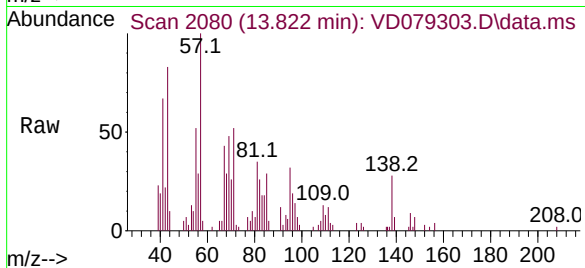

#93

1,2,4-Trichlorobenzene

Concen: 3.564 ug/l




RT: 15.092 min Scan# 2296


Delta R.T. -0.000 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Tgt Ion:180	Resp:	3001
Ion Ratio	Lower	Upper
180	100	
182	140.8	46.9 140.7#
145	31.1	14.0 41.9

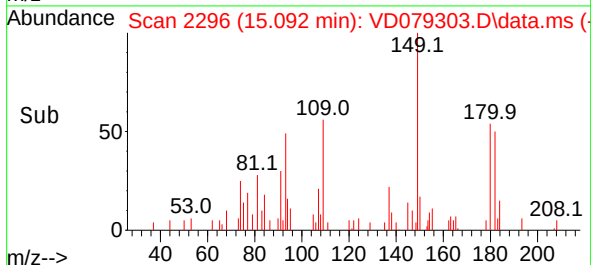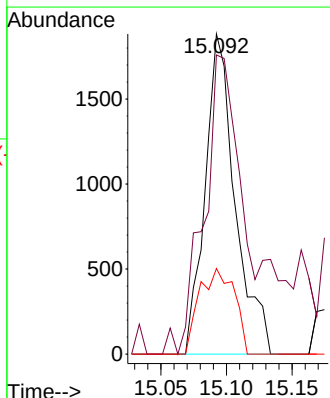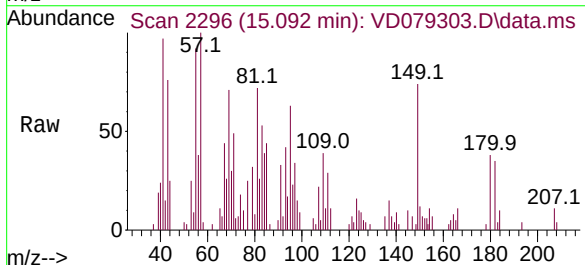



#94

Hexachlorobutadiene

Concen: 3.385 ug/l

RT: 15.198 min Scan# 2314

Delta R.T. -0.000 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30

Instrument :

MSVOA_D

ClientSampleId :





Tgt Ion:225 Resp: 1585

Ion Ratio Lower Upper

225 100

223 59.3 33.3 99.9

227 50.7 33.6 100.6

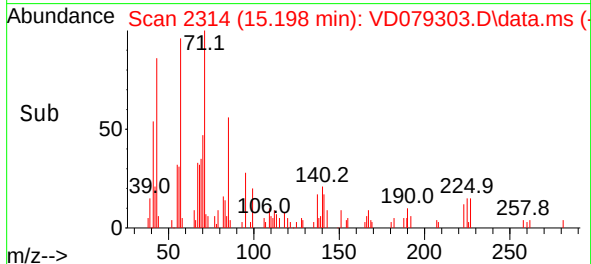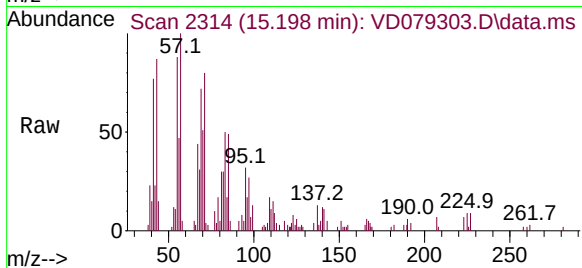

#95

Naphthalene

Concen: 2.133 ug/l

RT: 15.334 min Scan# 2337

Delta R.T. 0.006 min

Lab File: VD079303.D

Acq: 01 Jul 2024 18:30




Tgt Ion:128 Resp: 3506


Ion Ratio Lower Upper

128 100

127 23.7 10.2 15.4#

129 10.0 8.5 12.7

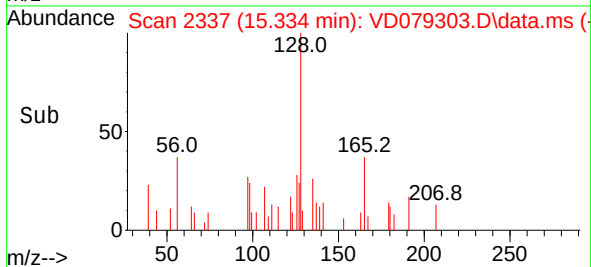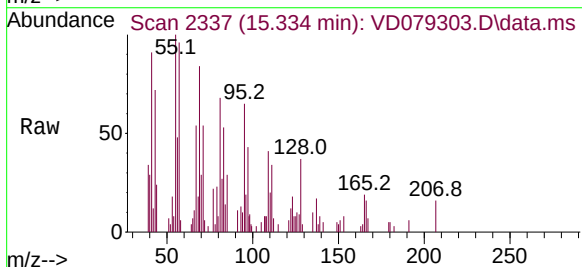



#96
 1,2,3-Trichlorobenzene
 Concen: 6.765 ug/l
 RT: 15.510 min Scan# 24
 Delta R.T. -0.006 min
 Lab File: VD079303.D
 Acq: 01 Jul 2024 18:30

Instrument :
 MSVOA_D
 ClientSampleId :

Tgt Ion	Ratio	Lower	Upper
180	100		
182	81.1	47.8	143.3
145	18.4	16.1	48.2

