
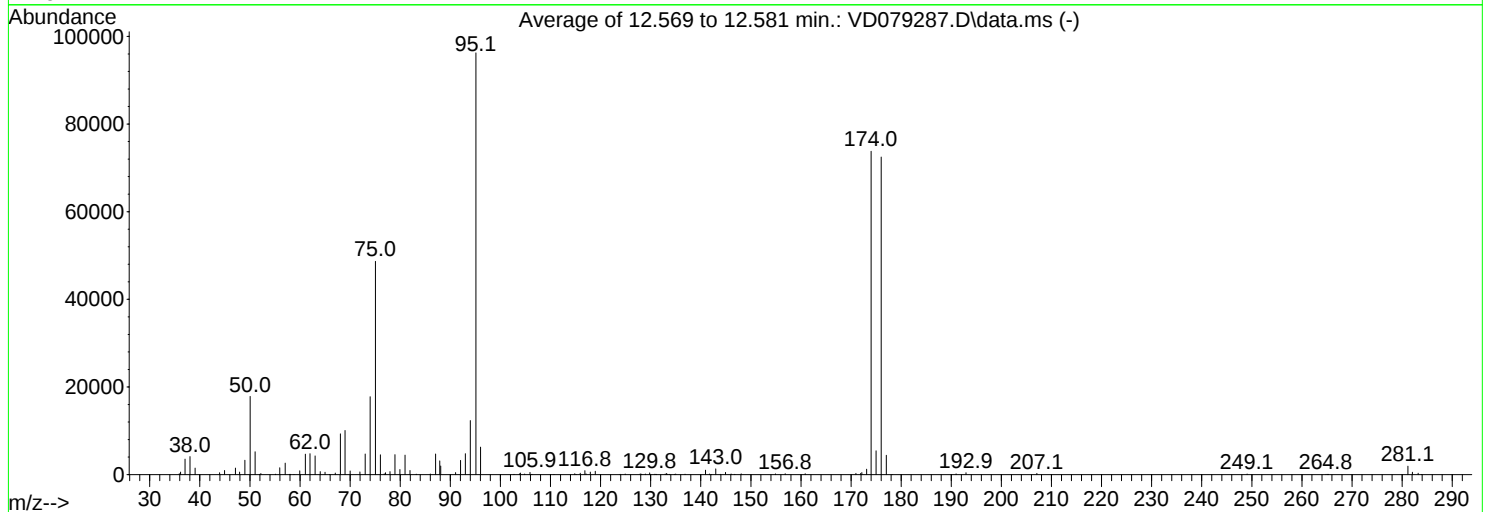


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070124\
Data File : VD079287.D
Acq On : 01 Jul 2024 08:19
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062824S.M
Title : SW846 8260
Last Update : Sat Jun 29 06:28:31 2024

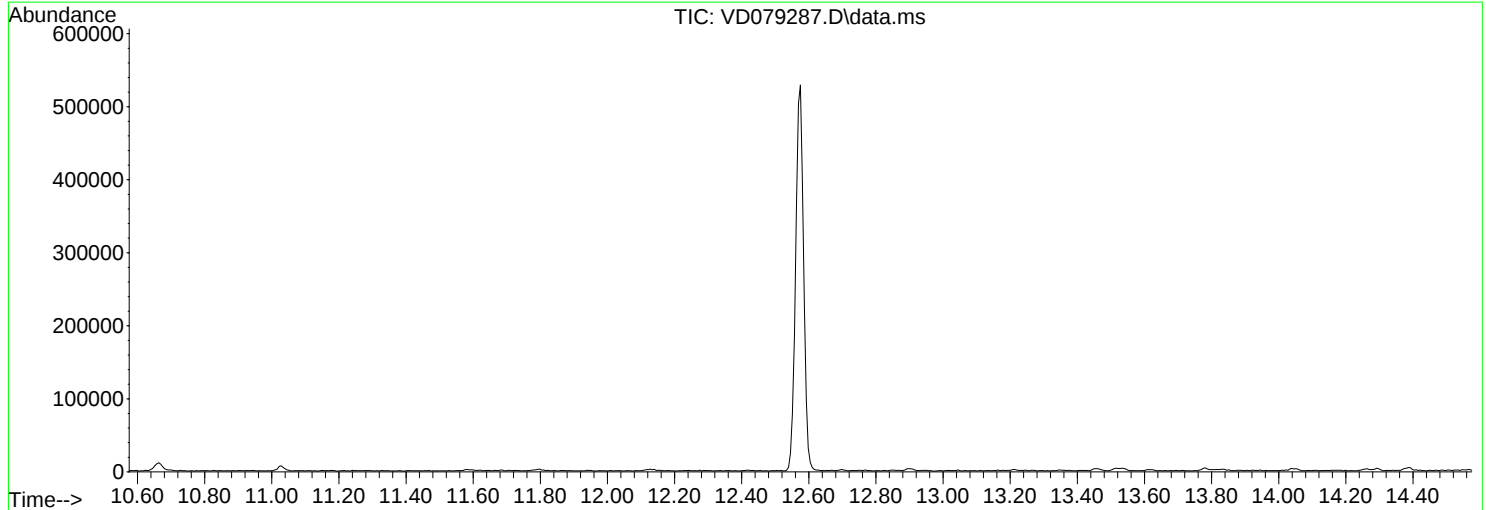

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	17837	PASS
75	95	30	60	50.6	48672	PASS
95	95	100	100	100.0	96245	PASS
96	95	5	9	6.5	6298	PASS
173	174	0.00	2	1.7	1248	PASS
174	95	50	100	76.7	73800	PASS
175	174	5	9	7.4	5437	PASS
176	174	95	101	98.2	72469	PASS
177	176	5	9	6.1	4410	PASS