
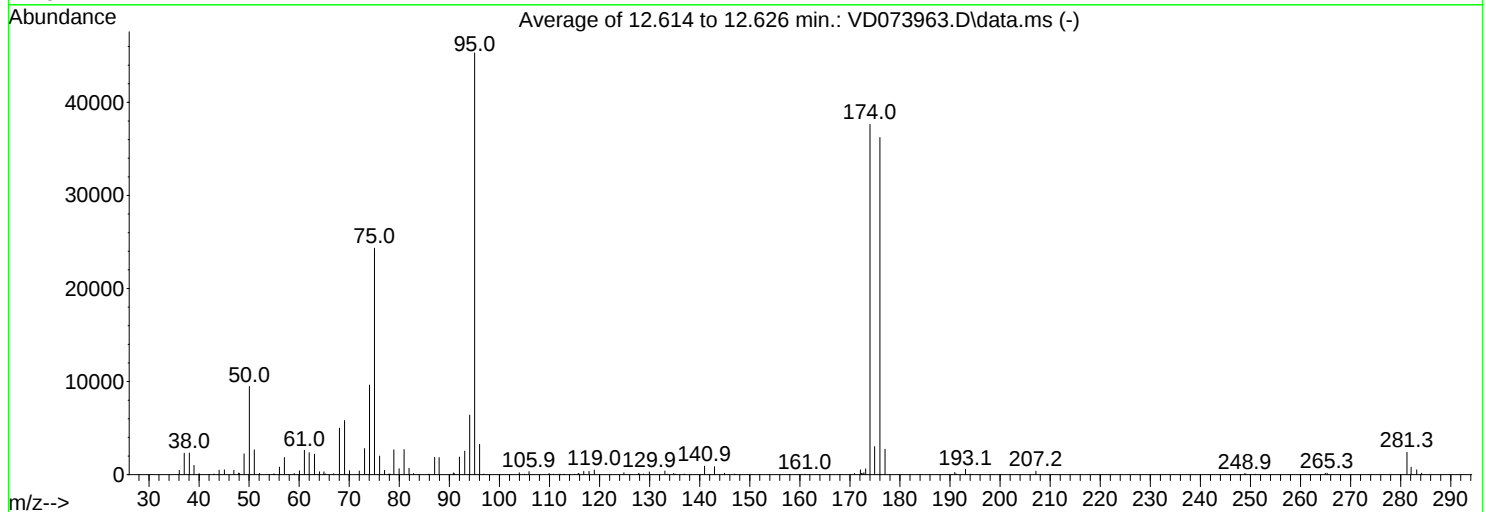


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD080522\  
 Data File : VD073963.D  
 Acq On : 05 Aug 2022 09:38  
 Operator : VA/SY  
 Sample : BFB  
 Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D080522S.M  
 Title : SW846 8260  
 Last Update : Sat Aug 06 00:36:42 2022

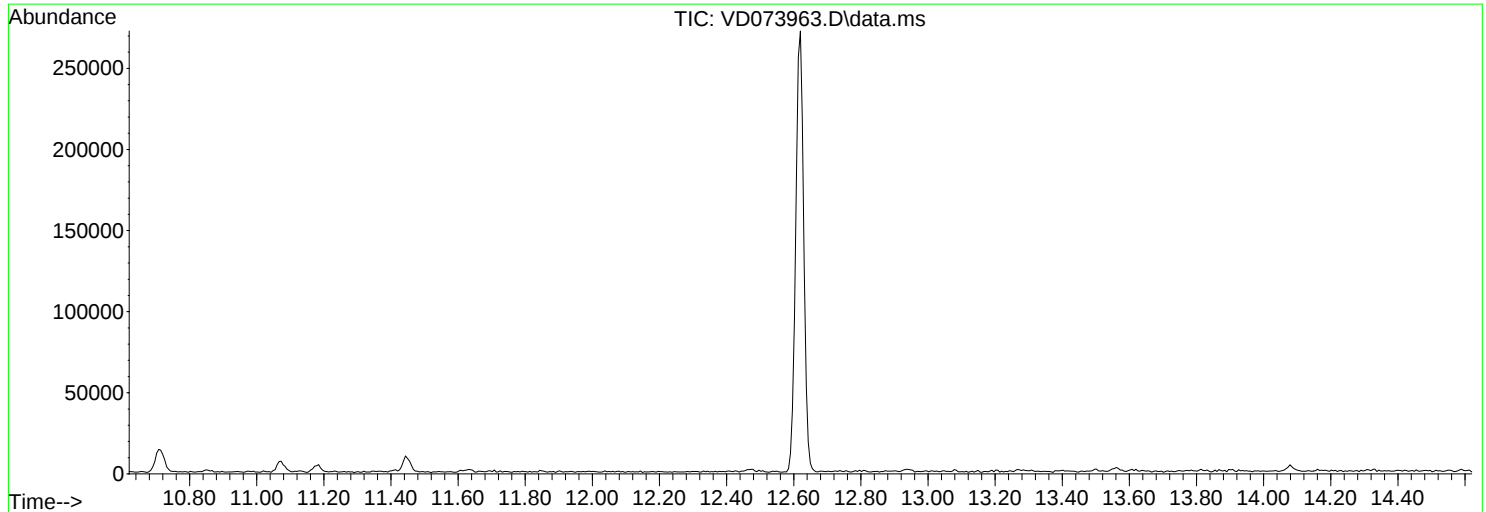

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 20.9         | 9472       | PASS                |
| 75             | 95              | 30              | 60              | 53.7         | 24331      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 45323      | PASS                |
| 96             | 95              | 5               | 9               | 7.2          | 3255       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.7          | 628        | PASS                |
| 174            | 95              | 50              | 100             | 83.0         | 37635      | PASS                |
| 175            | 174             | 5               | 9               | 8.0          | 3013       | PASS                |
| 176            | 174             | 95              | 101             | 96.3         | 36227      | PASS                |
| 177            | 176             | 5               | 9               | 7.6          | 2738       | PASS                |