
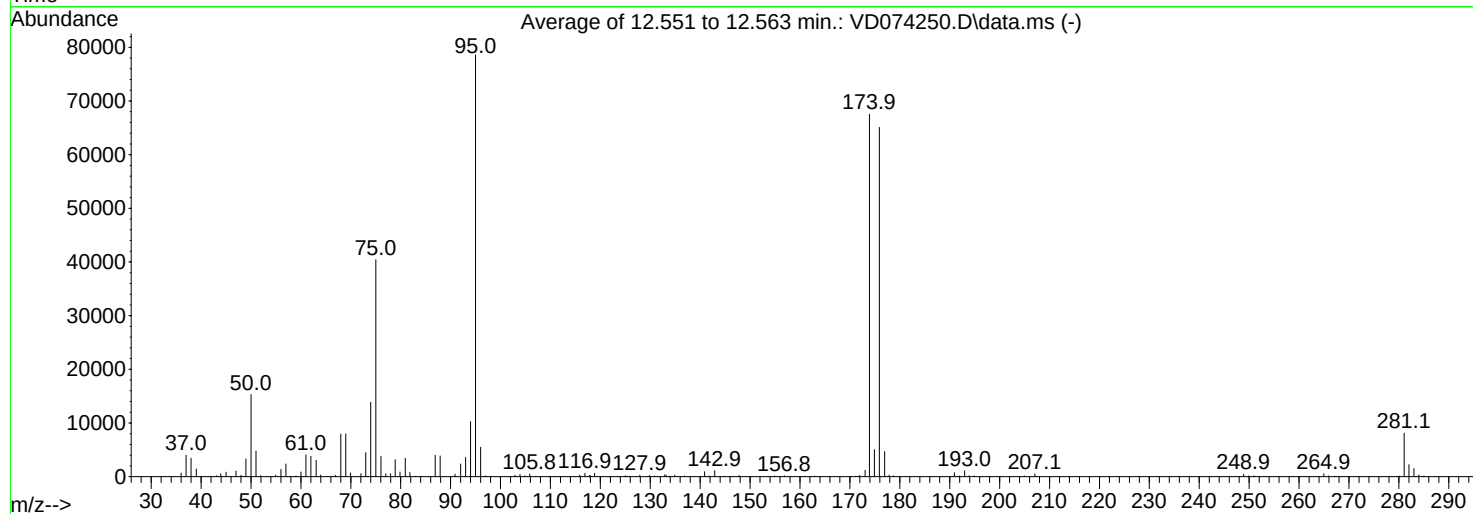


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD091222\  
Data File : VD074250.D  
Acq On : 12 Sep 2022 09:51  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D090922S.M  
Title : SW846 8260  
Last Update : Sat Sep 10 04:45:19 2022

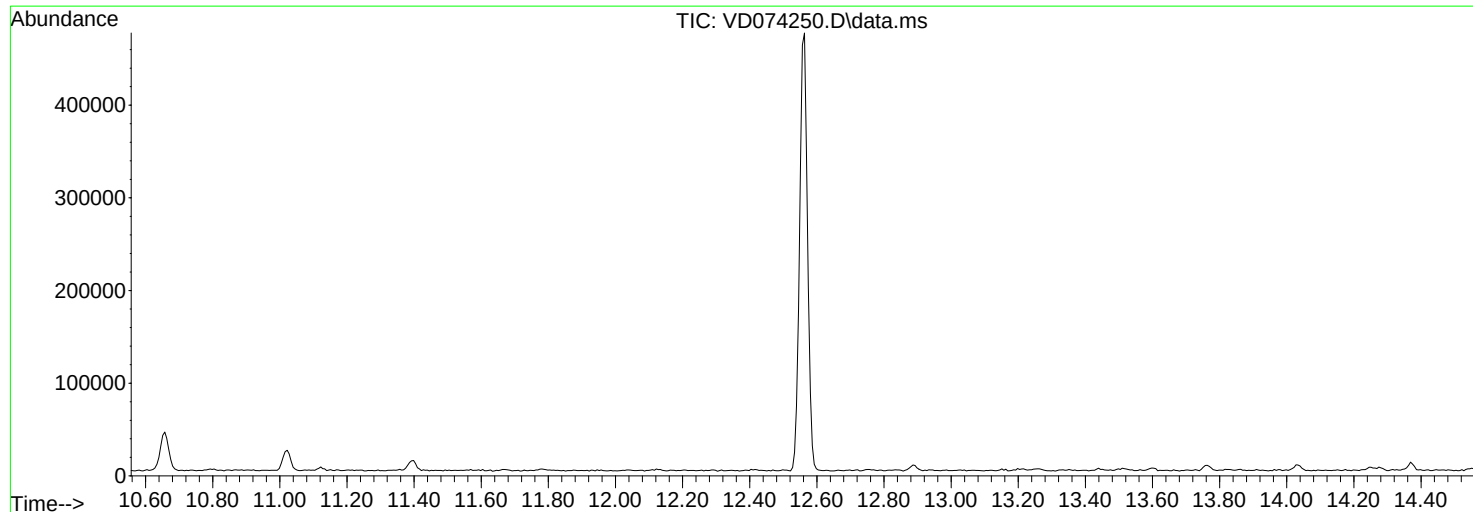

AutoFind: Scans 1864, 1865, 1866; Background Corrected with Scan 1857

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.4         | 15286      | PASS                |
| 75             | 95              | 30              | 60              | 51.4         | 40435      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 78600      | PASS                |
| 96             | 95              | 5               | 9               | 7.0          | 5502       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.8          | 1203       | PASS                |
| 174            | 95              | 50              | 100             | 85.9         | 67528      | PASS                |
| 175            | 174             | 5               | 9               | 7.5          | 5035       | PASS                |
| 176            | 174             | 95              | 101             | 96.4         | 65088      | PASS                |
| 177            | 176             | 5               | 9               | 7.2          | 4688       | PASS                |