
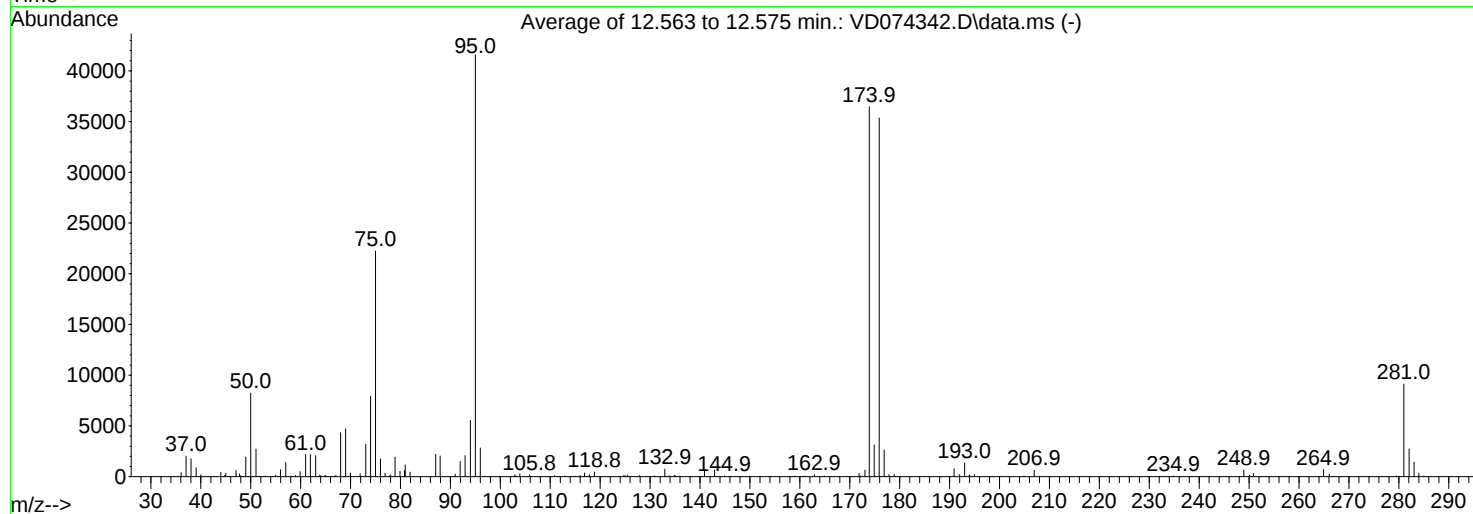


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091922\
Data File : VD074342.D
Acq On : 19 Sep 2022 10:06
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D091622S.M
Title : SW846 8260
Last Update : Sat Sep 17 04:16:54 2022

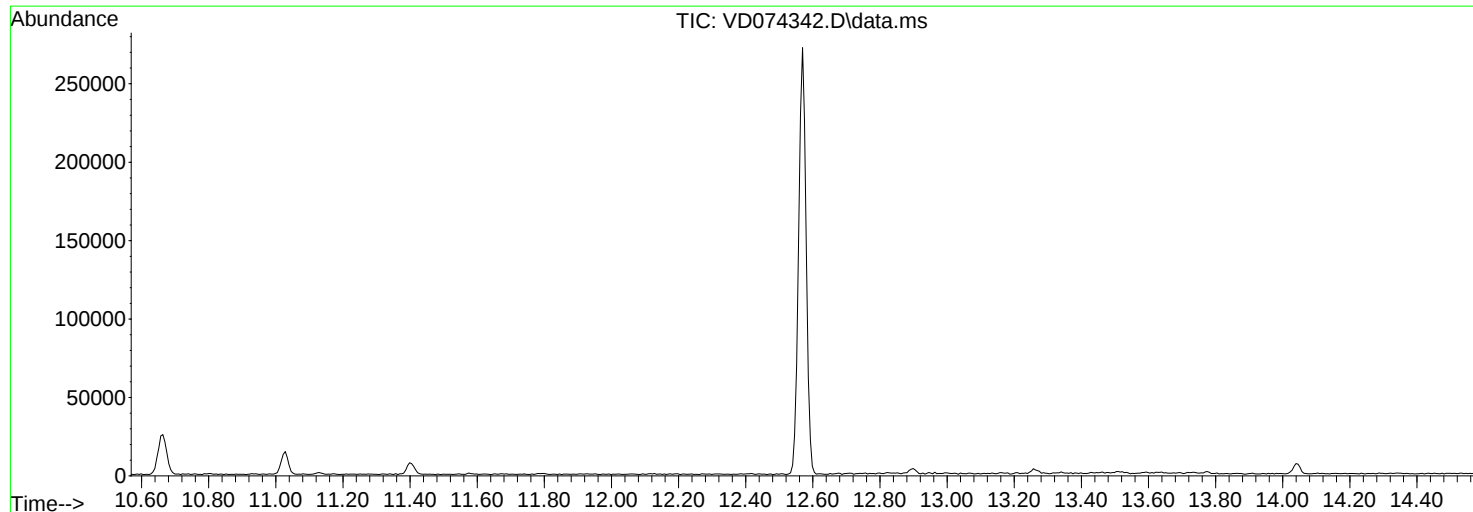

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	8222	PASS
75	95	30	60	53.5	22248	PASS
95	95	100	100	100.0	41584	PASS
96	95	5	9	6.8	2820	PASS
173	174	0.00	2	1.8	652	PASS
174	95	50	100	87.7	36475	PASS
175	174	5	9	8.6	3124	PASS
176	174	95	101	96.9	35360	PASS
177	176	5	9	7.5	2638	PASS