


Chloromethane

Response Ratio

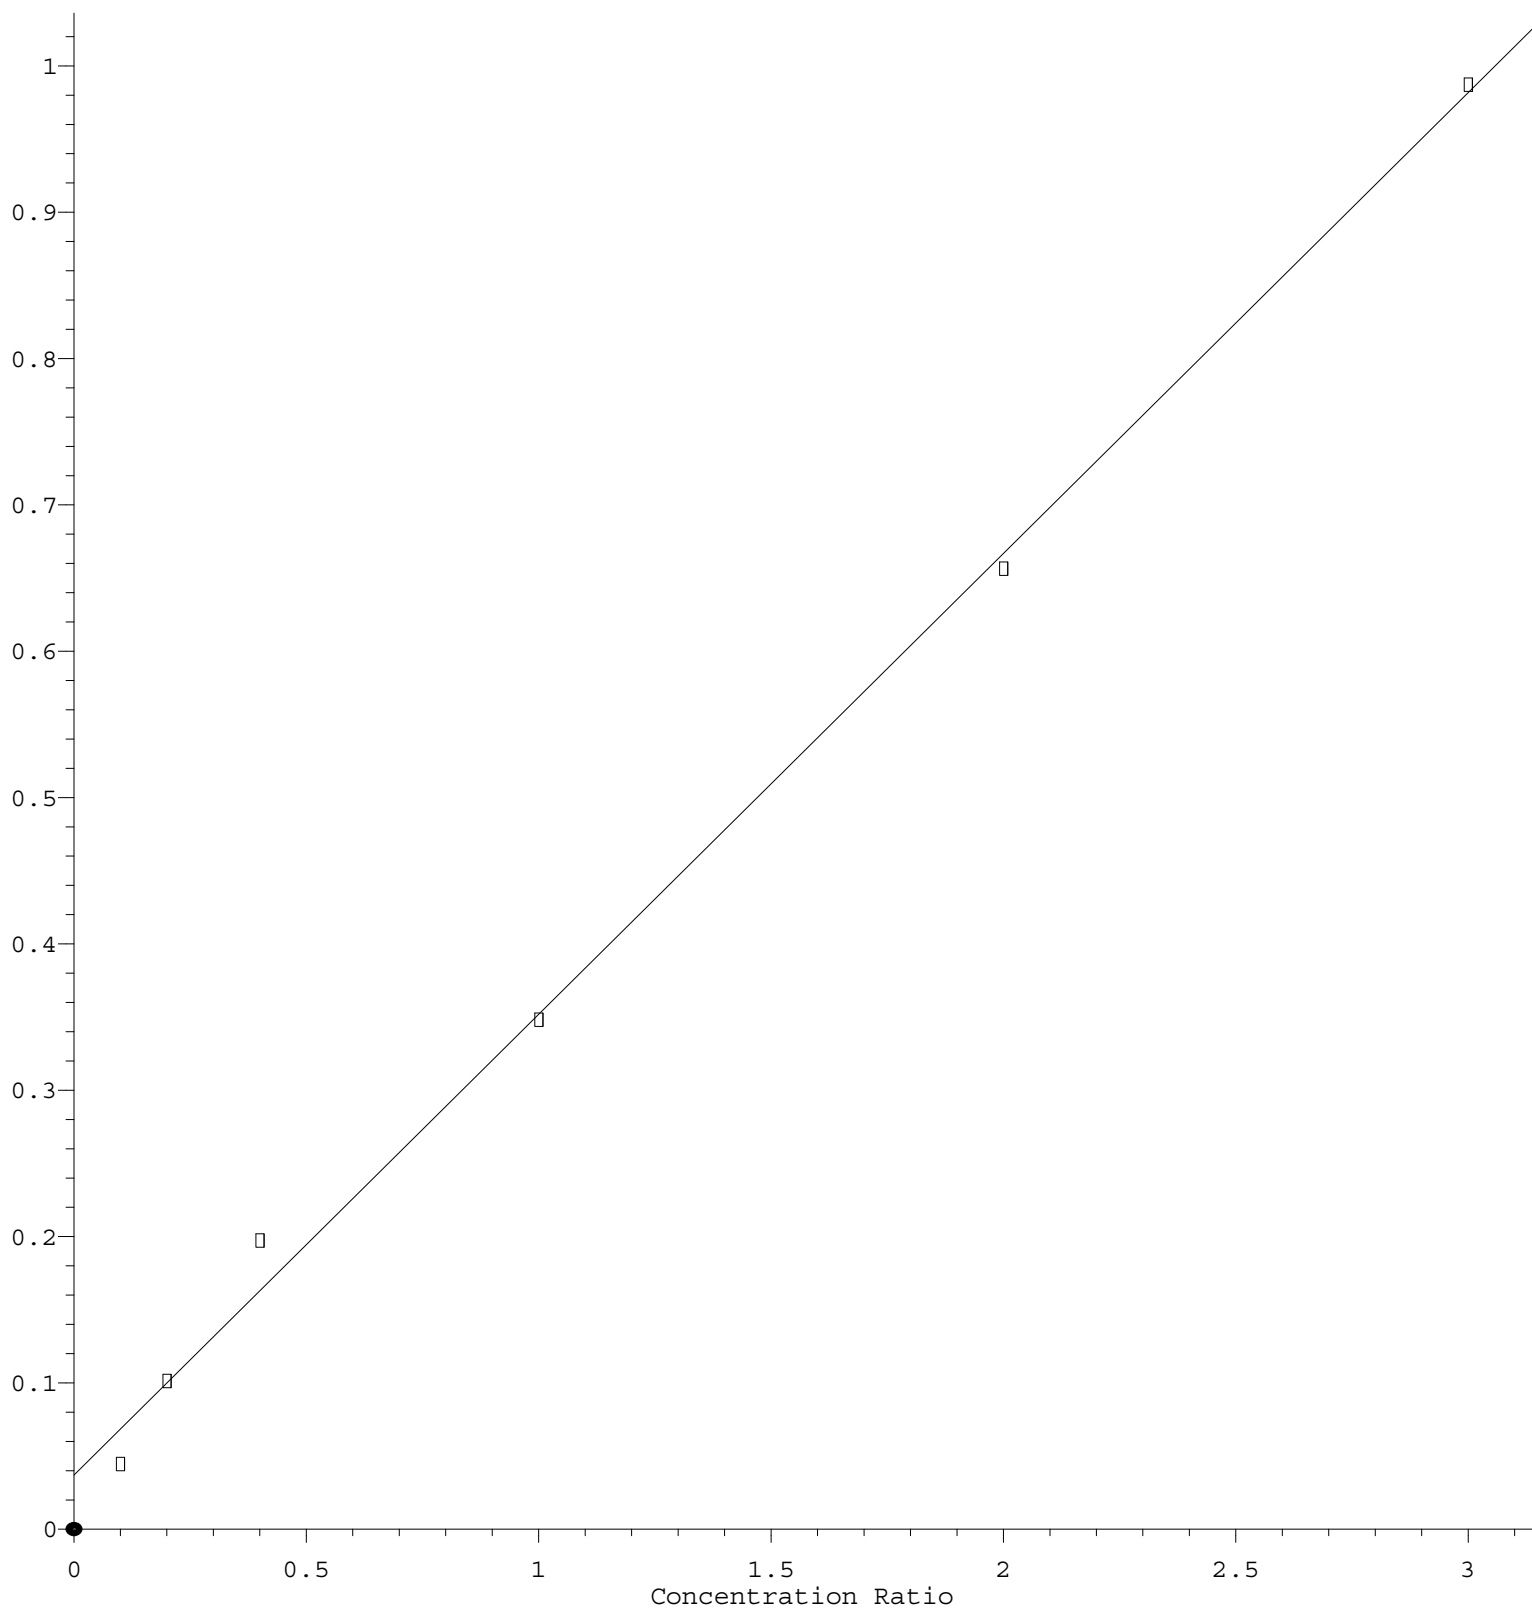

$$\text{Response} = 3.149\text{e-}001 * \text{Amt} + 3.743\text{e-}002$$


Coef of Det (r^2) = 0.997159 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M

Calibration Table Last Updated: Tue Sep 27 03:19:14 2022

Methyl Iodide

Response Ratio

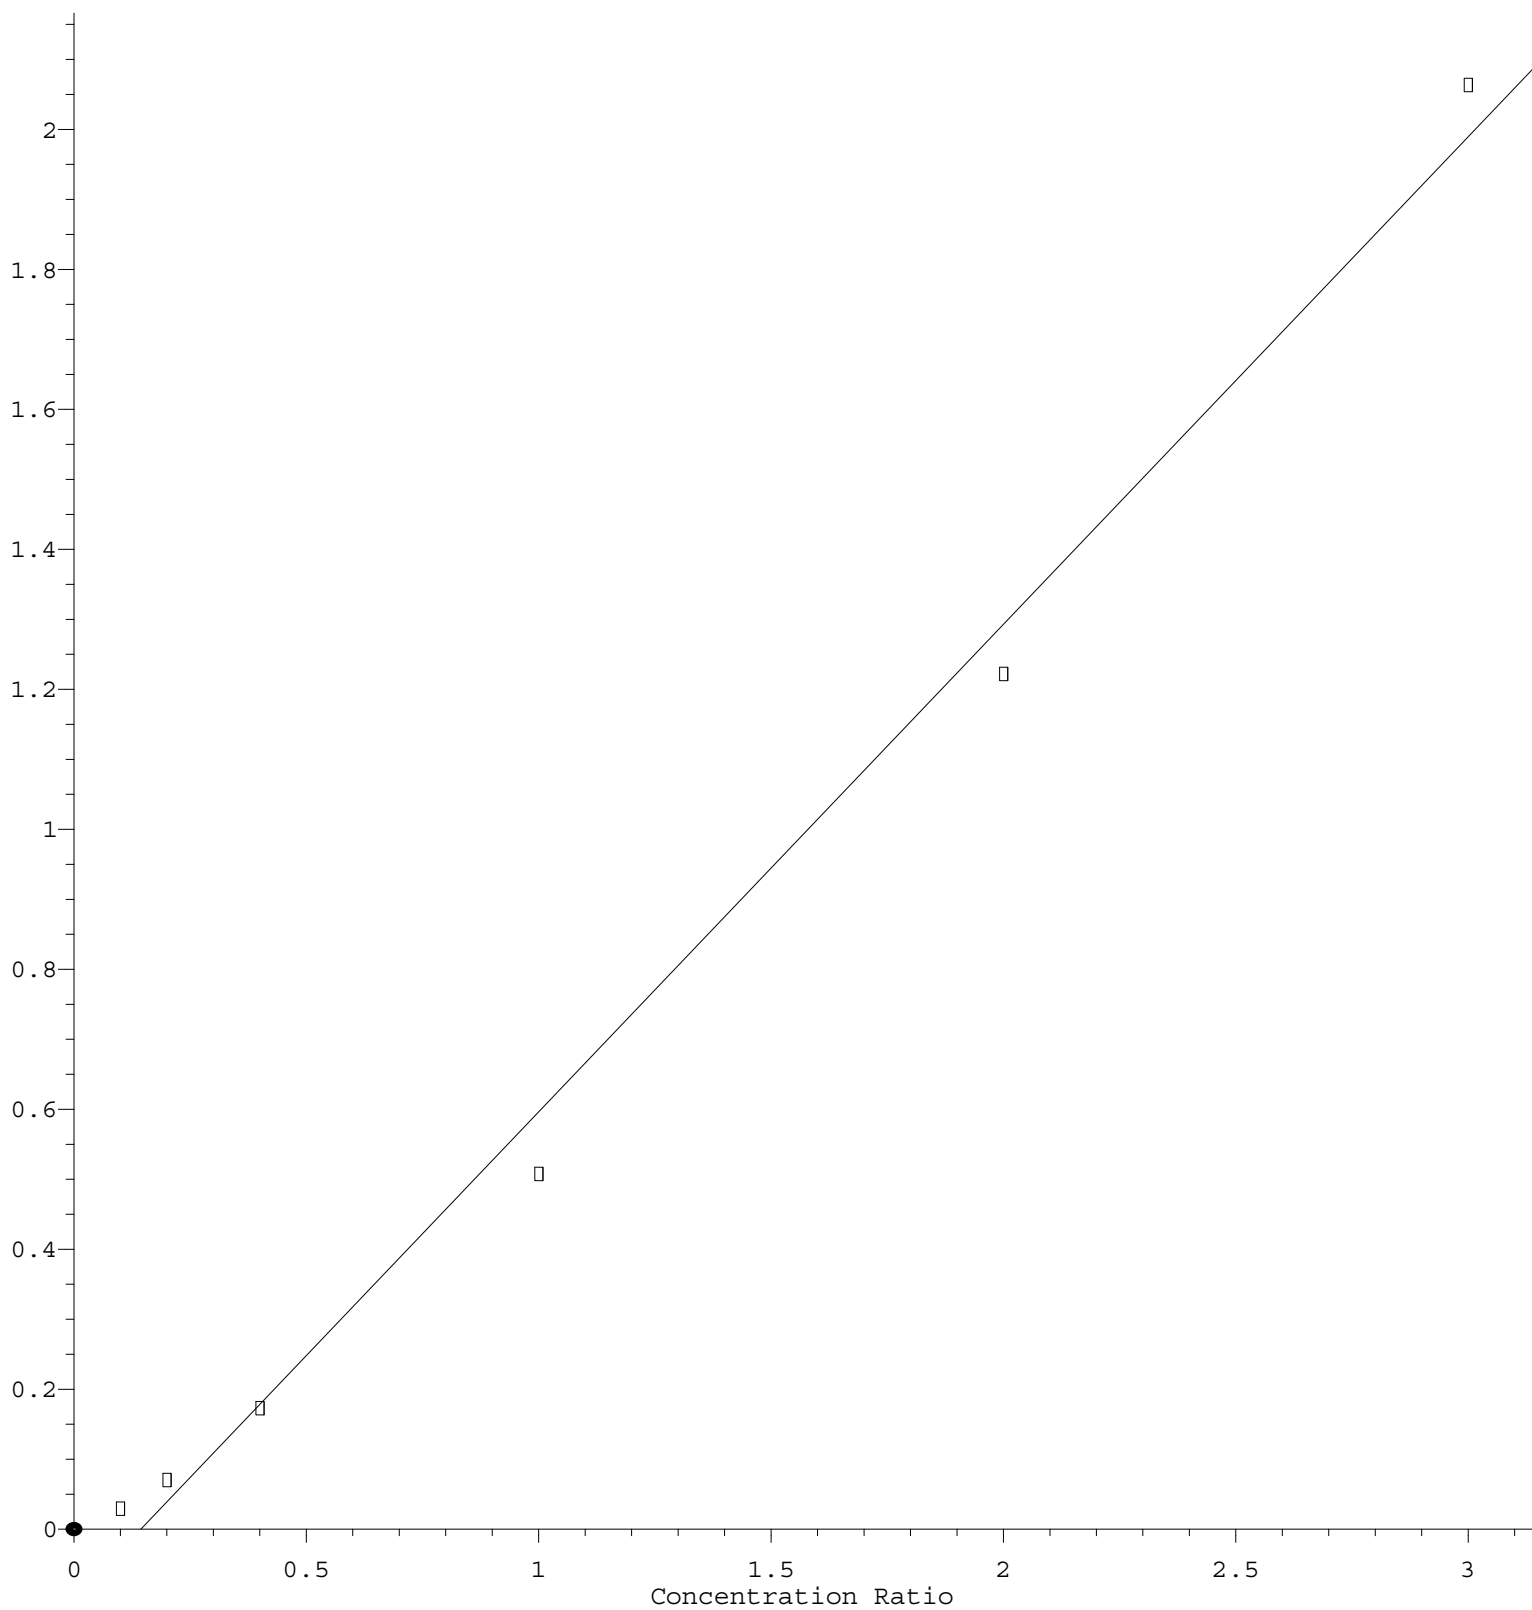

$$\text{Response} = 6.968\text{e-}001 * \text{Amt} - 1.006\text{e-}001$$


Coef of Det (r^2) = 0.993027 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M

Calibration Table Last Updated: Tue Sep 27 03:19:14 2022

Tert butyl alcohol


Response Ratio

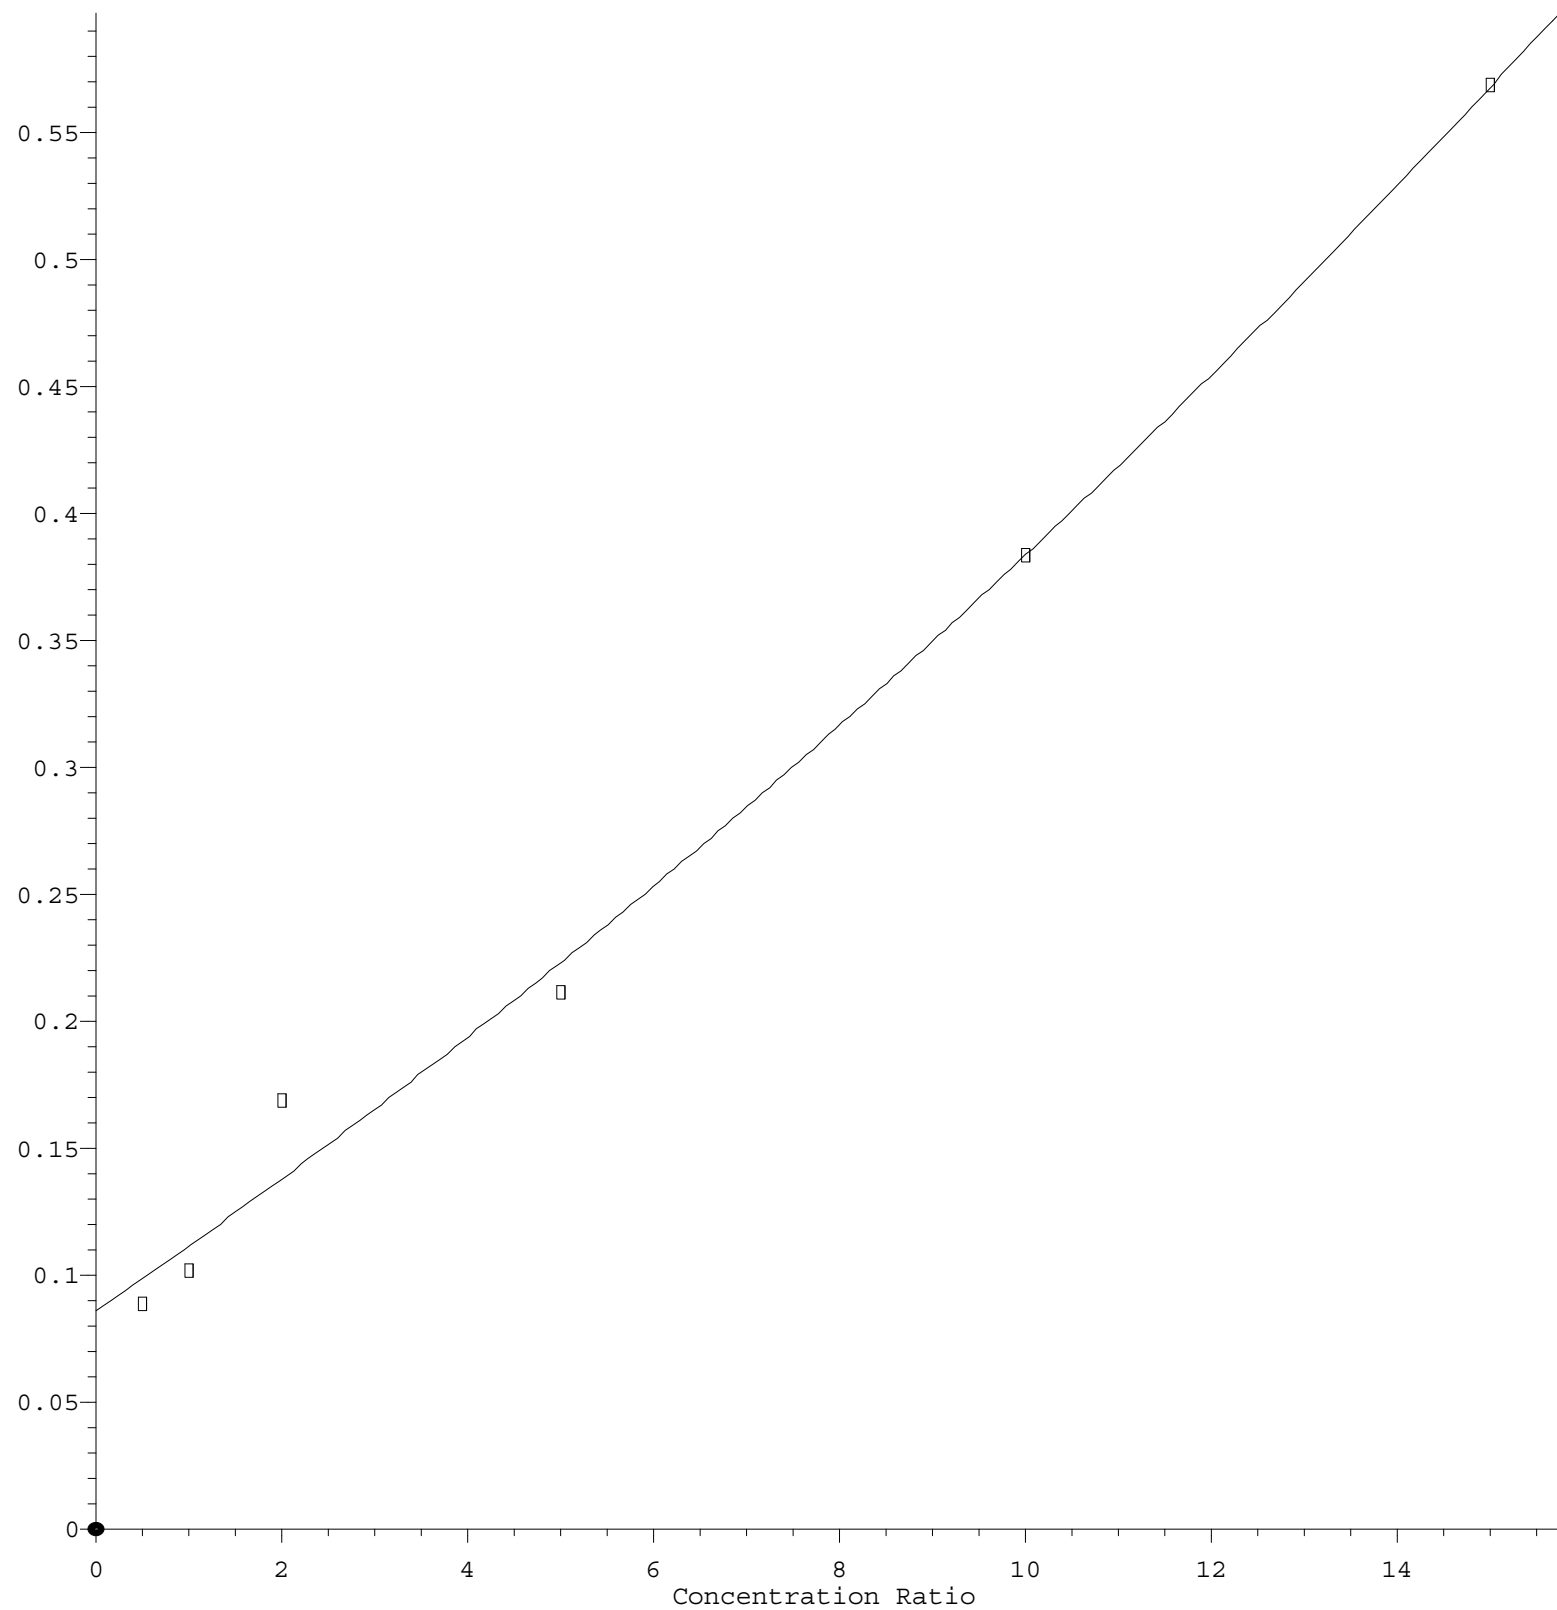

$R = 4.720e-004 A^2 + 2.504e-002 A + 8.609e-002$
 Coef of Det (r^2) = 0.992695 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M
 Calibration Table Last Updated: Tue Sep 27 03:19:14 2022

Carbon Disulfide

Response Ratio

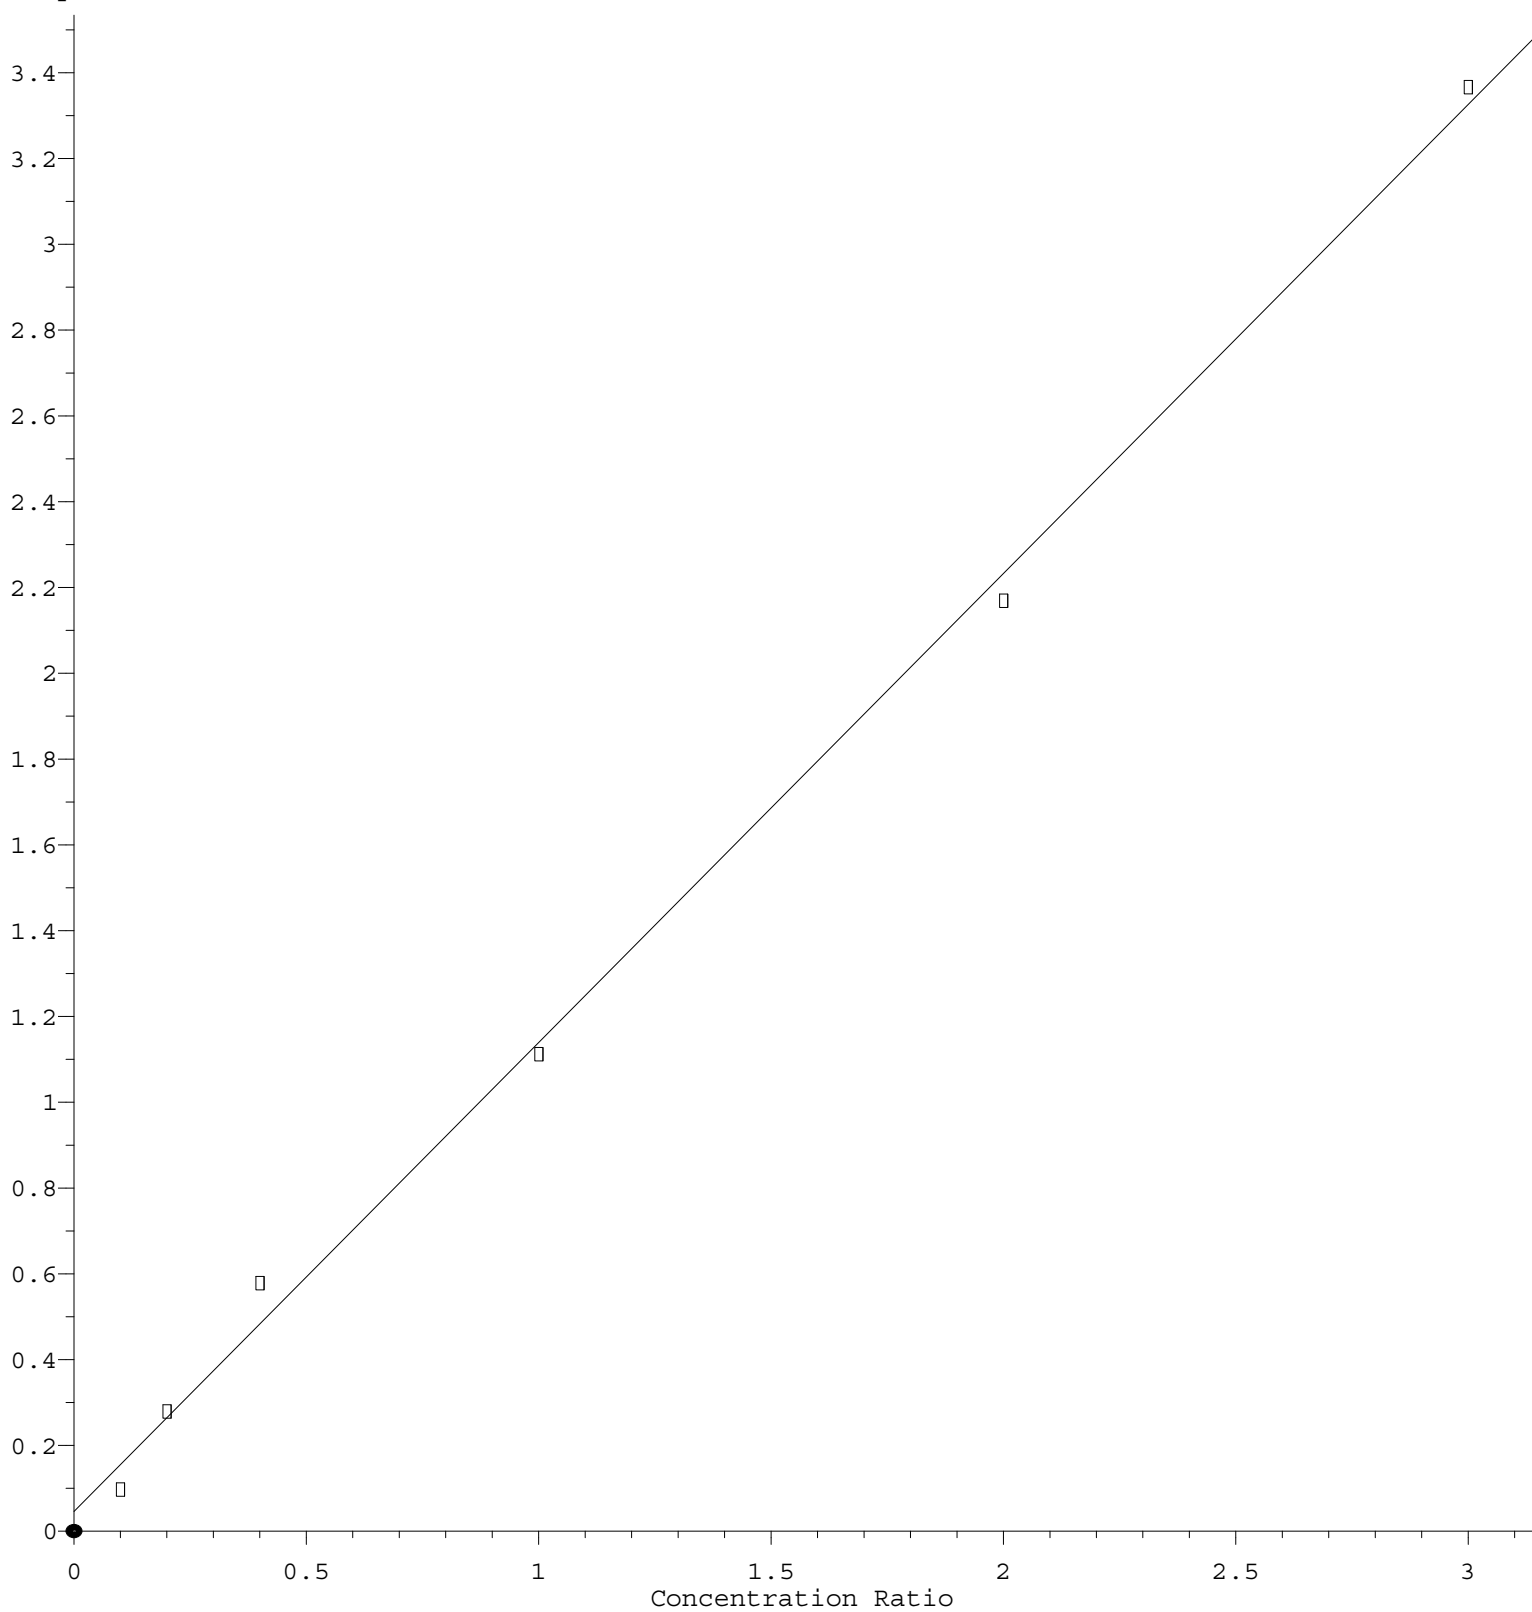


$$\text{Response} = 1.093\text{e}+000 * \text{Amt} + 4.578\text{e}-002$$

Coef of Det (r^2) = 0.997638 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M

Calibration Table Last Updated: Tue Sep 27 03:19:14 2022


Methyl Acetate

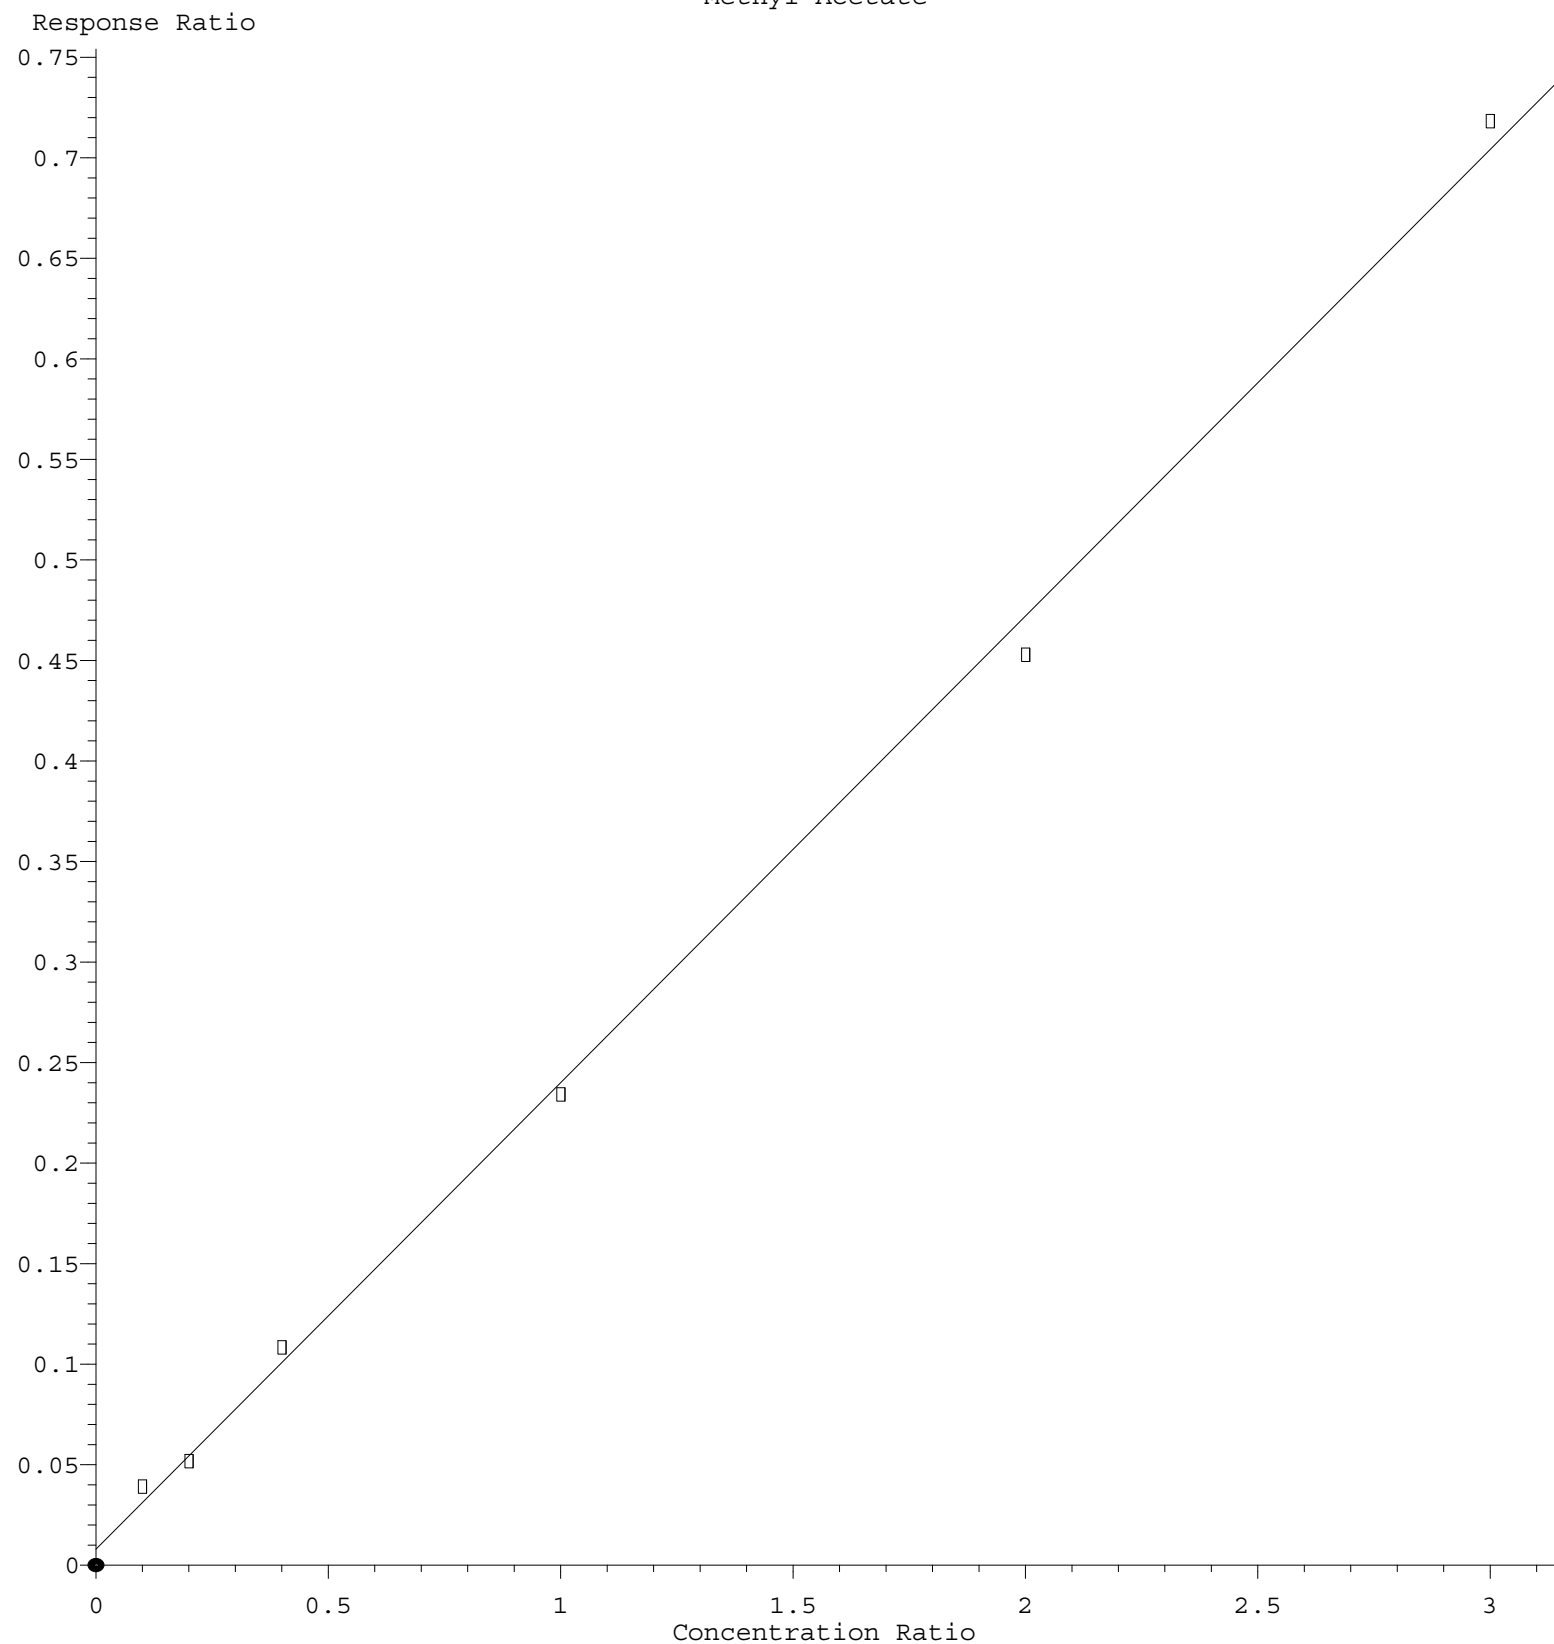

Response = 2.319e-001 * Amt + 8.390e-003
Coef of Det (r^2) = 0.997986 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M
Calibration Table Last Updated: Tue Sep 27 03:19:14 2022

Methylene Chloride

Response Ratio

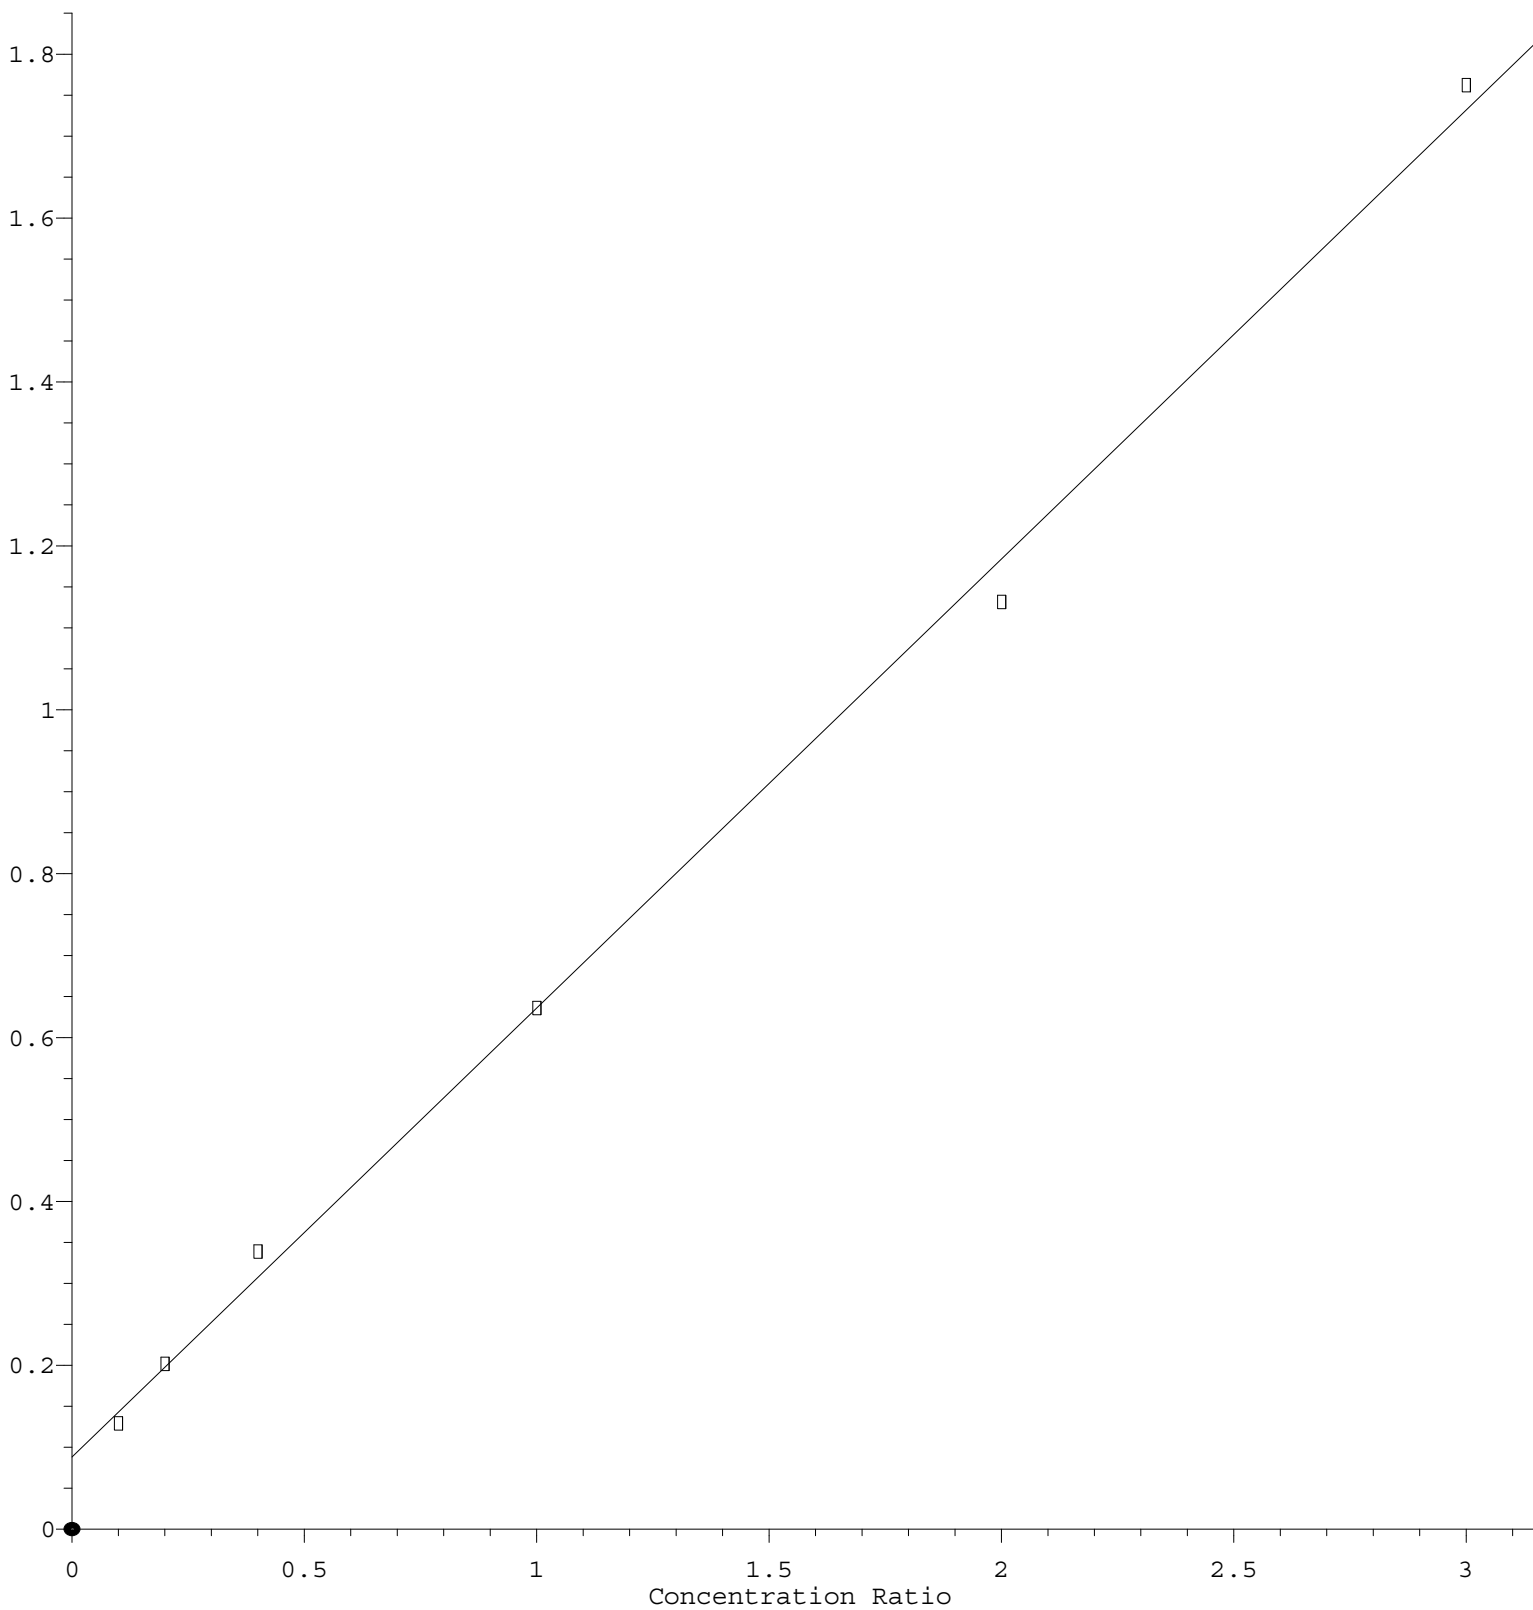

$$\text{Response} = 5.477\text{e-}001 * \text{Amt} + 8.830\text{e-}002$$


Coef of Det (r^2) = 0.997595 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M

Calibration Table Last Updated: Tue Sep 27 03:19:14 2022

Dibromofluoromethane

Response Ratio

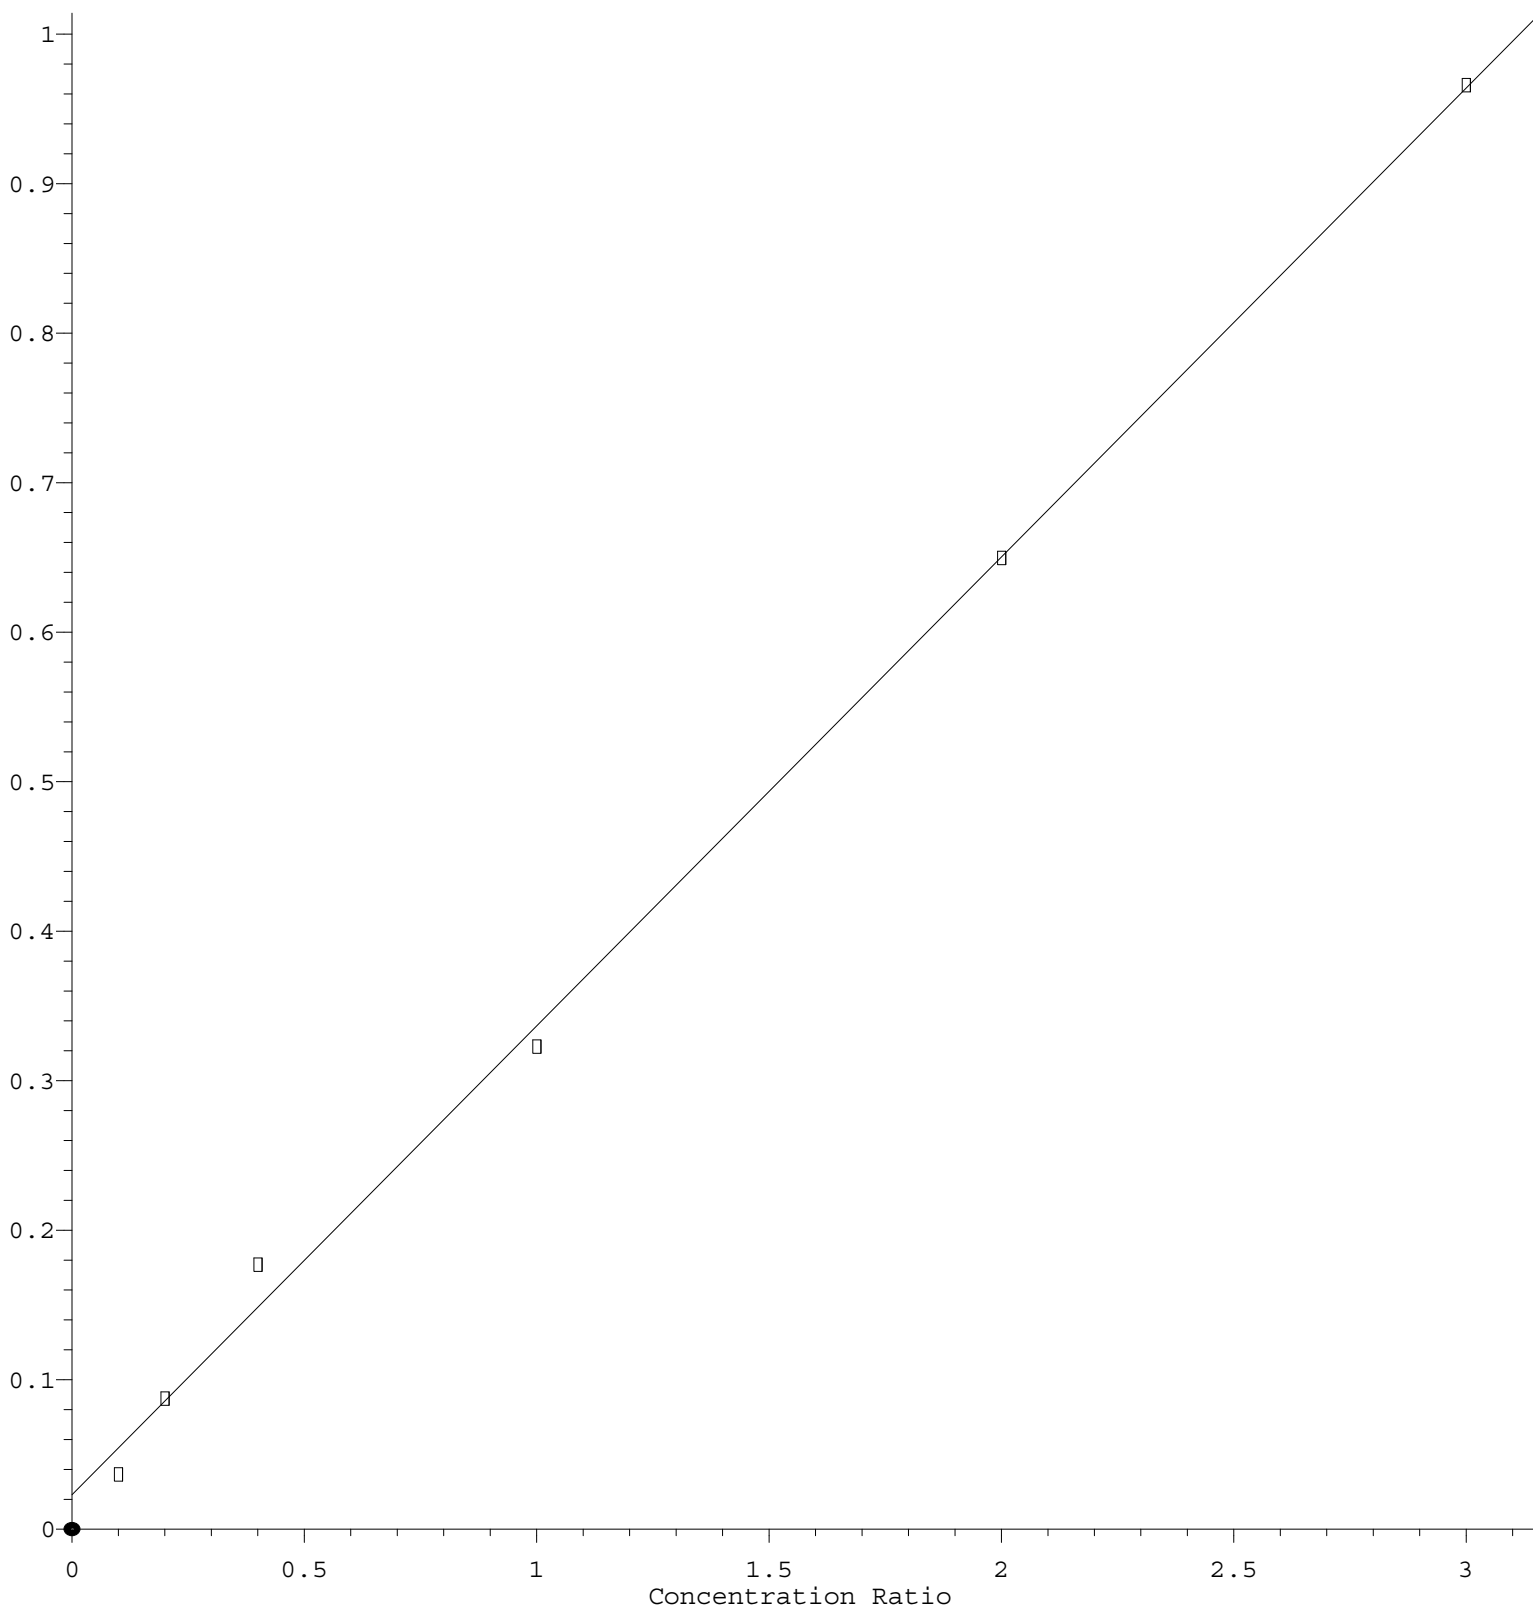


$$\text{Response} = 3.138\text{e-}001 * \text{Amt} + 2.278\text{e-}002$$

Coef of Det (r^2) = 0.998004 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M

Calibration Table Last Updated: Tue Sep 27 03:19:14 2022


1,4-Dioxane

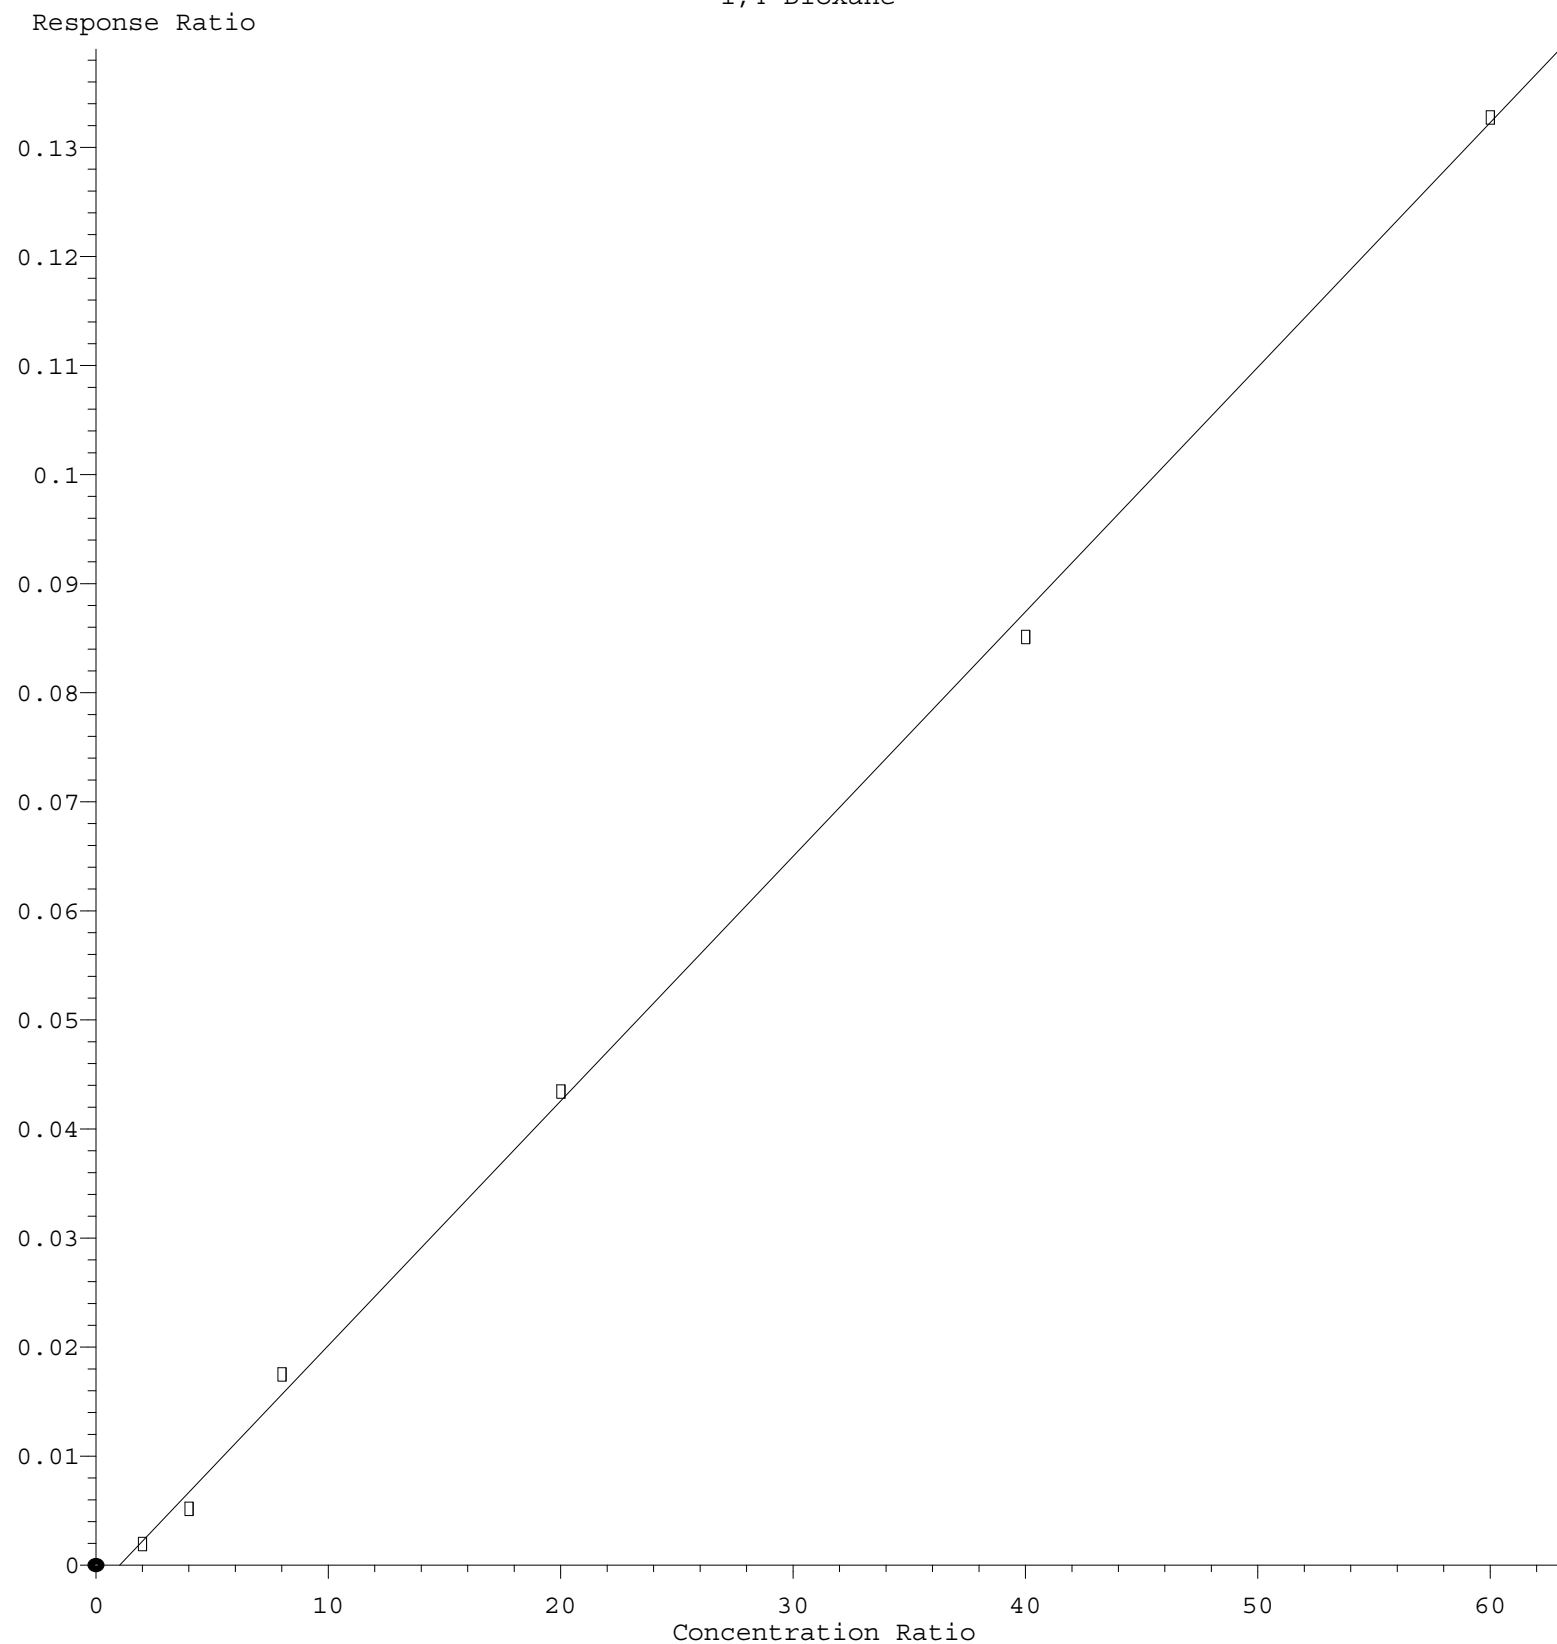

Response = $2.236 \times 10^{-3} \times \text{Amt} - 2.288 \times 10^{-3}$
 Coef of Det (r^2) = 0.999123 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M
 Calibration Table Last Updated: Tue Sep 27 03:19:14 2022

2-Chloroethyl Vinyl ether


Response Ratio

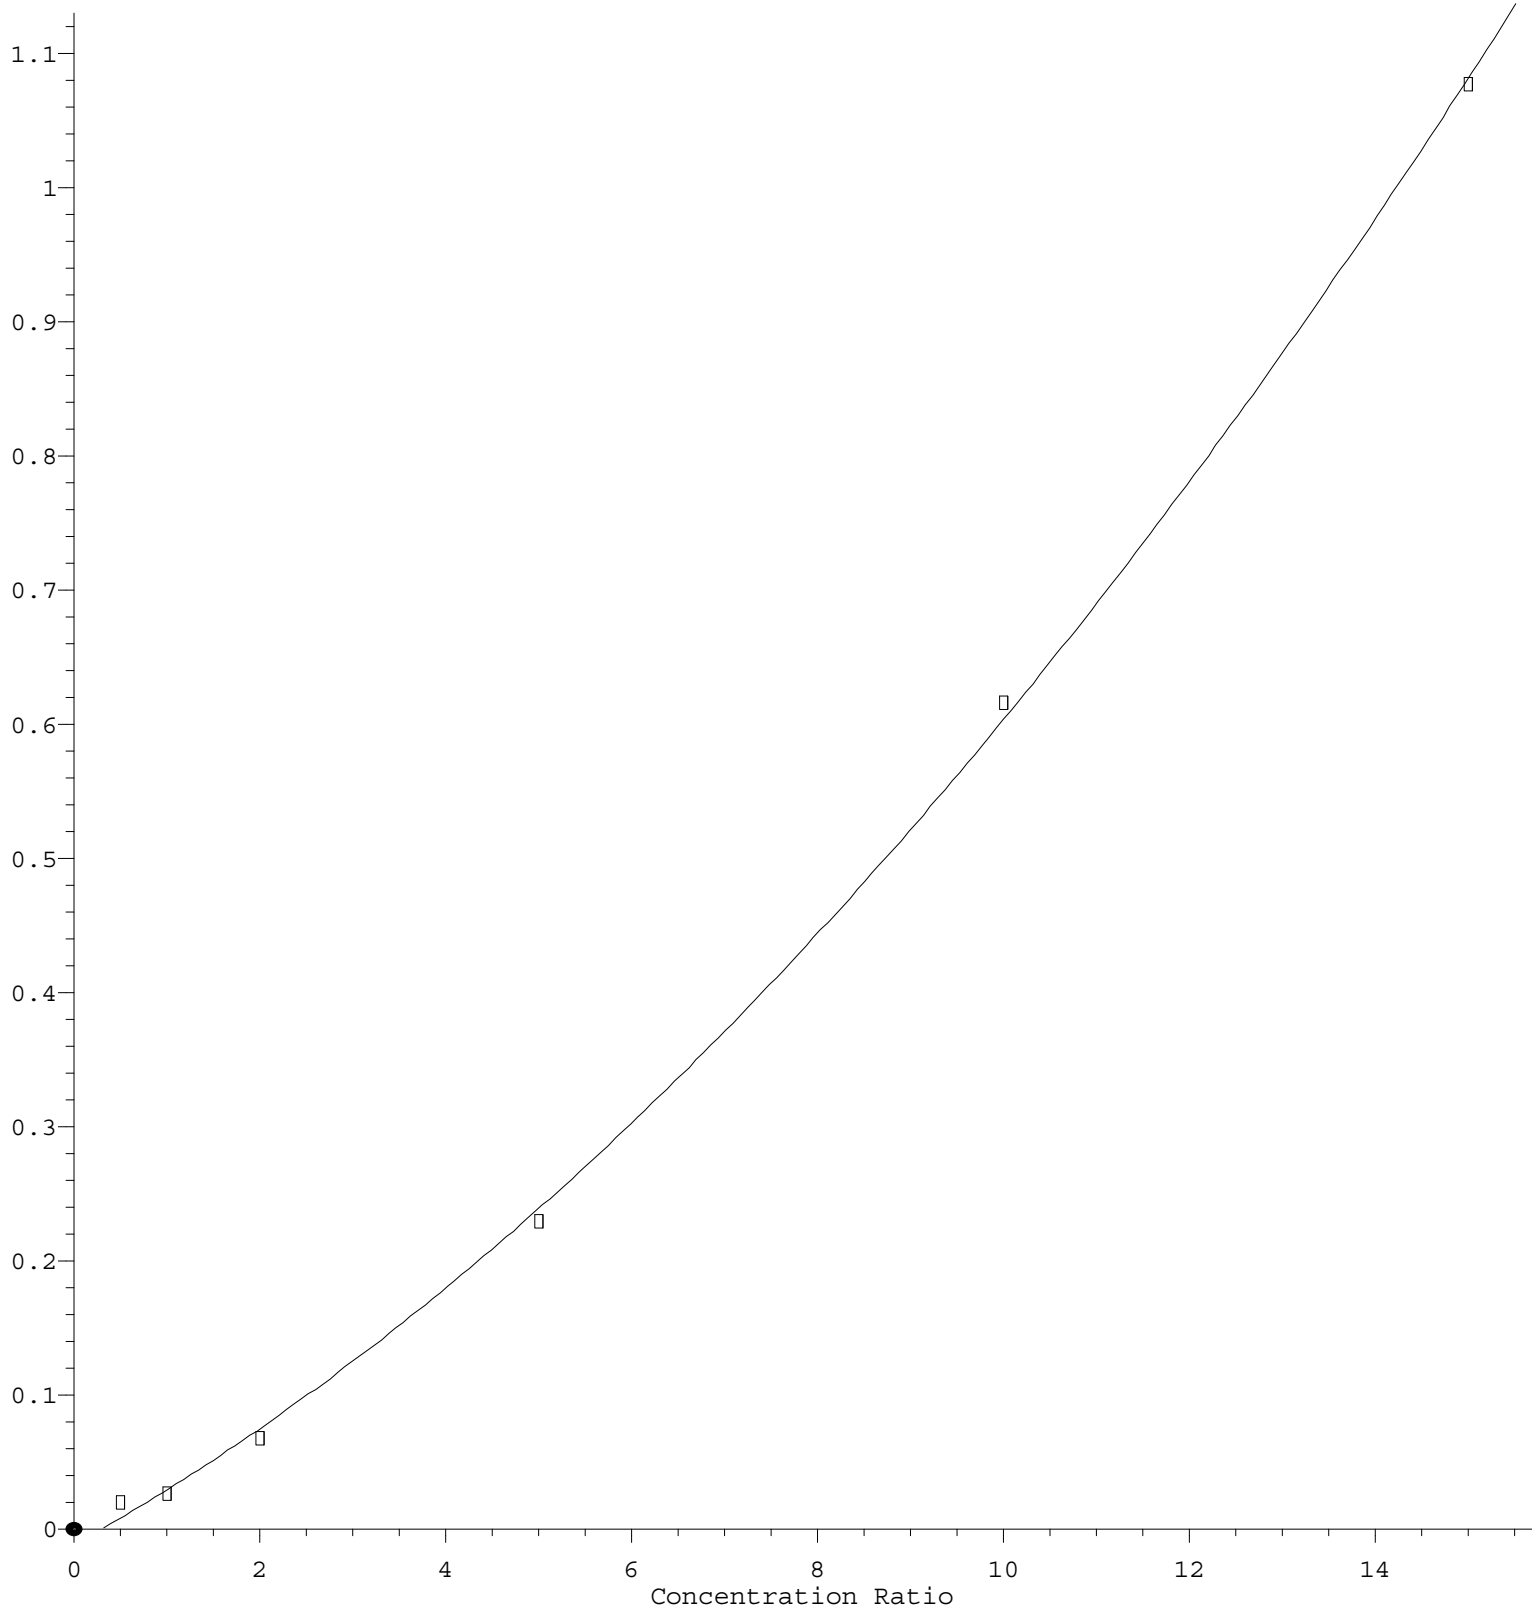

$R = 2.272e-003 A^2 + 3.879e-002 A - 1.168e-002$
 Coef of Det (r^2) = 0.999490 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M
 Calibration Table Last Updated: Tue Sep 27 03:19:14 2022

2-Chloroethyl Vinyl ether


Response Ratio

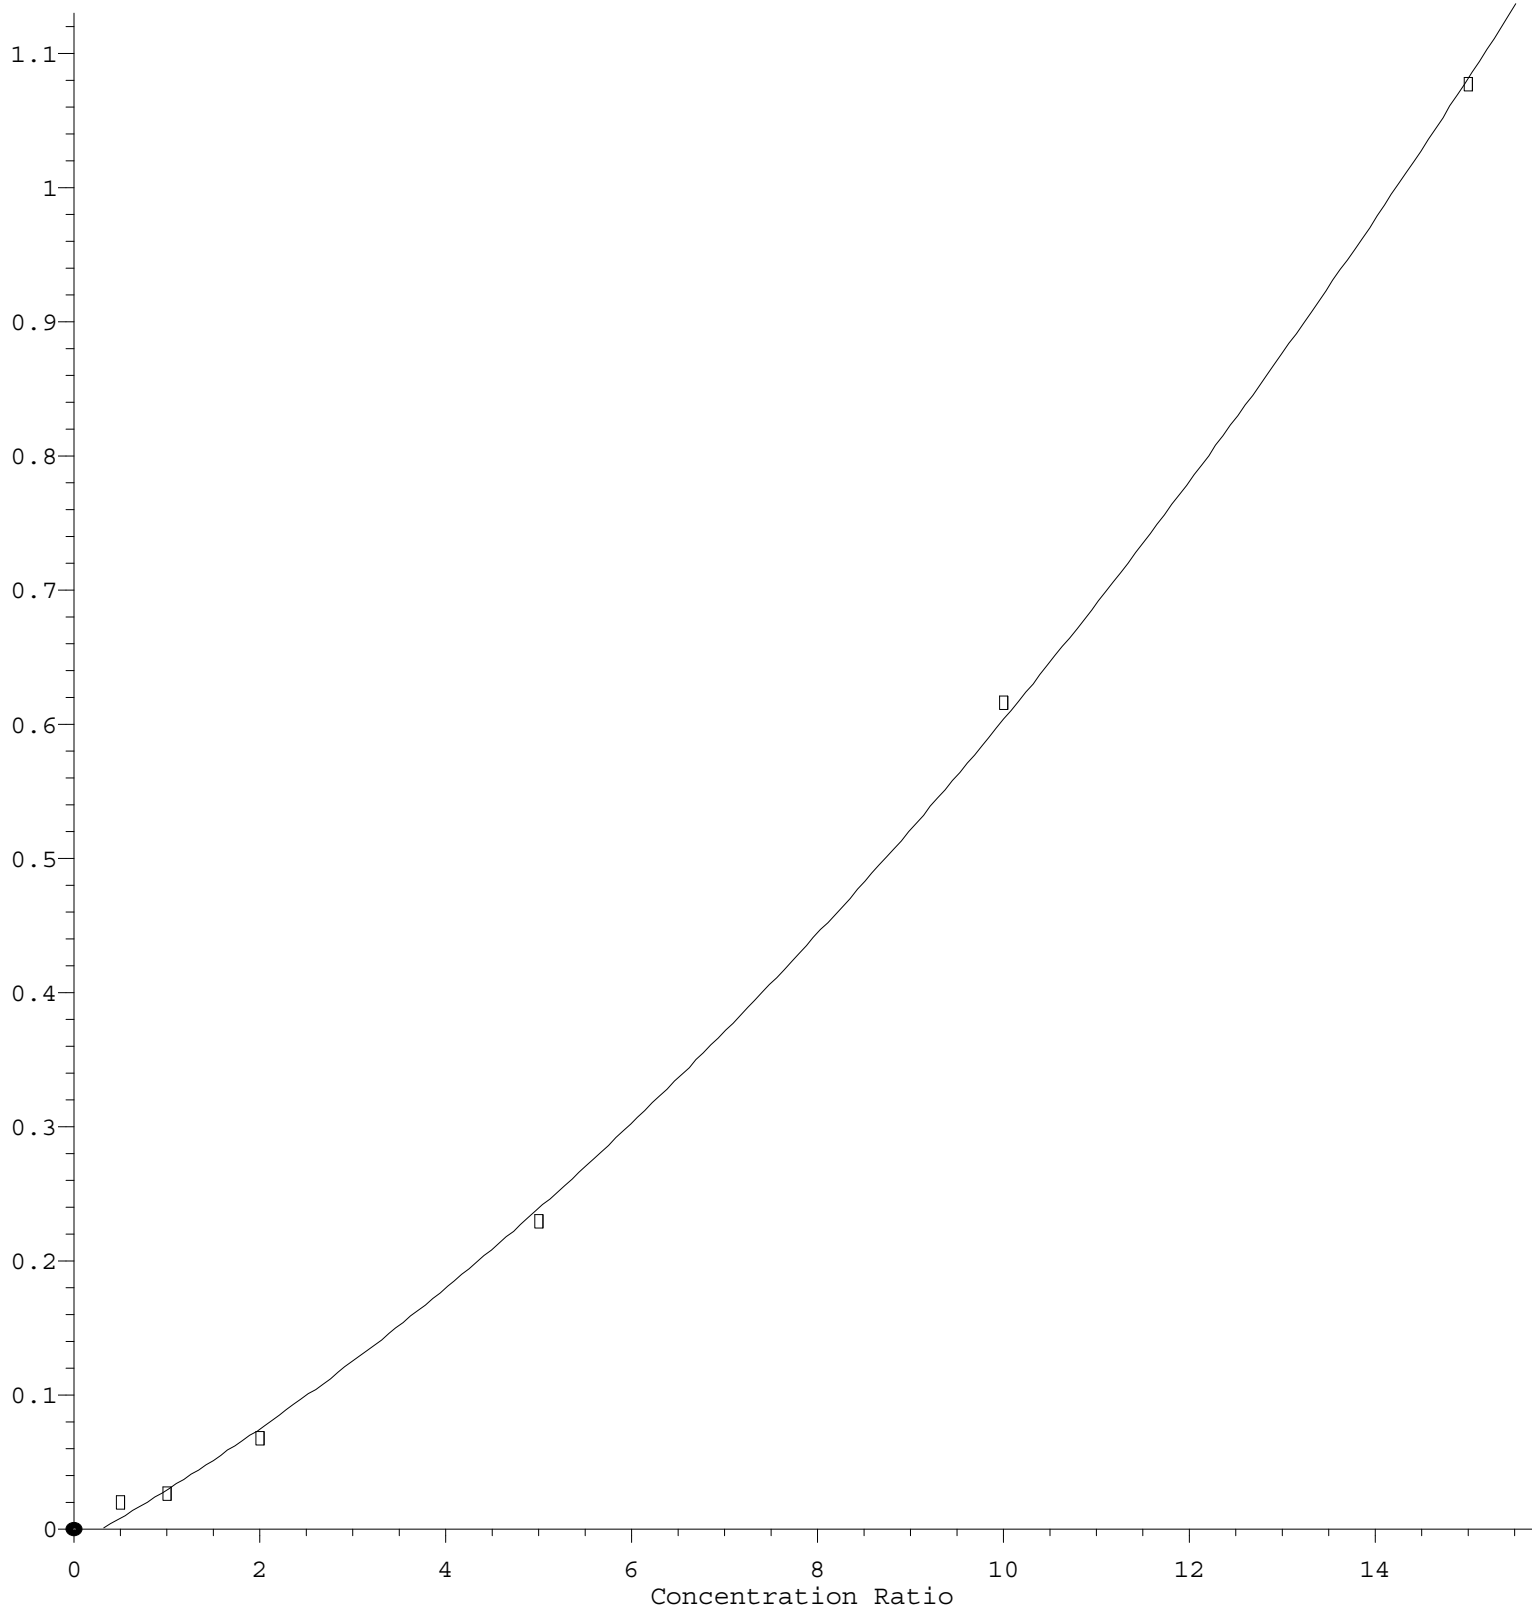

$R = 2.272e-003 A^2 + 3.879e-002 A - 1.168e-002$
 Coef of Det (r^2) = 0.999490 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M
 Calibration Table Last Updated: Tue Sep 27 03:19:14 2022

4-Bromofluorobenzene

Response Ratio

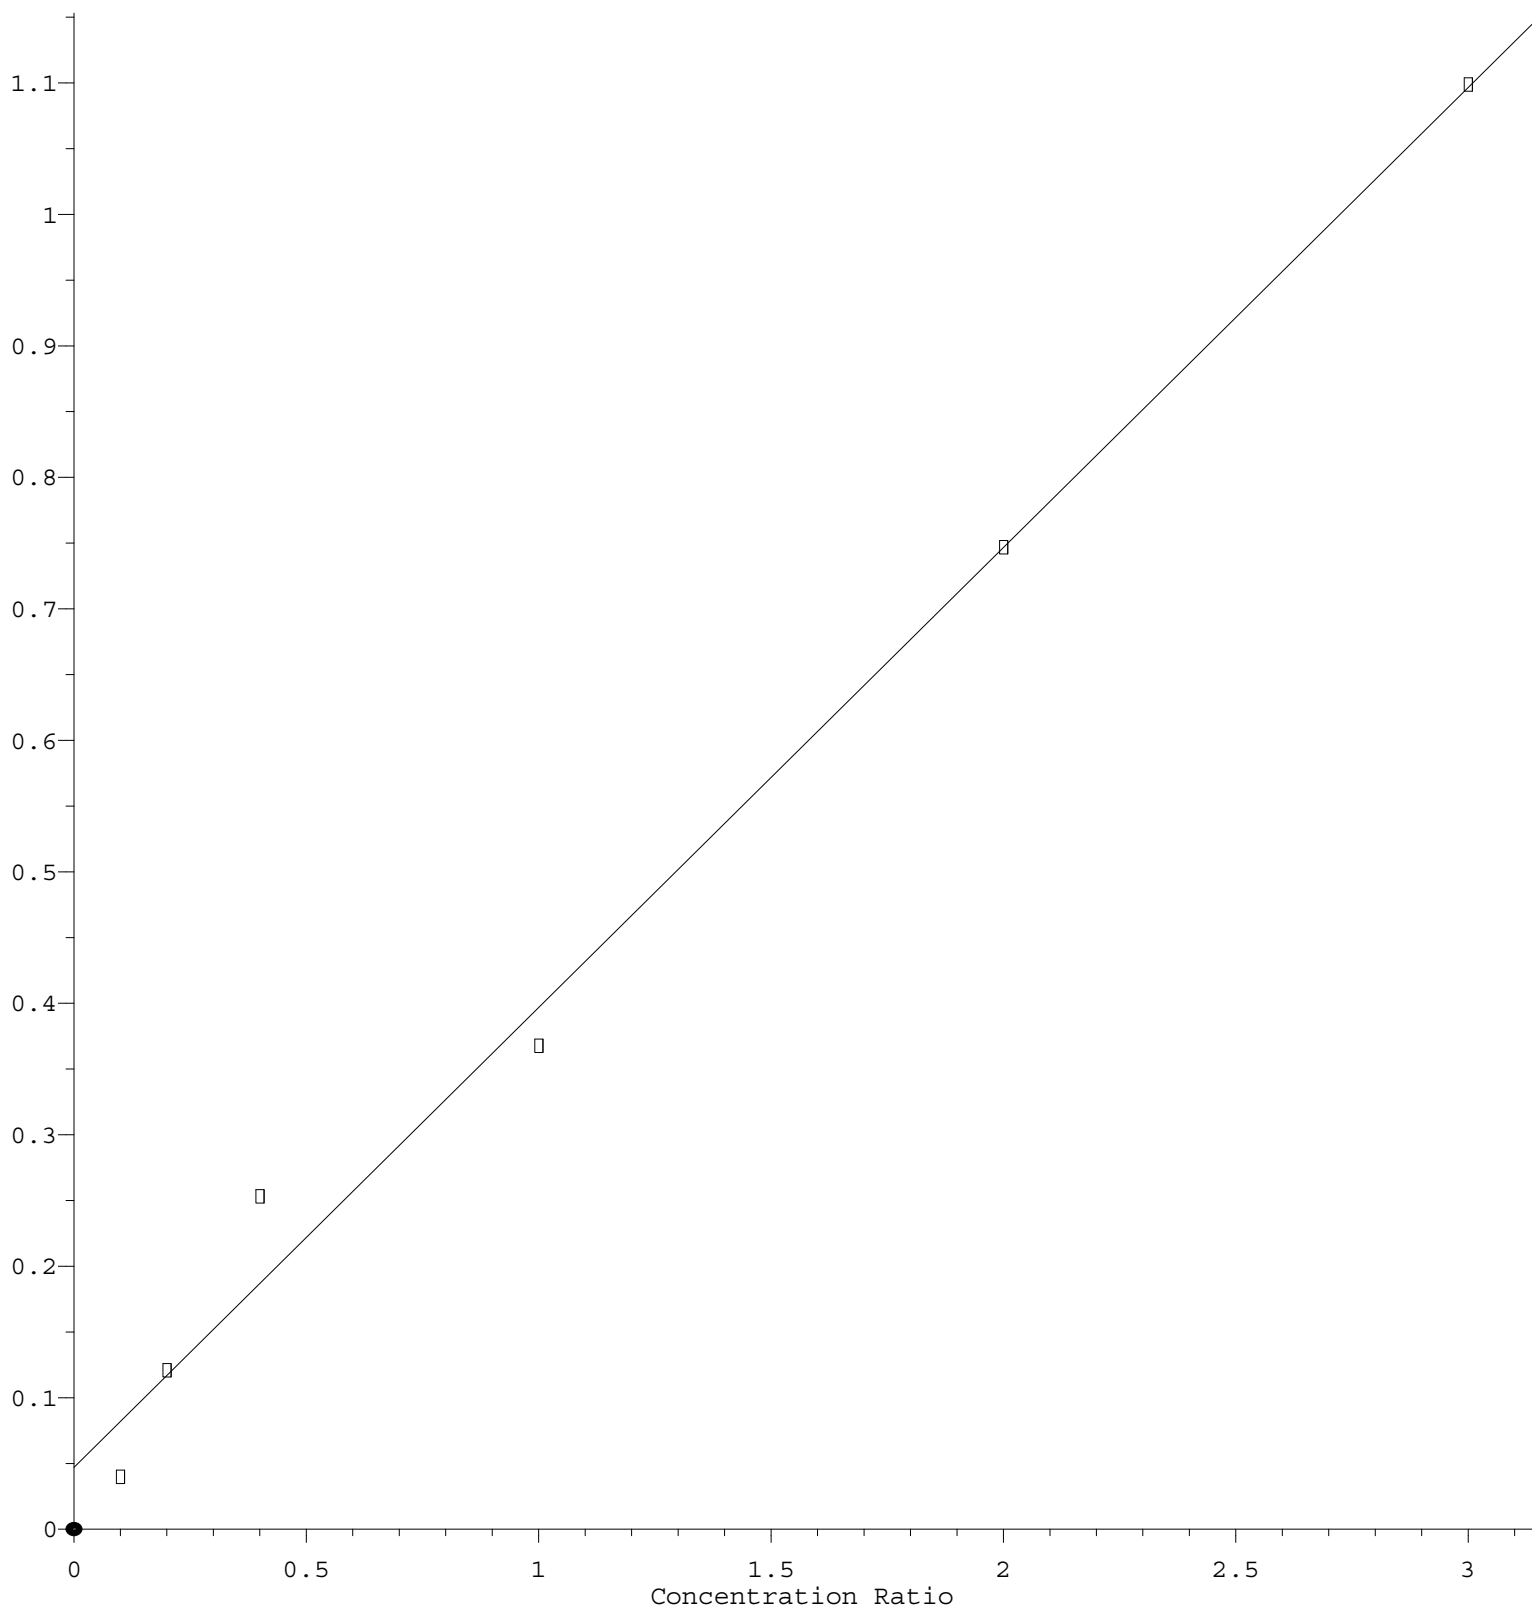


$$\text{Response} = 3.498\text{e-}001 * \text{Amt} + 4.722\text{e-}002$$

Coef of Det (r^2) = 0.991533 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M

Calibration Table Last Updated: Tue Sep 27 03:19:14 2022

1,2-Dibromo-3-Chloropropane

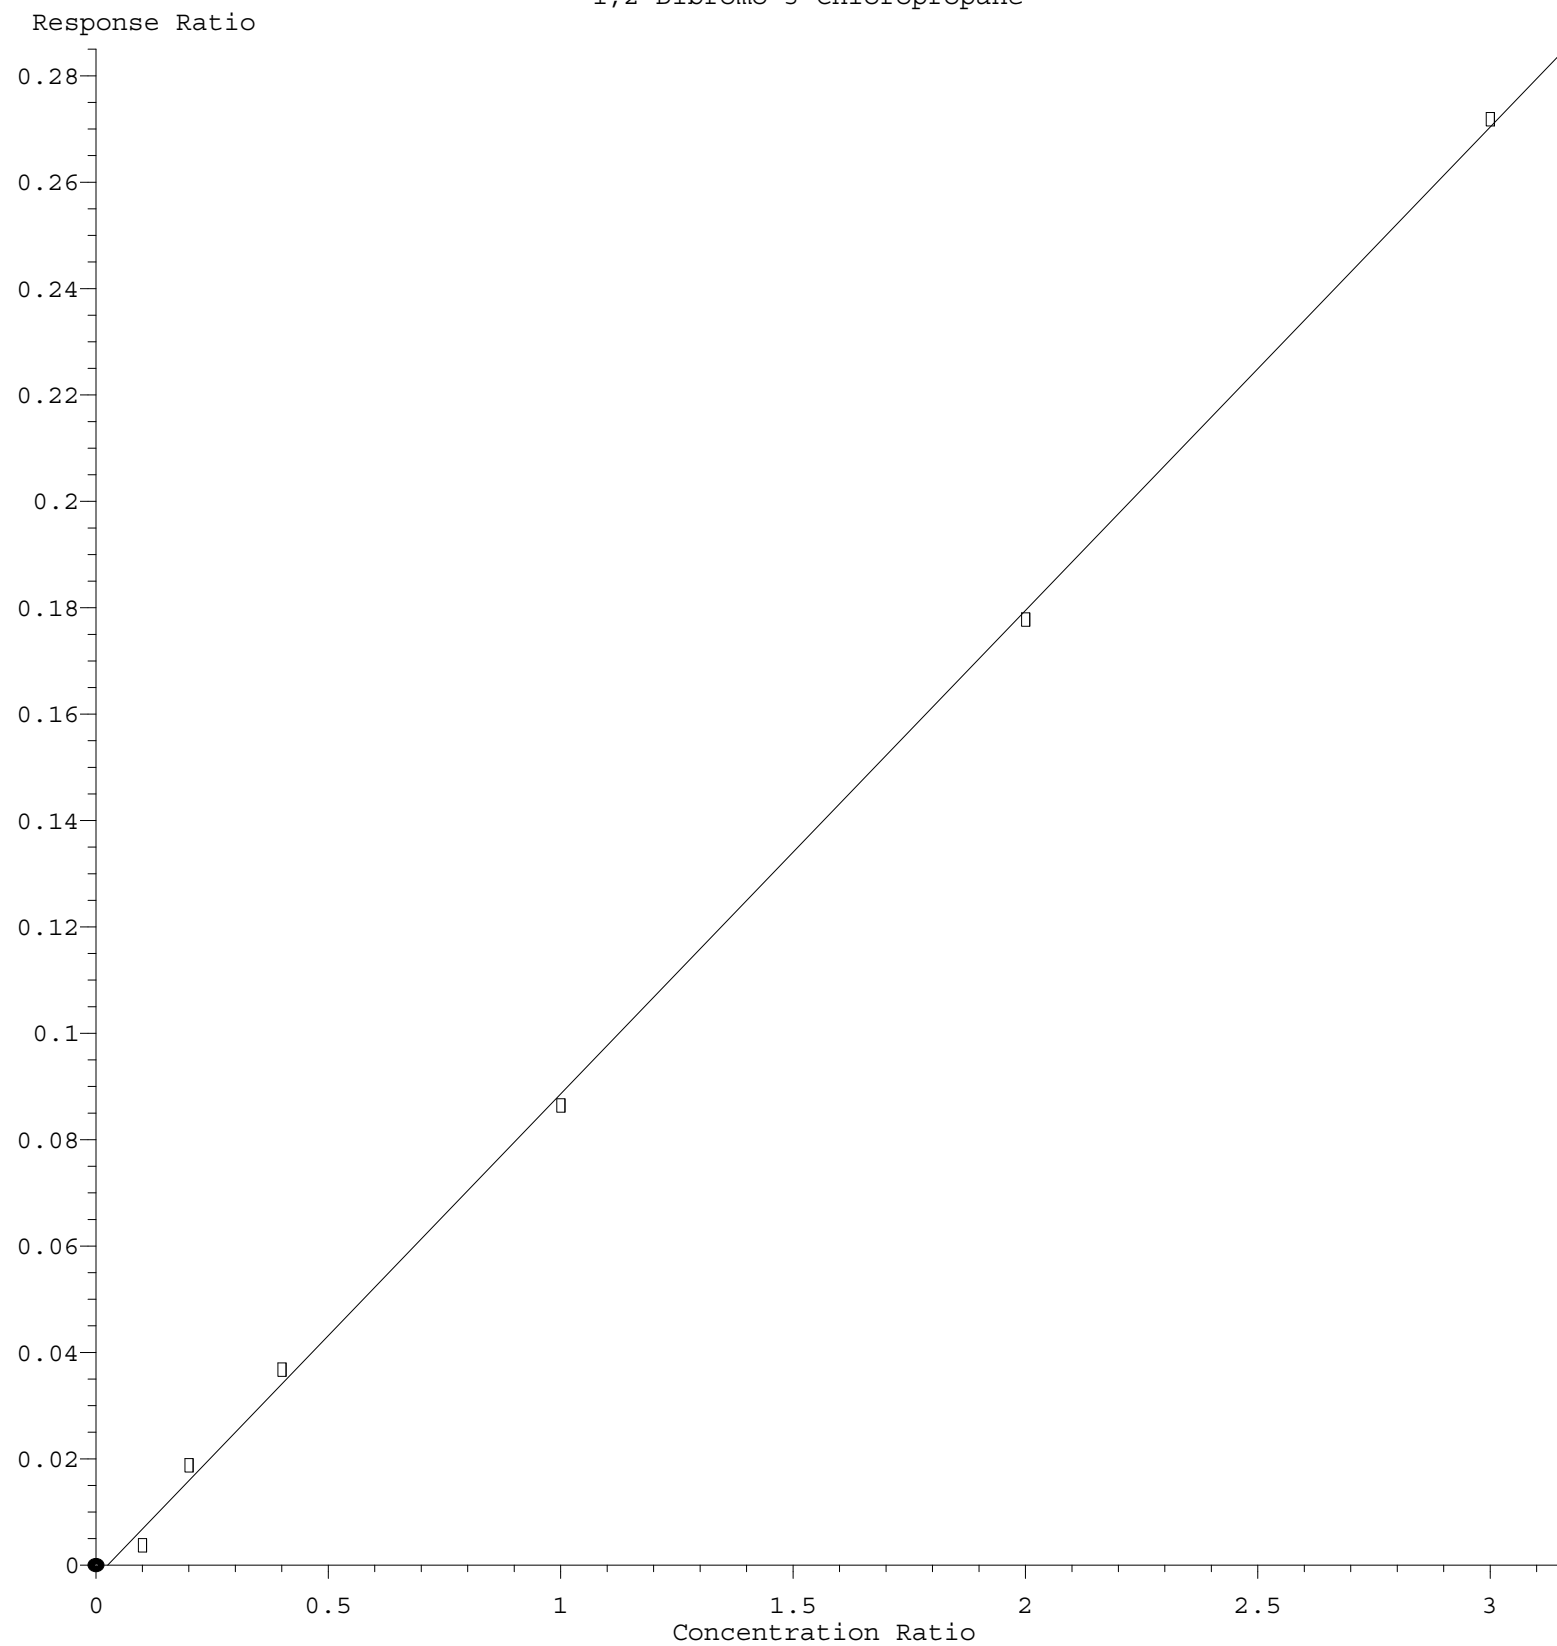

Response = $9.089 \times 10^{-2} \times \text{Amt} - 2.284 \times 10^{-3}$
 Coef of Det (r^2) = 0.999373 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D092622S.M
 Calibration Table Last Updated: Tue Sep 27 03:19:14 2022