
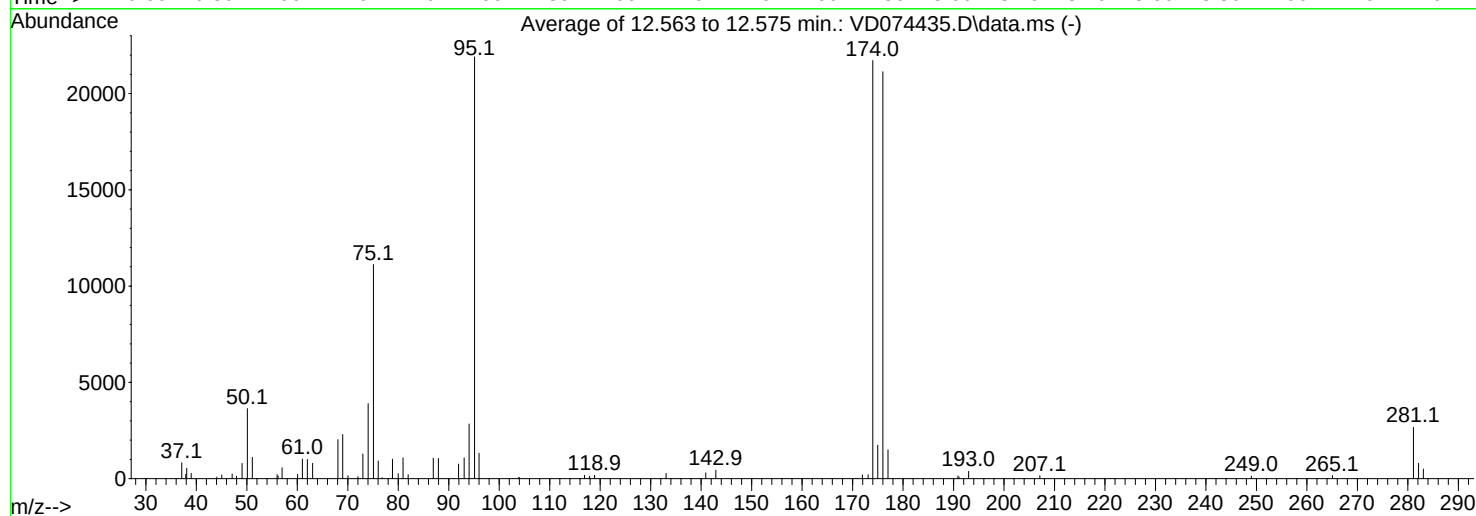


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092722\
 Data File : VD074435.D
 Acq On : 27 Sep 2022 09:44
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D092622S.M
 Title : SW846 8260
 Last Update : Tue Sep 27 03:19:14 2022

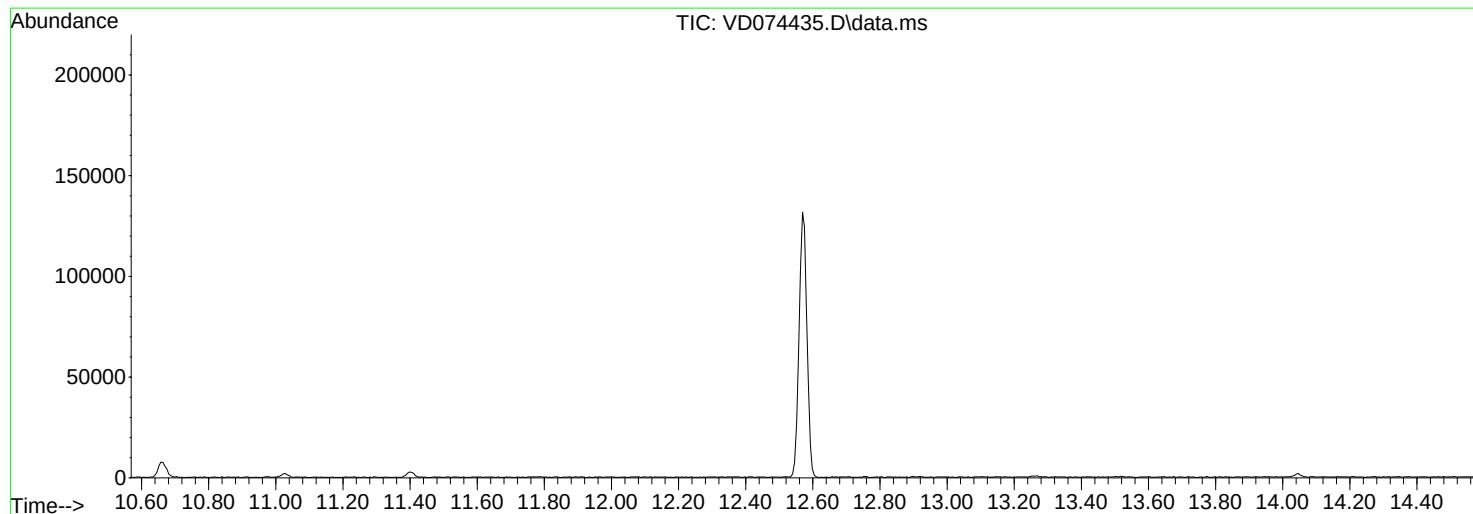

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	3641	PASS
75	95	30	60	50.8	11119	PASS
95	95	100	100	100.0	21907	PASS
96	95	5	9	6.0	1325	PASS
173	174	0.00	2	0.9	202	PASS
174	95	50	100	99.1	21712	PASS
175	174	5	9	8.0	1738	PASS
176	174	95	101	97.3	21133	PASS
177	176	5	9	7.1	1499	PASS