


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD102822\
 Data File : VD074662.D
 Acq On : 28 Oct 2022 09:10
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D102722S.M
 Title : SW846 8260
 Last Update : Fri Oct 28 00:18:17 2022

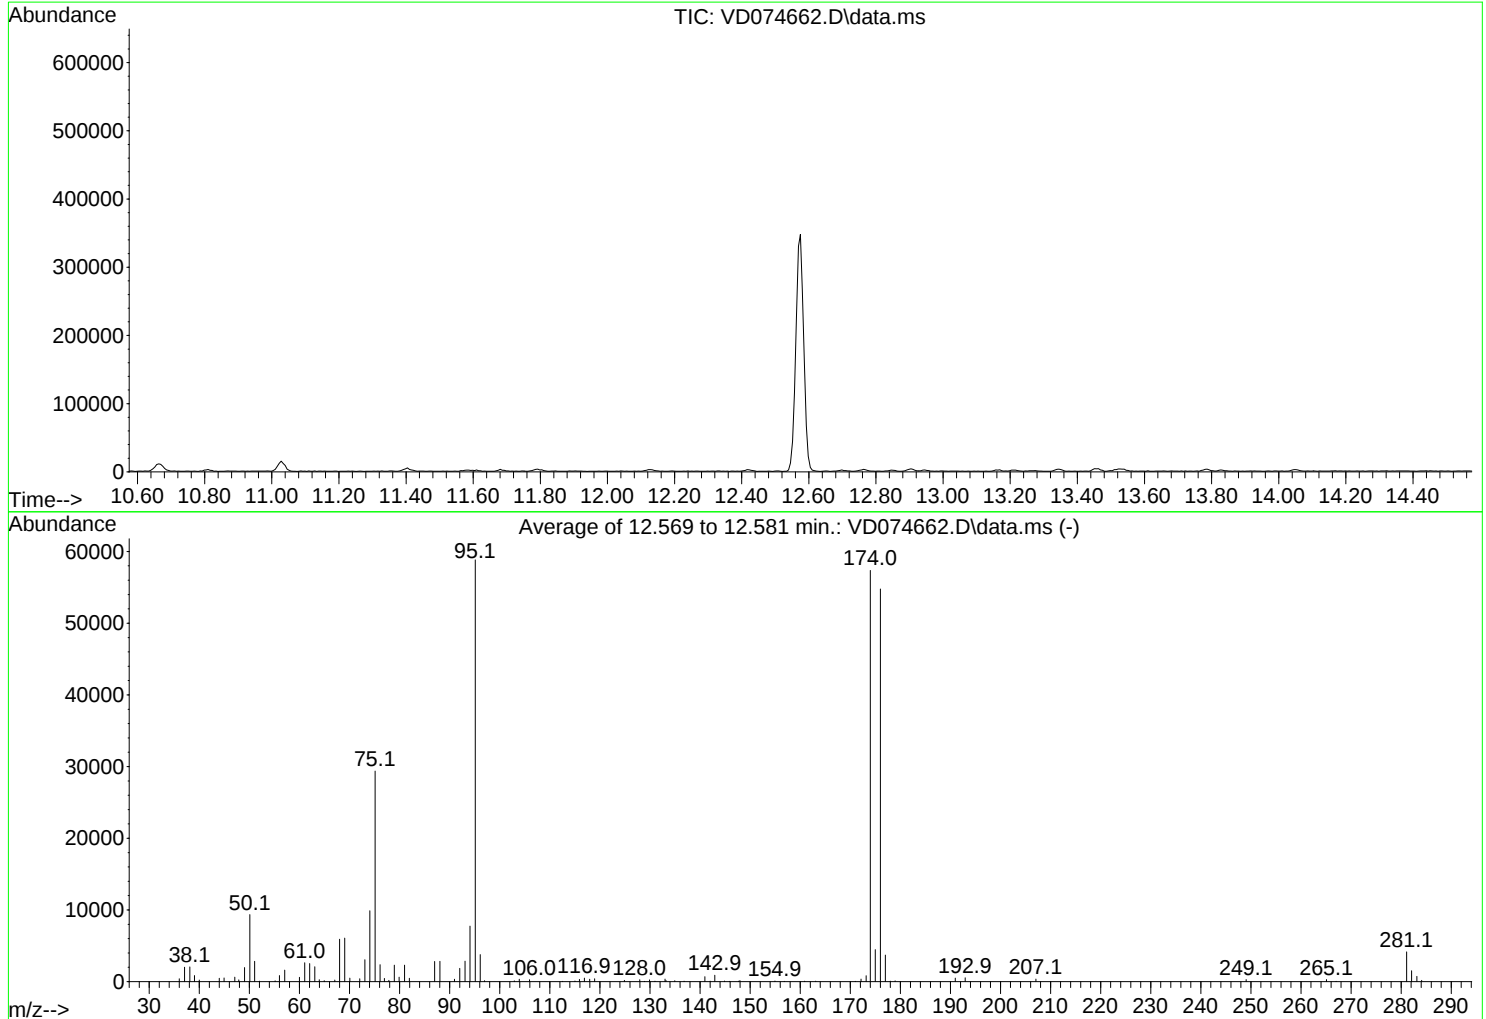

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	9354	PASS
75	95	30	60	49.9	29365	PASS
95	95	100	100	100.0	58840	PASS
96	95	5	9	6.4	3764	PASS
173	174	0.00	2	1.4	825	PASS
174	95	50	100	97.5	57373	PASS
175	174	5	9	7.8	4461	PASS
176	174	95	101	95.5	54773	PASS
177	176	5	9	6.8	3711	PASS