
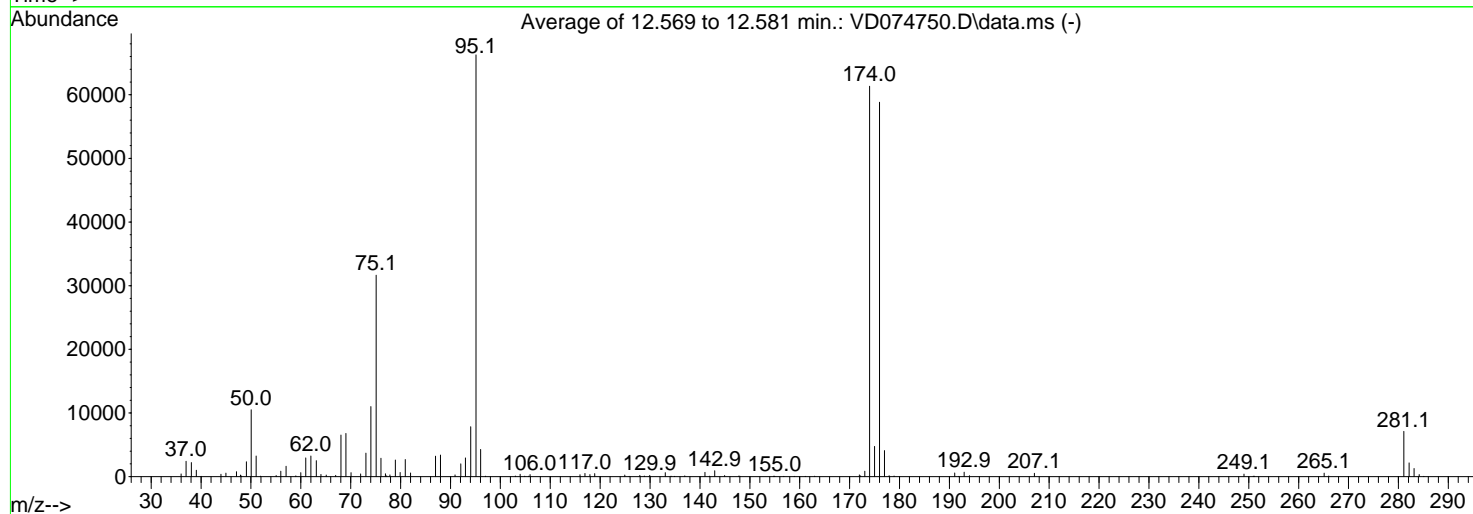


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD110722\
 Data File : VD074750.D
 Acq On : 07 Nov 2022 09:06
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D110222S.M
 Title : SW846 8260
 Last Update : Thu Nov 03 02:30:45 2022

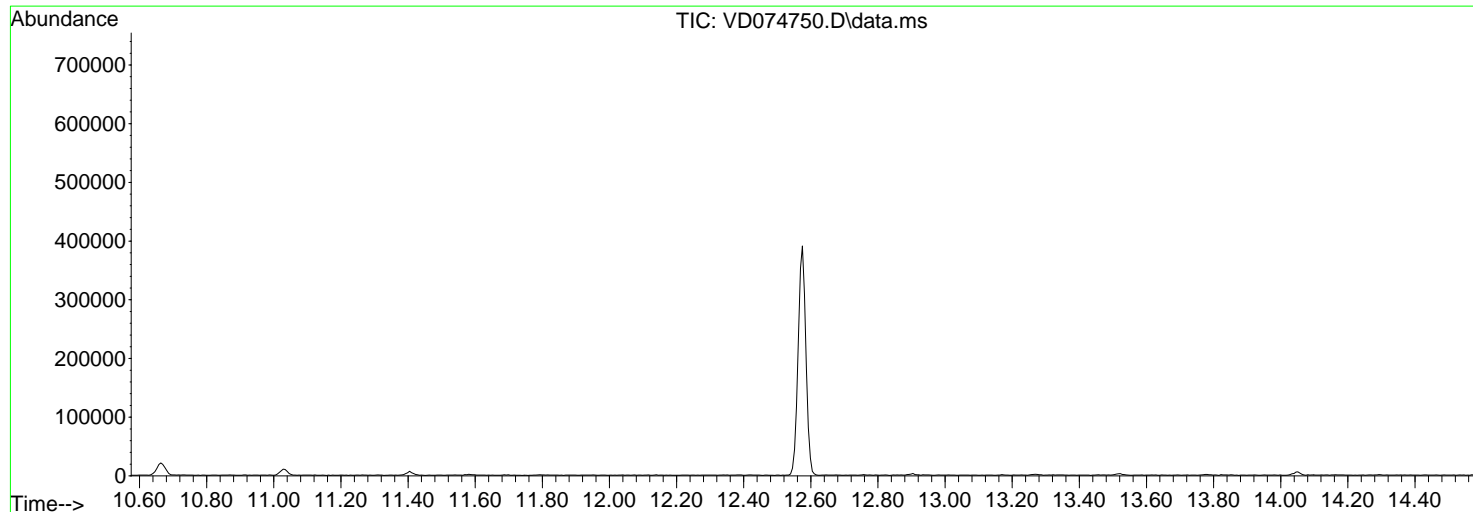

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50 | 95 | 15 | 40 | 15.9 | 10508 | PASS |
| 75 | 95 | 30 | 60 | 47.8 | 31659 | PASS |
| 95 | 95 | 100 | 100 | 100.0 | 66267 | PASS |
| 96 | 95 | 5 | 9 | 6.4 | 4272 | PASS |
| 173 | 174 | 0.00 | 2 | 1.4 | 848 | PASS |
| 174 | 95 | 50 | 100 | 92.6 | 61347 | PASS |
| 175 | 174 | 5 | 9 | 7.8 | 4755 | PASS |
| 176 | 174 | 95 | 101 | 95.9 | 58832 | PASS |
| 177 | 176 | 5 | 9 | 7.0 | 4094 | PASS |