

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111722\
 Data File : VD074971.D
 Acq On : 17 Nov 2022 15:56
 Operator : VA/SY
 Sample : N5642-11
 Misc : 6.69G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 LEFT-SIDE-FLATS-31

Quant Time: Nov 17 22:36:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111122S.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 14 00:51:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	128595	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	235005	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	219458	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	95513	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	61919	75.485	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	150.980%
35) Dibromofluoromethane	7.810	113	80751	55.743	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	111.480%
50) Toluene-d8	10.269	98	293187	61.440	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	122.880%
62) 4-Bromofluorobenzene	12.575	95	83388	56.909	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	113.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111722\
Data File : VD074971.D
Acq On : 17 Nov 2022 15:56
Operator : VA/SY
Sample : N5642-11
Misc : 6.69G/5.00ml/MSVOA_D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
LEFT-SIDE-FLATS-31

Quant Time: Nov 17 22:36:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111122S.M
Quant Title : SW846 8260
QLast Update : Mon Nov 14 00:51:58 2022
Response via : Initial Calibration




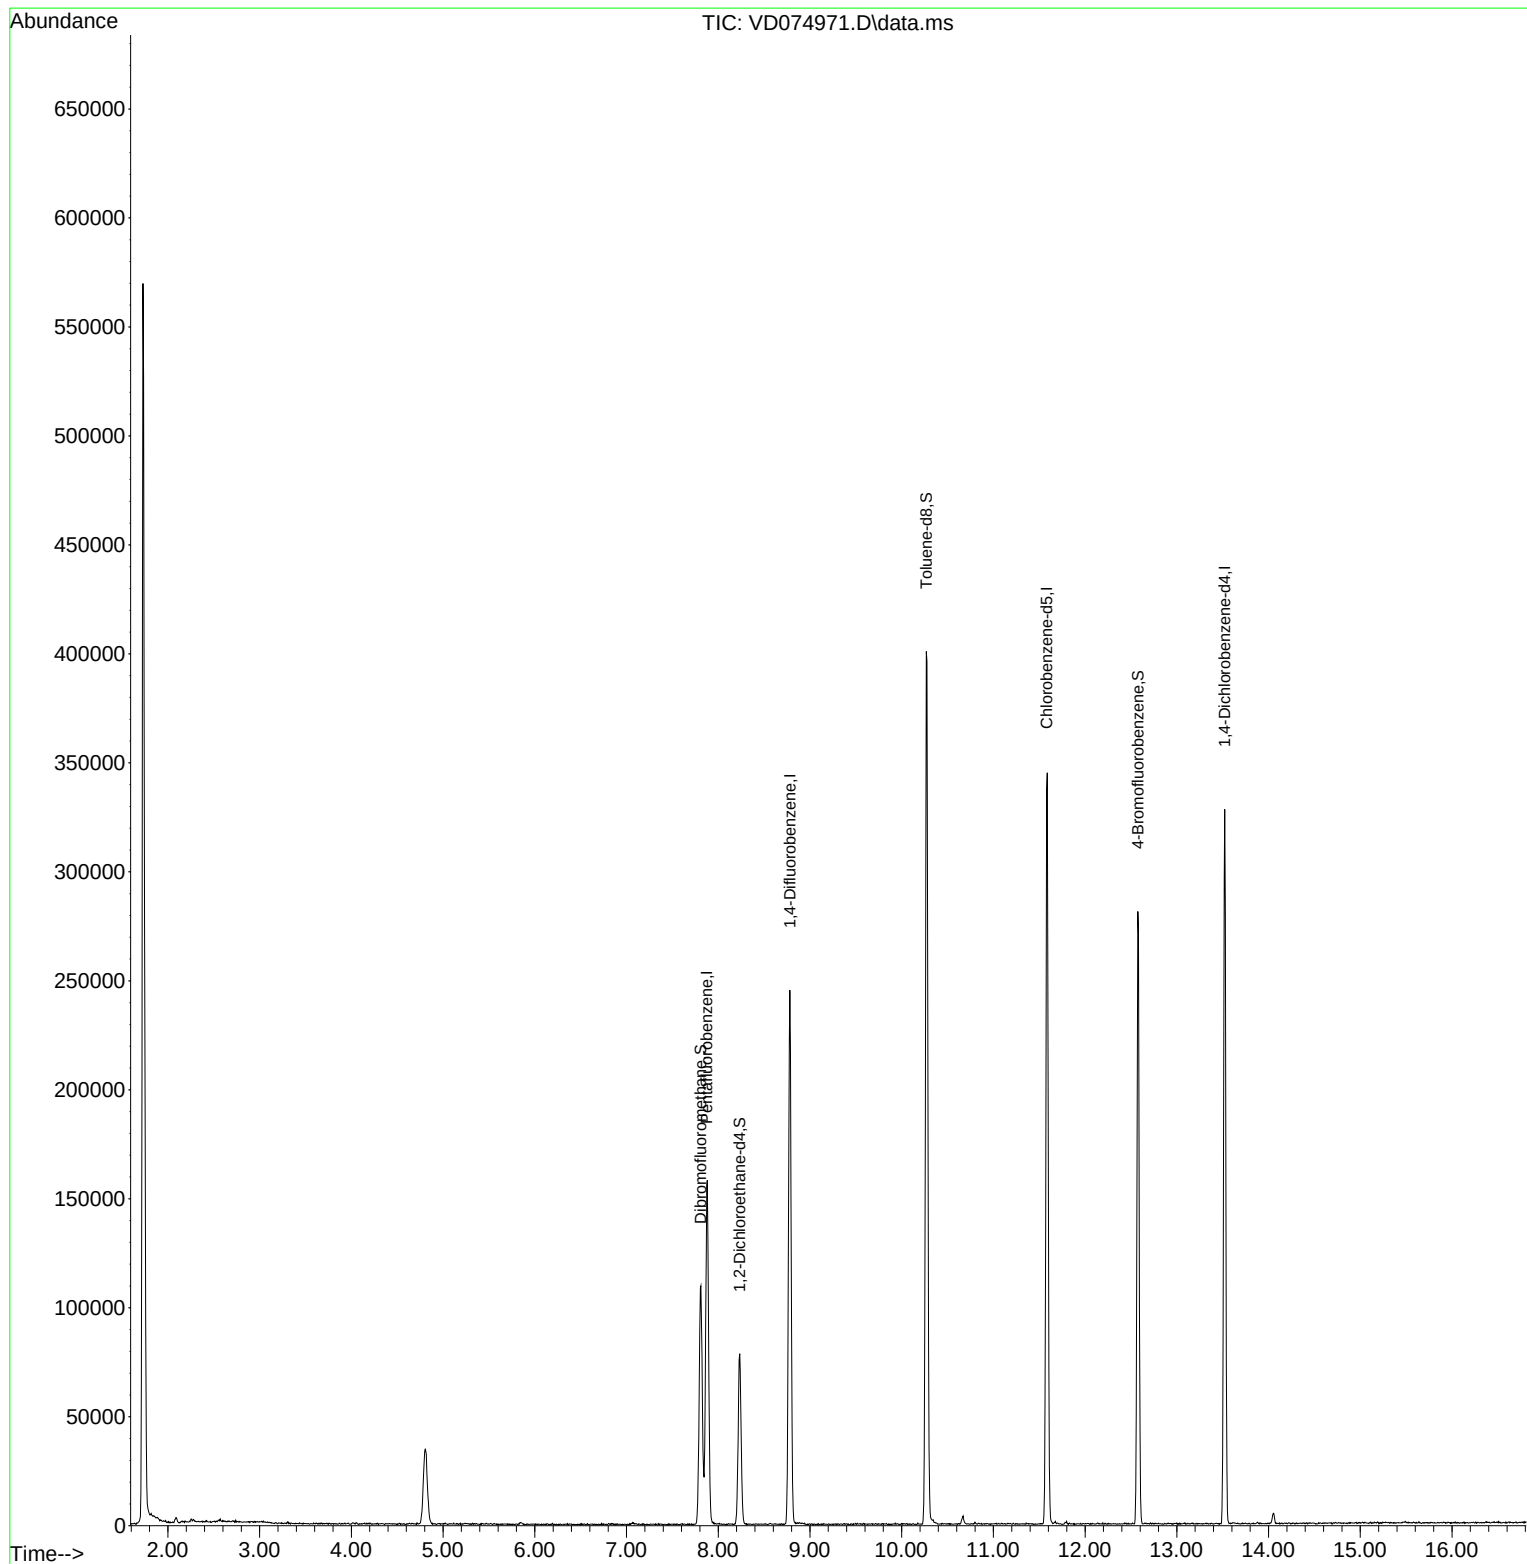


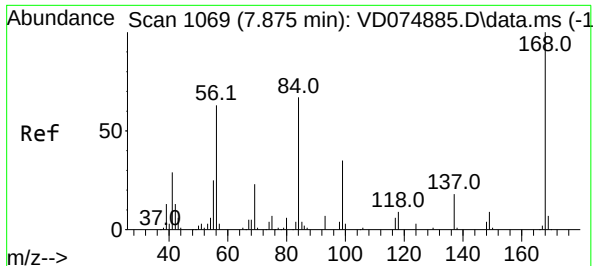

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1130
Delta R.T. 0.000 min
Lab File: VD074971.D
Acq: 17 Nov 2022 15:56




Instrument :
MSVOA_D
ClientSampleId :
LEFT-SIDE-FLATS-31


Tgt Ion:168 Resp: 128595
Ion Ratio Lower Upper
168 100
99 49.7 40.9 61.3

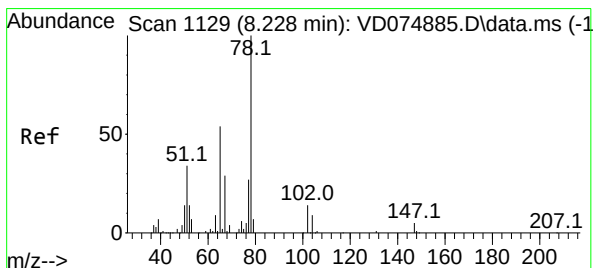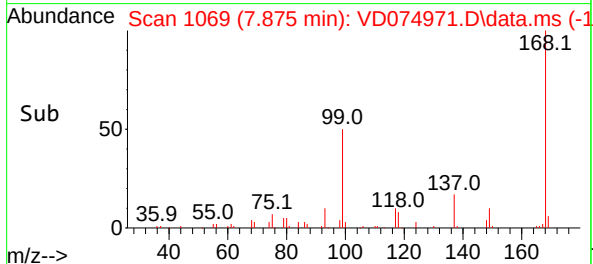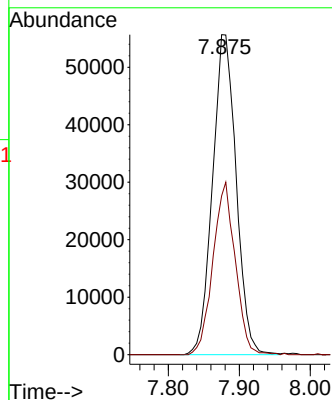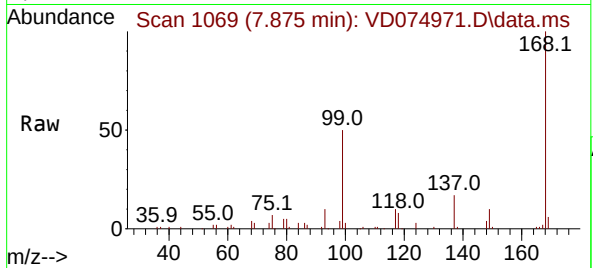

#33
1,2-Dichloroethane-d4
Concen: 75.485 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD074971.D
Acq: 17 Nov 2022 15:56

Tgt Ion: 65 Resp: 61919
Ion Ratio Lower Upper
65 100
67 54.7 0.0 110.2

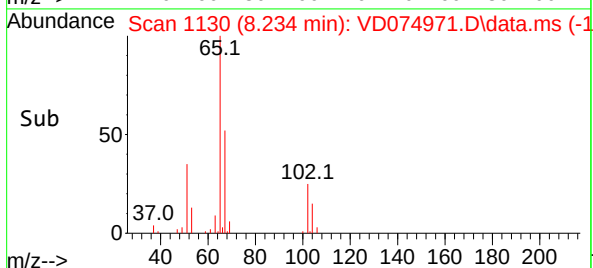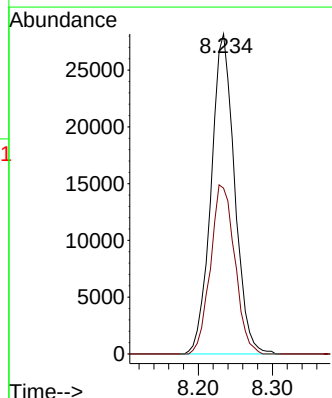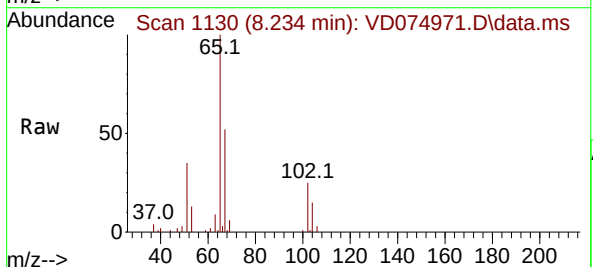

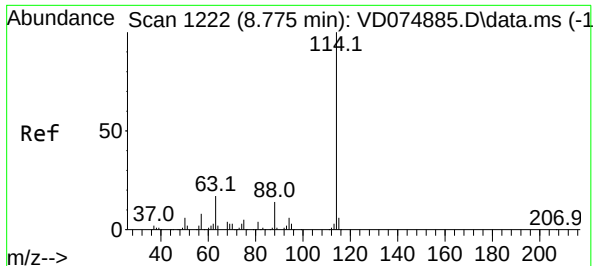

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD074971.D

Acq: 17 Nov 2022 15:56

Instrument :

MSVOA_D

ClientSampleId :

LEFT-SIDE-FLATS-31





Tgt Ion:114 Resp: 235005

Ion Ratio Lower Upper

114 100

63 15.7 0.0 33.2

88 13.1 0.0 28.2

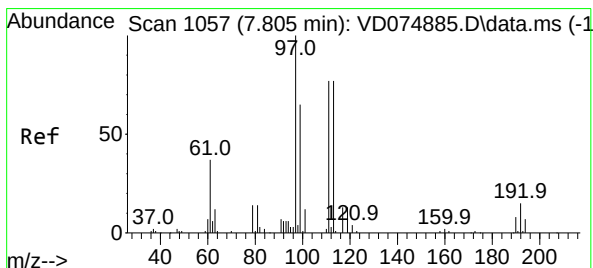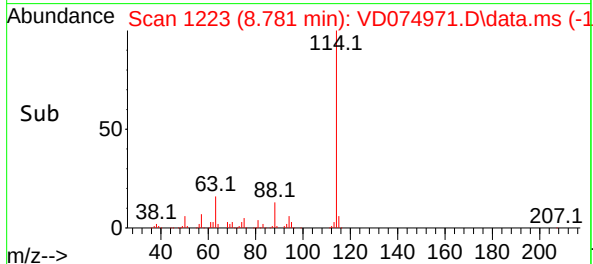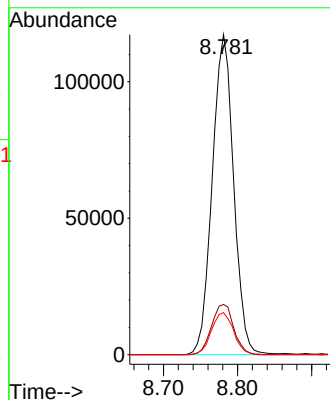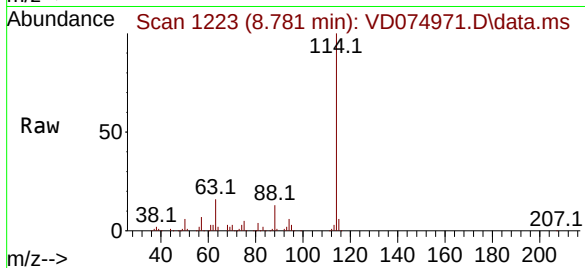

#35

Dibromofluoromethane

Concen: 55.743 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.005 min

Lab File: VD074971.D

Acq: 17 Nov 2022 15:56




Tgt Ion:113 Resp: 80751


Ion Ratio Lower Upper

113 100

111 102.8 82.3 123.5

192 18.6 16.4 24.6


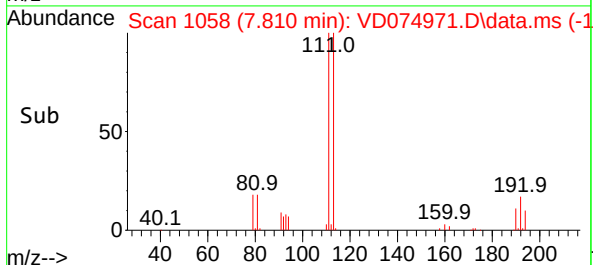
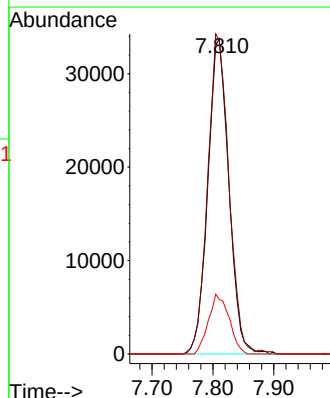
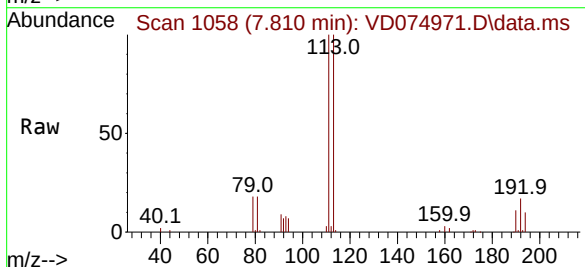


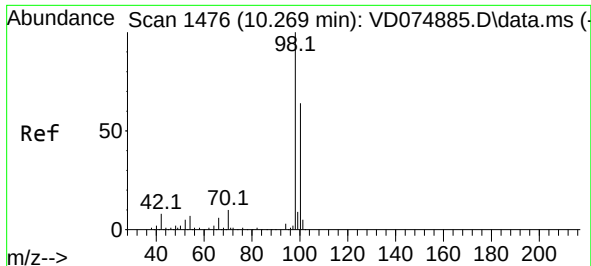

#50
Toluene-d8
Concen: 61.440 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD074971.D
Acq: 17 Nov 2022 15:56




Instrument :
MSVOA_D
ClientSampleId :
LEFT-SIDE-FLATS-31


Tgt Ion: 98 Resp: 293187
Ion Ratio Lower Upper
98 100
100 64.9 51.4 77.0

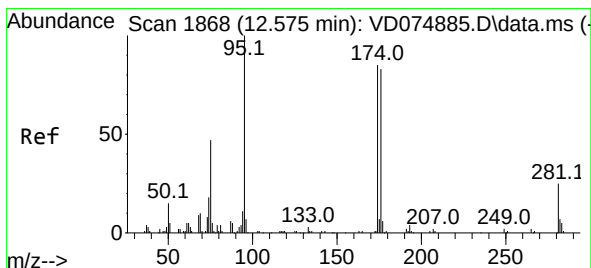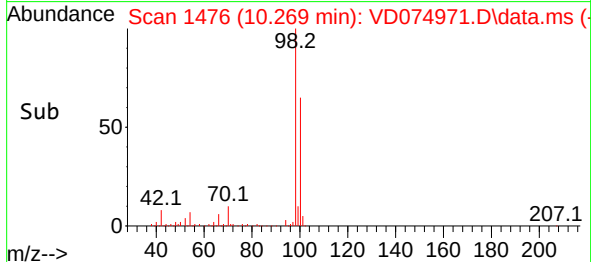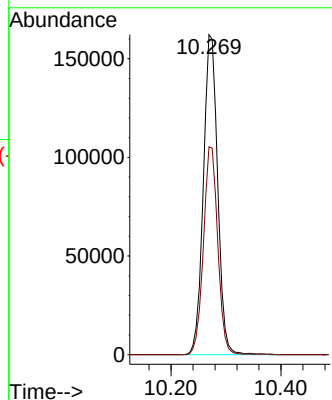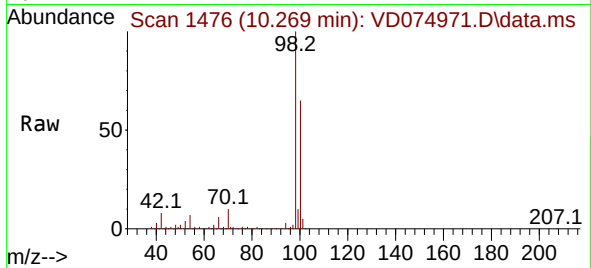

#62
4-Bromofluorobenzene
Concen: 56.909 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD074971.D
Acq: 17 Nov 2022 15:56

Tgt Ion: 95 Resp: 83388
Ion Ratio Lower Upper
95 100
174 94.1 0.0 197.0
176 91.3 0.0 182.6


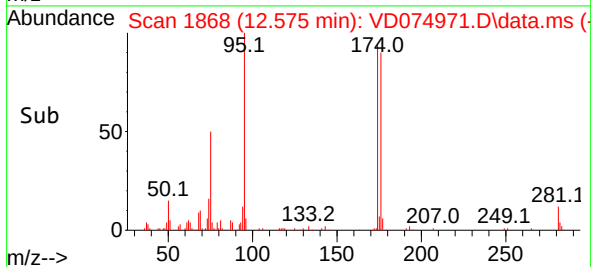
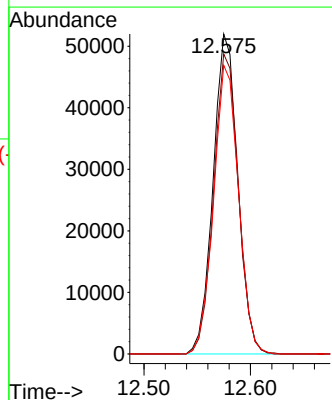
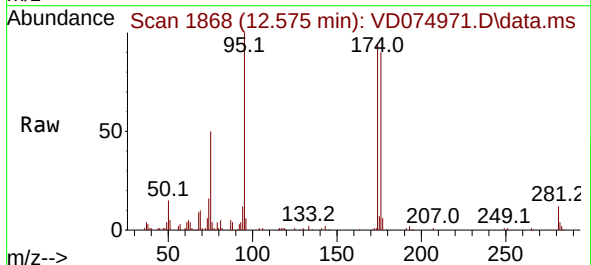


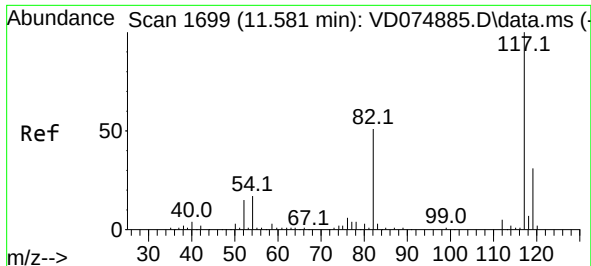

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD074971.D
Acq: 17 Nov 2022 15:56

Instrument :
MSVOA_D
ClientSampleId :
LEFT-SIDE-FLATS-31

Tgt Ion:117 Resp: 219458
Ion Ratio Lower Upper
117 100
82 47.5 41.6 62.4
119 31.1 25.2 37.8

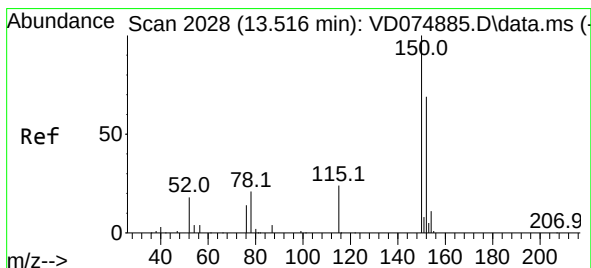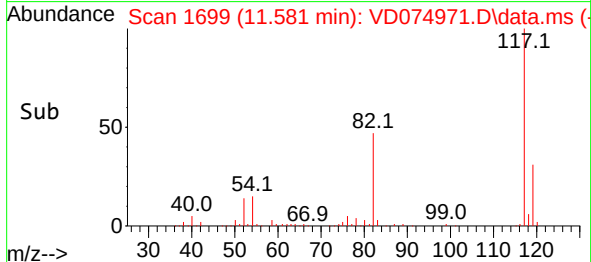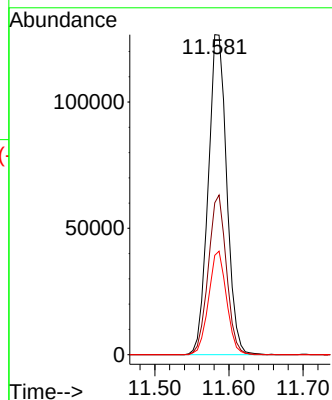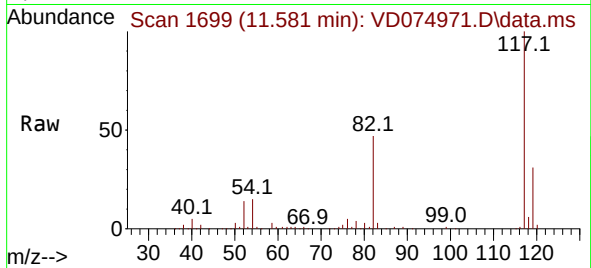

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. 0.006 min
Lab File: VD074971.D
Acq: 17 Nov 2022 15:56

Tgt Ion:152 Resp: 95513
Ion Ratio Lower Upper
152 100
115 54.7 26.8 80.4
150 156.9 0.0 348.2

