

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111722\
 Data File : VD074978.D
 Acq On : 17 Nov 2022 19:06
 Operator : VA/SY
 Sample : N5678-05
 Misc : 6.93G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 250FB-BP-BACKFILL-03

Quant Time: Nov 17 22:37:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111122S.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 14 00:51:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	133889	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	247241	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.587	117	225933	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	97070	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	66282	77.798	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	155.600%
35) Dibromofluoromethane	7.810	113	86977	57.069	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	114.140%
50) Toluene-d8	10.269	98	312985	62.343	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	124.680%
62) 4-Bromofluorobenzene	12.575	95	87327	56.648	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	113.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD111722\
Data File : VD074978.D
Acq On : 17 Nov 2022 19:06
Operator : VA/SY
Sample : N5678-05
Misc : 6.93G/5.00ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
250FB-BP-BACKFILL-03

Quant Time: Nov 17 22:37:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111122S.M
Quant Title : SW846 8260
QLast Update : Mon Nov 14 00:51:58 2022
Response via : Initial Calibration




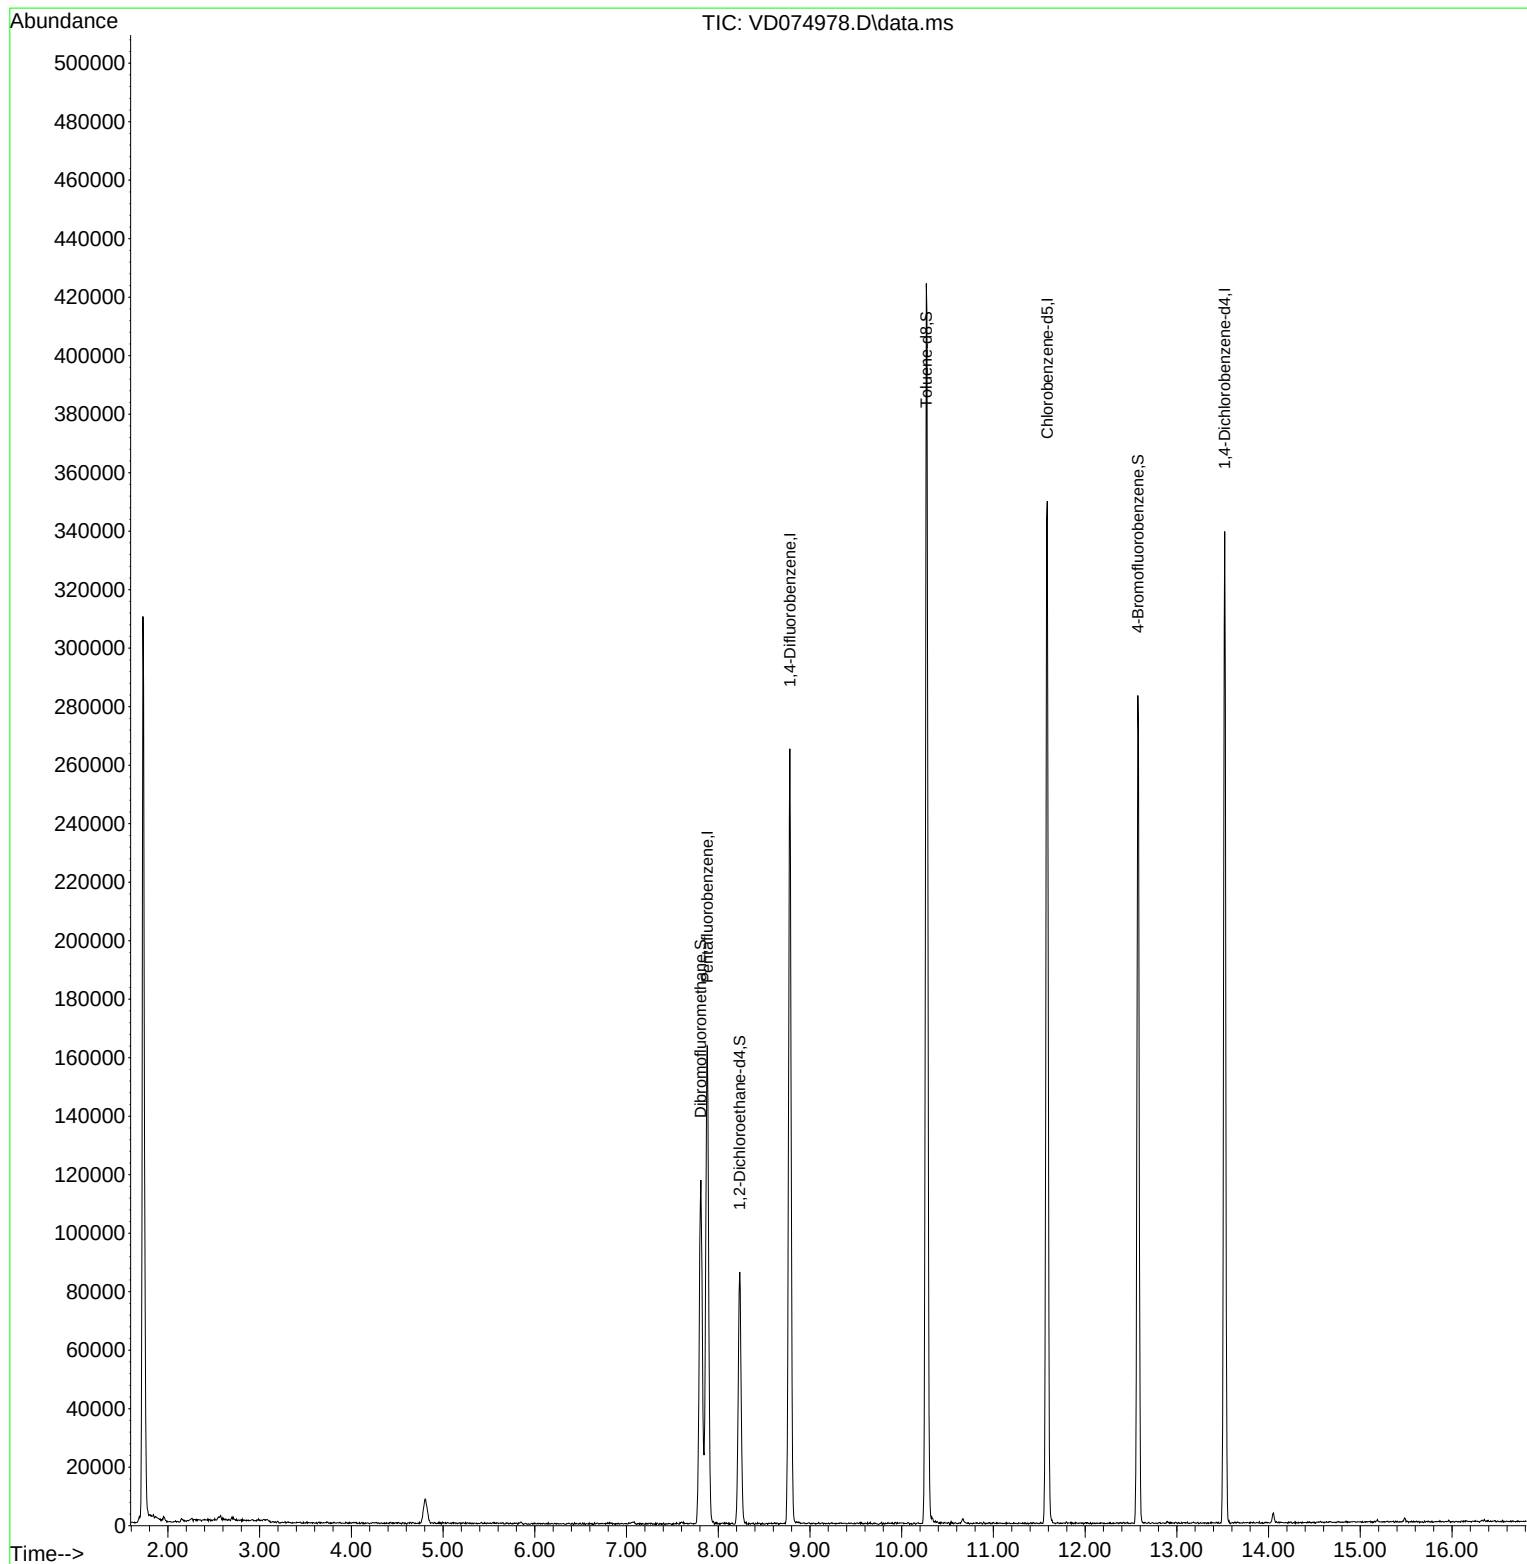


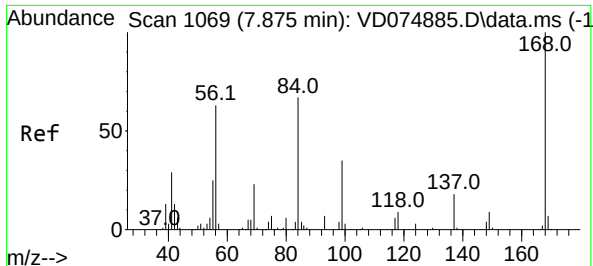

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD074978.D
Acq: 17 Nov 2022 19:06




Instrument :
MSVOA_D
ClientSampleId :
250FB-BP-BACKFILL-03


Tgt Ion:168 Resp: 133889
Ion Ratio Lower Upper
168 100
99 49.5 40.9 61.3

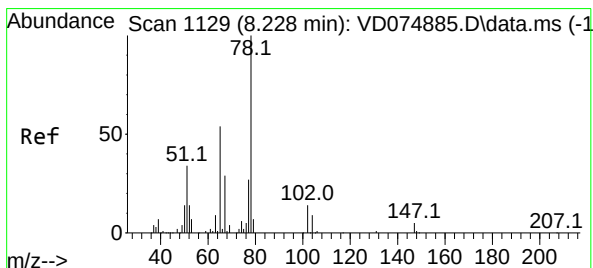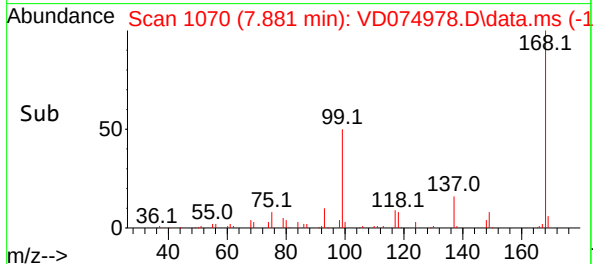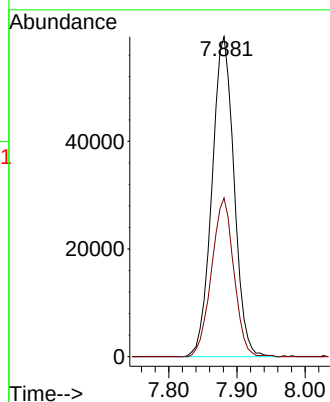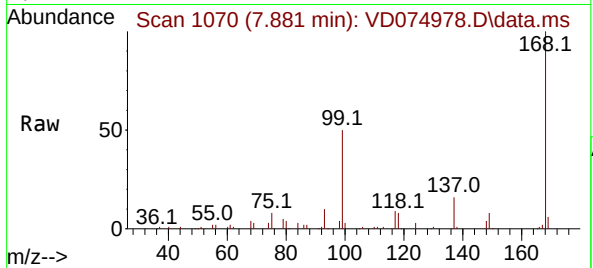

#33
1,2-Dichloroethane-d4
Concen: 77.798 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD074978.D
Acq: 17 Nov 2022 19:06

Tgt Ion: 65 Resp: 66282
Ion Ratio Lower Upper
65 100
67 54.2 0.0 110.2

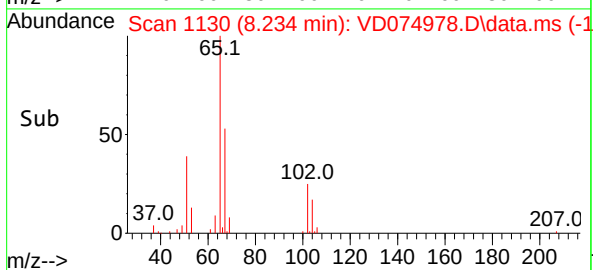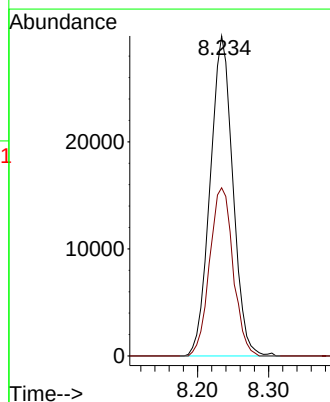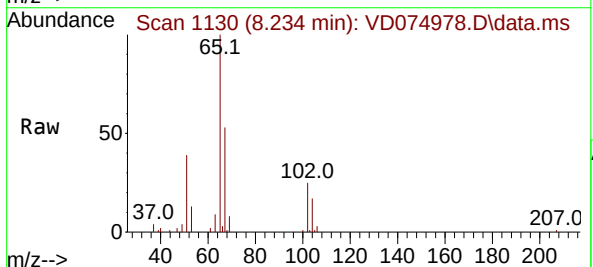

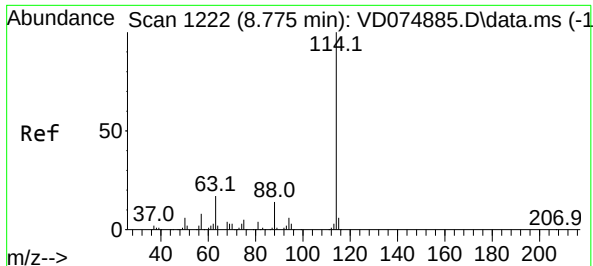

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD074978.D

Acq: 17 Nov 2022 19:06

Instrument :

MSVOA_D

ClientSampleId :

250FB-BP-BACKFILL-03





Tgt Ion:114 Resp: 247241

Ion Ratio Lower Upper

114 100

63 15.6 0.0 33.2

88 13.4 0.0 28.2

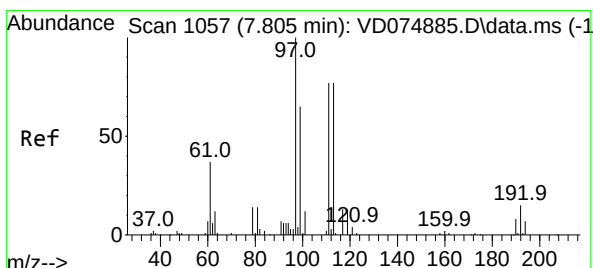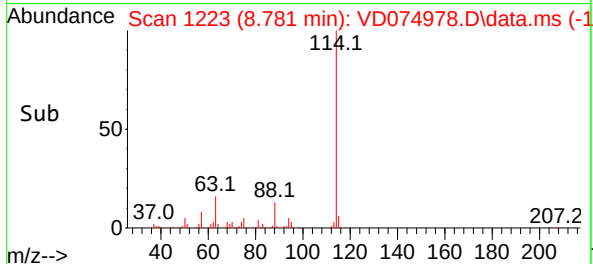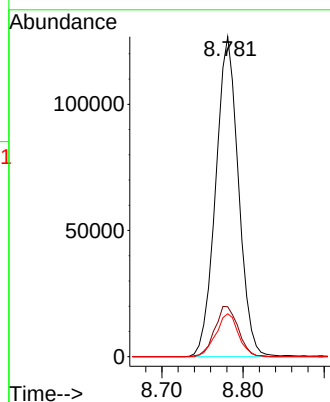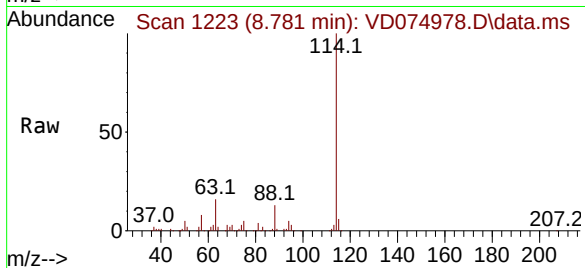

#35

Dibromofluoromethane

Concen: 57.069 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.005 min

Lab File: VD074978.D

Acq: 17 Nov 2022 19:06




Tgt Ion:113 Resp: 86977


Ion Ratio Lower Upper

113 100

111 102.5 82.3 123.5

192 18.8 16.4 24.6


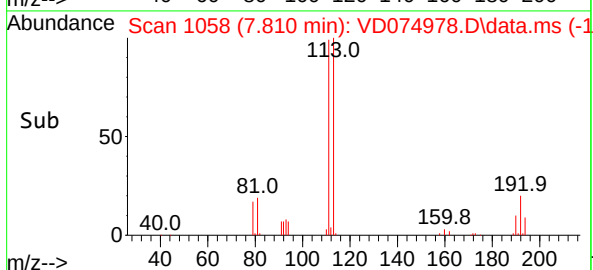
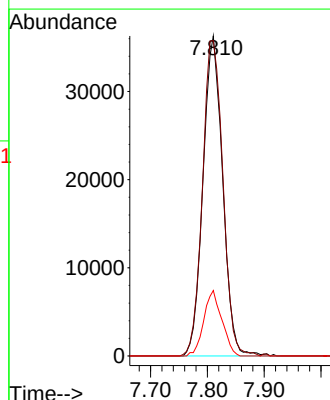
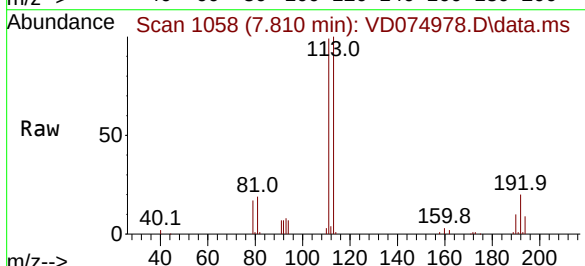


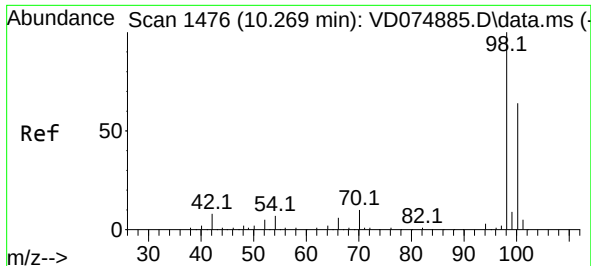

#50
Toluene-d8
Concen: 62.343 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD074978.D
Acq: 17 Nov 2022 19:06




Instrument :
MSVOA_D
ClientSampleId :
250FB-BP-BACKFILL-03


Tgt Ion: 98 Resp: 312985
Ion Ratio Lower Upper
98 100
100 64.1 51.4 77.0

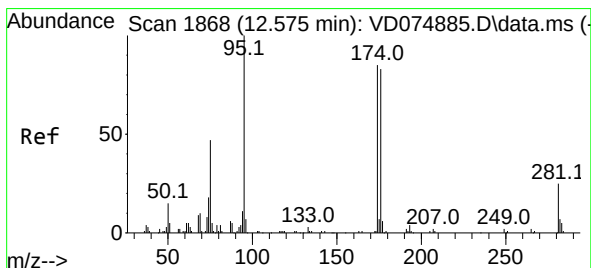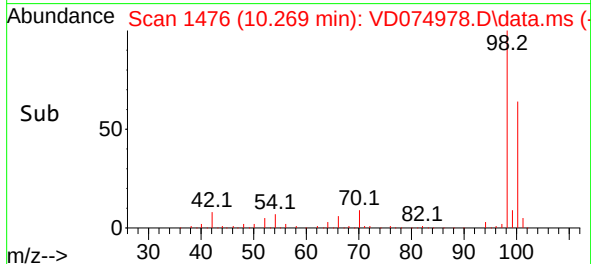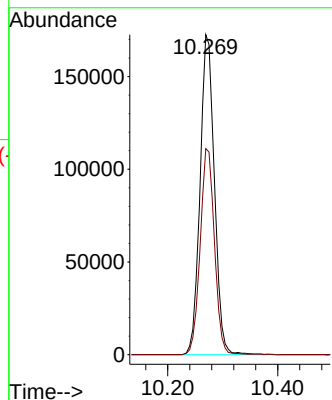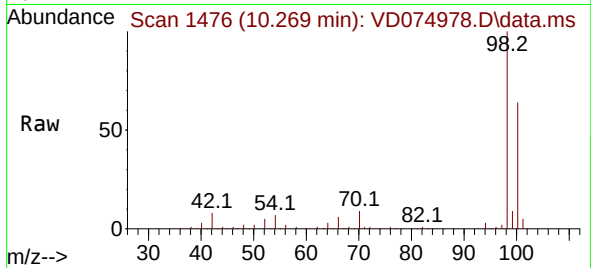

#62
4-Bromofluorobenzene
Concen: 56.648 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD074978.D
Acq: 17 Nov 2022 19:06

Tgt Ion: 95 Resp: 87327
Ion Ratio Lower Upper
95 100
174 95.4 0.0 197.0
176 90.6 0.0 182.6


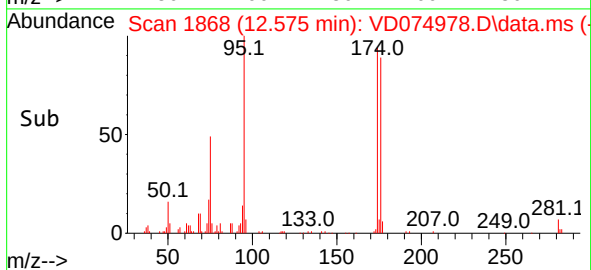
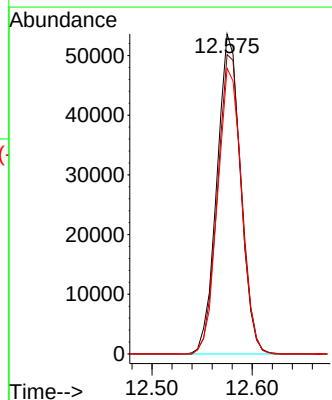
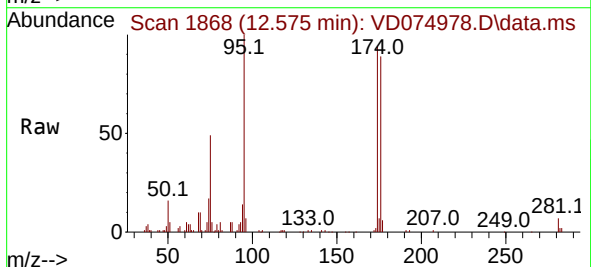


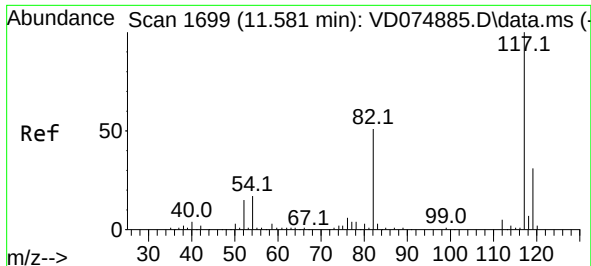

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.587 min Scan# 11
Delta R.T. 0.006 min
Lab File: VD074978.D
Acq: 17 Nov 2022 19:06

Instrument :
MSVOA_D
ClientSampleId :
250FB-BP-BACKFILL-03

Tgt Ion:117 Resp: 225933
Ion Ratio Lower Upper
117 100
82 50.1 41.6 62.4
119 32.5 25.2 37.8

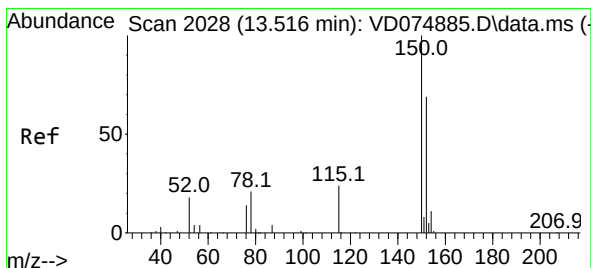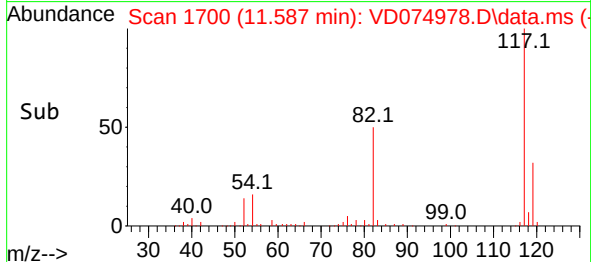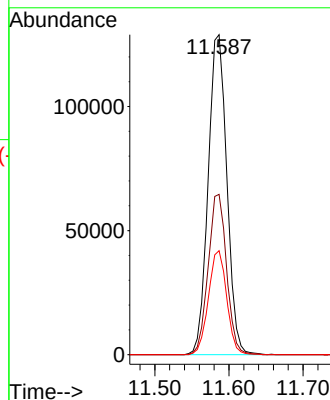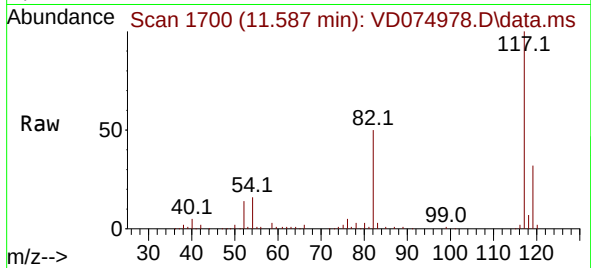

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. 0.006 min
Lab File: VD074978.D
Acq: 17 Nov 2022 19:06

Tgt Ion:152 Resp: 97070
Ion Ratio Lower Upper
152 100
115 55.6 26.8 80.4
150 157.7 0.0 348.2

