
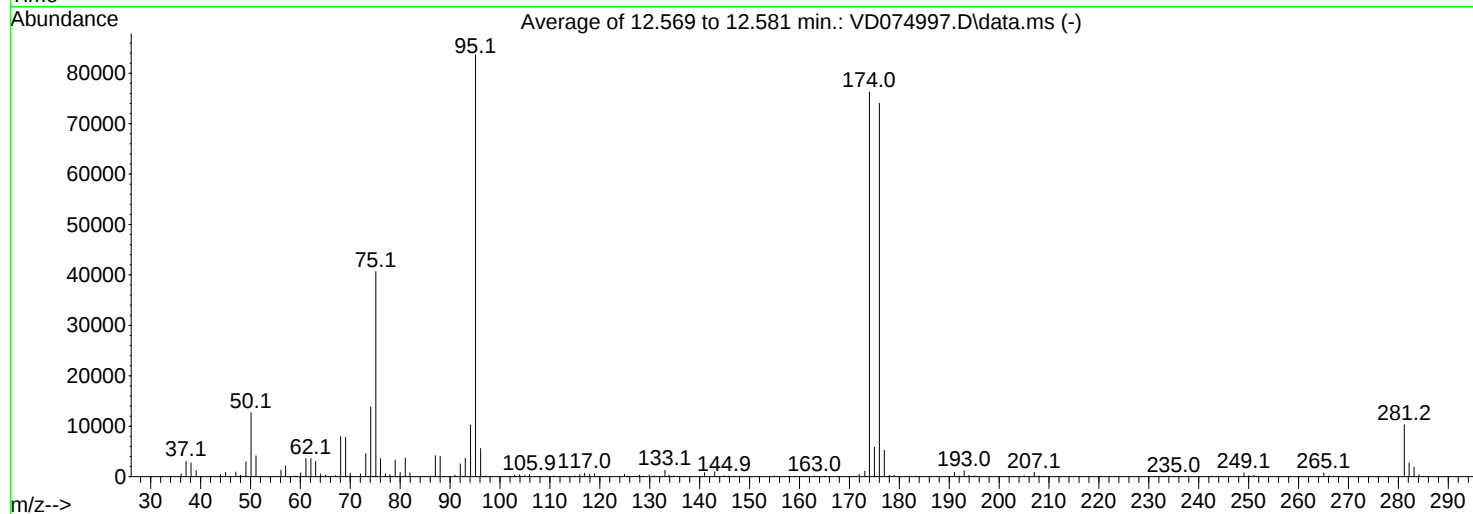


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD112122\
Data File : VD074997.D
Acq On : 21 Nov 2022 09:34
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D111122S.M
Title : SW846 8260
Last Update : Mon Nov 14 00:51:58 2022

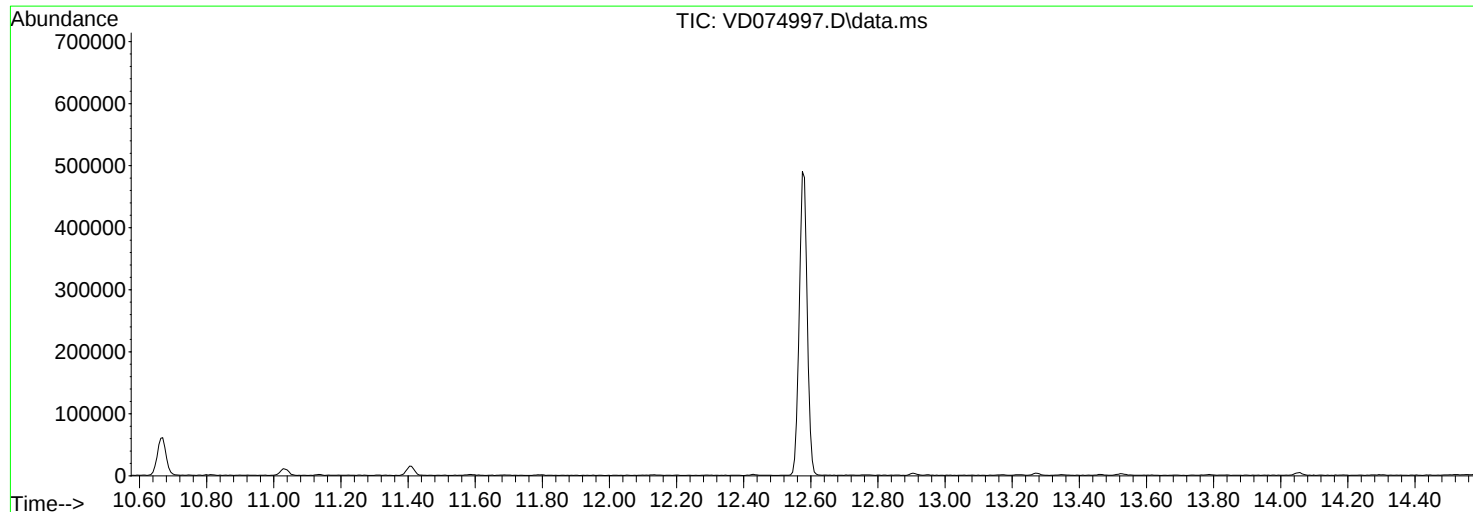

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.1	12663	PASS
75	95	30	60	48.6	40653	PASS
95	95	100	100	100.0	83643	PASS
96	95	5	9	6.7	5583	PASS
173	174	0.00	2	1.4	1072	PASS
174	95	50	100	91.2	76264	PASS
175	174	5	9	7.6	5811	PASS
176	174	95	101	97.1	74067	PASS
177	176	5	9	7.1	5231	PASS