

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122822\
 Data File : VD075067.D
 Acq On : 28 Dec 2022 15:51
 Operator : KP/SY
 Sample : N6219-04
 Misc : 4.63G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 72-12016

Quant Time: Dec 29 03:51:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D12222S.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 23 05:54:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	314	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.775	114	1240	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.587	117	1185	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	349	50.000	ug/l	# 0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	310	101.002	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 202.000%#	
35) Dibromofluoromethane	7.799	113	129	17.679	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 35.360%#	
50) Toluene-d8	10.275	98	1491	50.573	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 101.140%	
62) 4-Bromofluorobenzene	12.575	95	585	61.249	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 122.500%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122822\
Data File : VD075067.D
Acq On : 28 Dec 2022 15:51
Operator : KP/SY
Sample : N6219-04
Misc : 4.63G/5.00ml/MSVOA_D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
72-12016

Quant Time: Dec 29 03:51:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122222S.M
Quant Title : SW846 8260
QLast Update : Fri Dec 23 05:54:19 2022
Response via : Initial Calibration




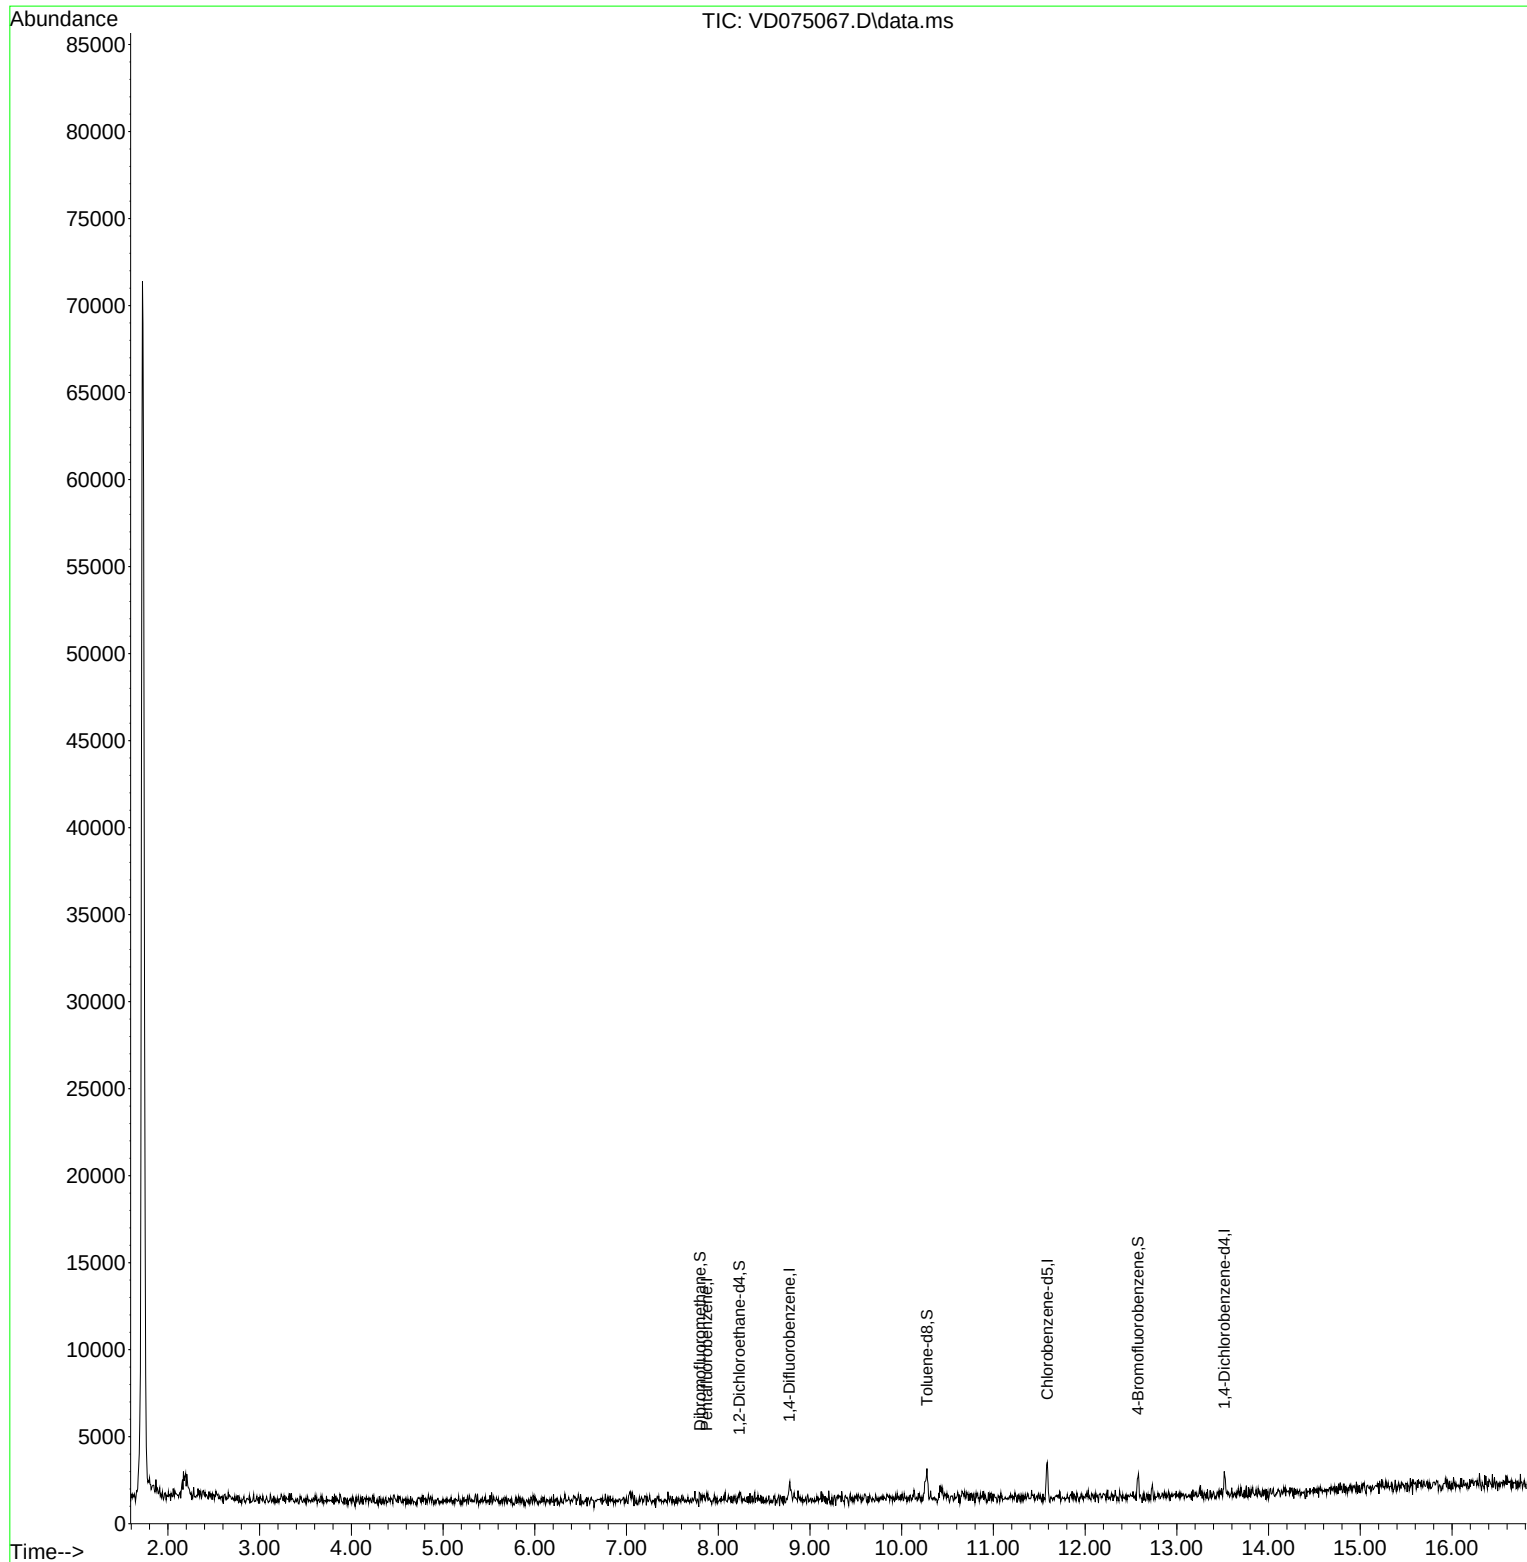


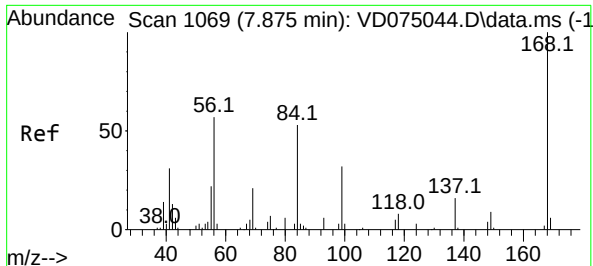

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD075067.D
Acq: 28 Dec 2022 15:51




Instrument :
MSVOA_D
ClientSampleId :
72-12016


Tgt Ion:168 Resp: 314
Ion Ratio Lower Upper
168 100
99 0.0 40.3 60.5#

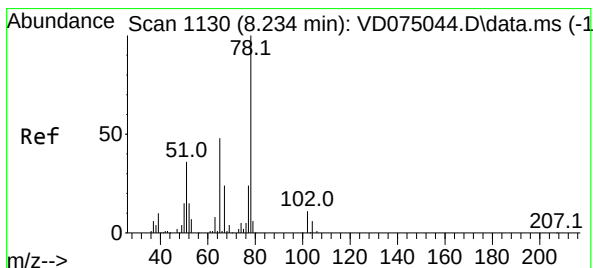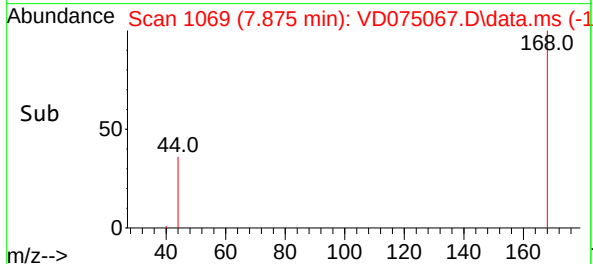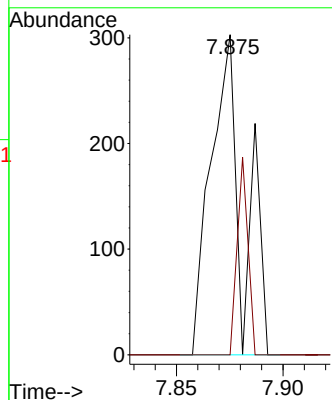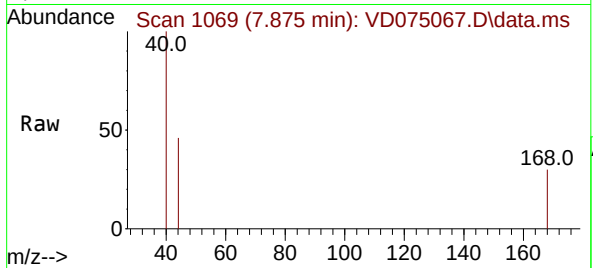

#33
1,2-Dichloroethane-d4
Concen: 101.002 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. 0.000 min
Lab File: VD075067.D
Acq: 28 Dec 2022 15:51

Tgt Ion: 65 Resp: 310
Ion Ratio Lower Upper
65 100
67 38.7 0.0 111.2

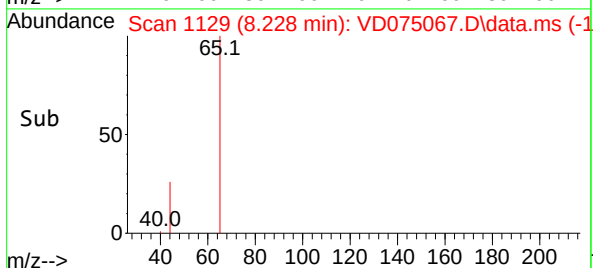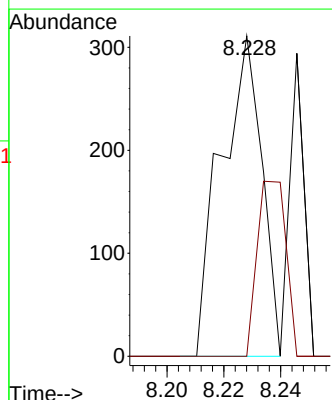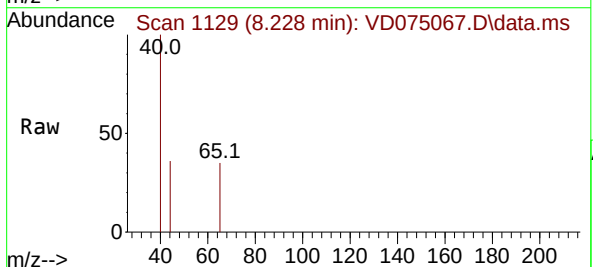

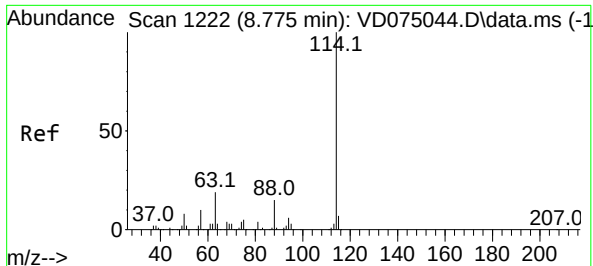

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 114

Delta R.T. 0.000 min

Lab File: VD075067.D

Acq: 28 Dec 2022 15:51





Instrument :

MSVOA_D

ClientSampleId :

72-12016

Tgt Ion:114	Resp:	1240
Ion Ratio	Lower	Upper
114	100	
63	0.0	33.8
88	23.6	27.8

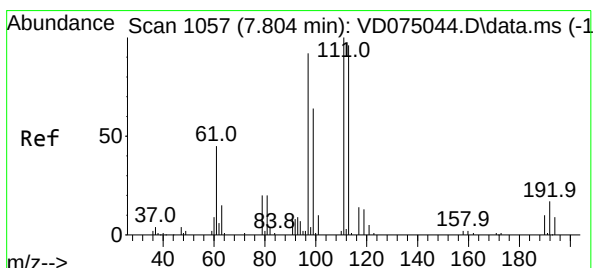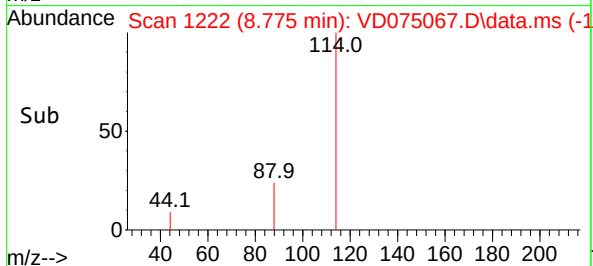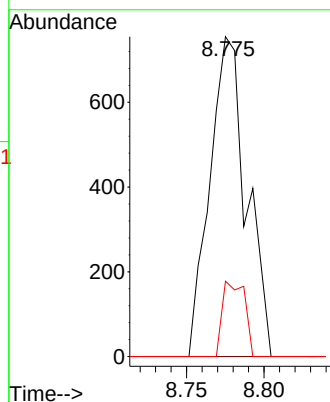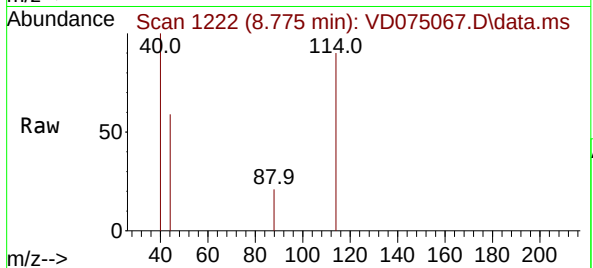

#35

Dibromofluoromethane

Concen: 17.679 ug/l




RT: 7.799 min Scan# 1056


Delta R.T. -0.006 min

Lab File: VD075067.D

Acq: 28 Dec 2022 15:51

Tgt Ion:113	Resp:	129
Ion Ratio	Lower	Upper
113	100	
111	107.8	123.1
192	0.0	22.7


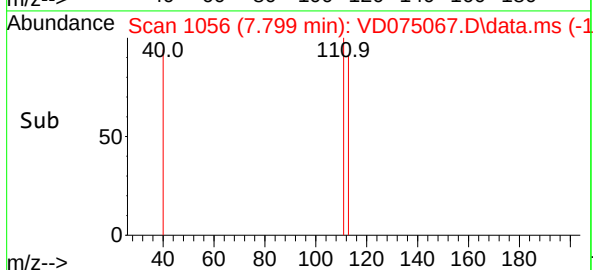
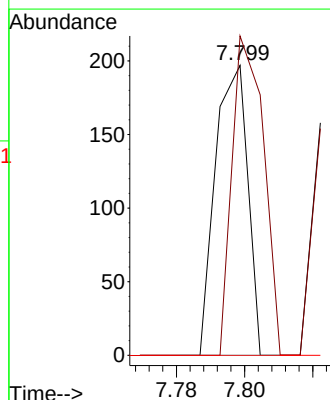
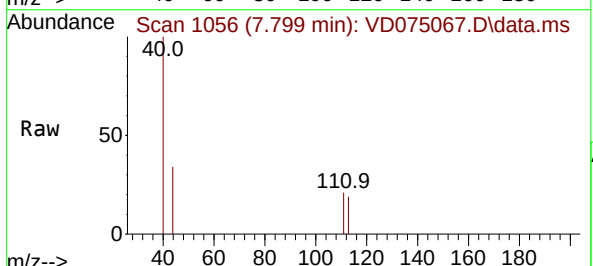


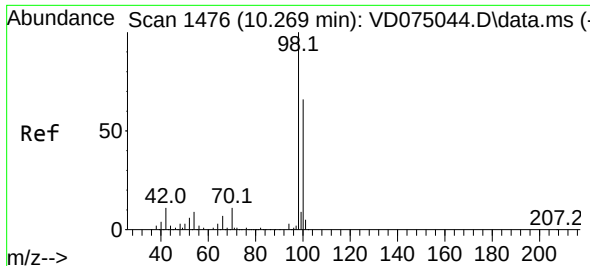

#50
Toluene-d8
Concen: 50.573 ug/l
RT: 10.275 min Scan# 1476
Delta R.T. 0.006 min
Lab File: VD075067.D
Acq: 28 Dec 2022 15:51




Instrument :
MSVOA_D
ClientSampleId :
72-12016


Tgt Ion: 98 Resp: 1491
Ion Ratio Lower Upper
98 100
100 65.2 52.2 78.2

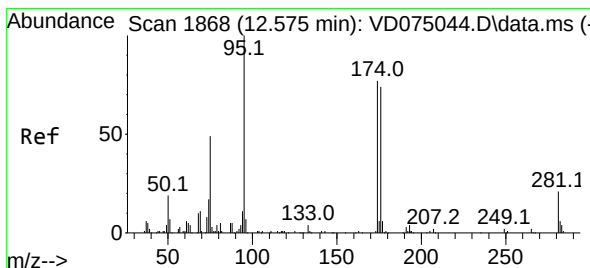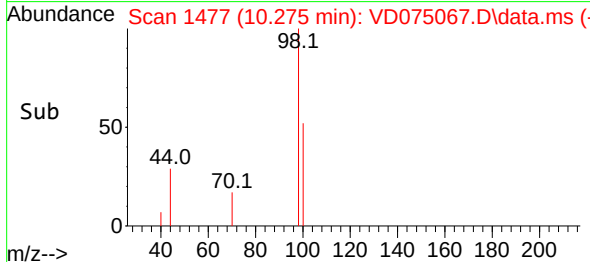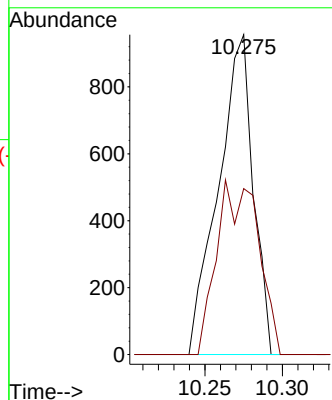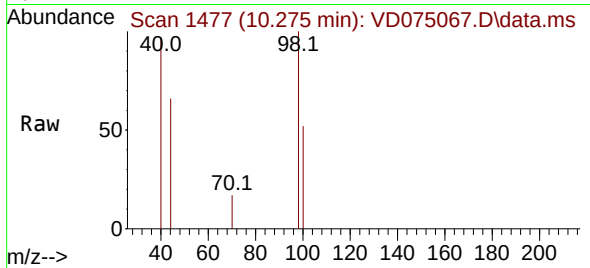

#62
4-Bromofluorobenzene
Concen: 61.249 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD075067.D
Acq: 28 Dec 2022 15:51

Tgt Ion: 95 Resp: 585
Ion Ratio Lower Upper
95 100
174 68.2 0.0 171.2
176 63.8 0.0 165.0


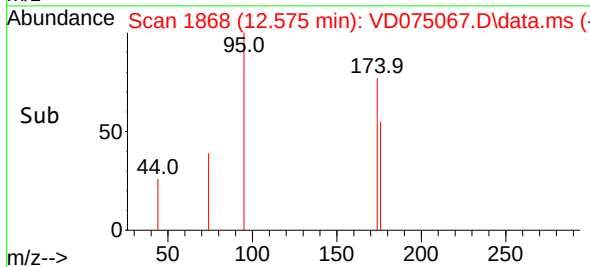
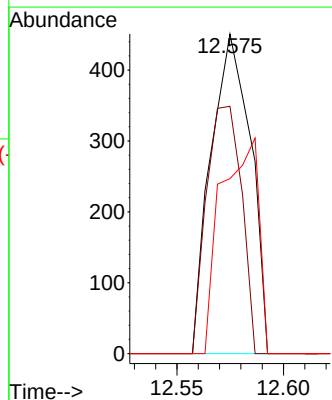
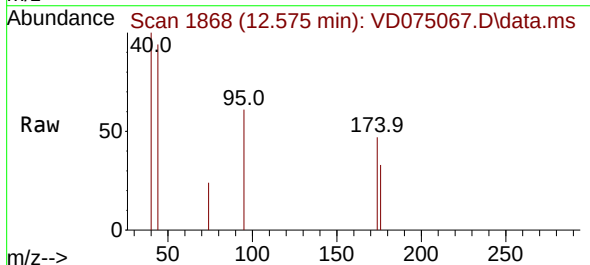


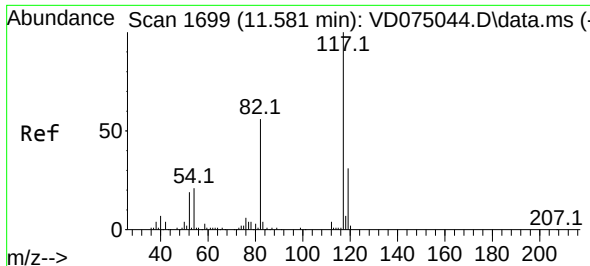

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.587 min Scan# 1185
Delta R.T. 0.006 min
Lab File: VD075067.D
Acq: 28 Dec 2022 15:51

Instrument :
MSVOA_D
ClientSampleId :
72-12016

Tgt Ion:	117	Resp:	1185
Ion Ratio	Lower	Upper	
117	100		
82	46.7	40.9	61.3
119	34.7	25.5	38.3

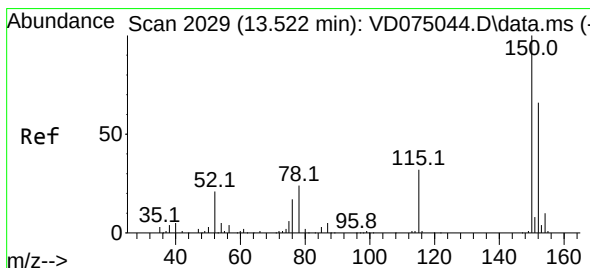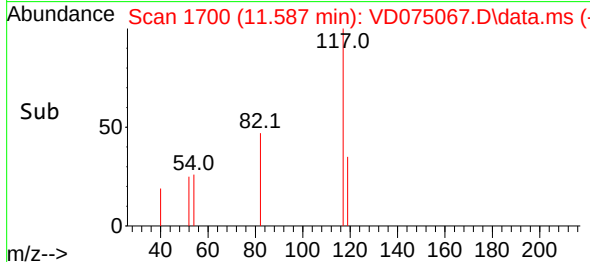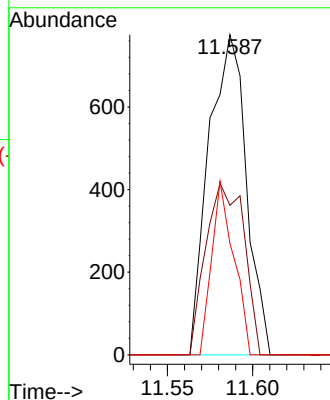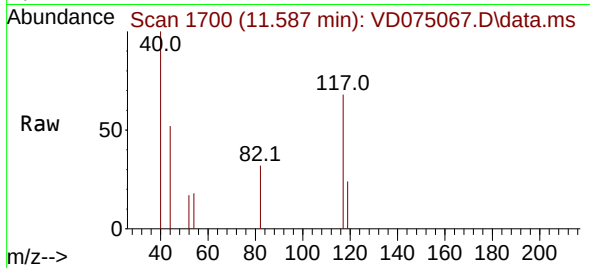

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. 0.000 min
Lab File: VD075067.D
Acq: 28 Dec 2022 15:51

Tgt Ion:	152	Resp:	349
Ion Ratio	Lower	Upper	
152	100		
115	92.0	28.8	86.5
150	172.5	0.0	354.2

