
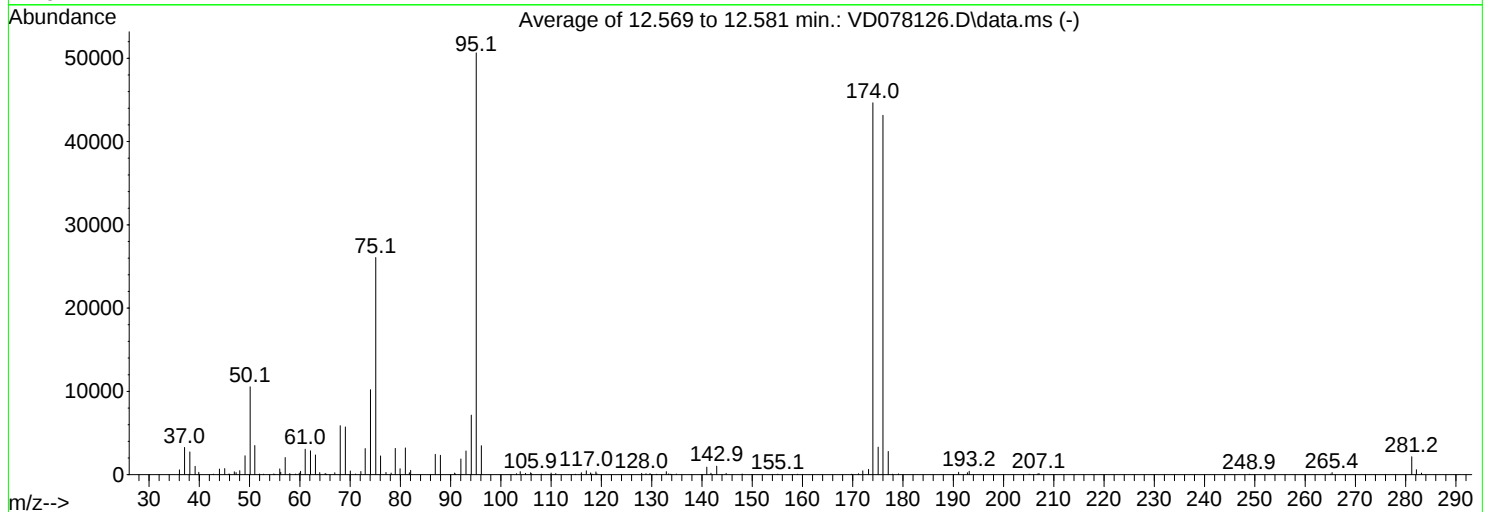


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010824\
Data File : VD078126.D
Acq On : 08 Jan 2024 11:53
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D010824S.M
Title : SW846 8260
Last Update : Tue Jan 09 01:29:14 2024

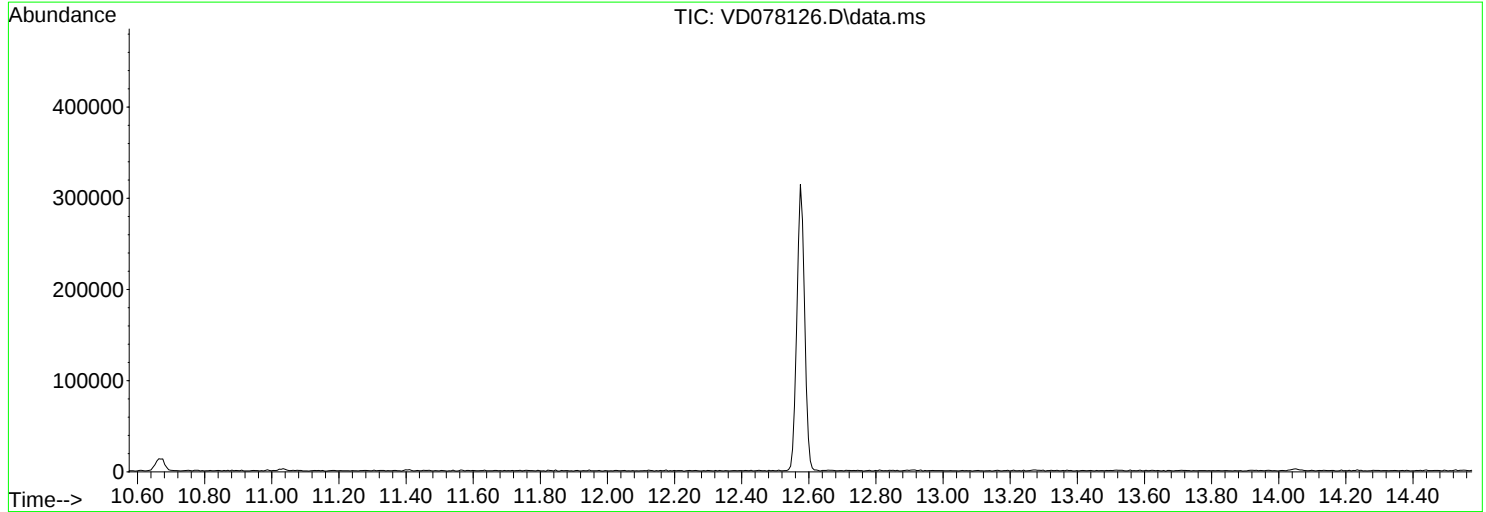

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.8	10545	PASS
75	95	30	60	51.5	26069	PASS
95	95	100	100	100.0	50656	PASS
96	95	5	9	6.9	3474	PASS
173	174	0.00	2	1.4	632	PASS
174	95	50	100	88.1	44651	PASS
175	174	5	9	7.4	3301	PASS
176	174	95	101	96.7	43163	PASS
177	176	5	9	6.4	2782	PASS