
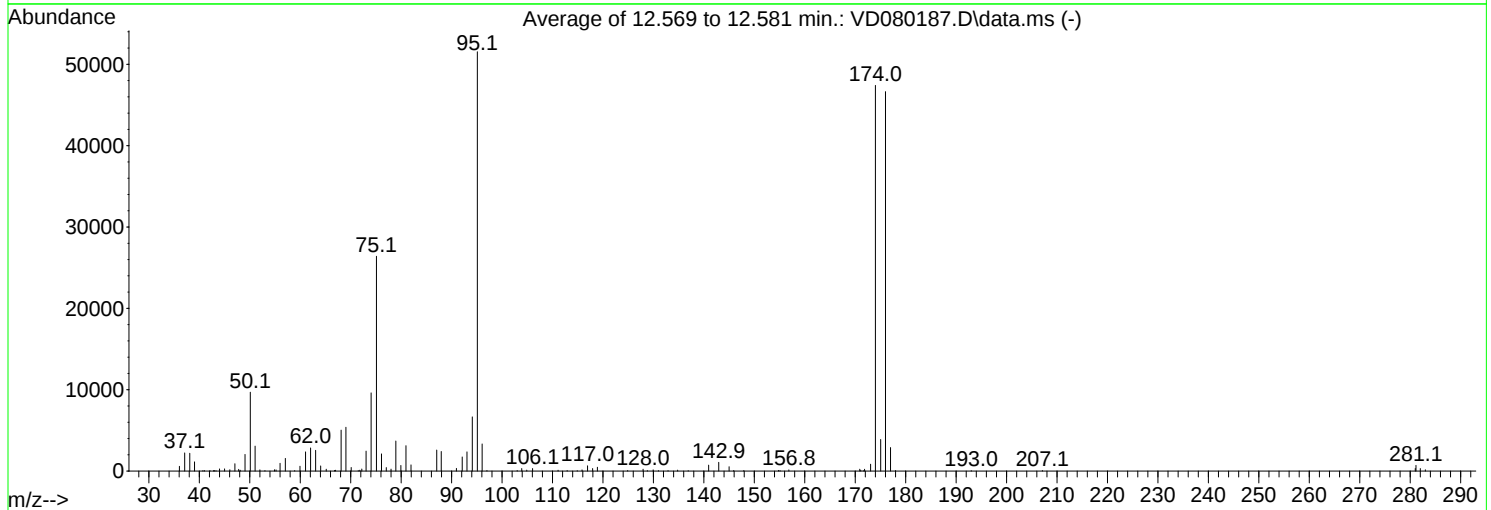


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010925\
Data File : VD080187.D
Acq On : 09 Jan 2025 10:03
Operator : RP/MD
Sample : BFB844
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB844

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM010925SMA.M
Title : SFAM01.0
Last Update : Thu Jan 09 20:13:33 2025

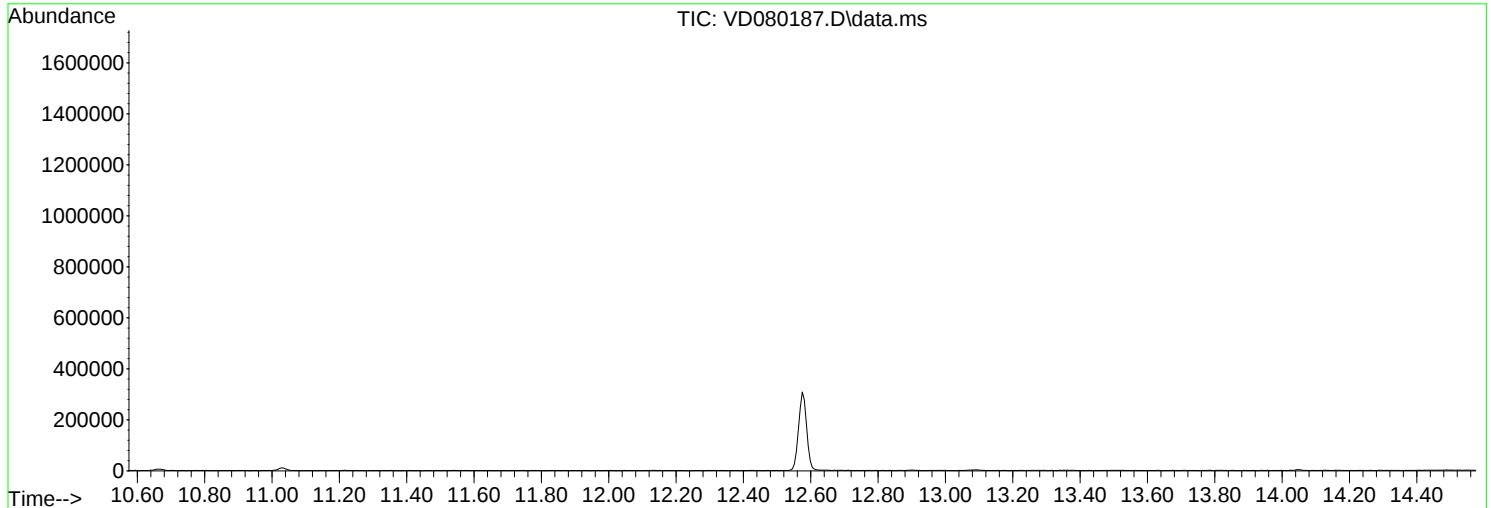

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	9693	PASS
75	95	30	80	51.2	26403	PASS
95	95	100	100	100.0	51547	PASS
96	95	5	9	6.5	3332	PASS
173	174	0.00	2	1.8	847	PASS
174	95	50	120	92.0	47413	PASS
175	174	5	9	8.2	3885	PASS
176	174	95	105	98.4	46645	PASS
177	176	5	10	6.2	2892	PASS

Scan 1860 (12.528 min): VD080187.D\data.ms
BFB844

m/z	Abundance
40.00	933.0
43.90	244.0
44.90	213.0
69.20	159.0

Instrument :
MSVOA_D
ClientSampleId :
BFB844

m/z	Abundance
36.10	658.0
37.10	1965.0
38.10	1907.0
39.00	847.0
40.20	740.0
41.00	193.0
43.30	153.0
44.00	320.0
45.00	462.0
46.10	263.0
47.00	734.0
47.80	301.0
49.10	1845.0
50.10	9002.0
51.10	3002.0
52.10	223.0
53.00	178.0
55.00	273.0
56.00	886.0
57.00	1488.0
59.90	630.0
61.00	2378.0
62.10	2284.0
63.00	2399.0
64.00	455.0
65.10	192.0
66.80	238.0
68.10	4466.0
69.00	5269.0
70.10	368.0
72.20	365.0
73.00	1864.0
74.00	8358.0
75.10	23776.0
76.10	1940.0
77.10	451.0
79.00	3128.0
79.90	669.0
80.90	3146.0
82.00	634.0
87.10	2249.0
88.00	2270.0
90.90	428.0
92.10	1481.0
93.10	2225.0
94.10	5612.0
95.10	46624.0
96.10	3218.0
104.00	361.0
106.10	268.0
111.10	157.0
115.90	189.0
117.00	604.0
117.90	265.0
119.00	463.0
128.00	175.0
128.80	189.0
131.00	167.0
141.00	616.0
143.00	889.0
145.10	578.0
156.80	204.0
171.00	268.0
171.60	158.0
173.00	1103.0
174.00	41648.0
175.00	3623.0
176.00	40720.0
177.00	2804.0
281.00	952.0
282.00	238.0

Instrument :
MSVOA_D
ClientSampleId :
BFB844

m/z	Abundance
36.00	628.0
37.10	2617.0
38.10	2595.0
39.10	1286.0
40.00	723.0
40.70	163.0
42.10	158.0
42.80	189.0
44.00	587.0
45.00	469.0
47.10	1090.0
47.80	337.0
49.00	2088.0
50.10	10712.0
51.00	3575.0
54.80	231.0
55.30	174.0
55.90	871.0
57.10	1533.0
58.90	175.0
60.00	610.0
61.10	2218.0
62.00	3343.0
63.10	2416.0
64.10	593.0
65.20	159.0
67.00	314.0
68.10	5669.0
69.10	5901.0
70.00	576.0
71.50	170.0
72.20	398.0
73.10	2712.0
74.10	10540.0
75.10	30040.0
76.10	2730.0
77.00	466.0
78.10	329.0
79.00	4357.0
80.00	653.0
81.00	3022.0
82.00	839.0
87.00	2397.0
87.90	2589.0
91.00	270.0
92.10	1858.0
93.00	2526.0
94.10	8689.0
95.10	57272.0
96.00	3685.0
97.00	213.0
103.00	220.0
103.80	364.0
104.90	351.0
106.00	315.0
111.10	163.0
112.90	210.0
115.80	255.0
116.90	850.0
118.00	318.0
118.80	420.0
124.90	213.0
127.90	237.0
129.90	285.0
134.80	358.0
140.90	871.0
143.00	1076.0
145.00	632.0
145.90	187.0
147.90	166.0
155.10	188.0
170.80	415.0
171.80	299.0
174.00	52480.0
175.00	4426.0
176.00	51856.0
177.00	3088.0
193.00	159.0
281.20	786.0
282.00	358.0
283.00	280.0

Instrument :
MSVOA_D
ClientSampleId :
BFB844

m/z	Abundance
36.00	476.0
37.10	2104.0
38.10	2066.0
39.10	1262.0
40.10	816.0
43.00	178.0
44.10	633.0
45.10	530.0
46.00	233.0
47.10	892.0
48.10	328.0
49.10	2217.0
50.10	9365.0
51.10	2636.0
51.90	239.0
55.10	280.0
56.10	1106.0
57.10	1655.0
60.00	549.0
61.10	2494.0
62.10	2913.0
63.10	2831.0
64.00	852.0
65.10	344.0
68.10	4977.0
69.10	5472.0
70.20	392.0
71.80	315.0
73.00	2785.0
74.10	9940.0
75.10	25392.0
76.10	1675.0
77.00	373.0
77.90	407.0
78.90	3593.0
80.00	756.0
80.90	3207.0
81.90	815.0
87.00	3106.0
88.00	2364.0
90.90	288.0
92.10	1870.0
93.00	2330.0
94.10	5686.0
95.10	50744.0
96.10	3093.0
103.80	216.0
106.00	361.0
114.90	160.0
117.00	506.0
118.00	362.0
118.90	529.0
127.90	275.0
130.00	178.0
132.90	179.0
136.90	162.0
140.90	710.0
142.90	1254.0
144.90	406.0
154.80	256.0
156.90	233.0
171.10	314.0
171.90	366.0
173.10	1438.0
174.00	48112.0
175.10	3607.0
176.00	47360.0
177.00	2785.0
178.00	161.0
207.10	193.0
281.10	1324.0
282.00	337.0
283.00	197.0

Instrument :
MSVOA_D
ClientSampleId :
BFB844