
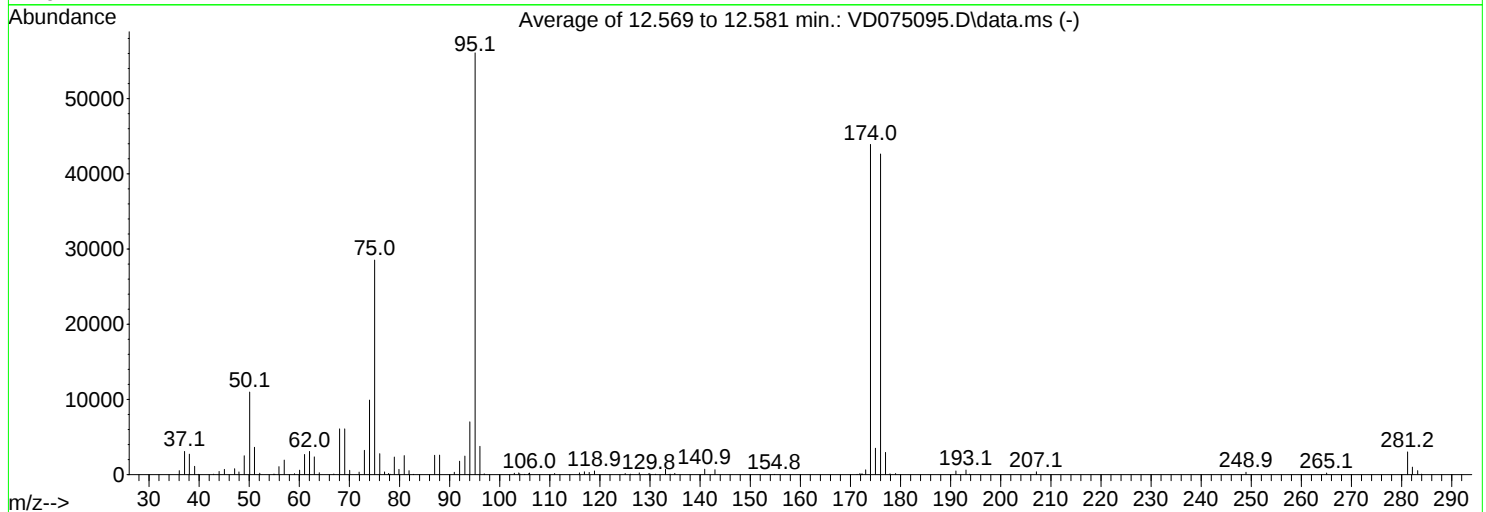


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011023\
Data File : VD075095.D
Acq On : 10 Jan 2023 09:09
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D010923S.M
Title : SW846 8260
Last Update : Tue Jan 10 03:36:33 2023

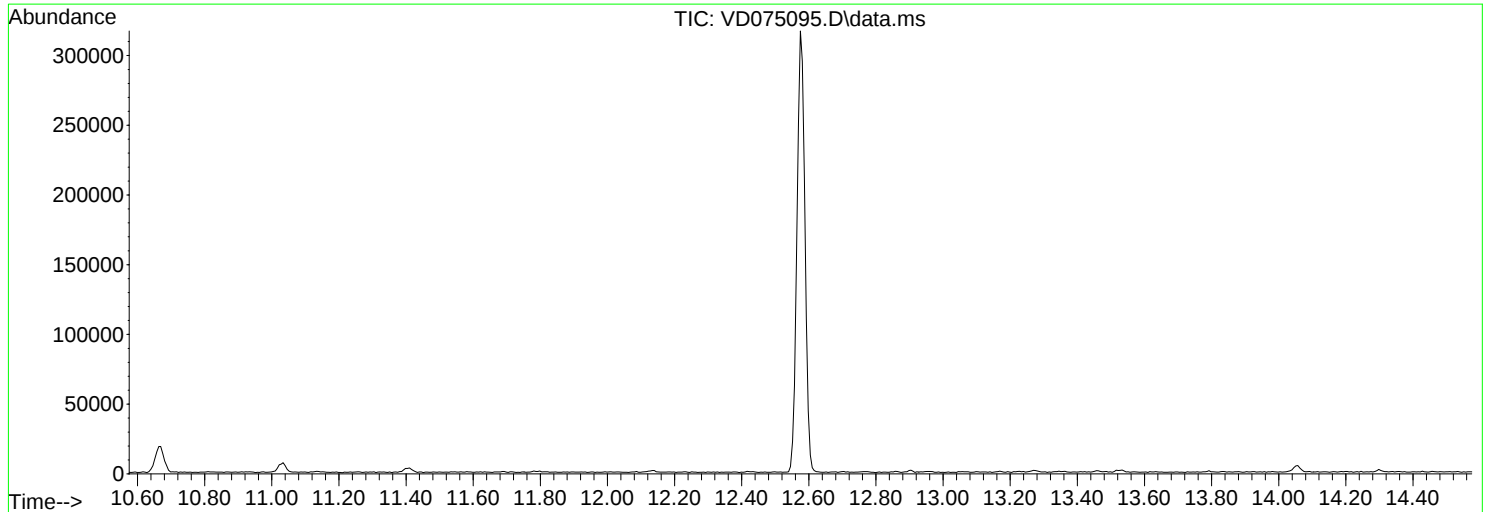

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	10987	PASS
75	95	30	60	50.9	28533	PASS
95	95	100	100	100.0	56091	PASS
96	95	5	9	6.7	3771	PASS
173	174	0.00	2	1.5	640	PASS
174	95	50	100	78.3	43912	PASS
175	174	5	9	8.0	3520	PASS
176	174	95	101	97.1	42632	PASS
177	176	5	9	6.9	2959	PASS