

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011025\
 Data File : VD080209.D
 Acq On : 10 Jan 2025 14:03
 Operator : RP/MD
 Sample : MDL05
 Misc : 5.00G/10ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Jan 13 00:14:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM010925SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 13 00:09:32 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	204316	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	197611	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	87143	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	124236	20.733	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.920%
7) Chloroethane-d5	2.805	69	103604	21.275	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.120%
11) 1,1-Dichloroethene-d2	3.916	65	27052	18.708	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.840%
21) 2-Butanone-d5	6.987	46	25950	37.435	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.880%
24) Chloroform-d	7.569	84	117519	18.329	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.320%
26) 1,2-Dichloroethane-d4	8.234	65	67798	20.188	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	80.760%
32) Benzene-d6	8.204	84	234507	18.382	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.520%
36) 1,2-Dichloropropane-d6	9.210	67	79589	18.849	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	75.400%
41) Toluene-d8	10.269	98	209317	18.003	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.000%
43) trans-1,3-Dichloroprop...	10.528	79	30421	17.634	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.520%
47) 2-Hexanone-d5	10.875	63	19247	36.576	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.160%
56) 1,1,2,2-Tetrachloroeth...	12.651	84	61057	19.297	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	77.200%
66) 1,2-Dichlorobenzene-d4	13.816	152	66043	20.161	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.640%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.934	85	4870	1.201	ug/L	98
3) Chloromethane	2.152	50	6976	1.262	ug/L	88
5) Vinyl chloride	2.281	62	8304	1.224	ug/L	94
6) Bromomethane	2.699	94	4332	1.097	ug/L	79
8) Chloroethane	2.840	64	5056	1.215	ug/L	94
9) Trichlorofluoromethane	3.175	101	6240	1.107	ug/L	96
10) 1,1,2-Trichloro-1,2,2-...	3.975	101	957	0.298	ug/L #	31
12) 1,1-Dichloroethene	3.940	96	3473	1.210	ug/L #	1
13) Acetone	4.028	43	1555	2.836	ug/L	97
14) Carbon disulfide	4.275	76	11076	1.035	ug/L #	88
15) Methyl Acetate	4.587	43	680	0.496	ug/L	95
17) trans-1,2-Dichloroethene	5.310	96	591	0.189	ug/L	97
18) Methyl tert-butyl Ether	5.328	73	4879	0.820	ug/L #	70
19) 1,1-Dichloroethane	6.105	63	6568	1.090	ug/L #	93
20) cis-1,2-Dichloroethene	7.087	96	3074	0.936	ug/L	92
22) 2-Butanone	7.093	43	1113	1.425	ug/L	80
23) Bromochloromethane	7.422	128	1229	0.774	ug/L #	69
25) Chloroform	7.593	83	19785	2.961	ug/L	88
27) 1,2-Dichloroethane	8.334	62	4003	1.027	ug/L #	91

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011025\
 Data File : VD080209.D
 Acq On : 10 Jan 2025 14:03
 Operator : RP/MD
 Sample : MDL05
 Misc : 5.00G/10ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Jan 13 00:14:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM010925SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 13 00:09:32 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


29) Cyclohexane	7.881	56	4202	0.845	ug/L #	89
30) 1,1,1-Trichloroethane	7.793	97	3692	0.705	ug/L #	48
31) Carbon tetrachloride	7.993	117	4785	1.036	ug/L	99
33) Benzene	8.251	78	13614	1.013	ug/L	100
34) Trichloroethene	9.028	95	3924	1.128	ug/L	88
35) Methylcyclohexane	9.269	83	4951	0.957	ug/L	92
38) Bromodichloromethane	9.593	83	4958	1.080	ug/L	79
39) cis-1,3-Dichloropropene	10.016	75	5251	1.015	ug/L	97
40) 4-Methyl-2-pentanone	10.157	43	3804	2.117	ug/L #	92
42) Toluene	10.334	91	14312	1.019	ug/L	93
44) trans-1,3-Dichloropropene	10.557	75	5932	1.328	ug/L	97
45) 1,1,2-Trichloroethane	10.734	97	2733	1.022	ug/L #	79
46) Tetrachloroethene	10.810	164	2905	1.036	ug/L	91
48) 2-Hexanone	10.922	43	2429	1.982	ug/L #	81
49) Dibromochloromethane	11.075	129	3170	1.065	ug/L #	73
50) 1,2-Dibromoethane	11.181	107	2585	1.064	ug/L #	84
51) Chlorobenzene	11.604	112	9252	1.028	ug/L	96
52) Ethylbenzene	11.687	91	13614	0.904	ug/L	96
53) m,p-Xylene	11.798	106	4690	0.833	ug/L	86
54) o-Xylene	12.128	106	4092	0.777	ug/L	68
55) Styrene	12.134	104	7391	0.775	ug/L	99
57) 1,1,2,2-Tetrachloroethane	12.669	83	3138	1.036	ug/L #	86
59) Bromoform	12.298	173	1772	1.133	ug/L #	92
60) Isopropylbenzene	12.422	105	10978	0.903	ug/L	95
61) 1,2,3-Trichloropropane	12.728	75	2084	1.131	ug/L	93
62) 1,3,5-Trimethylbenzene	12.898	105	8737	0.902	ug/L	100
63) 1,2,4-Trimethylbenzene	13.210	105	8517	0.901	ug/L	98
64) 1,3-Dichlorobenzene	13.457	146	5830	0.981	ug/L	97
65) 1,4-Dichlorobenzene	13.539	146	6111	0.996	ug/L #	75
67) 1,2-Dichlorobenzene	13.828	146	6026	1.132	ug/L	93
69) 1,3,5-Trichlorobenzene	14.592	180	4354	1.077	ug/L #	40
70) 1,2,4-trichlorobenzene	15.098	180	3249	0.985	ug/L #	85
71) Naphthalene	15.328	128	5782	0.996	ug/L	97
72) 1,2,3-Trichlorobenzene	15.522	180	3299	1.077	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011025\
Data File : VD080209.D
Acq On : 10 Jan 2025 14:03
Operator : RP/MD
Sample : MDL05
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :

Quant Time: Jan 13 00:14:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM010925SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 13 00:09:32 2025
Response via : Initial Calibration




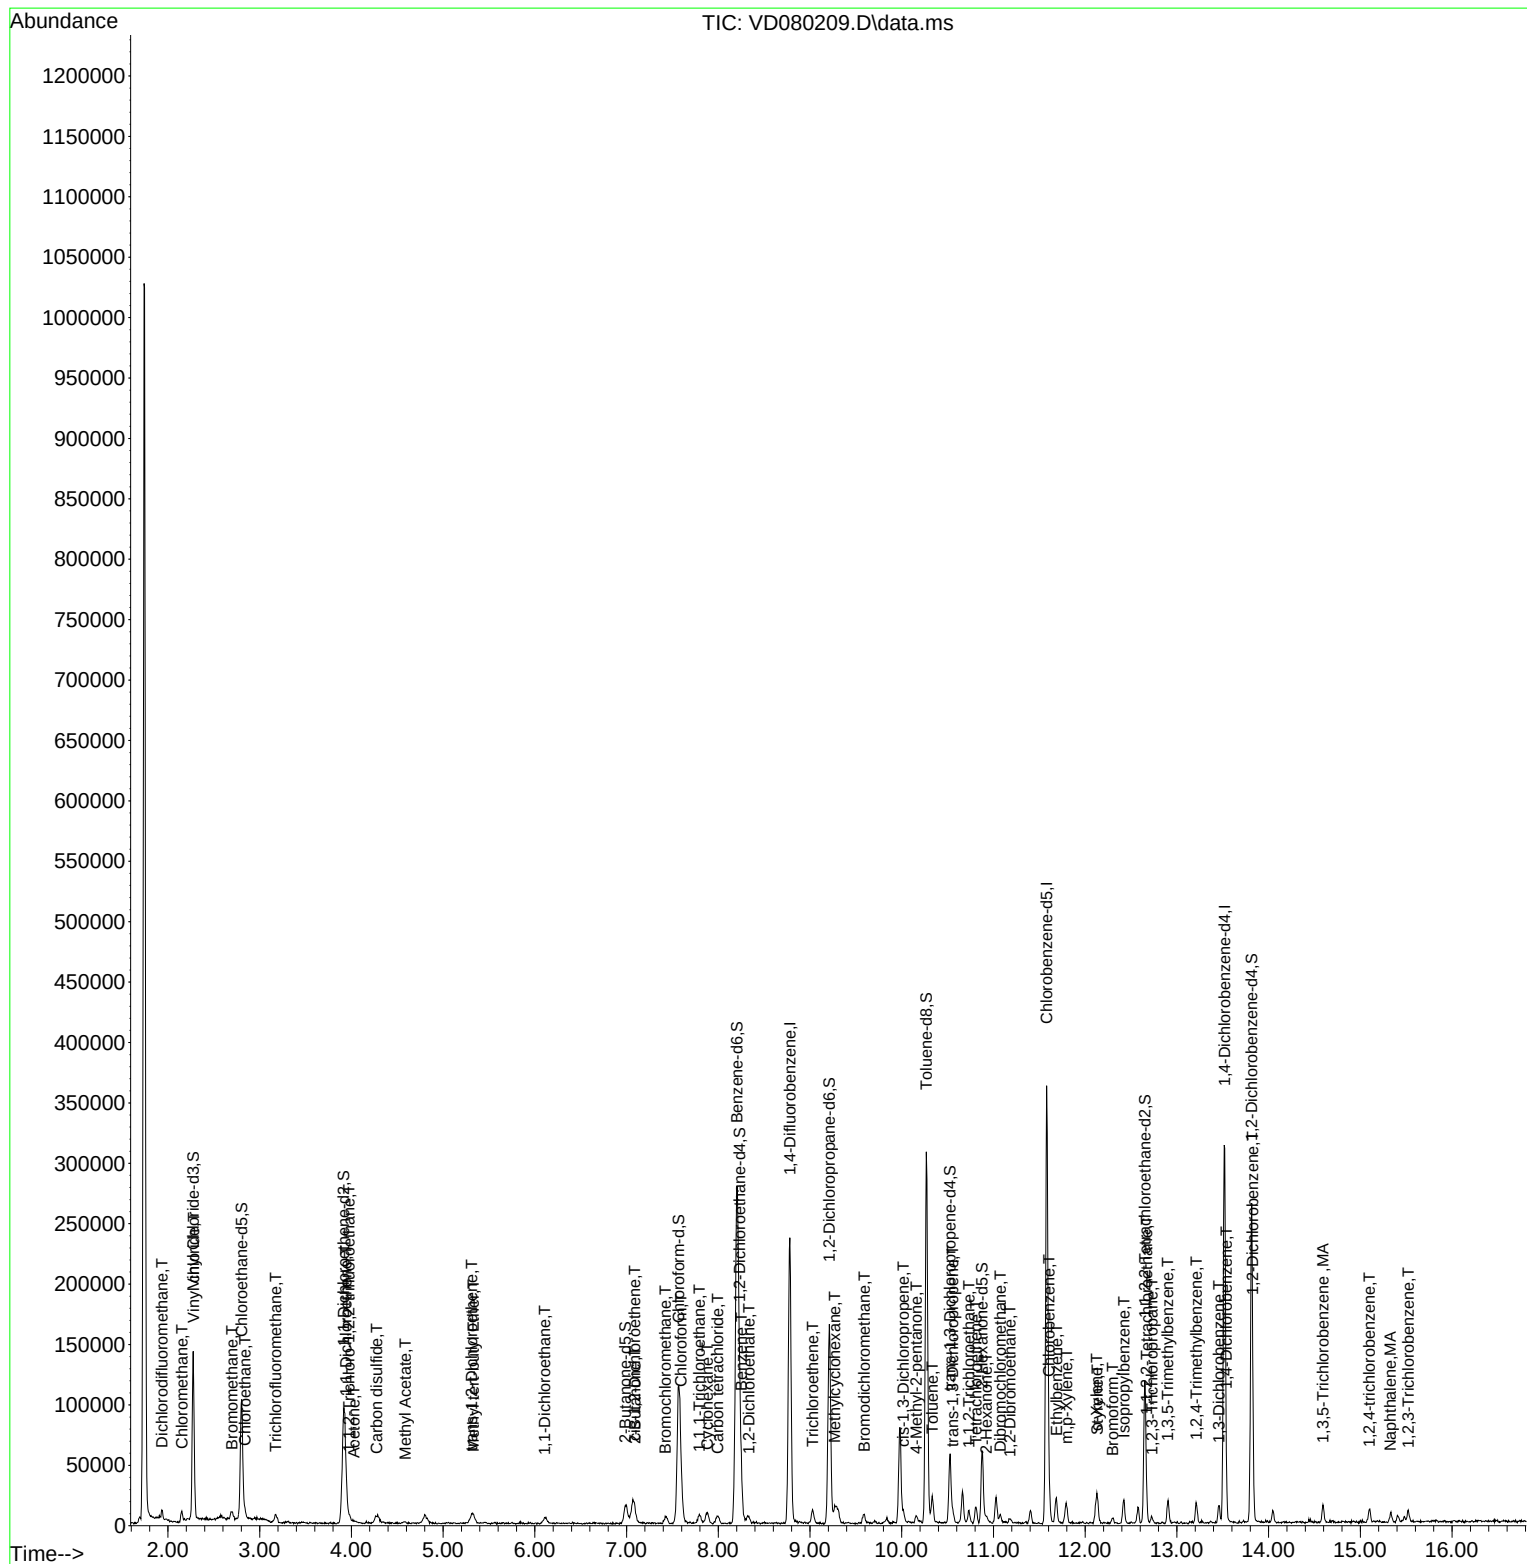


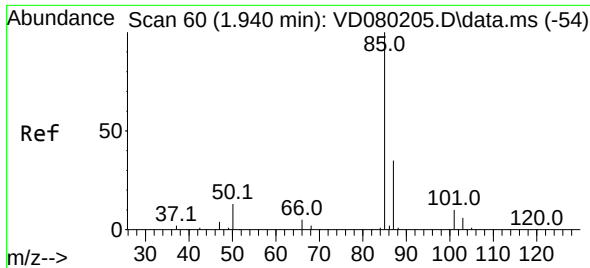

#2
 Dichlorodifluoromethane
 Concen: 1.201 ug/L
 RT: 1.934 min Scan# 59
 Delta R.T. -0.006 min
 Lab File: VD080209.D
 Acq: 10 Jan 2025 14:03




Instrument :
 MSVOA_D
 ClientSampleId :


Tgt Ion: 85 Resp: 4870
 Ion Ratio Lower Upper
 85 100
 87 31.7 26.4 39.6

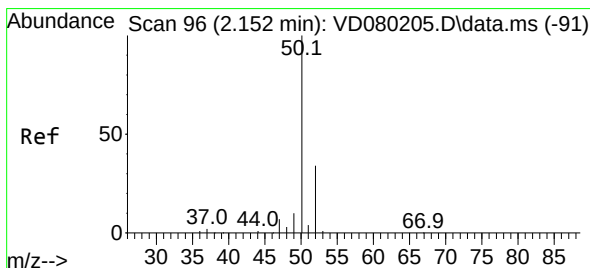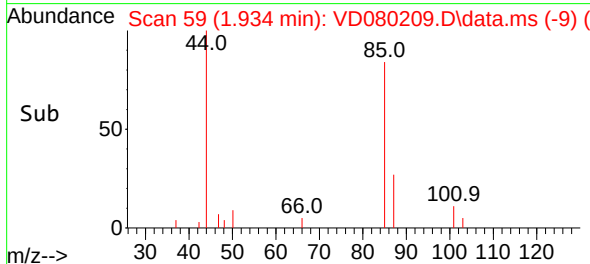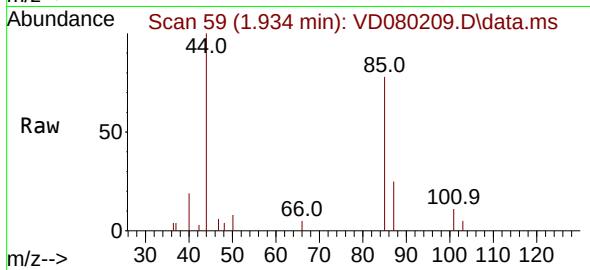

#3
 Chloromethane
 Concen: 1.262 ug/L
 RT: 2.152 min Scan# 96
 Delta R.T. -0.000 min
 Lab File: VD080209.D
 Acq: 10 Jan 2025 14:03

Tgt Ion: 50 Resp: 6976
 Ion Ratio Lower Upper
 50 100
 52 24.8 22.0 40.8


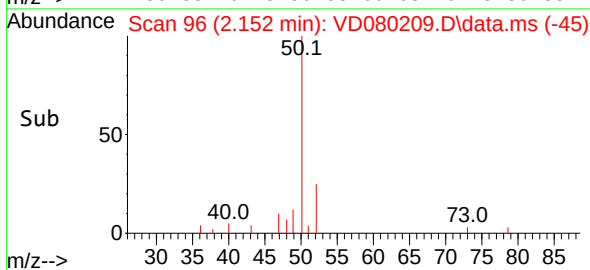

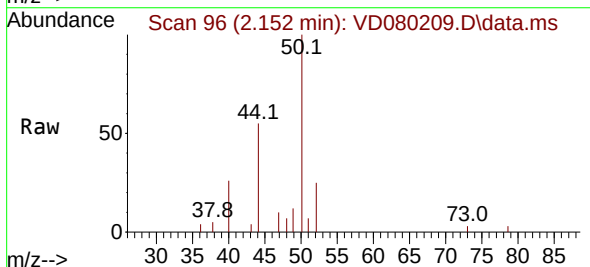


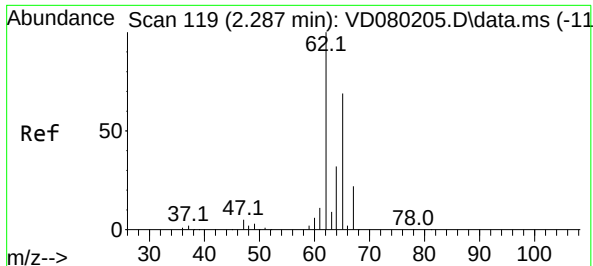

#5
 Vinyl chloride
 Concen: 1.224 ug/L
 RT: 2.281 min Scan# 119
 Delta R.T. -0.006 min
 Lab File: VD080209.D
 Acq: 10 Jan 2025 14:03




Instrument :
 MSVOA_D
 ClientSampleId :


Tgt Ion: 62 Resp: 8304
 Ion Ratio Lower Upper
 62 100
 64 35.3 22.3 41.5

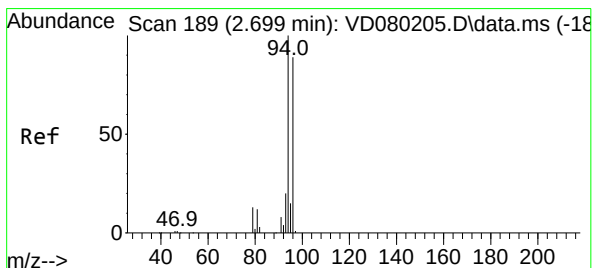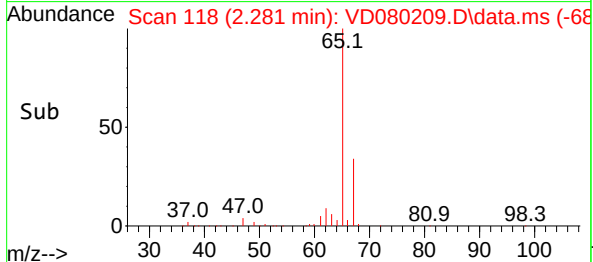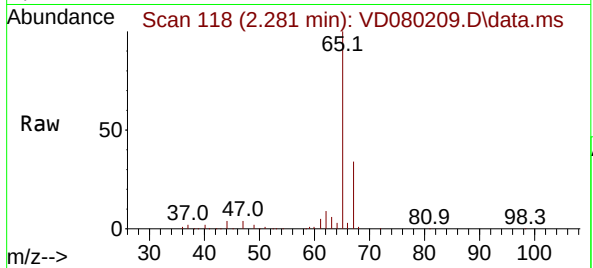

#6
 Bromomethane
 Concen: 1.097 ug/L
 RT: 2.699 min Scan# 189
 Delta R.T. -0.000 min
 Lab File: VD080209.D
 Acq: 10 Jan 2025 14:03

Tgt Ion: 94 Resp: 4332
 Ion Ratio Lower Upper
 94 100
 96 76.5 67.7 125.7


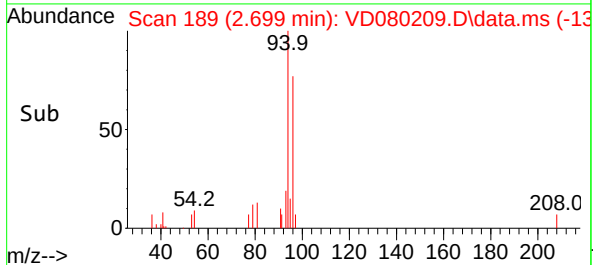

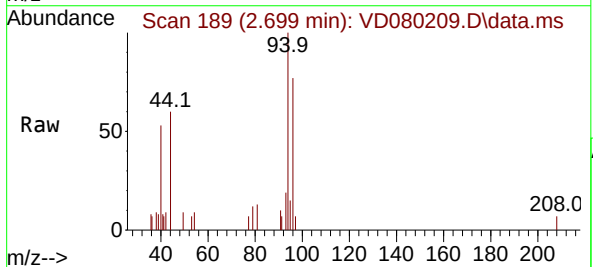




#8
Chloroethane
Concen: 1.215 ug/L
RT: 2.840 min Scan# 214
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 64 Resp: 5056
Ion Ratio Lower Upper
64 100
66 28.4 22.3 41.5



#9
Trichlorofluoromethane
Concen: 1.107 ug/L
RT: 3.175 min Scan# 270
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Tgt Ion:101 Resp: 6240
Ion Ratio Lower Upper
101 100
103 62.2 52.2 78.2









#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.298 ug/L
RT: 3.975 min Scan# 405
Delta R.T. 0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:101 Resp: 957
Ion Ratio Lower Upper
101 100
85 69.0 35.6 53.4#
151 0.0 60.0 90.0#

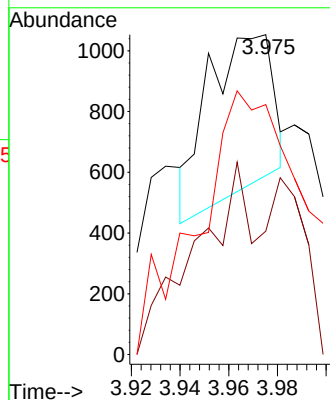

#12
1,1-Dichloroethene
Concen: 1.210 ug/L
RT: 3.940 min Scan# 400
Delta R.T. -0.012 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Tgt Ion: 96 Resp: 3473
Ion Ratio Lower Upper
96 100
61 284.8 123.1 228.7#
63 1084.1 89.6 166.4#

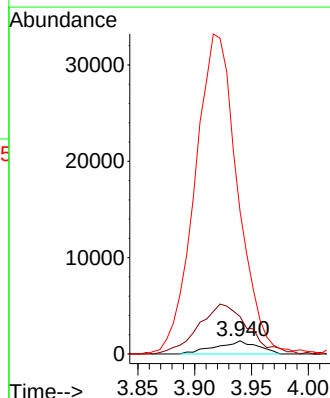



#13

Acetone

Concen: 2.836 ug/L

RT: 4.028 min Scan# 416

Delta R.T. -0.006 min

Lab File: VD080209.D

Acq: 10 Jan 2025 14:03

Instrument :

MSVOA_D





ClientSampleId :

Tgt Ion: 43 Resp: 1555

Ion Ratio Lower Upper

43 100

58 27.9 0.0 52.8



#14

Carbon disulfide

Concen: 1.035 ug/L

RT: 4.275 min Scan# 457

Delta R.T. -0.000 min

Lab File: VD080209.D




Acq: 10 Jan 2025 14:03


Tgt Ion: 76 Resp: 11076

Ion Ratio Lower Upper

76 100

78 4.9 7.5 11.3#







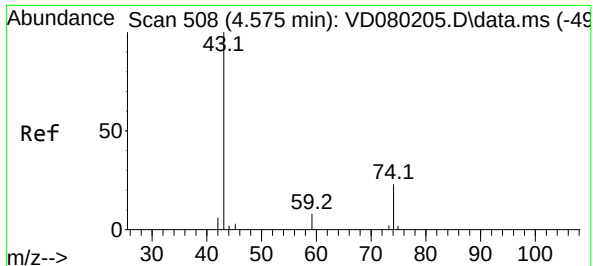

#15
Methyl Acetate
Concen: 0.496 ug/L
RT: 4.587 min Scan# 510
Delta R.T. 0.012 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 43 Resp: 680
Ion Ratio Lower Upper
43 100
74 10.7 10.1 15.1

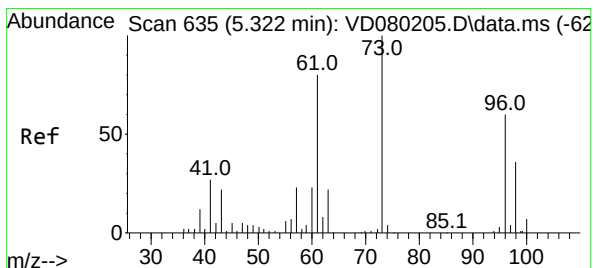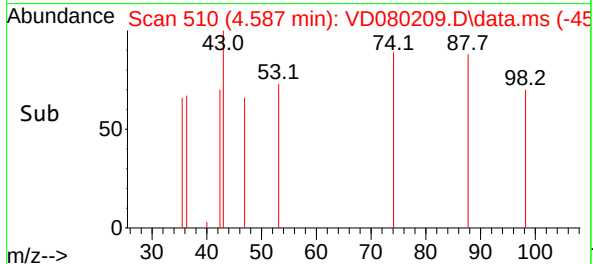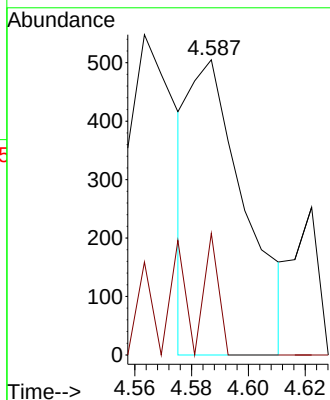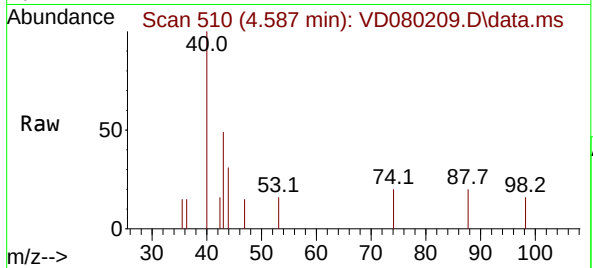

#17
trans-1,2-Dichloroethene
Concen: 0.189 ug/L
RT: 5.310 min Scan# 633
Delta R.T. -0.012 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03


Tgt Ion: 96 Resp: 591
Ion Ratio Lower Upper
96 100
61 139.4 93.7 173.9
98 59.5 42.1 78.1

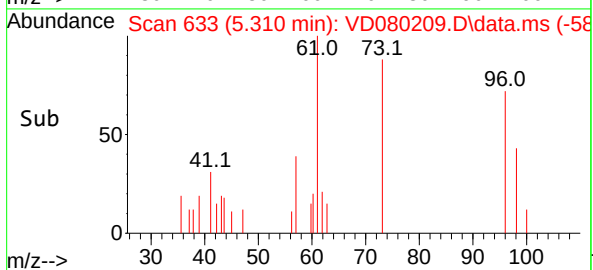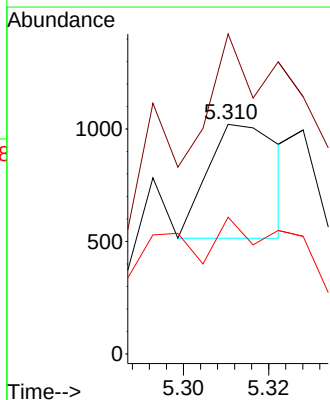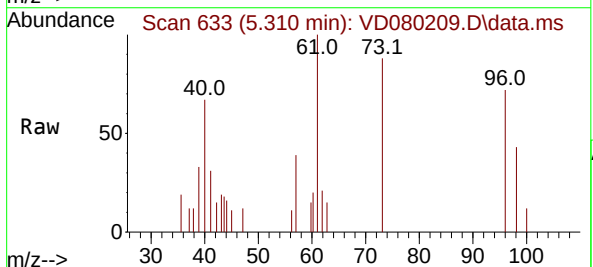






#18
Methyl tert-butyl Ether
Concen: 0.820 ug/L
RT: 5.328 min Scan# 61
Delta R.T. 0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03


Instrument :
MSVOA_D
ClientSampleId :





Tgt Ion: 73 Resp: 4879
Ion Ratio Lower Upper
73 100
43 0.0 16.6 24.8#
57 15.2 18.9 28.3#




#19
1,1-Dichloroethane
Concen: 1.090 ug/L
RT: 6.105 min Scan# 768
Delta R.T. -0.018 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03



Tgt Ion: 63 Resp: 6568
Ion Ratio Lower Upper
63 100
65 29.5 21.7 40.3
83 19.4 8.8 16.4#









#20
 cis-1,2-Dichloroethene
 Concen: 0.936 ug/L
 RT: 7.087 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: VD080209.D
 Acq: 10 Jan 2025 14:03

Instrument :
 MSVOA_D
 ClientSampleId :

Tgt Ion: 96 Resp: 3074




Ion	Ratio	Lower	Upper
96	100		
61	107.5	80.8	150.0
98	53.7	42.6	79.0

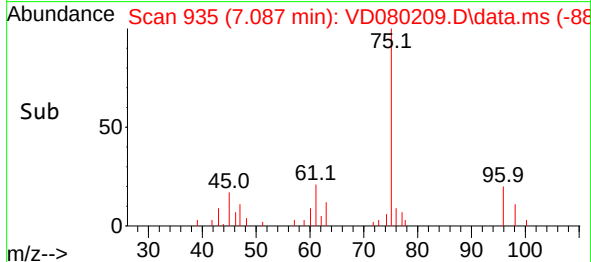


#22
 2-Butanone
 Concen: 1.425 ug/L
 RT: 7.093 min Scan# 936
 Delta R.T. 0.006 min
 Lab File: VD080209.D
 Acq: 10 Jan 2025 14:03

Tgt Ion: 43 Resp: 1113


Ion	Ratio	Lower	Upper
43	100		
72	17.4	14.0	42.0

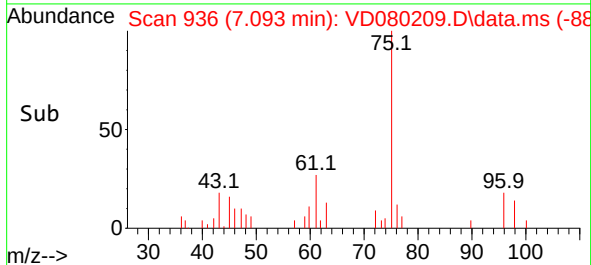






#23
Bromochloromethane
Concen: 0.774 ug/L
RT: 7.422 min Scan# 992
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Instrument :
MSVOA_D
ClientSampleId :







Tgt Ion:128 Resp: 1229
Ion Ratio Lower Upper
128 100
49 91.9 110.7 205.7#
130 110.1 83.1 154.3
51 36.4 42.0 63.0#

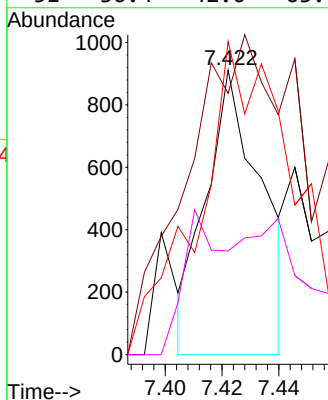

#25
Chloroform
Concen: 2.961 ug/L
RT: 7.593 min Scan# 1021
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Tgt Ion: 83 Resp: 19785
Ion Ratio Lower Upper
83 100
85 74.1 45.1 83.9

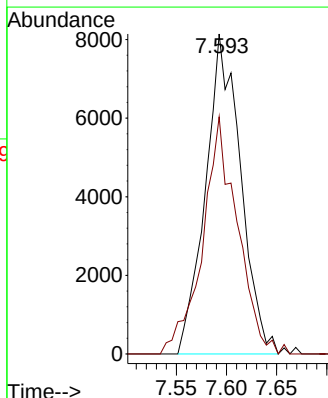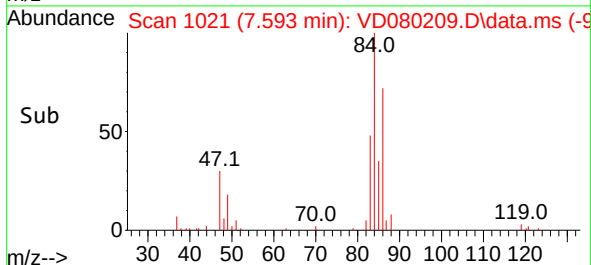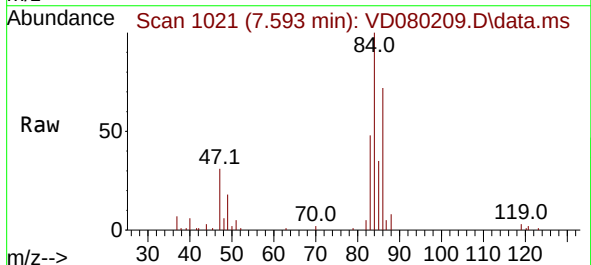

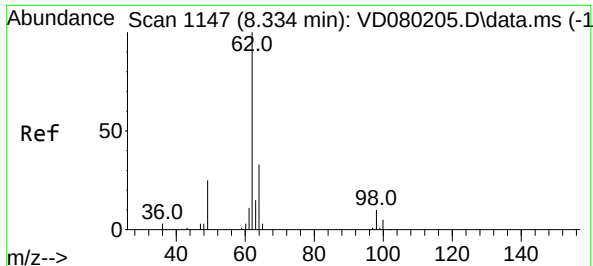

#27

1,2-Dichloroethane

Concen: 1.027 ug/L

RT: 8.334 min Scan# 1147

Delta R.T. -0.000 min

Lab File: VD080209.D

Acq: 10 Jan 2025 14:03

Instrument :

MSVOA_D





ClientSampleId :

Tgt Ion: 62 Resp: 4003

Ion Ratio Lower Upper

62 100

98 7.5 8.6 13.0#

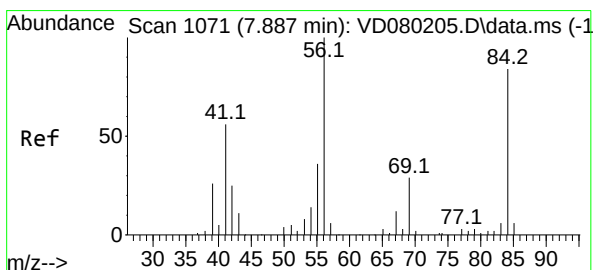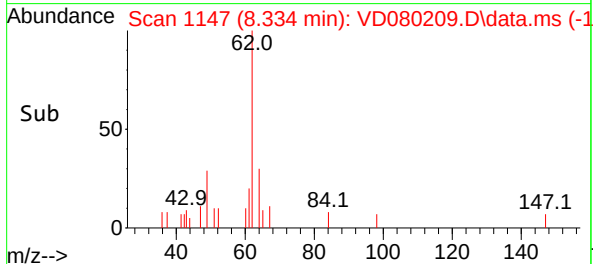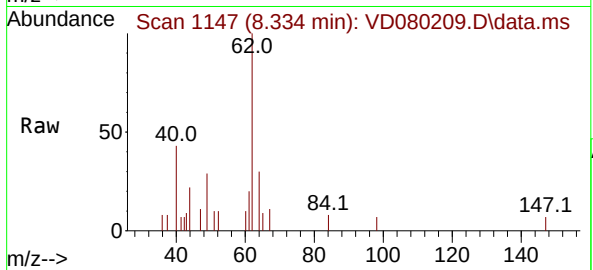

#29

Cyclohexane

Concen: 0.845 ug/L

RT: 7.881 min Scan# 1070

Delta R.T. -0.006 min

Lab File: VD080209.D

Acq: 10 Jan 2025 14:03




Tgt Ion: 56 Resp: 4202


Ion Ratio Lower Upper

56 100

69 20.4 24.2 36.4#

84 78.8 68.8 103.2


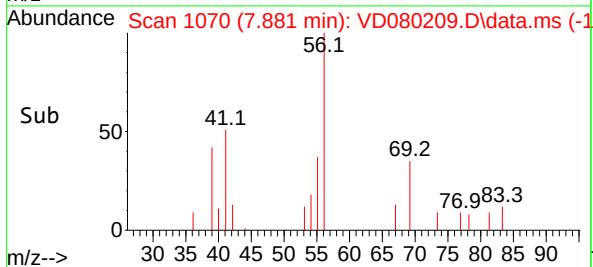

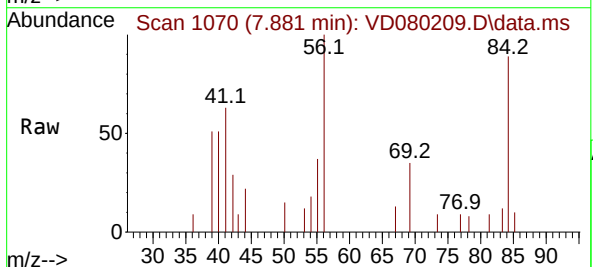




#30
1,1,1-Trichloroethane
Concen: 0.705 ug/L
RT: 7.793 min Scan# 1055
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 97 Resp: 3692
Ion Ratio Lower Upper
97 100
99 114.7 51.7 77.5#
61 67.3 35.8 53.6#



#31
Carbon tetrachloride
Concen: 1.036 ug/L
RT: 7.993 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Tgt Ion: 117 Resp: 4785
Ion Ratio Lower Upper
117 100
119 93.7 75.8 113.8



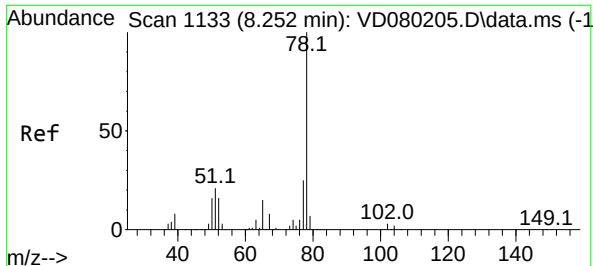

#33

Benzene

Concen: 1.013 ug/L

RT: 8.251 min Scan# 1133

Delta R.T. -0.000 min

Lab File: VD080209.D





Acq: 10 Jan 2025 14:03

Instrument :

MSVOA_D

ClientSampleId :

Tgt Ion: 78 Resp: 13614

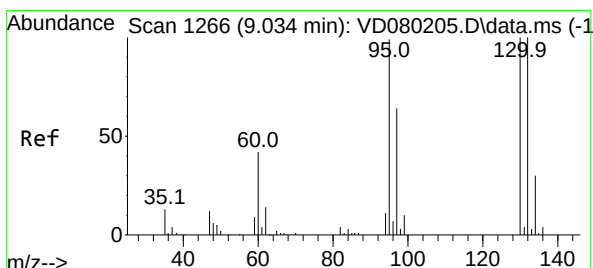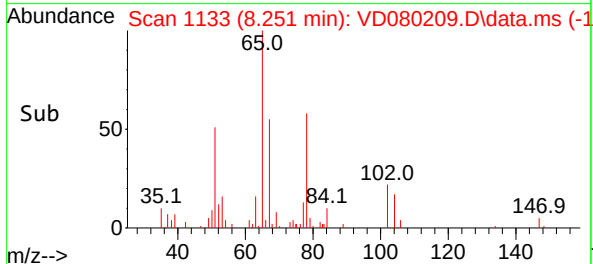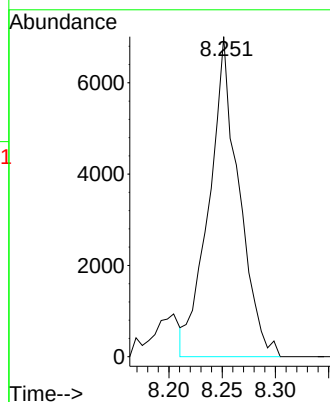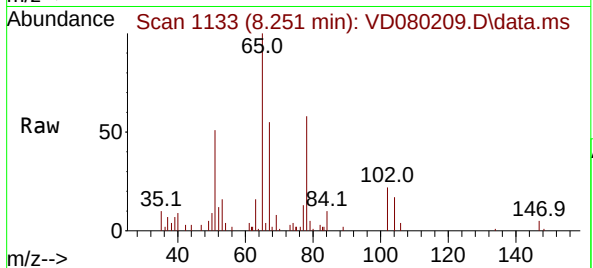

#34

Trichloroethene

Concen: 1.128 ug/L

RT: 9.028 min Scan# 1265

Delta R.T. -0.006 min

Lab File: VD080209.D

Acq: 10 Jan 2025 14:03

Tgt Ion: 95 Resp: 3924




Ion Ratio Lower Upper


95 100

97 63.7 45.6 84.6

132 80.2 67.2 124.8

130 85.6 71.0 131.8

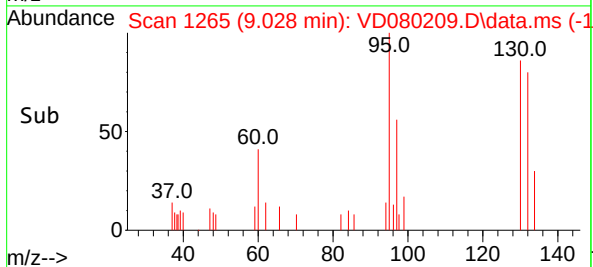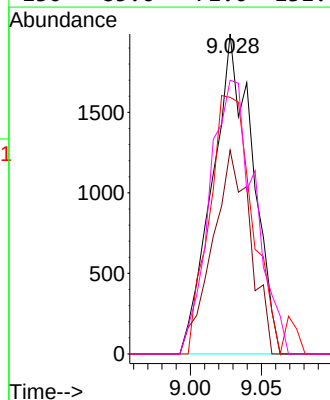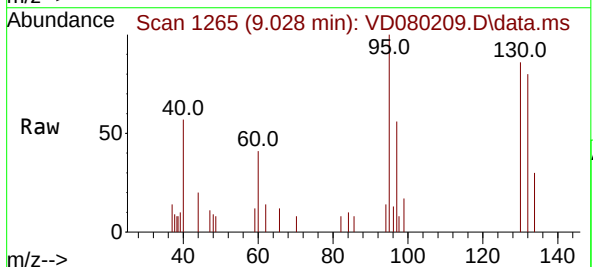

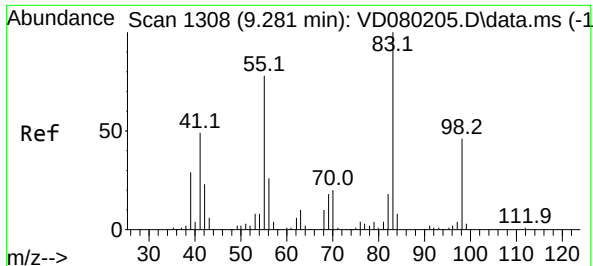

#35

Methylcyclohexane

Concen: 0.957 ug/L

RT: 9.269 min Scan# 1306

Delta R.T. -0.012 min

Lab File: VD080209.D

Acq: 10 Jan 2025 14:03

Instrument :

MSVOA_D

ClientSampleId :





Tgt Ion: 83 Resp: 4951

Ion Ratio Lower Upper

83 100

55 73.5 65.6 98.4

98 43.6 37.7 56.5

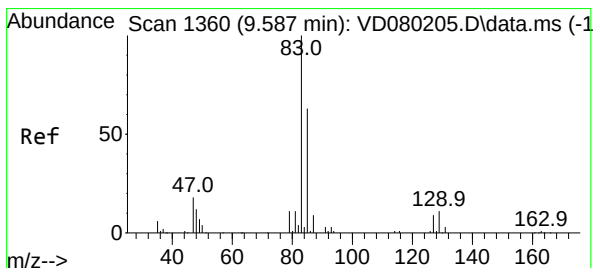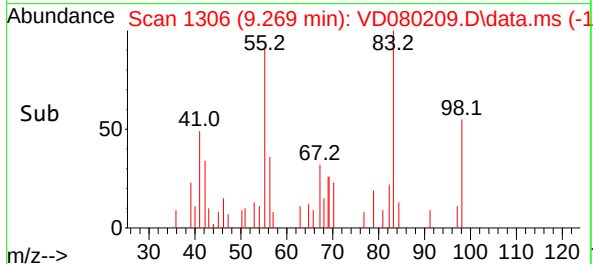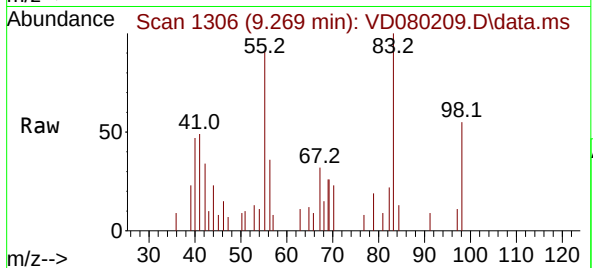

#38

Bromodichloromethane

Concen: 1.080 ug/L

RT: 9.593 min Scan# 1361

Delta R.T. 0.006 min

Lab File: VD080209.D

Acq: 10 Jan 2025 14:03




Tgt Ion: 83 Resp: 4958


Ion Ratio Lower Upper

83 100

85 45.0 44.6 82.8


127 9.0 6.7 10.1

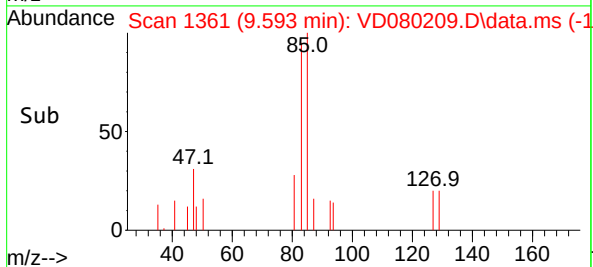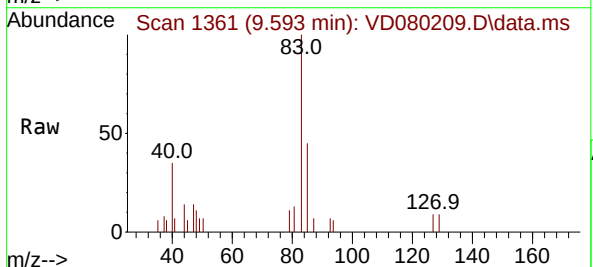






#39
cis-1,3-Dichloropropene
Concen: 1.015 ug/L
RT: 10.016 min Scan# 1433
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Instrument :
MSVOA_D
ClientSampleId :







Tgt Ion: 75 Resp: 5251
Ion Ratio Lower Upper
75 100
77 29.6 22.0 40.8



#40
4-Methyl-2-pentanone
Concen: 2.117 ug/L
RT: 10.157 min Scan# 1457
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Tgt Ion: 43 Resp: 3804
Ion Ratio Lower Upper
43 100
58 41.4 31.0 46.6
100 22.6 12.1 18.1#





#42

Toluene

Concen: 1.019 ug/L

RT: 10.334 min Scan# 1487

Delta R.T. -0.000 min

Lab File: VD080209.D

Acq: 10 Jan 2025 14:03

Instrument :

MSVOA_D





ClientSampleId :

Tgt Ion: 91 Resp: 14312

Ion Ratio Lower Upper

91 100

92 62.0 39.8 73.8



#44

trans-1,3-Dichloropropene

Concen: 1.328 ug/L

RT: 10.557 min Scan# 1525

Delta R.T. -0.000 min

Lab File: VD080209.D




Acq: 10 Jan 2025 14:03


Tgt Ion: 75 Resp: 5932

Ion Ratio Lower Upper

75 100

77 29.6 22.0 40.8




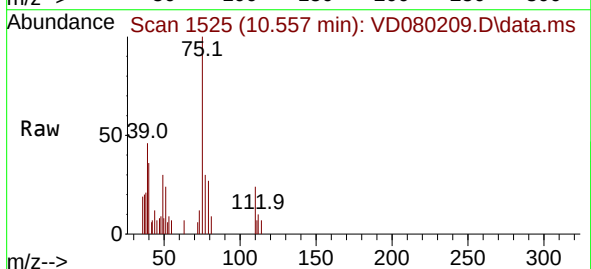




#45
1,1,2-Trichloroethane
Concen: 1.022 ug/L
RT: 10.734 min Scan# 1555
Delta R.T. -0.000 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 97	Resp: 2733
Ion Ratio	Lower Upper
97 100	
99 67.4	44.0 81.8
83 60.3	64.4 119.6#
85 43.3	38.9 72.3



#46
Tetrachloroethene
Concen: 1.036 ug/L
RT: 10.810 min Scan# 1568
Delta R.T. -0.000 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Tgt	Ion:164	Resp:	2905
Ion	Ratio	Lower	Upper
164	100		
129	120.9	67.8	125.8
131	103.0	67.6	125.6
166	133.3	93.7	174.1







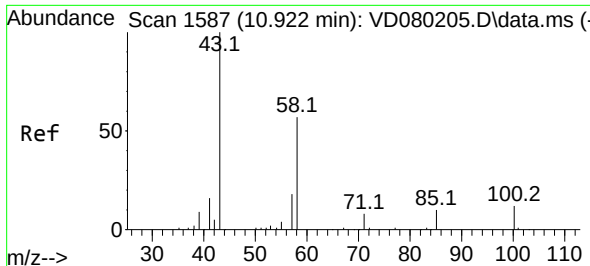

#48
2-Hexanone
Concen: 1.982 ug/L
RT: 10.922 min Scan# 1587
Delta R.T. -0.000 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 43 Resp: 2429
Ion Ratio Lower Upper
43 100
58 42.7 42.5 63.7
57 9.8 15.5 23.3#
100 0.0 9.7 14.5#

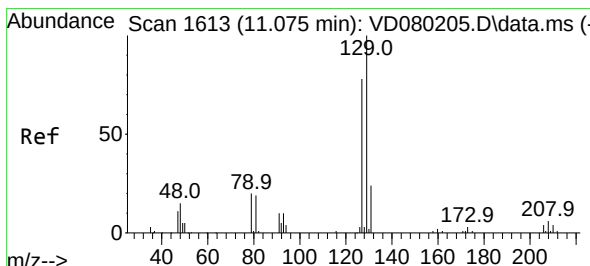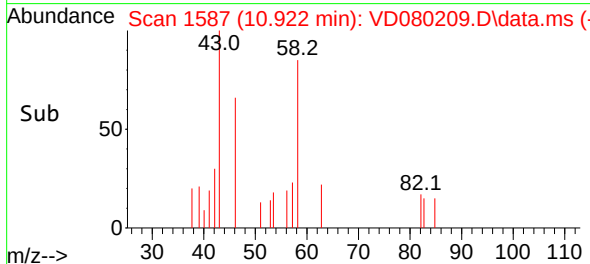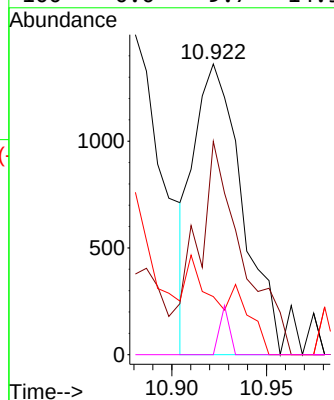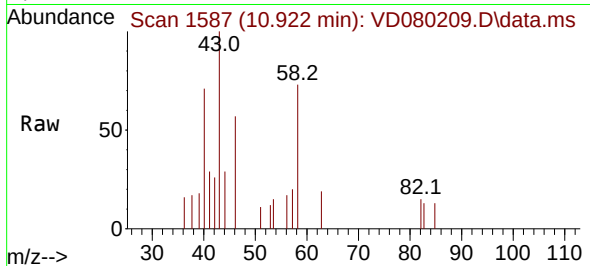

#49
Dibromochloromethane
Concen: 1.065 ug/L
RT: 11.075 min Scan# 1613
Delta R.T. -0.000 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Tgt Ion: 129 Resp: 3170
Ion Ratio Lower Upper
129 100
127 97.9 52.3 97.1#


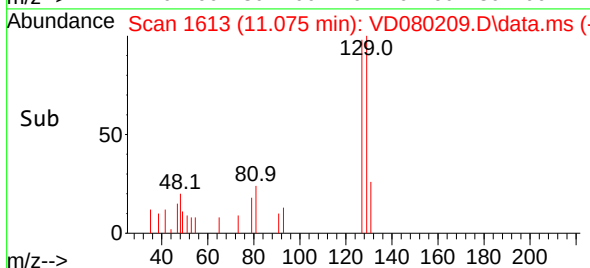
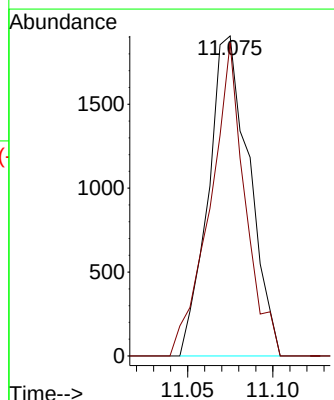
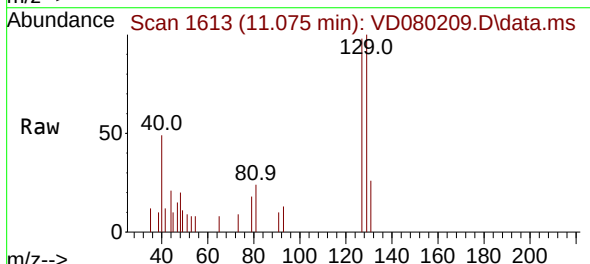




#50
1,2-Dibromoethane
Concen: 1.064 ug/L
RT: 11.181 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:107 Resp: 2585
Ion Ratio Lower Upper
107 100
109 75.6 63.8 118.6
188 0.0 2.8 4.2#

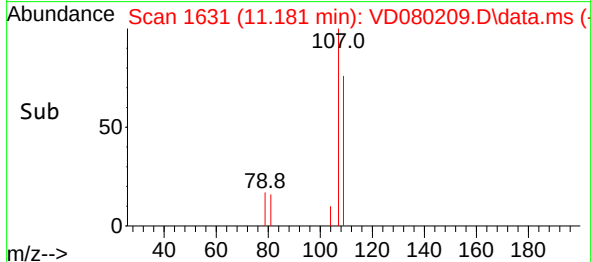

#51
Chlorobenzene
Concen: 1.028 ug/L
RT: 11.604 min Scan# 1703
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Tgt Ion:112 Resp: 9252
Ion Ratio Lower Upper
112 100
114 36.2 21.8 40.6
77 59.5 46.8 70.2




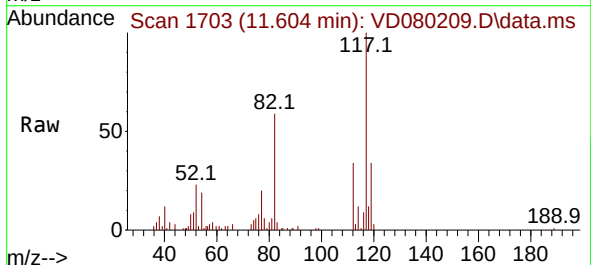




#52
Ethylbenzene
Concen: 0.904 ug/L
RT: 11.687 min Scan# 1717
Delta R.T. -0.000 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 91 Resp: 13614
Ion Ratio Lower Upper
91 100
106 28.8 21.8 40.6



#53
m,p-Xylene
Concen: 0.833 ug/L
RT: 11.798 min Scan# 1736
Delta R.T. -0.000 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Tgt Ion: 106 Resp: 4690
Ion Ratio Lower Upper
106 100
91 183.7 144.1 267.7





#54

o-Xylene

Concen: 0.777 ug/L

RT: 12.128 min Scan# 1792

Delta R.T. 0.006 min

Lab File: VD080209.D

Acq: 10 Jan 2025 14:03

Instrument :

MSVOA_D





ClientSampleId :

Tgt Ion:106 Resp: 4092

Ion Ratio Lower Upper

106 100

91 168.0 153.8 285.6



#55

Styrene

Concen: 0.775 ug/L

RT: 12.134 min Scan# 1793

Delta R.T. -0.000 min

Lab File: VD080209.D




Acq: 10 Jan 2025 14:03


Tgt Ion:104 Resp: 7391

Ion Ratio Lower Upper

104 100

78 46.5 31.9 59.3





#57

1,1,2,2-Tetrachloroethane

Concen: 1.036 ug/L

RT: 12.669 min Scan# 1884

Delta R.T. -0.006 min

Lab File: VD080209.D

Acq: 10 Jan 2025 14:03





Instrument :

MSVOA_D

ClientSampleId :

Tgt Ion: 83 Resp: 3138

Ion	Ratio	Lower	Upper
83	100		
85	63.4	40.7	75.5
131	31.5	6.2	9.2#

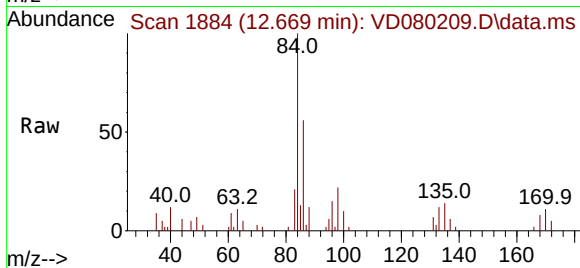

#59

Bromoform

Concen: 1.133 ug/L

RT: 12.298 min Scan# 1821




Delta R.T. -0.006 min


Lab File: VD080209.D

Acq: 10 Jan 2025 14:03

Tgt Ion: 173 Resp: 1772

Ion	Ratio	Lower	Upper
173	100		
175	45.0	38.2	57.4
254	0.0	8.3	12.5#




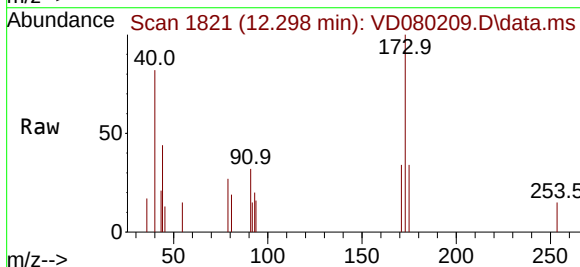




#60
Isopropylbenzene
Concen: 0.903 ug/L
RT: 12.422 min Scan# 1842
Delta R.T. -0.000 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:	105	Resp:	10978
Ion	Ratio	Lower	Upper
105	100		
120	29.7	20.6	30.8
77	17.0	13.0	19.6

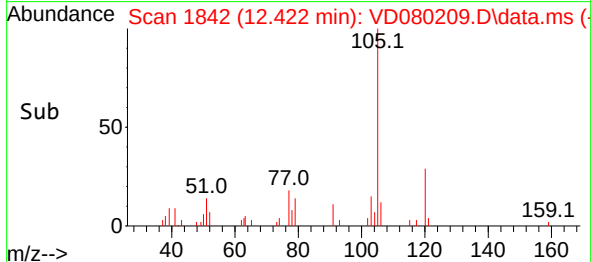

#61
1,2,3-Trichloropropane
Concen: 1.131 ug/L
RT: 12.728 min Scan# 1894
Delta R.T. -0.000 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Tgt Ion:	75	Resp:	2084
Ion	Ratio	Lower	Upper
75	100		
77	29.6	25.7	38.5
110	44.7	31.5	47.3




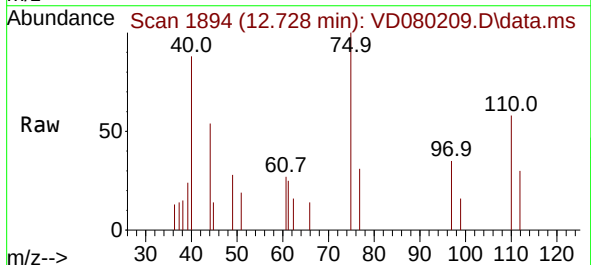




#62
1,3,5-Trimethylbenzene
Concen: 0.902 ug/L
RT: 12.898 min Scan# 1923
Delta R.T. -0.012 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:105 Resp: 8737
Ion Ratio Lower Upper
105 100
120 48.4 38.9 58.3



#63
1,2,4-Trimethylbenzene
Concen: 0.901 ug/L
RT: 13.210 min Scan# 1976
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03


Tgt Ion:105 Resp: 8517
Ion Ratio Lower Upper
105 100
120 44.0 36.1 54.1

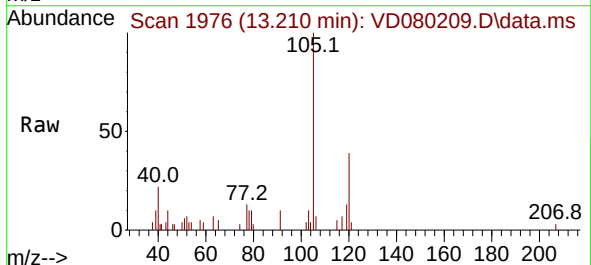






#64
1,3-Dichlorobenzene
Concen: 0.981 ug/L
RT: 13.457 min Scan# 2019
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03


Instrument :
MSVOA_D
ClientSampleId :





Tgt Ion:146 Resp: 5830
Ion Ratio Lower Upper
146 100
111 36.3 27.2 50.6
148 62.8 44.8 83.2




#65
1,4-Dichlorobenzene
Concen: 0.996 ug/L
RT: 13.539 min Scan# 2032
Delta R.T. -0.000 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Tgt Ion:146 Resp: 6111
Ion Ratio Lower Upper
146 100
111 48.9 26.7 49.7
148 86.2 44.1 81.9#





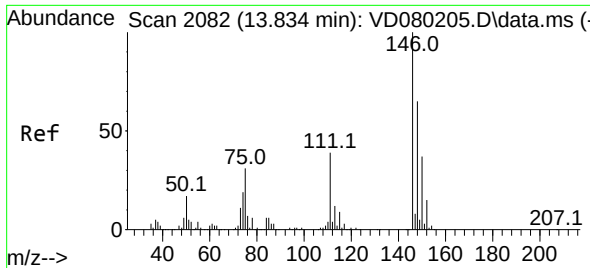


#67
1,2-Dichlorobenzene
Concen: 1.132 ug/L
RT: 13.828 min Scan# 2081
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03

Instrument :
MSVOA_D
ClientSampleId :



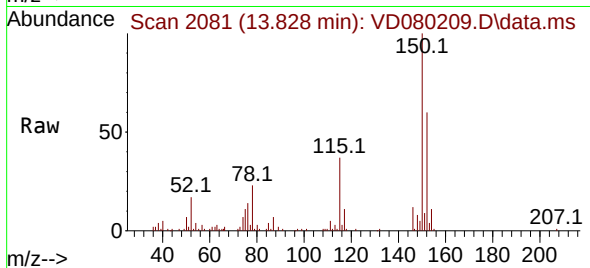



Tgt Ion:146 Resp: 6026
Ion Ratio Lower Upper
146 100
111 44.9 31.4 47.0
148 65.8 48.8 73.2

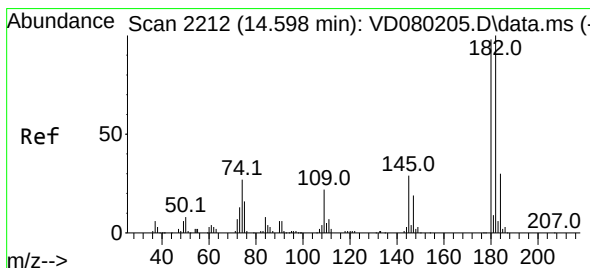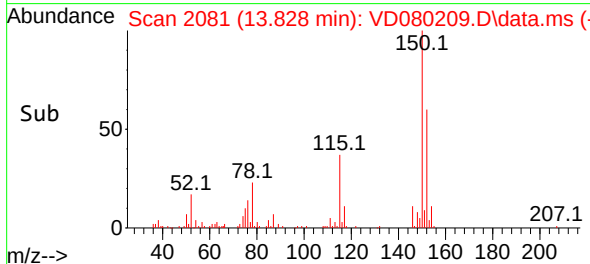

#69
1,3,5-Trichlorobenzene
Concen: 1.077 ug/L
RT: 14.592 min Scan# 2211
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03


Tgt Ion:180 Resp: 4354
Ion Ratio Lower Upper
180 100
182 0.0 75.4 113.0#
184 30.6 24.0 36.0
145 29.2 23.4 35.0

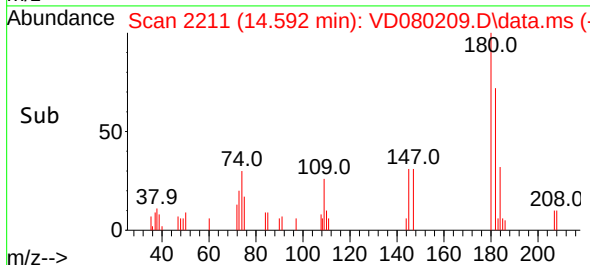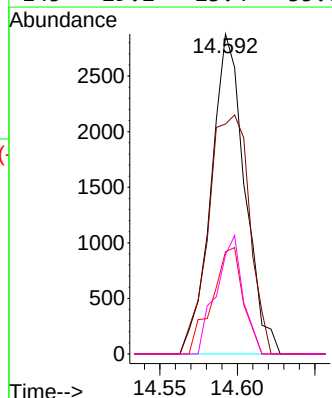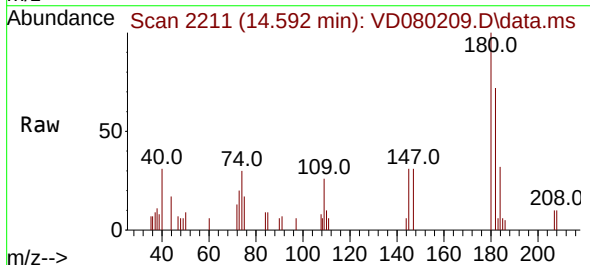






#70
1,2,4-trichlorobenzene
Concen: 0.985 ug/L
RT: 15.098 min Scan# 21
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03


Instrument :
MSVOA_D
ClientSampleId :





Tgt Ion:180 Resp: 3249
Ion Ratio Lower Upper
180 100
182 107.8 76.9 115.3
145 15.9 23.5 35.3#

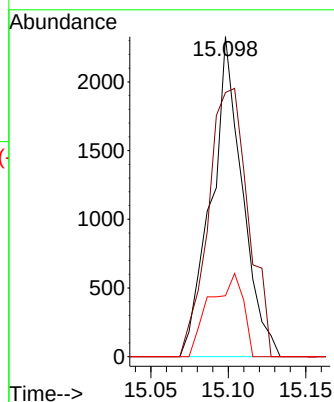


#71
Naphthalene
Concen: 0.996 ug/L
RT: 15.328 min Scan# 2336
Delta R.T. -0.006 min
Lab File: VD080209.D
Acq: 10 Jan 2025 14:03




Tgt Ion:128 Resp: 5782
Ion Ratio Lower Upper
128 100
127 14.1 11.5 17.3
129 9.4 9.0 13.6

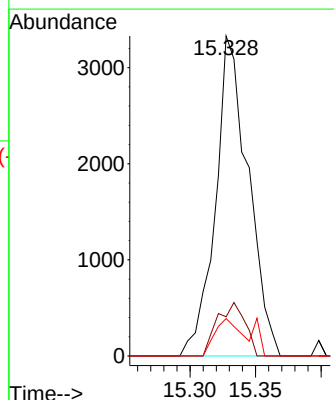

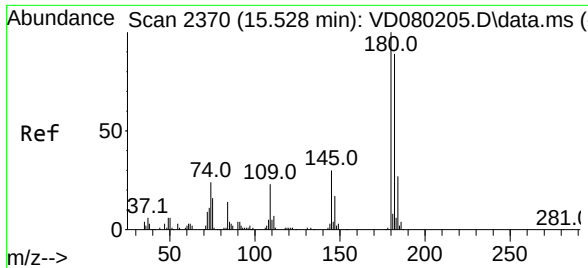

#72
 1,2,3-Trichlorobenzene
 Concen: 1.077 ug/L
 RT: 15.522 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VD080209.D
 Acq: 10 Jan 2025 14:03

Instrument :
 MSVOA_D
 ClientSampleId :

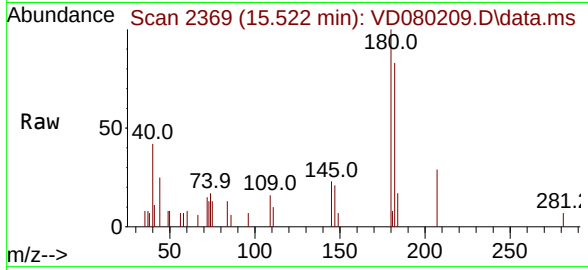

Tgt Ion:	180	Resp:	3299
Ion	Ratio	Lower	Upper
180	100		
182	86.5	74.8	112.2
145	30.8	24.2	36.4

