
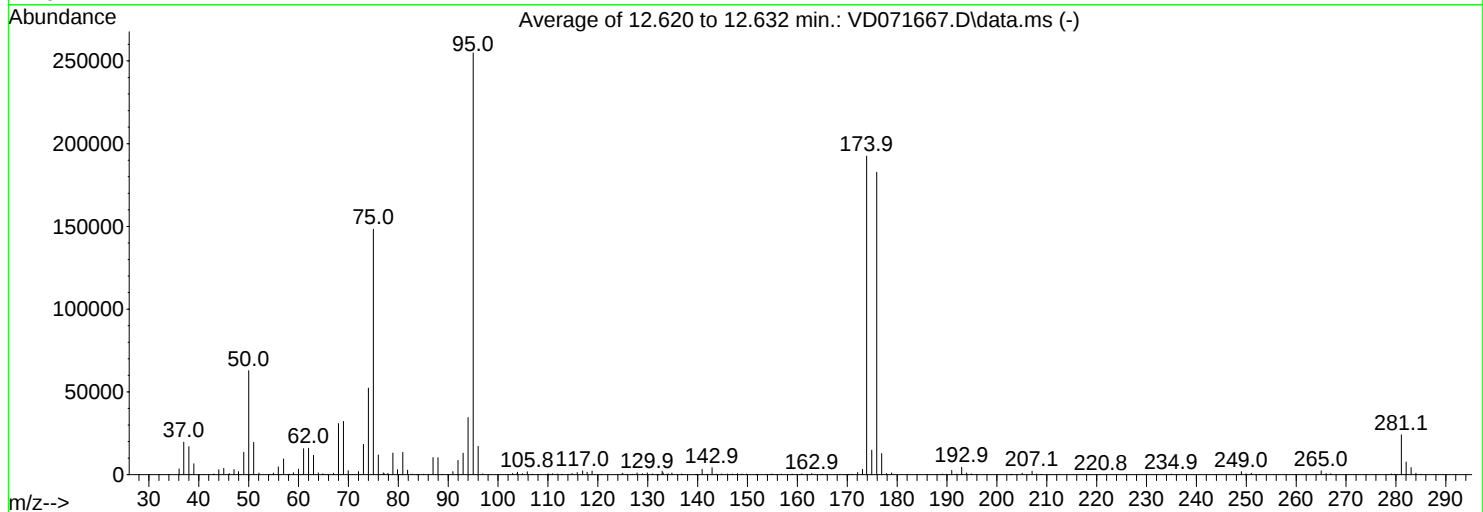


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD011122\  
Data File : VD071667.D  
Acq On : 11 Jan 2022 09:10  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D010722S.M  
Title : SW846 8260  
Last Update : Fri Jan 07 15:39:14 2022

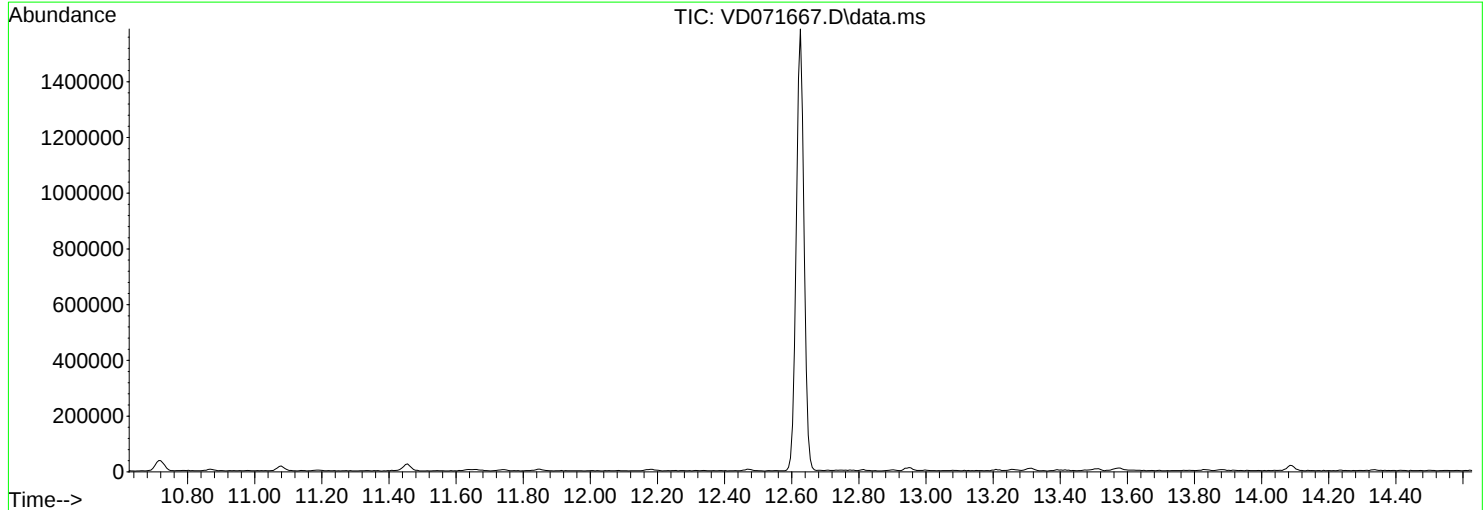

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 50     | 95      | 15     | 40     | 24.6  | 62824  | PASS      |
| 75     | 95      | 30     | 60     | 58.2  | 148352 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 254891 | PASS      |
| 96     | 95      | 5      | 9      | 6.7   | 17116  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.6   | 3168   | PASS      |
| 174    | 95      | 50     | 100    | 75.5  | 192512 | PASS      |
| 175    | 174     | 5      | 9      | 7.7   | 14822  | PASS      |
| 176    | 174     | 95     | 101    | 94.9  | 182763 | PASS      |
| 177    | 176     | 5      | 9      | 7.0   | 12724  | PASS      |