
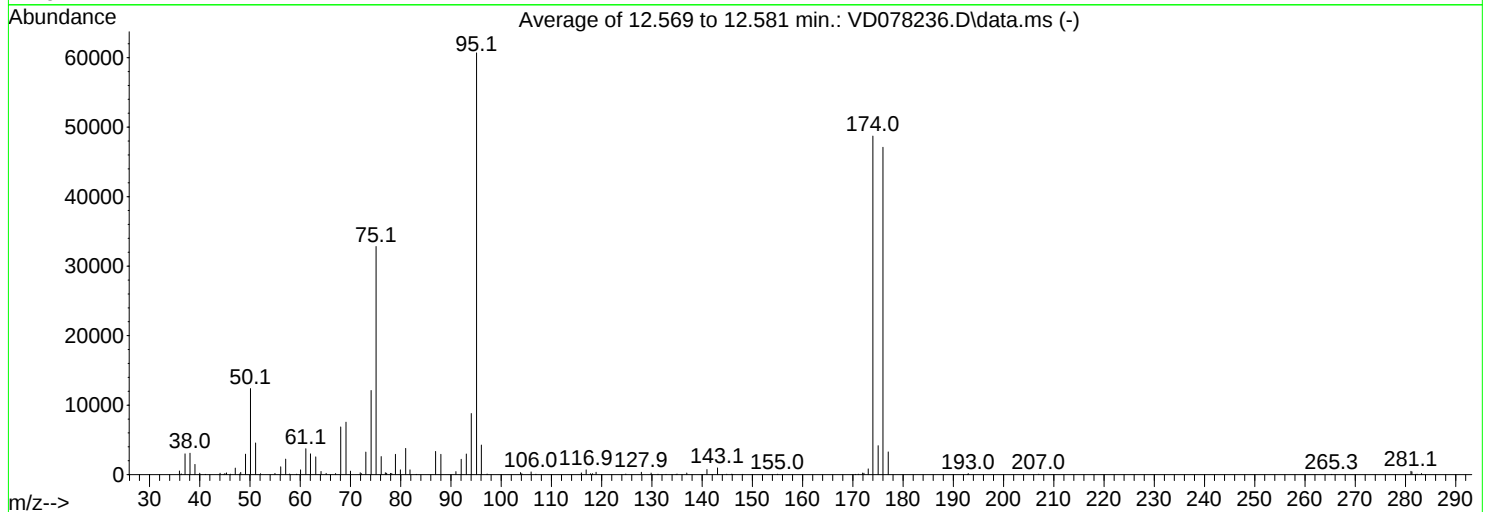


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012524\
Data File : VD078236.D
Acq On : 25 Jan 2024 09:00
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012224S.M
Title : SW846 8260
Last Update : Tue Jan 23 05:43:07 2024

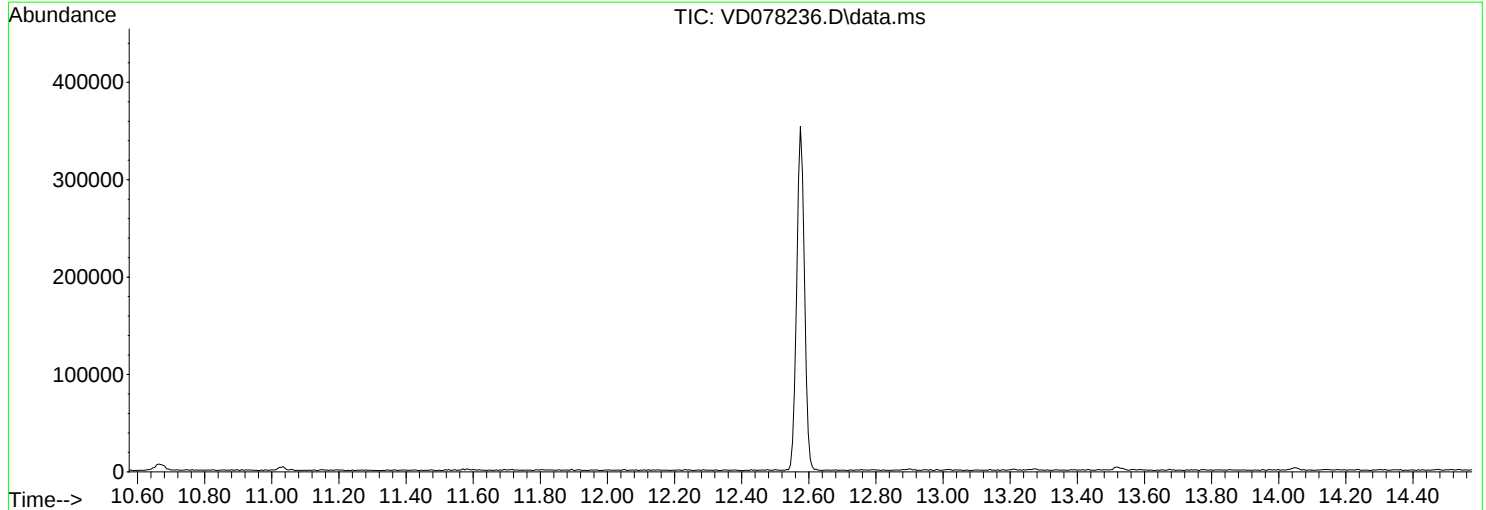

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	12396	PASS
75	95	30	60	54.1	32837	PASS
95	95	100	100	100.0	60691	PASS
96	95	5	9	7.0	4266	PASS
173	174	0.00	2	1.7	829	PASS
174	95	50	100	80.3	48707	PASS
175	174	5	9	8.6	4177	PASS
176	174	95	101	96.7	47096	PASS
177	176	5	9	6.9	3269	PASS