

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012721\
 Data File : VD068202.D
 Acq On : 27 Jan 2021 17:08
 Operator : VA/SY
 Sample : M1251-02
 Misc : 6.76G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 400026

Quant Time: Jan 27 23:58:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 19 13:19:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	500990	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	892449	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.649	117	780570	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	311457	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	296353	61.84	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 123.68%	
35) Dibromofluoromethane	7.920	113	271211	54.97	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 109.94%	
50) Toluene-d8	10.344	98	1103158	55.90	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 111.80%	
62) 4-Bromofluorobenzene	12.632	95	344784	48.51	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 97.02%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012721\
Data File : VD068202.D
Acq On : 27 Jan 2021 17:08
Operator : VA/SY
Sample : M1251-02
Misc : 6.76G/5.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
400026

Quant Time: Jan 27 23:58:00 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 19 13:19:08 2021
Response via : Initial Calibration




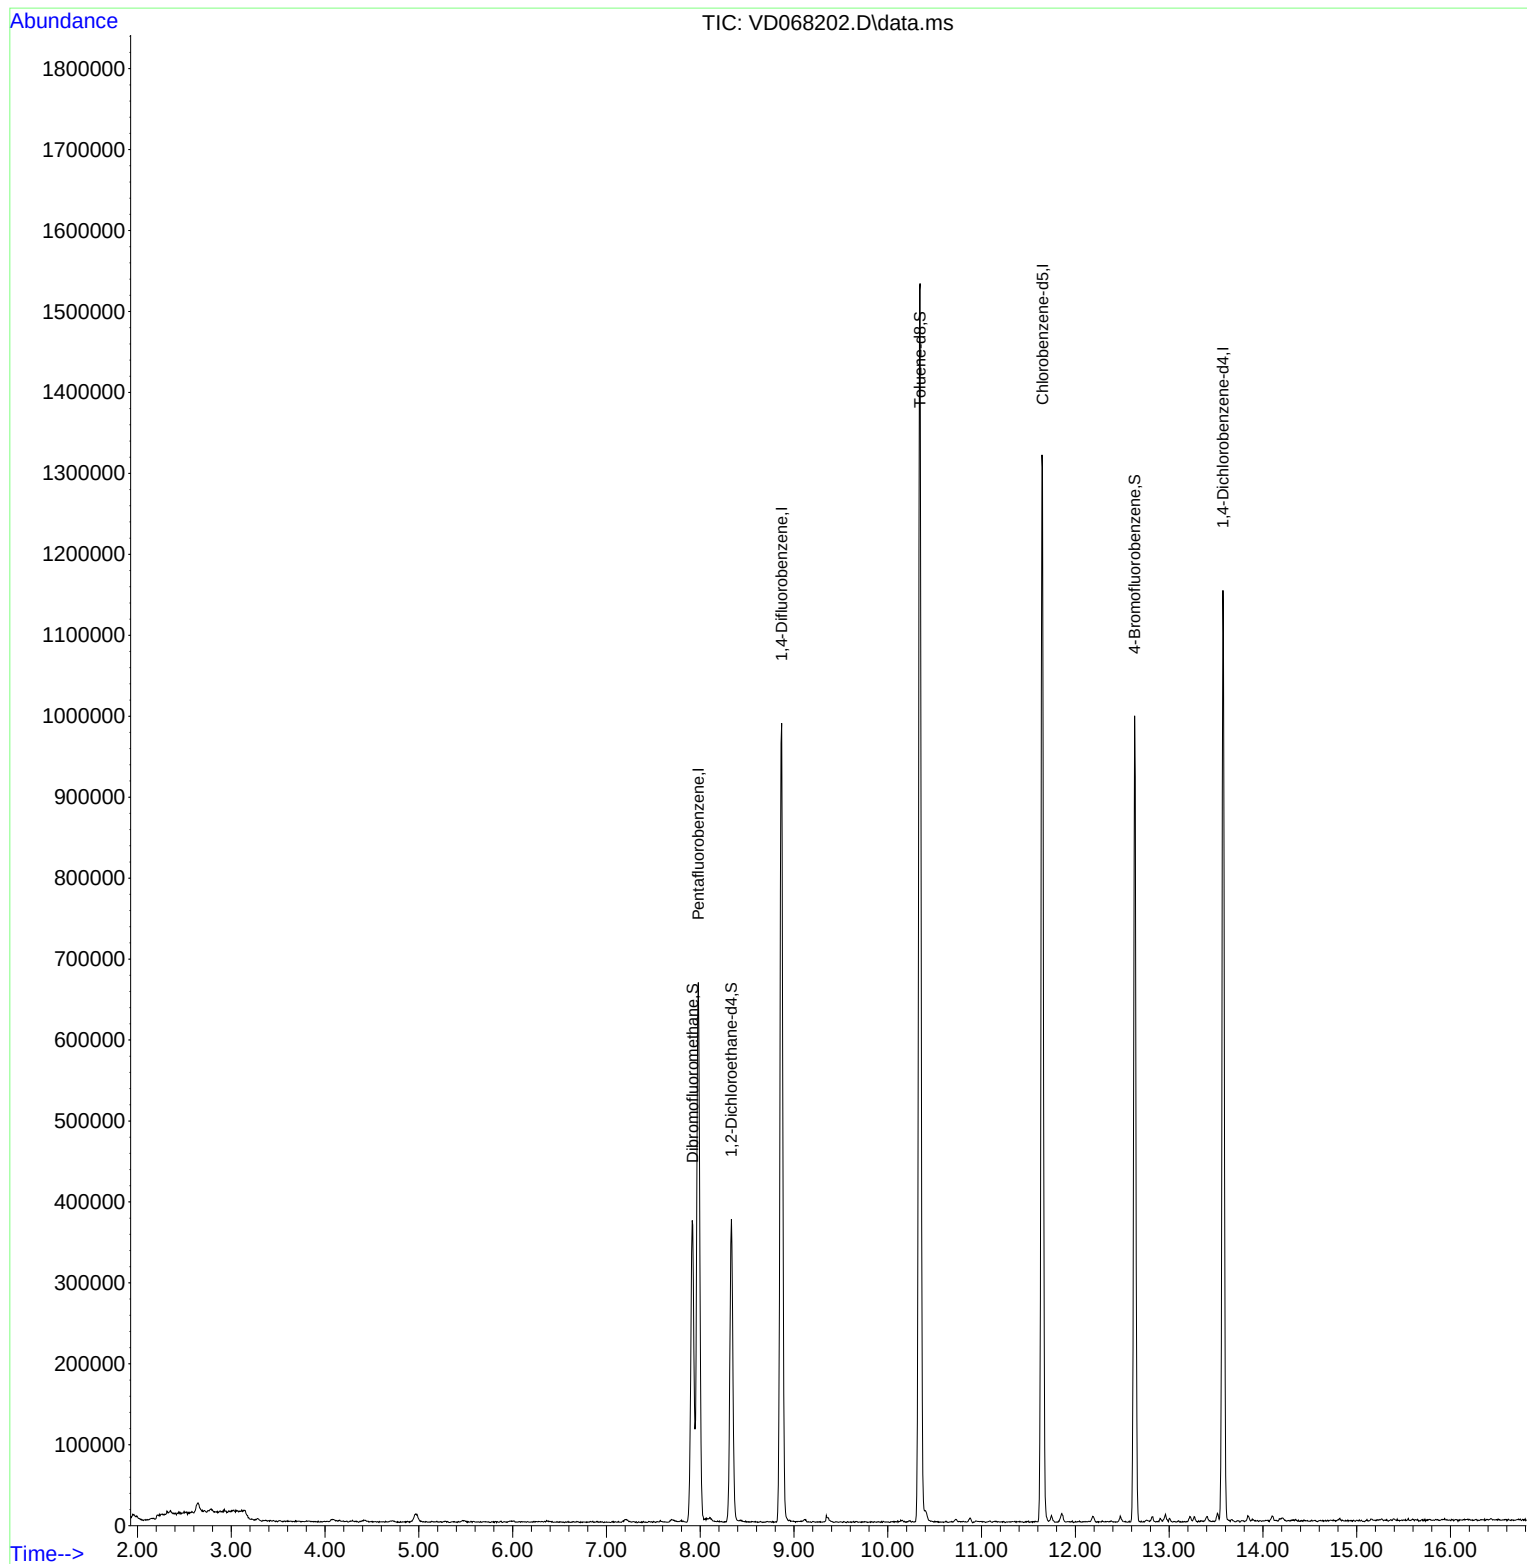


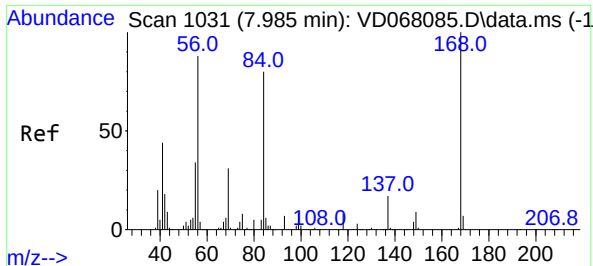

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD068202.D
Acq: 27 Jan 2021 17:08




Instrument :
MSVOA_D
ClientSampleId :
400026


Tgt Ion:168 Resp: 500990
Ion Ratio Lower Upper
168 100
99 58.8 43.5 65.3

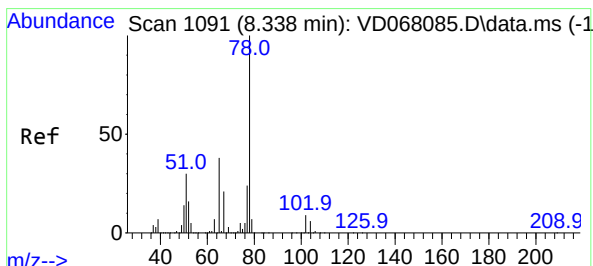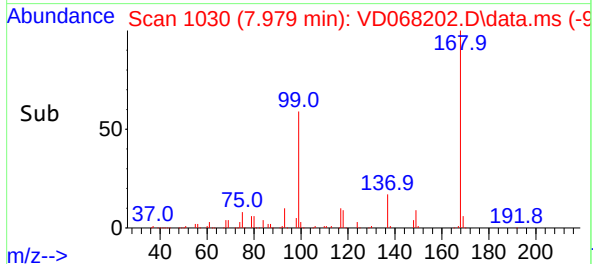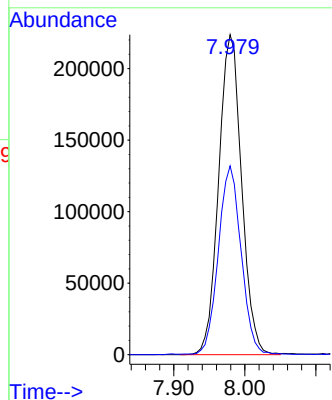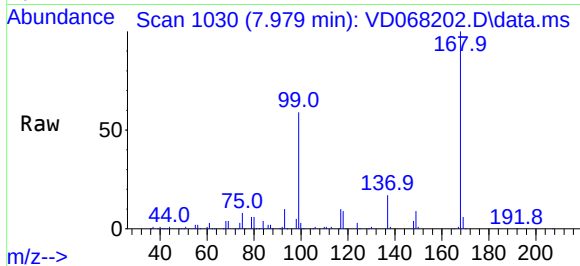

#33
1,2-Dichloroethane-d4
Concen: 61.84 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. -0.006 min
Lab File: VD068202.D
Acq: 27 Jan 2021 17:08

Tgt Ion: 65 Resp: 296353
Ion Ratio Lower Upper
65 100
67 53.2 0.0 105.0

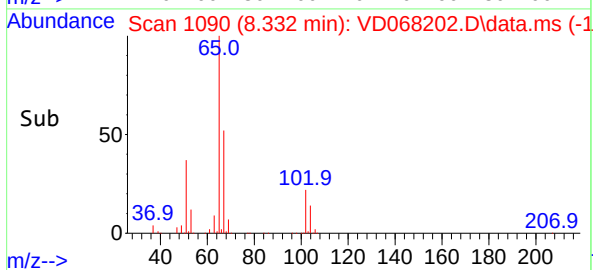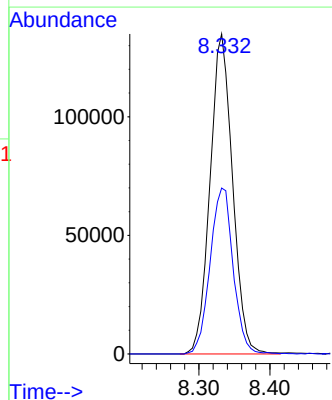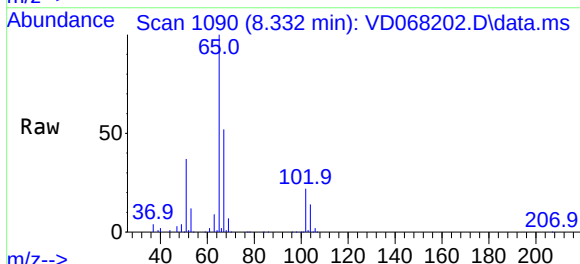




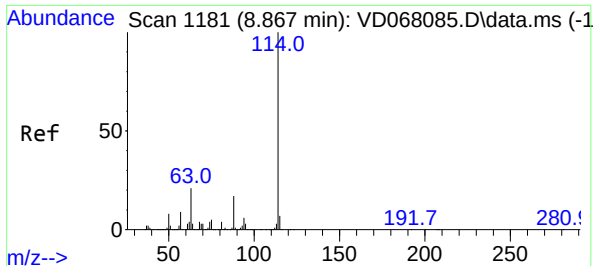


#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068202.D
Acq: 27 Jan 2021 17:08

Instrument :
MSVOA_D
ClientSampleId :
400026

Tgt Ion:114 Resp: 892449




Ion	Ratio	Lower	Upper
114	100		
63	19.9	0.0	34.8
88	16.4	0.0	31.6

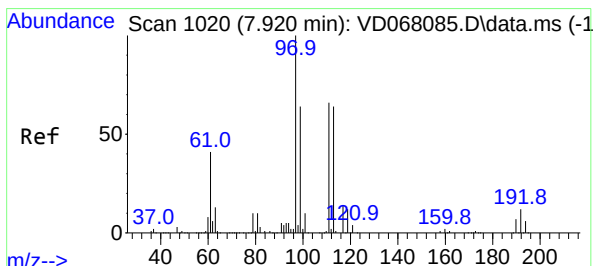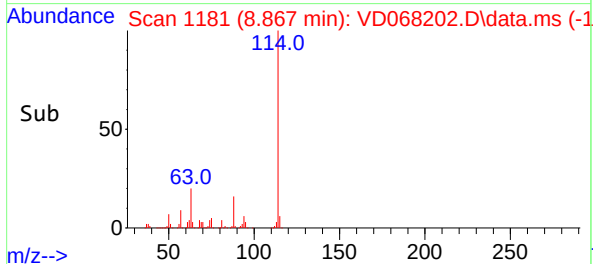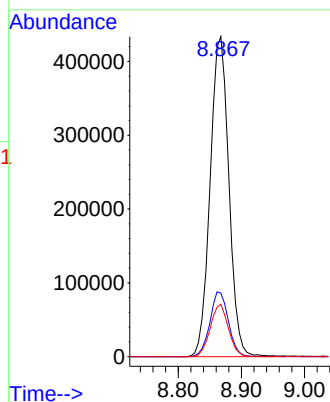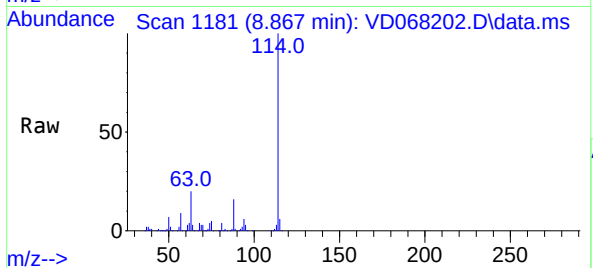


#35
Dibromofluoromethane
Concen: 54.97 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. 0.000 min
Lab File: VD068202.D
Acq: 27 Jan 2021 17:08

Tgt Ion:113 Resp: 271211

Ion	Ratio	Lower	Upper
113	100		
111	103.5	81.4	122.0
192	18.5	16.1	24.1


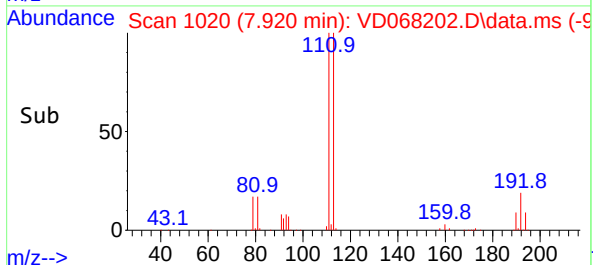
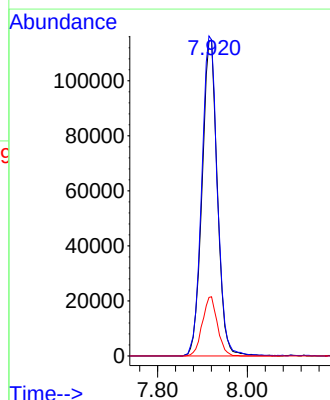
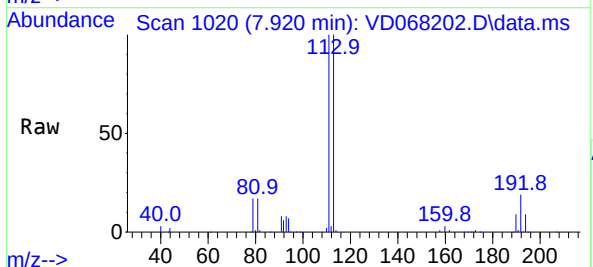


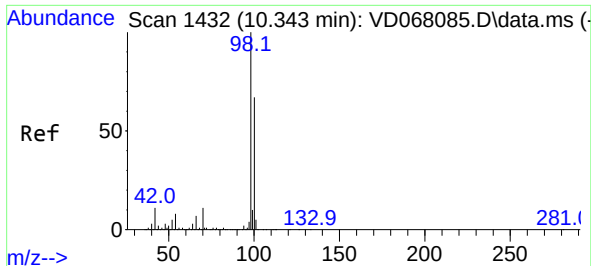

#50
Toluene-d8
Concen: 55.90 ug/l
RT: 10.344 min Scan# 1432
Delta R.T. 0.000 min
Lab File: VD068202.D
Acq: 27 Jan 2021 17:08




Instrument :
MSVOA_D
ClientSampleId :
400026


Tgt Ion: 98 Resp: 1103158
Ion Ratio Lower Upper
98 100
100 64.2 53.0 79.4

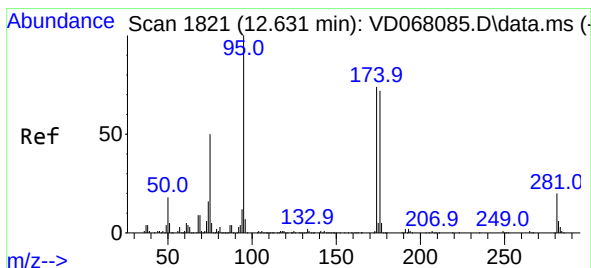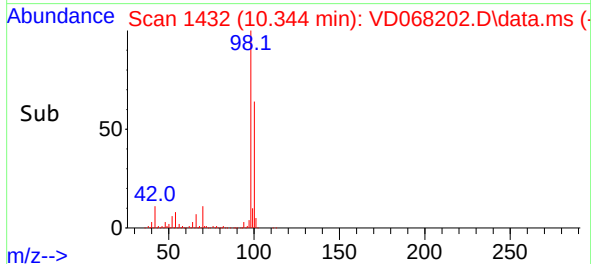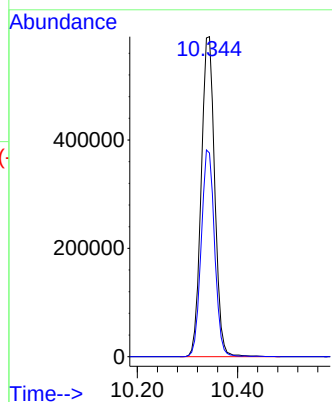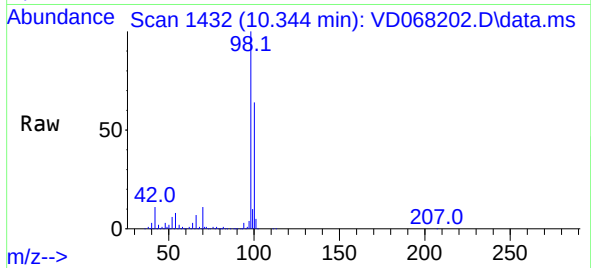

#62
4-Bromofluorobenzene
Concen: 48.51 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.000 min
Lab File: VD068202.D
Acq: 27 Jan 2021 17:08

Tgt Ion: 95 Resp: 344784
Ion Ratio Lower Upper
95 100
174 76.1 0.0 172.4
176 74.3 0.0 168.4


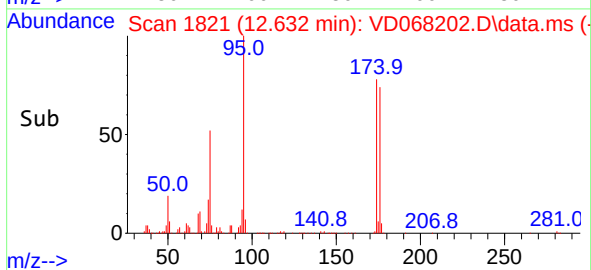
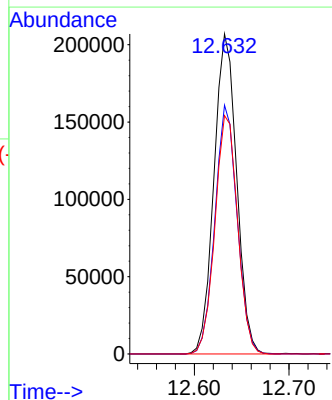
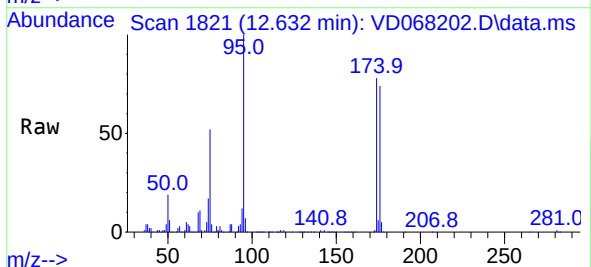


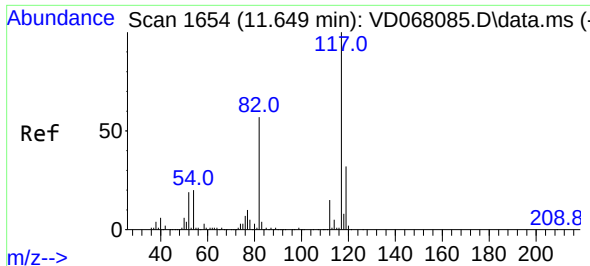

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.649 min Scan# 1654
Delta R.T. 0.000 min
Lab File: VD068202.D
Acq: 27 Jan 2021 17:08

Instrument :
MSVOA_D
ClientSampleId :
400026

Tgt Ion:117 Resp: 780570
Ion Ratio Lower Upper
117 100
82 54.4 41.4 62.0
119 31.0 26.1 39.1

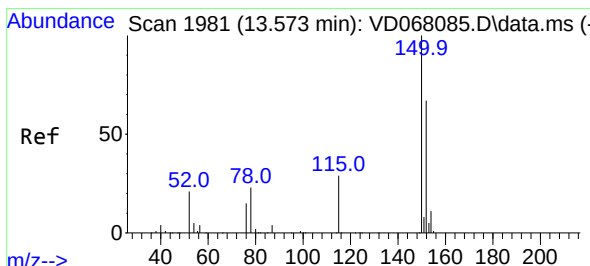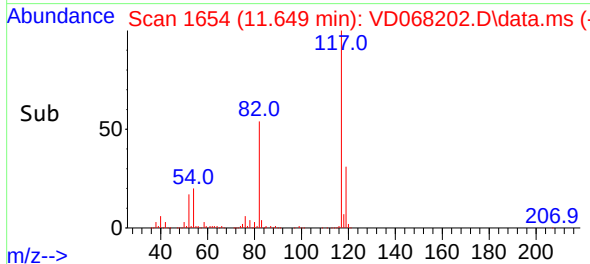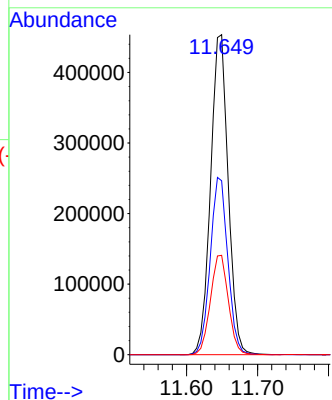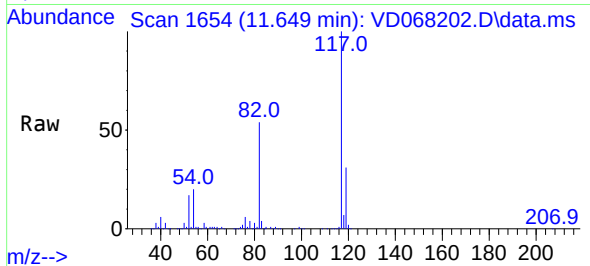

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.000 min
Lab File: VD068202.D
Acq: 27 Jan 2021 17:08

Tgt Ion:152 Resp: 311457
Ion Ratio Lower Upper
152 100
115 60.9 28.9 86.8
150 159.1 0.0 344.4

