

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012723\
 Data File : VD075224.D
 Acq On : 27 Jan 2023 14:32
 Operator : KP/SY
 Sample : 01293-01
 Misc : 5.07G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 PL-3-012523

Quant Time: Jan 30 01:03:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011823S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 19 01:32:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	1885	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.781	114	3688	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	3642	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	1427	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	1590	82.662	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	165.320%#
35) Dibromofluoromethane	7.805	113	1082	48.552	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.100%
50) Toluene-d8	10.269	98	4277	48.743	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	97.480%
62) 4-Bromofluorobenzene	12.575	95	1385	49.734	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	99.460%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012723\
Data File : VD075224.D
Acq On : 27 Jan 2023 14:32
Operator : KP/SY
Sample : 01293-01
Misc : 5.07G/5.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
PL-3-012523

Quant Time: Jan 30 01:03:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011823S.M
Quant Title : SW846 8260
QLast Update : Thu Jan 19 01:32:27 2023
Response via : Initial Calibration




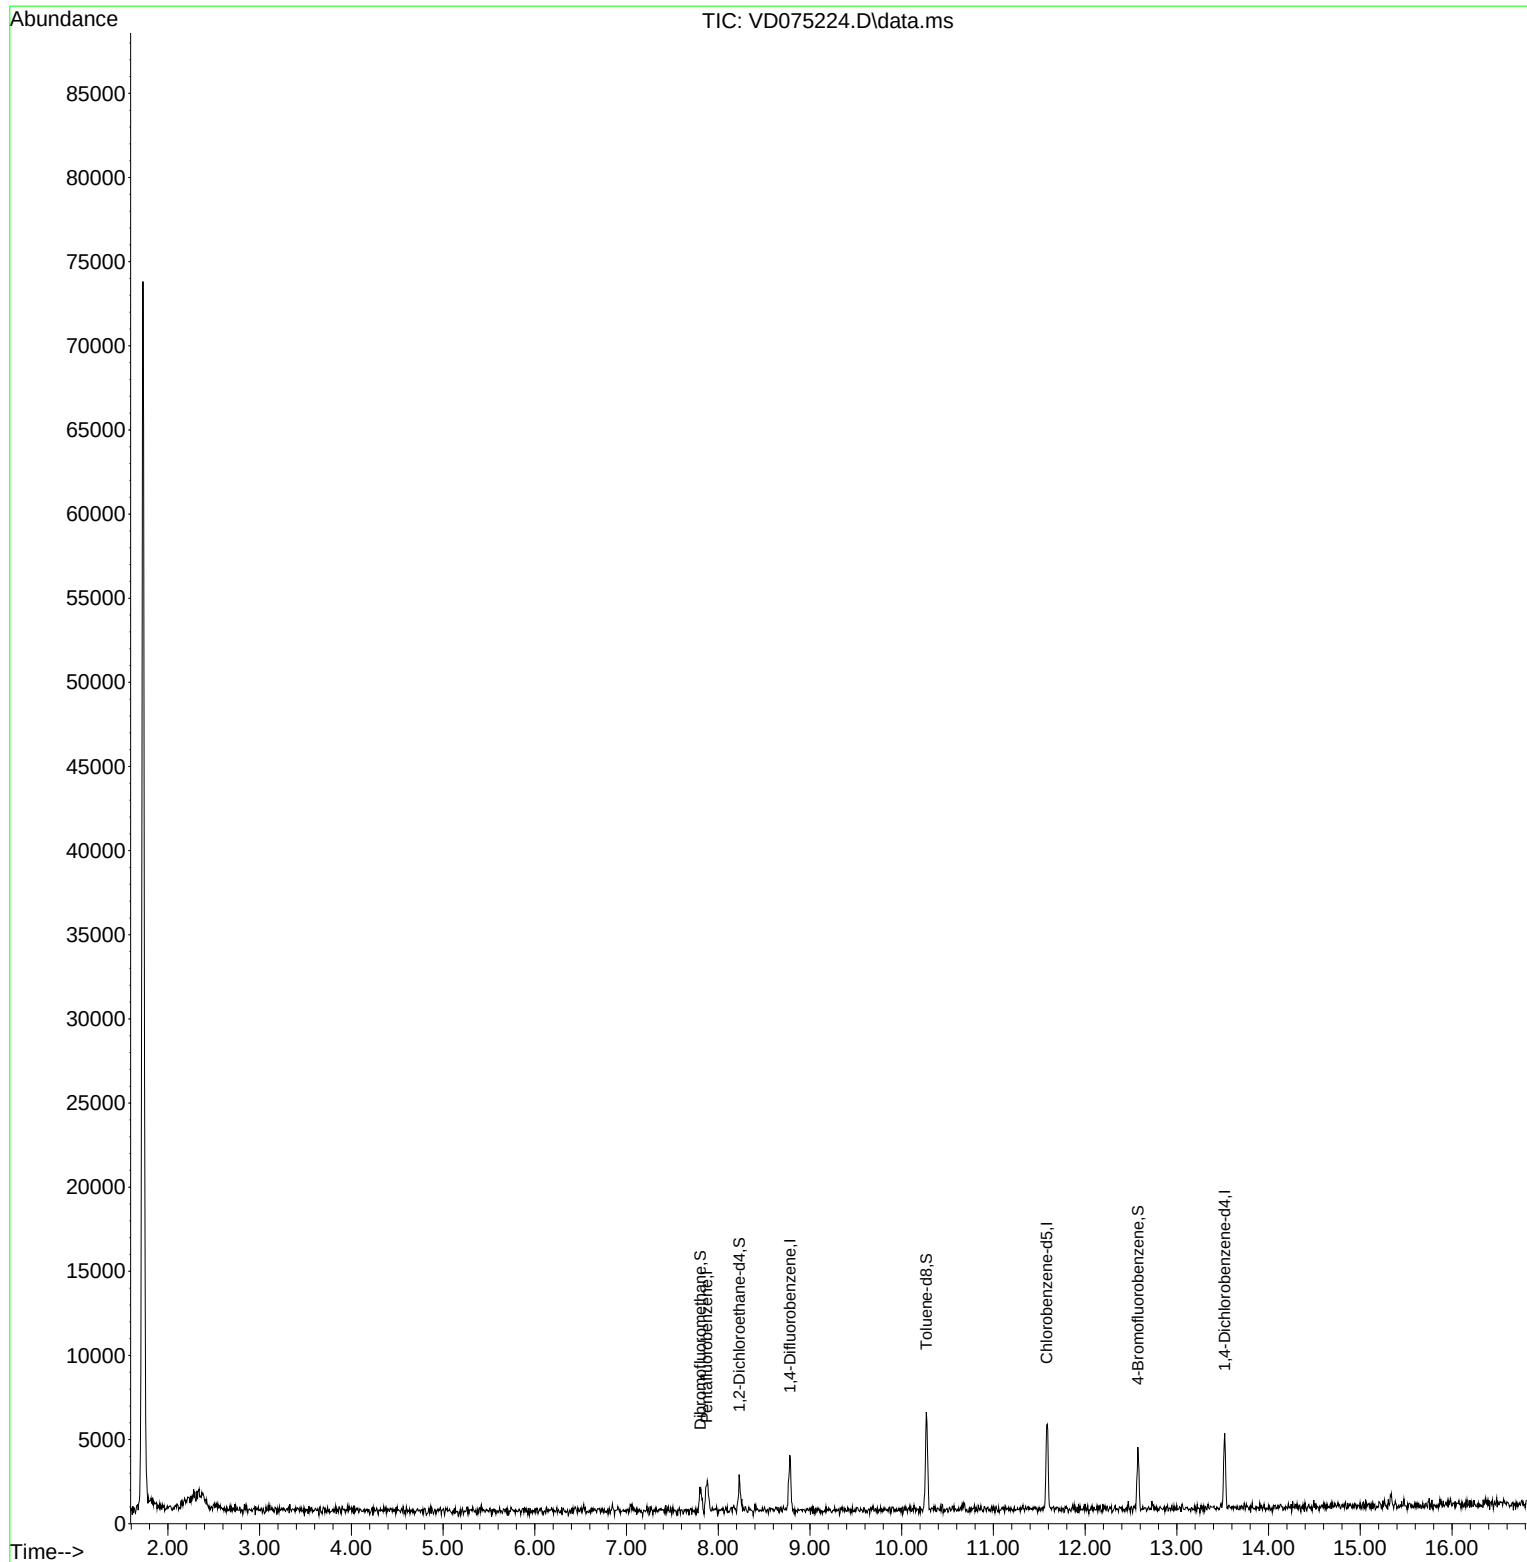


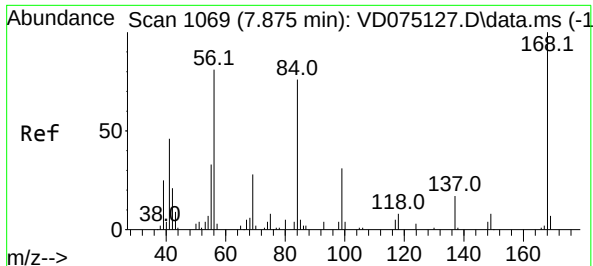

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD075224.D
Acq: 27 Jan 2023 14:32




Instrument :
MSVOA_D
ClientSampleId :
PL-3-012523


Tgt Ion:168 Resp: 1885
Ion Ratio Lower Upper
168 100
99 42.4 45.2 67.8#

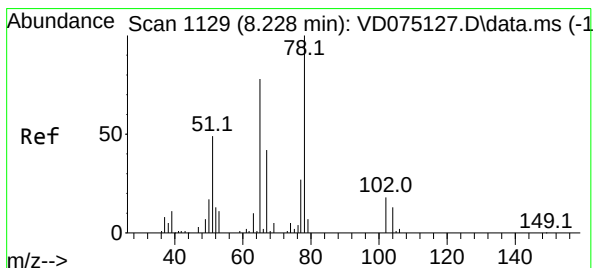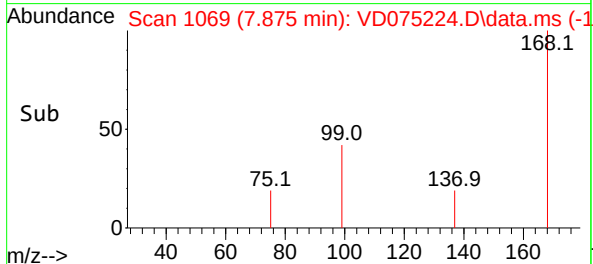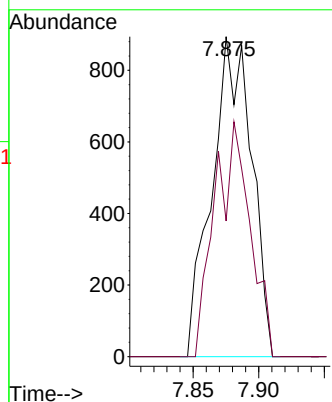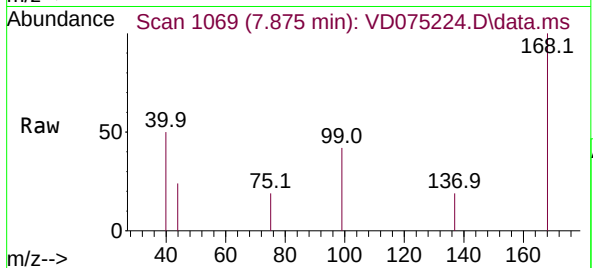

#33
1,2-Dichloroethane-d4
Concen: 82.662 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD075224.D
Acq: 27 Jan 2023 14:32

Tgt Ion: 65 Resp: 1590
Ion Ratio Lower Upper
65 100
67 50.3 0.0 105.2

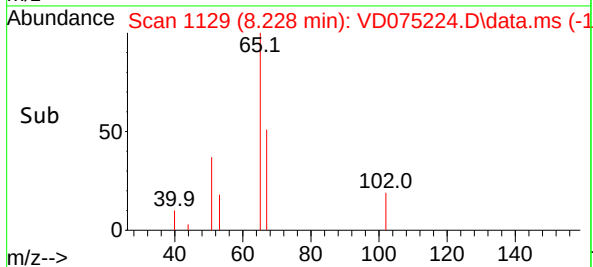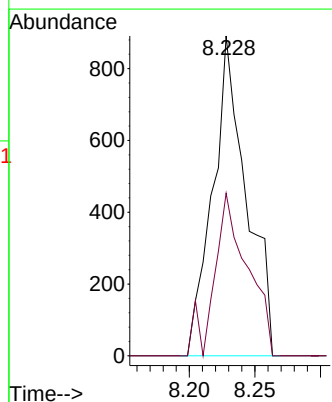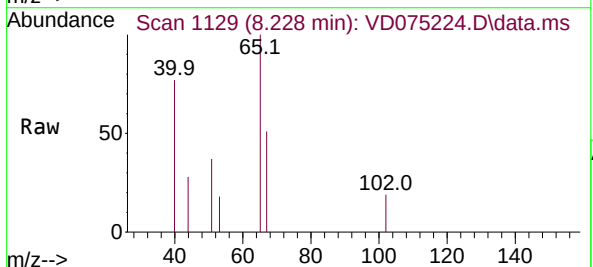

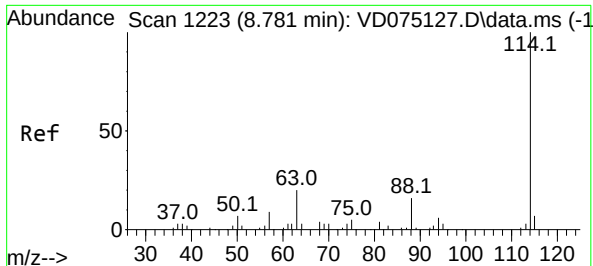

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 1

Delta R.T. -0.000 min

Lab File: VD075224.D

Acq: 27 Jan 2023 14:32

Instrument :

MSVOA_D

ClientSampleId :

PL-3-012523





Tgt Ion:114 Resp: 3688

Ion Ratio Lower Upper

114 100

63 25.4 0.0 40.2

88 14.2 0.0 32.2

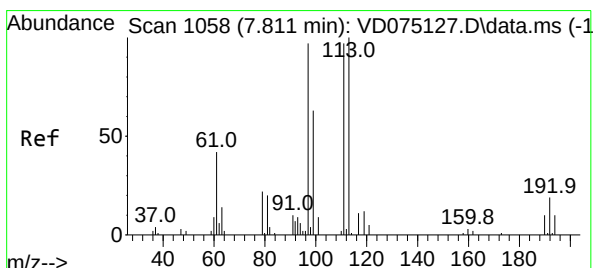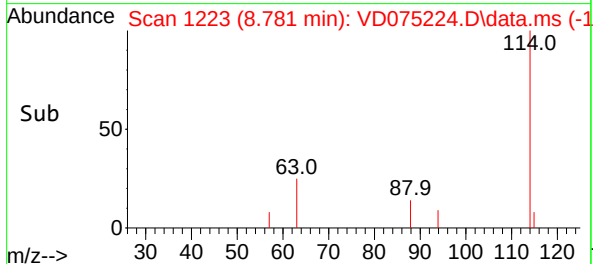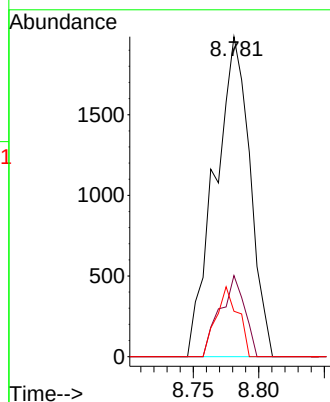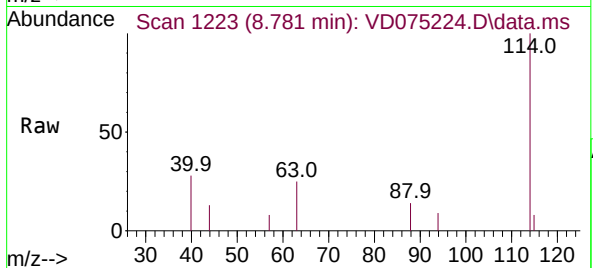

#35

Dibromofluoromethane

Concen: 48.552 ug/l

RT: 7.805 min Scan# 1057

Delta R.T. -0.006 min

Lab File: VD075224.D

Acq: 27 Jan 2023 14:32




Tgt Ion:113 Resp: 1082


Ion Ratio Lower Upper

113 100

111 108.1 80.1 120.1

192 5.0 15.4 23.0#


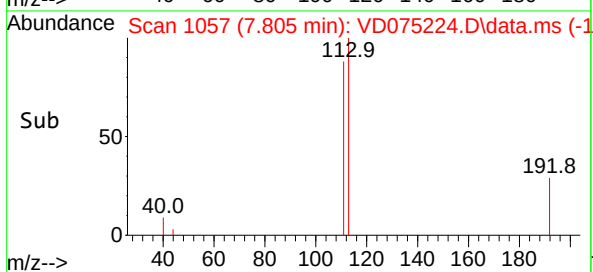
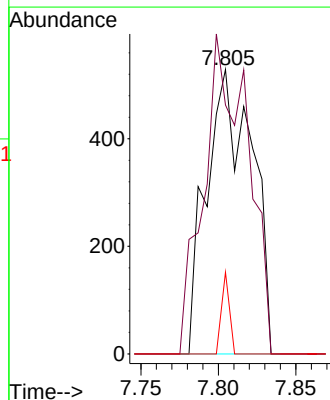
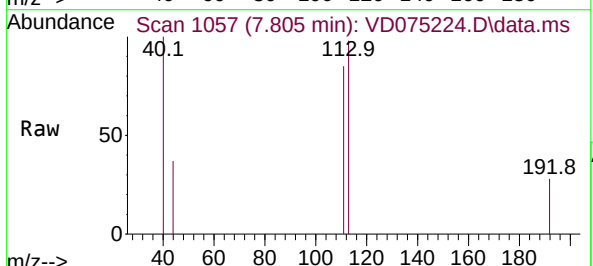


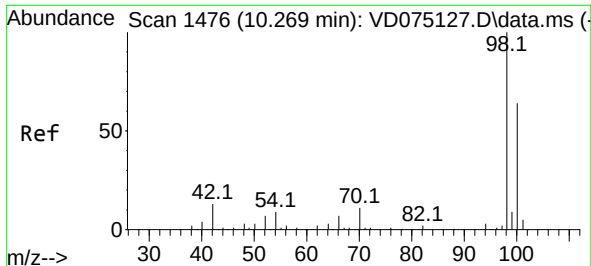

#50
Toluene-d8
Concen: 48.743 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD075224.D
Acq: 27 Jan 2023 14:32




Instrument :
MSVOA_D
ClientSampleId :
PL-3-012523


Tgt Ion: 98 Resp: 4277
Ion Ratio Lower Upper
98 100
100 69.2 52.7 79.1

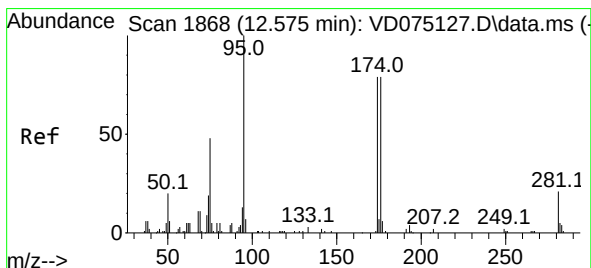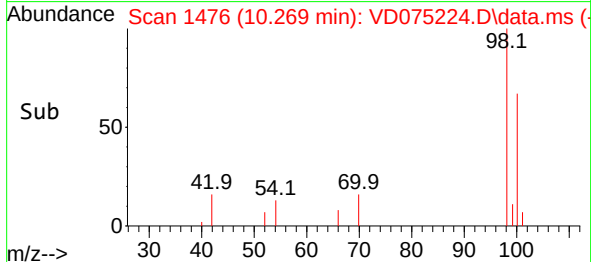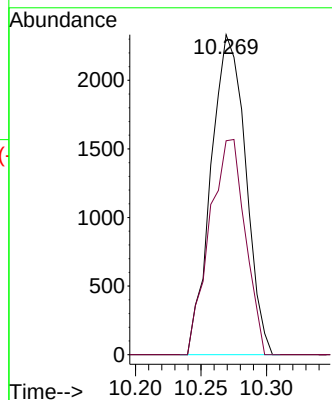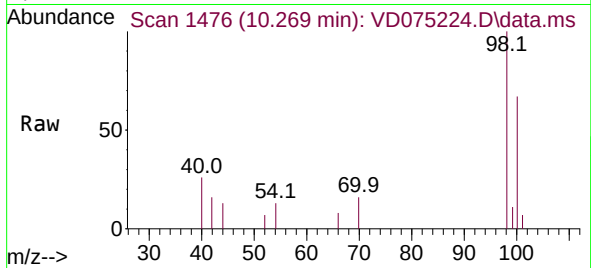

#62
4-Bromofluorobenzene
Concen: 49.734 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD075224.D
Acq: 27 Jan 2023 14:32

Tgt Ion: 95 Resp: 1385
Ion Ratio Lower Upper
95 100
174 81.9 0.0 161.2
176 79.2 0.0 160.2


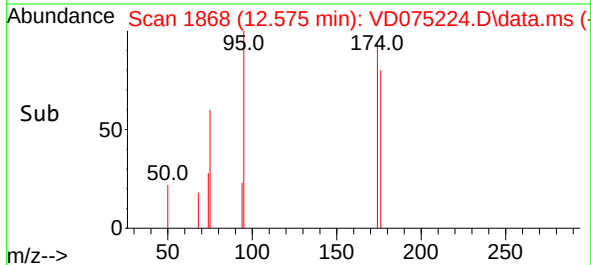
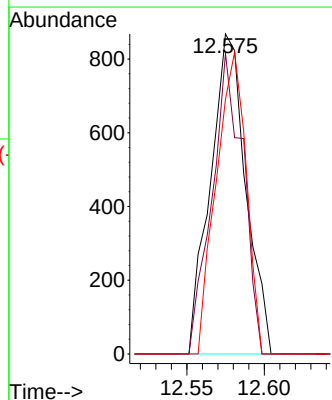
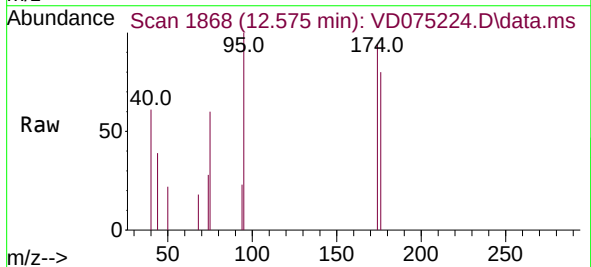


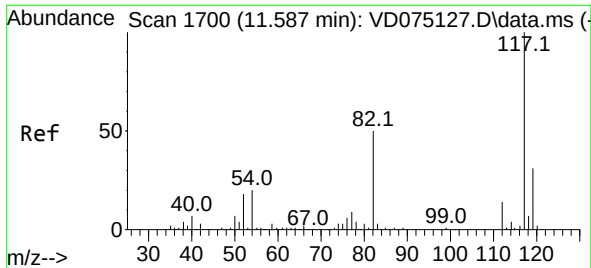

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1699
Delta R.T. -0.006 min
Lab File: VD075224.D
Acq: 27 Jan 2023 14:32

Instrument :
MSVOA_D
ClientSampleId :
PL-3-012523

Tgt Ion:117 Resp: 3642
Ion Ratio Lower Upper
117 100
82 45.5 39.6 59.4
119 24.8 24.6 37.0

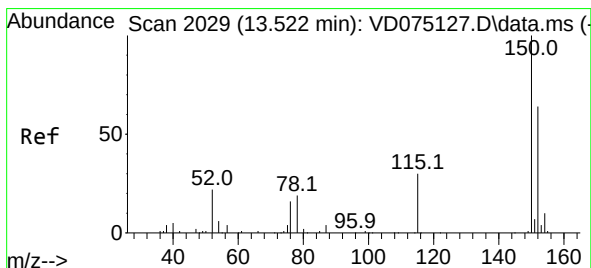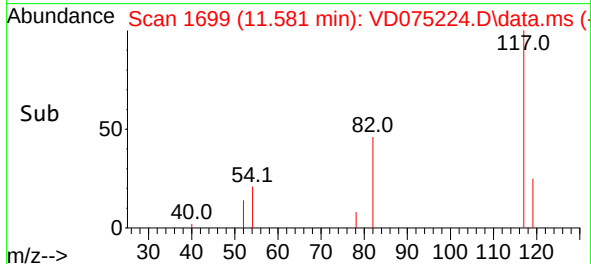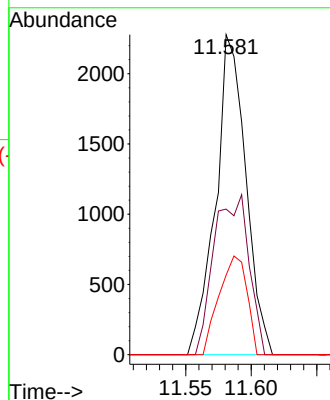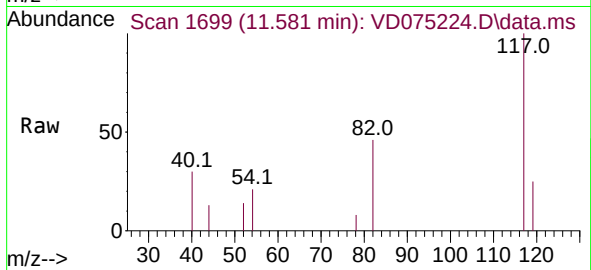

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. -0.000 min
Lab File: VD075224.D
Acq: 27 Jan 2023 14:32

Tgt Ion:152 Resp: 1427
Ion Ratio Lower Upper
152 100
115 48.2 28.8 86.4
150 148.1 0.0 348.6

