


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD013019\
Data File : VD060798.D
Acq On : 30 Jan 2019 10:16
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D012819S.M
Title : SW846 8260
Last Update : Tue Jan 29 13:53:55 2019

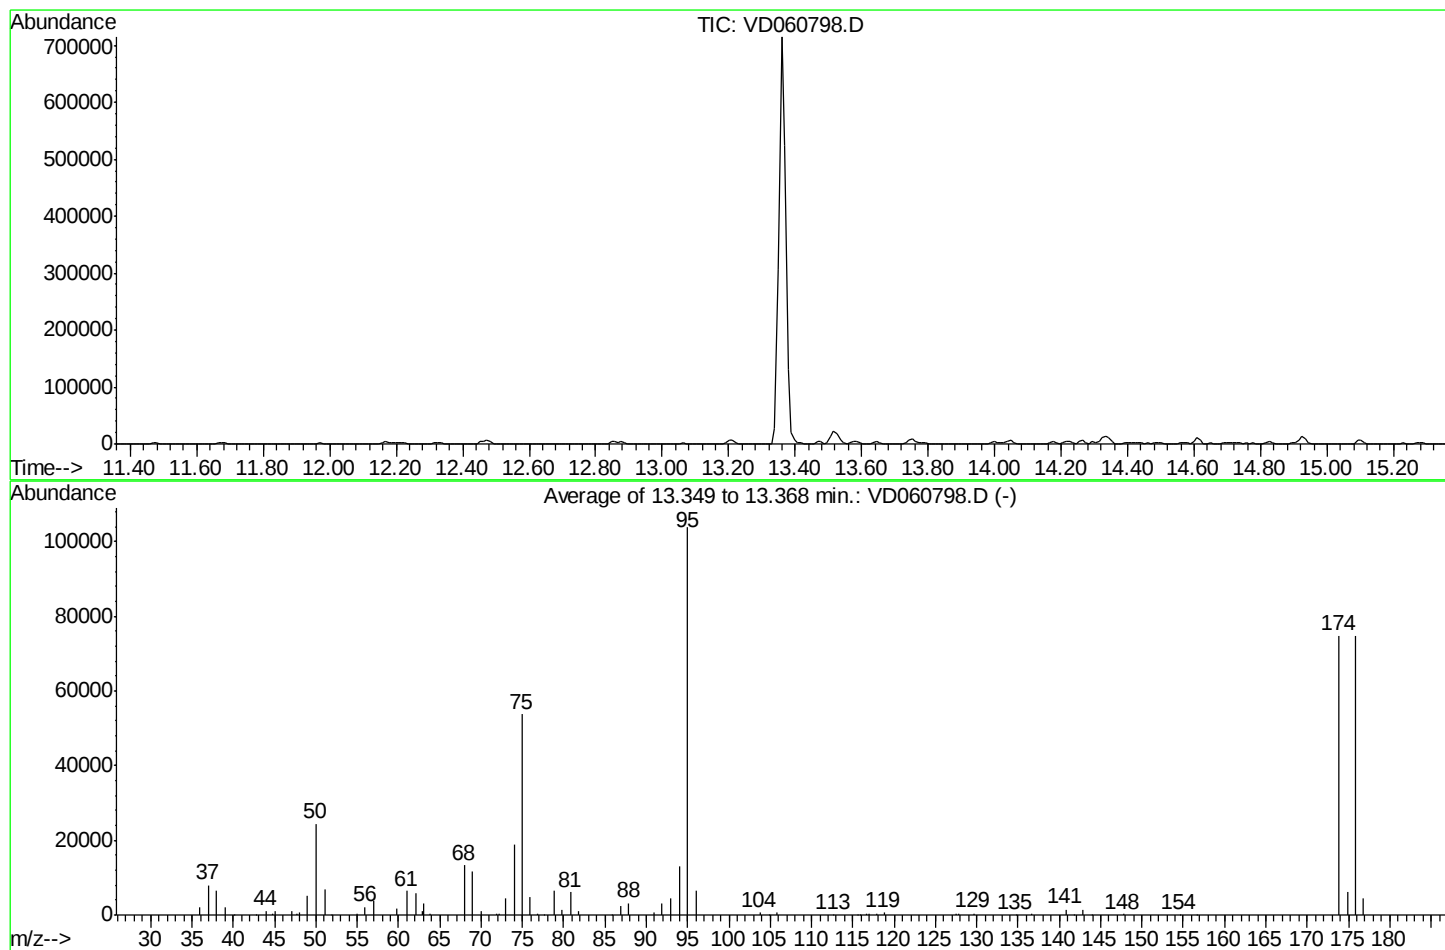

AutoFind: Scans 1252, 1253, 1254; Background Corrected with Scan 1248

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	24501	PASS
75	95	30	60	51.8	53805	PASS
95	95	100	100	100.0	103808	PASS
96	95	5	9	6.3	6500	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.0	74757	PASS
175	174	5	9	8.2	6131	PASS
176	174	95	101	99.9	74672	PASS
177	176	5	9	6.1	4586	PASS