
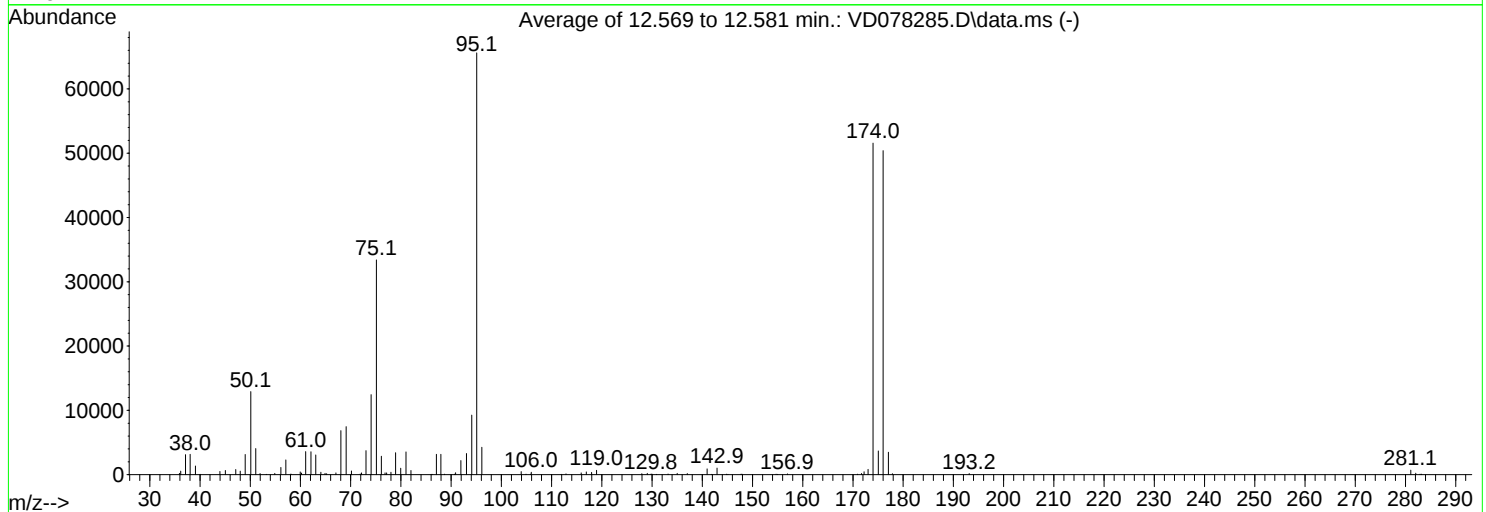


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD013124\
Data File : VD078285.D
Acq On : 31 Jan 2024 08:53
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D013024S.M
Title : SW846 8260
Last Update : Thu Feb 01 03:58:19 2024

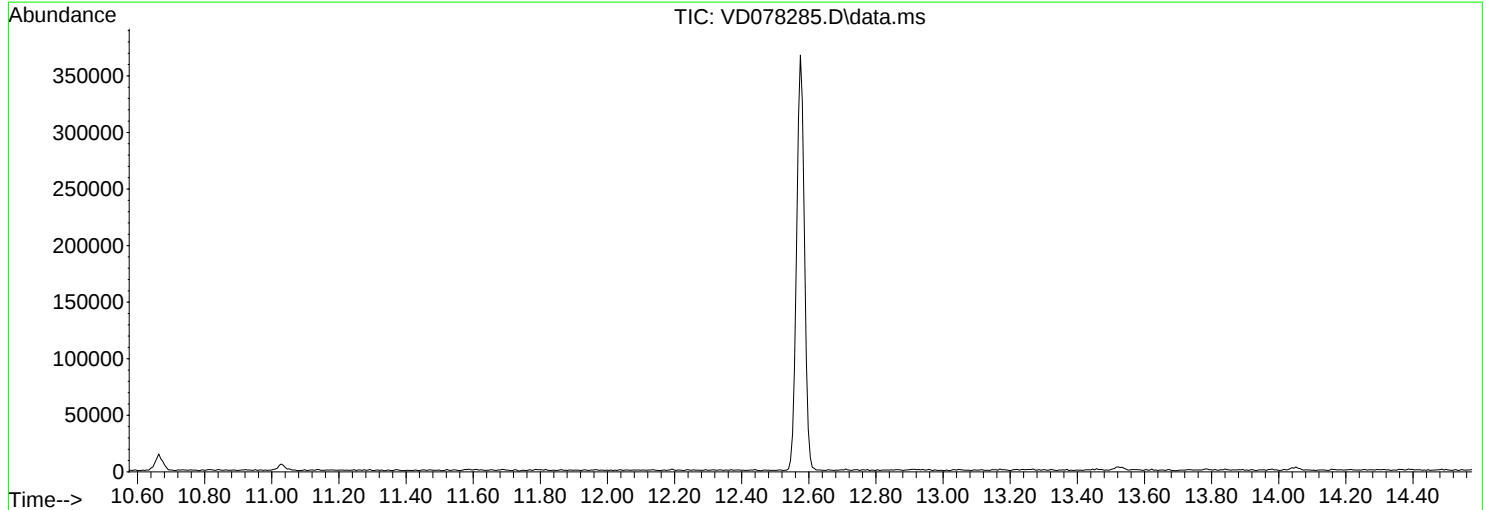

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	12926	PASS
75	95	30	60	50.9	33413	PASS
95	95	100	100	100.0	65613	PASS
96	95	5	9	6.5	4263	PASS
173	174	0.00	2	1.6	830	PASS
174	95	50	100	78.6	51581	PASS
175	174	5	9	7.1	3676	PASS
176	174	95	101	97.7	50392	PASS
177	176	5	9	6.9	3479	PASS