




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020124\
Data File : VD078305.D
Acq On : 01 Feb 2024 15:23
Operator : RP/MD
Sample : P1329-07
Misc : 5.75G/10ml/MSVOA_D/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0FL6

Manual IntegrationsAPPROVED

Quant Time: Feb 02 00:39:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 02 00:36:57 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/06/2024
Supervised By :Mahesh Dadoda 02/06/2024

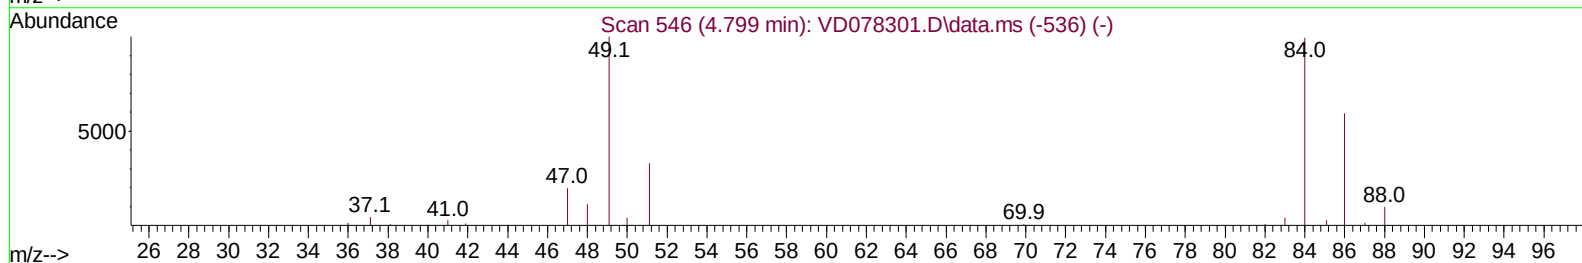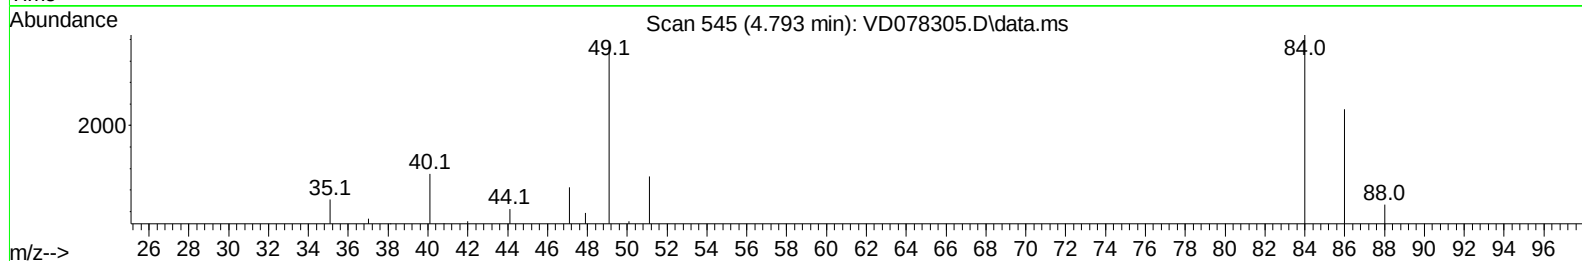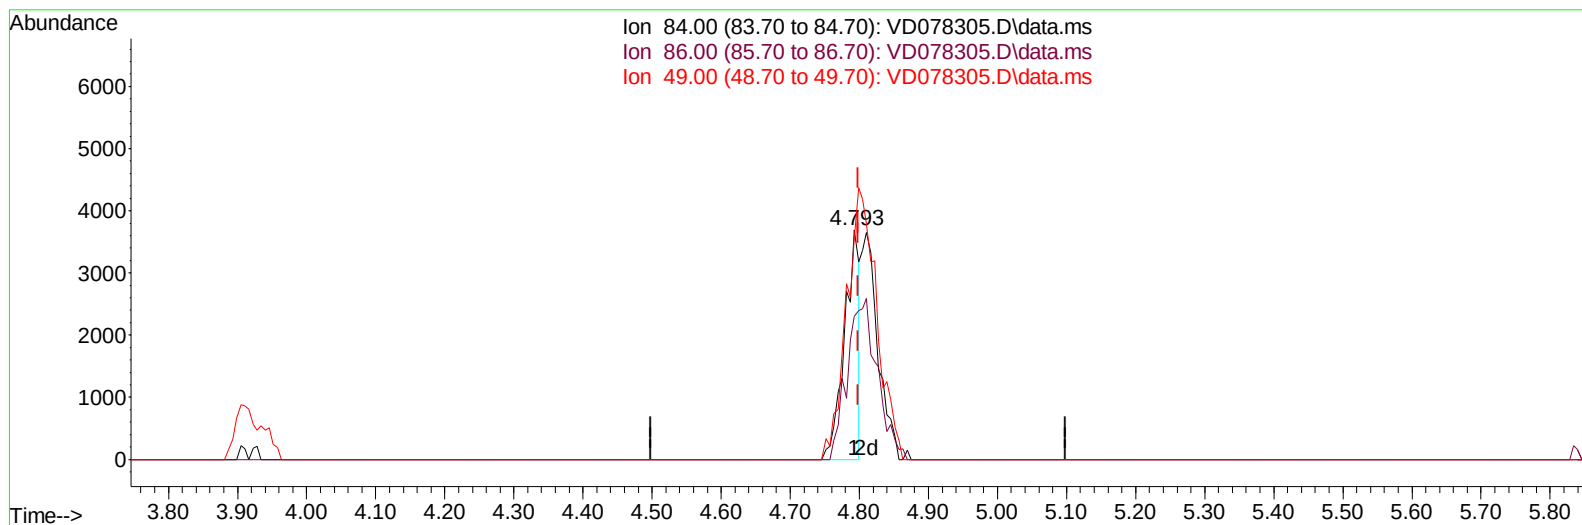

TIC: VD078305.D\data.ms

(16) Methylene chloride (T)

4.793min (-0.006) 1.83 ug/L

response 5438

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.80	62.33
49.00	110.50	96.12
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020124\
 Data File : VD078305.D
 Acq On : 01 Feb 2024 15:23
 Operator : RP/MD
 Sample : P1329-07
 Misc : 5.75G/10ml/MSVOA_D/SOIL/A
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0FL6

Manual IntegrationsAPPROVED

Quant Time: Feb 02 00:39:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Feb 02 00:36:57 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/06/2024
 Supervised By :Mahesh Dadoda 02/06/2024

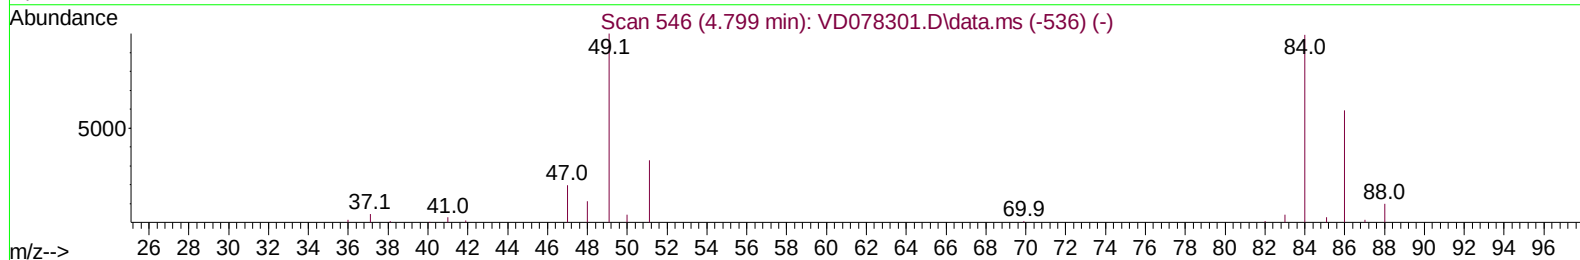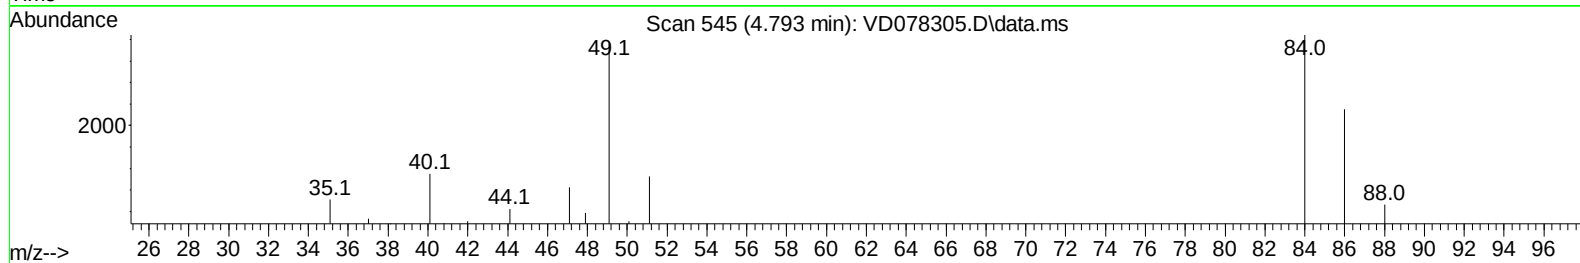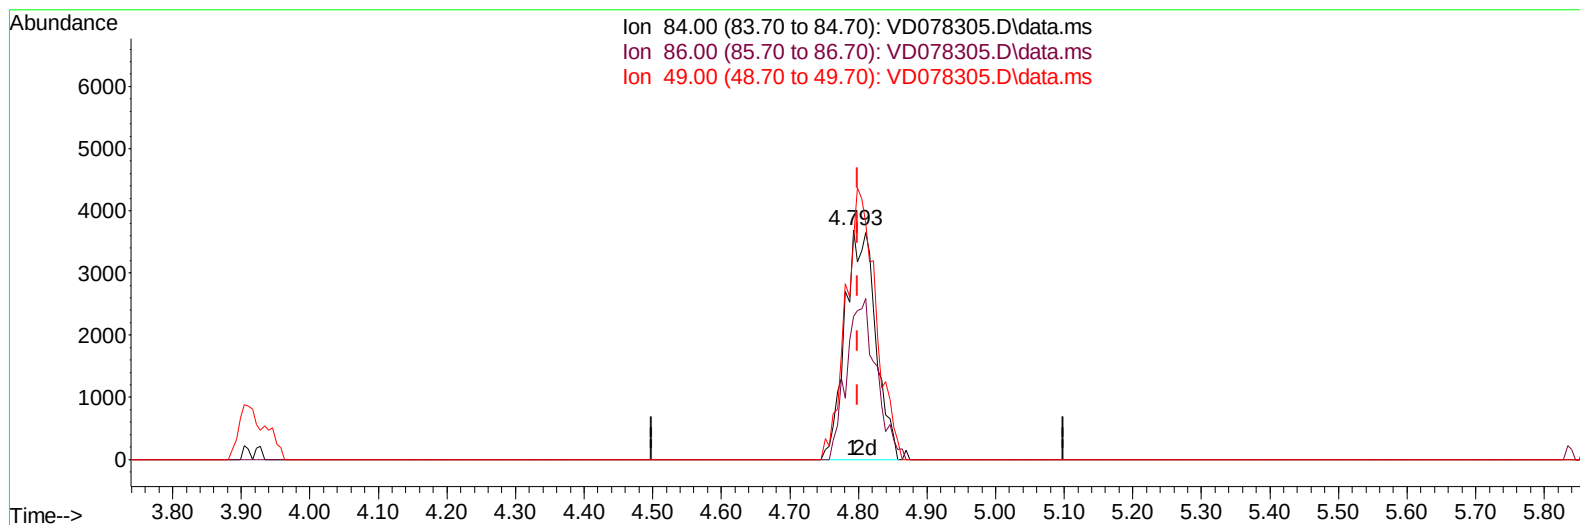

TIC: VD078305.D\data.ms

(16) Methylene chloride (T)

4.793min (-0.006) 3.86 ug/L m

response 11512

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.80	62.33
49.00	110.50	96.12
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020124\
 Data File : VD078305.D
 Acq On : 01 Feb 2024 15:23
 Operator : RP/MD
 Sample : P1329-07
 Misc : 5.75G/10mL/MSVOA_D/SOIL/A
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0FL6

Manual IntegrationsAPPROVED

Quant Time: Feb 02 00:39:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Feb 02 00:36:57 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/06/2024
 Supervised By :Mahesh Dadoda 02/06/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		151887	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		148639	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		56870	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.275	65		114067	26.470	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	105.880%	
7) Chloroethane-d5	2.805	69		88977	24.564	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	98.240%	
11) 1,1-Dichloroethene-d2	3.910	65		24877	26.737	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	106.960%	
21) 2-Butanone-d5	6.993	46		34337	54.119	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	108.240%	
24) Chloroform-d	7.563	84		101239	23.378	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	93.520%	
26) 1,2-Dichloroethane-d4	8.234	65		57680	24.681	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	98.720%	
32) Benzene-d6	8.204	84		213816	24.601	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	98.400%	
36) 1,2-Dichloropropane-d6	9.216	67		64391	24.065	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	96.280%	
41) Toluene-d8	10.269	98		183462	23.501	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	94.000%	
43) trans-1,3-Dichloroprop...	10.522	79		28985	24.261	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	97.040%	
47) 2-Hexanone-d5	10.875	63		29290	53.954	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	107.900%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		63461	25.524	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	102.080%	
66) 1,2-Dichlorobenzene-d4	13.816	152		54188	26.615	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	106.480%	
Target Compounds							
16) Methylene chloride	4.793	84		11512m	3.865	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020124\
Data File : VD078305.D
Acq On : 01 Feb 2024 15:23
Operator : RP/MD
Sample : P1329-07
Misc : 5.75G/10ml/MSVOA_D/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0FL6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/06/2024
Supervised By :Mahesh Dadoda 02/06/2024

Quant Time: Feb 02 00:39:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 02 00:36:57 2024
Response via : Initial Calibration

