




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020124\
Data File : VD078307.D
Acq On : 01 Feb 2024 16:14
Operator : RP/MD
Sample : P1329-05
Misc : 4.58G/10ml/MSVOA_D/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0FL3

Manual IntegrationsAPPROVED

Quant Time: Feb 02 00:40:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 02 00:36:57 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/06/2024
Supervised By :Mahesh Dadoda 02/06/2024

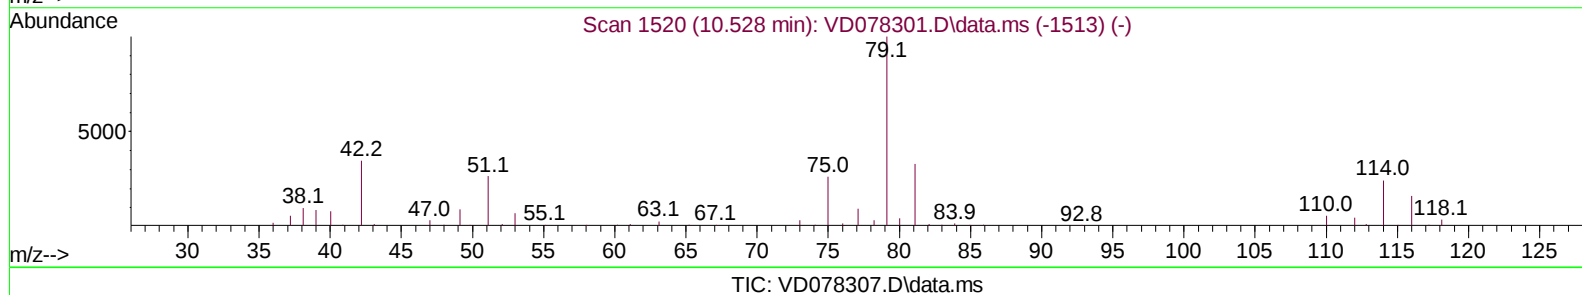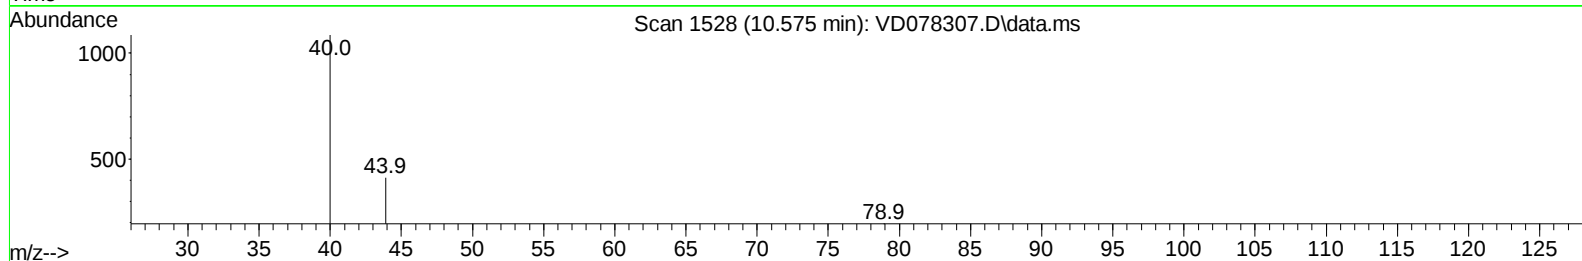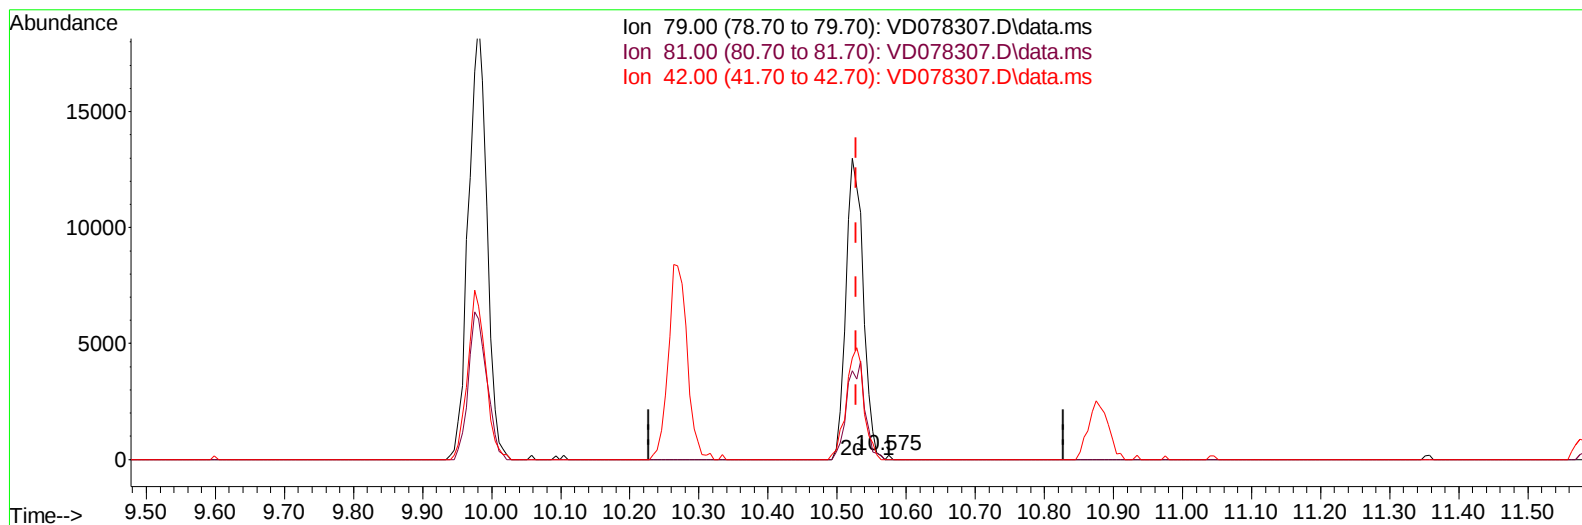

(43) trans-1,3-Dichloropropene-d4 (S)

10.575min (+ 0.047) 0.20 ug/L

response 68

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	30.90	3752.94#
42.00	35.10	12664.71#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020124\
Data File : VD078307.D
Acq On : 01 Feb 2024 16:14
Operator : RP/MD
Sample : P1329-05
Misc : 4.58G/10ml/MSVOA_D/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0FL3

Manual IntegrationsAPPROVED

Quant Time: Feb 02 00:40:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 02 00:36:57 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/06/2024
Supervised By :Mahesh Dadoda 02/06/2024

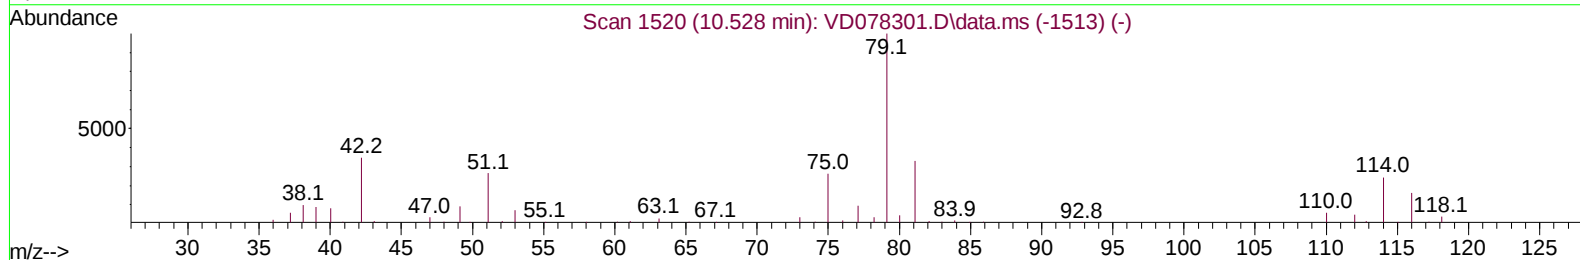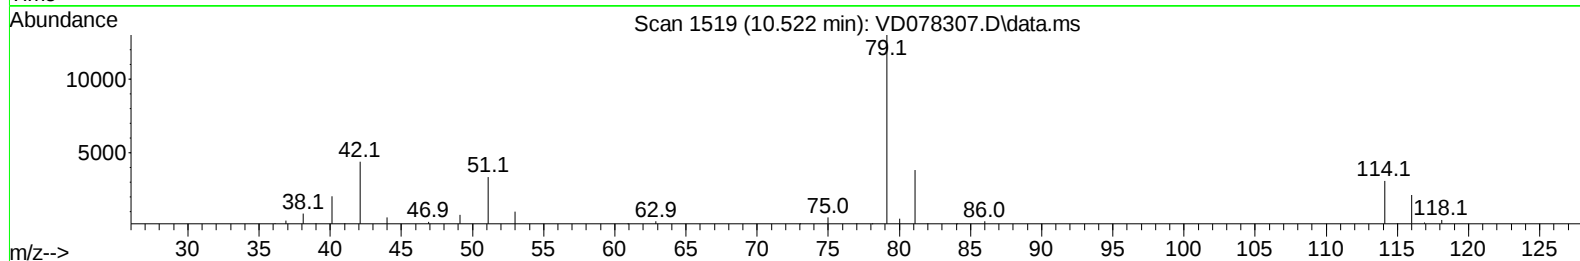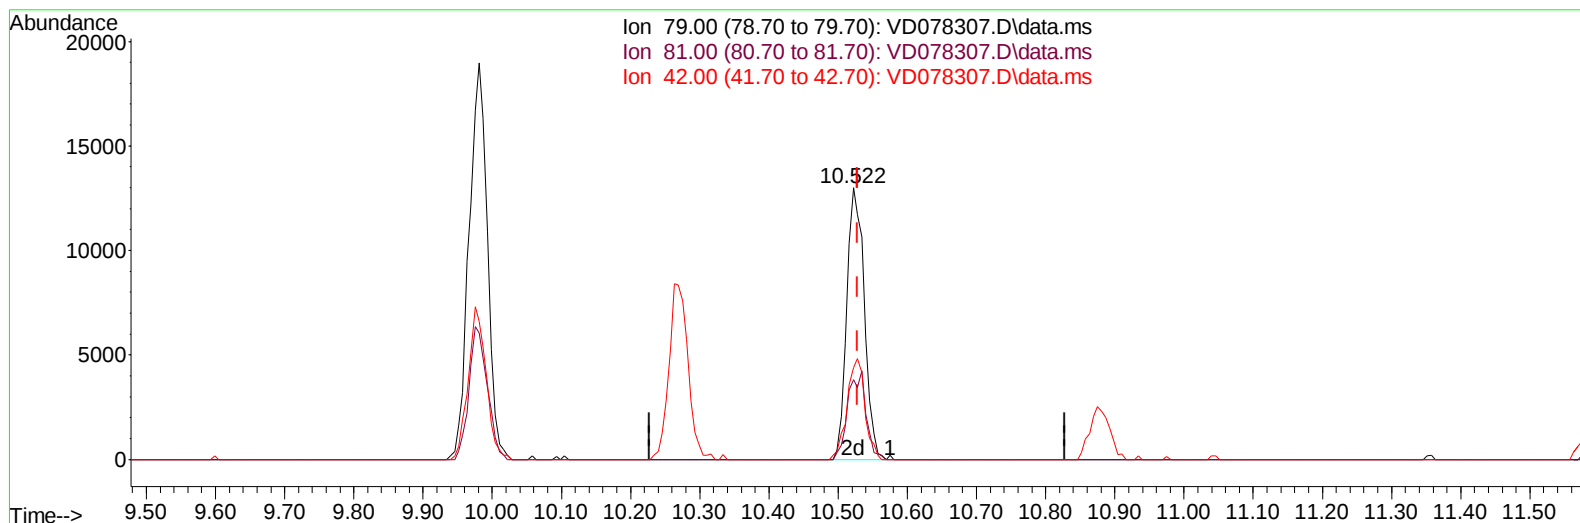

TIC: VD078307.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

10.522min (-0.006) 66.96 ug/L m

response 22600

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	30.90	11.29#
42.00	35.10	38.11
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020124\
 Data File : VD078307.D
 Acq On : 01 Feb 2024 16:14
 Operator : RP/MD
 Sample : P1329-05
 Misc : 4.58G/10ml/MSVOA_D/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0FL3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/06/2024
 Supervised By :Mahesh Dadoda 02/06/2024

Quant Time: Feb 02 00:40:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Feb 02 00:36:57 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.775	114		43989	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		41991	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152		15950	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.276	65		92308	73.963	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	= 295.840%#		
7) Chloroethane-d5	2.799	69		75504	71.972	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	= 287.880%#		
11) 1,1-Dichloroethene-d2	3.923	65		18547	68.827	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	= 275.320%#		
21) 2-Butanone-d5	6.993	46		41708	226.980	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	= 453.960%#		
24) Chloroform-d	7.569	84		78226	62.371	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	= 249.480%#		
26) 1,2-Dichloroethane-d4	8.234	65		48549	71.728	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	= 286.920%#		
32) Benzene-d6	8.205	84		169200	68.912	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	= 275.640%#		
36) 1,2-Dichloropropane-d6	9.210	67		50638	66.991	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	= 267.960%#		
41) Toluene-d8	10.269	98		140163	63.556	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	= 254.240%#		
43) trans-1,3-Dichloroprop...	10.522	79		22600m	66.960	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	= 267.840%#		
47) 2-Hexanone-d5	10.881	63		32154	209.660	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	= 419.320%#		
56) 1,1,2,2-Tetrachloroeth...	12.651	84		58484	83.264	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	= 333.040%#		
66) 1,2-Dichlorobenzene-d4	13.816	152		37680	65.988	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	= 263.960%#		
Target Compounds							Qvalue
16) Methylene chloride	4.805	84		7977	9.247	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020124\
Data File : VD078307.D
Acq On : 01 Feb 2024 16:14
Operator : RP/MD
Sample : P1329-05
Misc : 4.58G/10ml/MSVOA_D/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0FL3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/06/2024
Supervised By :Mahesh Dadoda 02/06/2024

Quant Time: Feb 02 00:40:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 02 00:36:57 2024
Response via : Initial Calibration

