
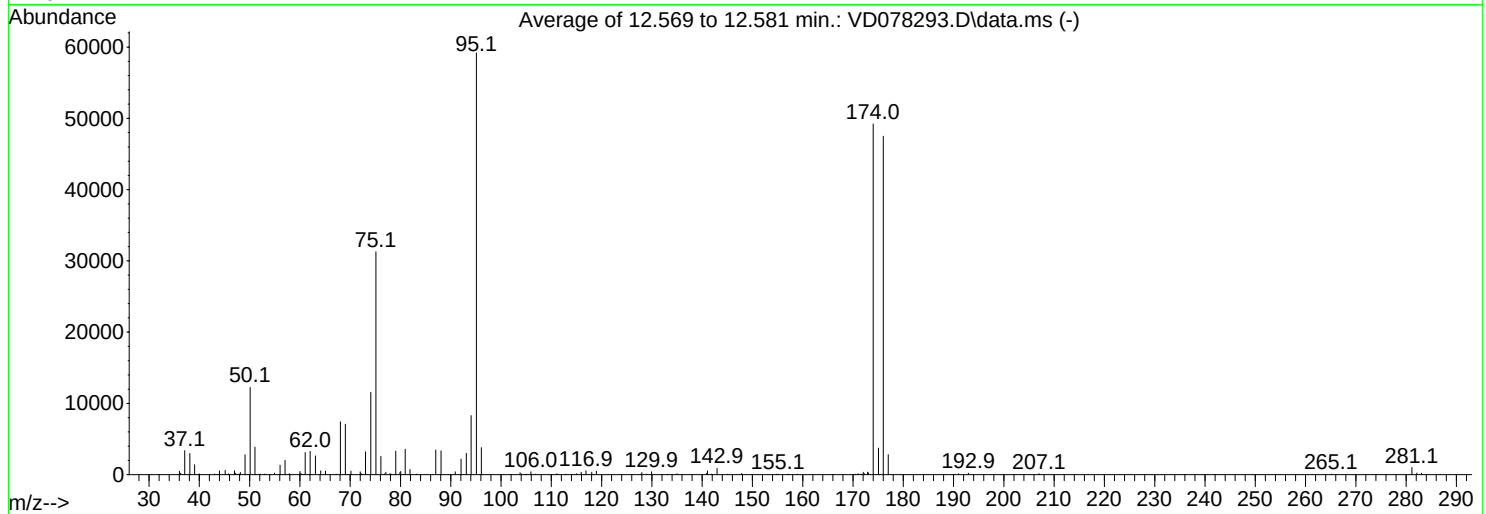


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD078293\
Data File : VD078293.D
Acq On : 31 Jan 2024 15:47
Operator : RP/MD
Sample : BFB198
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB198

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Title : SFAM01.0
Last Update : Tue Feb 06 00:51:05 2024

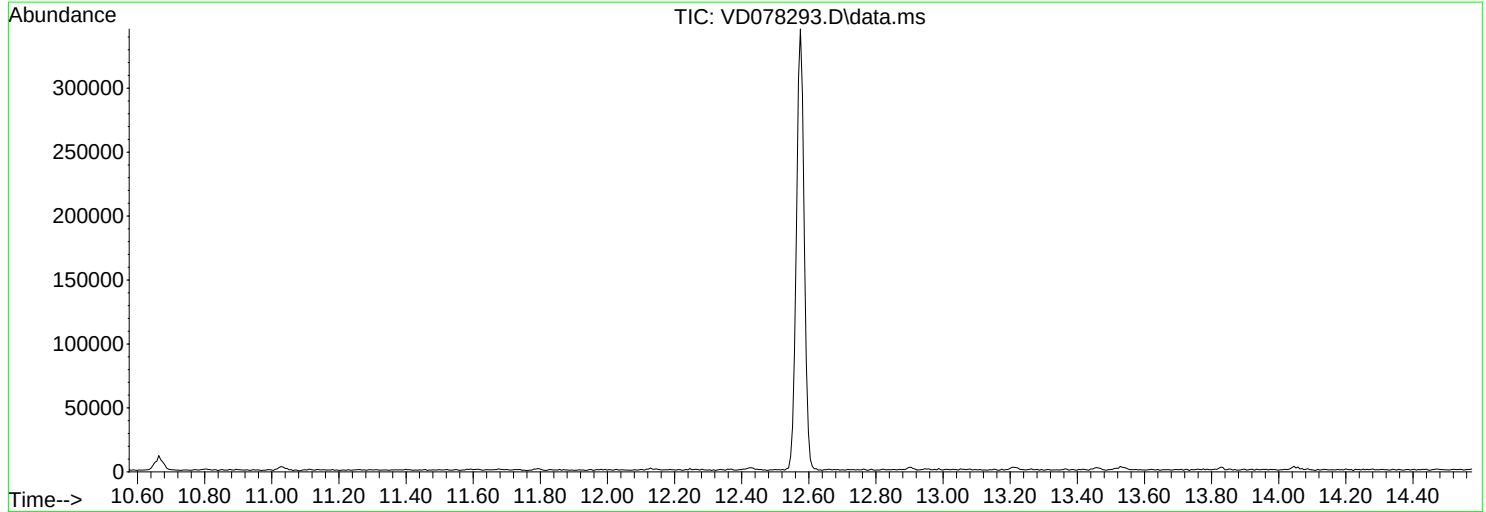

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	12240	PASS
75	95	30	80	52.8	31283	PASS
95	95	100	100	100.0	59197	PASS
96	95	5	9	6.4	3787	PASS
173	174	0.00	2	0.8	370	PASS
174	95	50	120	83.1	49219	PASS
175	174	5	9	7.6	3727	PASS
176	174	95	105	96.5	47499	PASS
177	176	5	10	5.9	2803	PASS

Scan 1860 (12.528 min): VD078293.D\data.ms
BFB198

m/z	Abundance
40.00	989.0
44.00	429.0

Instrument :
MSVOA_D
ClientSampleId :
BFB198

m/z	Abundance
36.30	614.0
37.10	3346.0
38.10	2481.0
39.10	1463.0
40.10	1303.0
44.10	707.0
45.10	420.0
45.80	169.0
47.00	826.0
47.90	347.0
49.10	3052.0
50.10	12343.0
51.00	3439.0
51.90	222.0
54.90	243.0
56.10	1596.0
57.10	1299.0
57.90	241.0
60.10	662.0
61.10	2980.0
62.00	2926.0
63.10	2373.0
64.10	346.0
65.10	863.0
68.00	7384.0
69.10	7631.0
70.20	455.0
72.00	626.0
73.00	2748.0
74.10	11670.0
75.10	31160.0
76.10	2431.0
77.00	251.0
77.90	236.0
79.00	3181.0
79.90	855.0
80.90	3091.0
81.90	965.0
83.20	178.0
87.00	3975.0
88.20	3266.0
91.00	345.0
92.00	2182.0
93.10	2709.0
94.00	7859.0
95.10	58432.0
96.10	3833.0
103.80	407.0
104.80	151.0
106.00	419.0
111.10	169.0
115.00	188.0
116.10	178.0
116.90	505.0
118.10	334.0
119.00	407.0
125.90	156.0
127.80	175.0
129.90	322.0
135.00	260.0
140.90	524.0
143.00	769.0
147.90	309.0
154.80	210.0
157.10	192.0
171.10	189.0
171.60	243.0
172.30	425.0
172.90	660.0
174.00	46760.0
175.10	3463.0
176.00	45280.0
177.00	2772.0
193.00	212.0
206.90	231.0
281.30	623.0
282.20	246.0
283.00	170.0

Instrument :
MSVOA_D
ClientSampleId :
BFB198

m/z	Abundance
36.00	598.0
37.10	3263.0
38.10	3286.0
39.00	1275.0
40.00	847.0
44.00	1232.0
45.10	921.0
45.80	173.0
47.20	597.0
48.10	566.0
49.10	2847.0
50.10	13102.0
51.10	4366.0
53.00	300.0
55.00	435.0
56.00	1426.0
57.00	2277.0
59.90	716.0
61.00	3122.0
62.10	3787.0
63.10	2920.0
64.20	745.0
65.10	349.0
67.20	202.0
68.10	7727.0
69.00	7043.0
70.20	502.0
72.00	594.0
73.10	3727.0
74.10	12630.0
75.10	35184.0
76.10	2823.0
77.10	753.0
77.90	248.0
79.00	3914.0
80.10	721.0
81.00	4106.0
81.90	768.0
87.00	3170.0
88.00	3211.0
90.90	506.0
92.00	2451.0
93.10	3243.0
94.10	9492.0
95.10	64080.0
96.10	3630.0
103.80	427.0
105.10	176.0
105.90	495.0
111.10	243.0
115.10	192.0
115.90	368.0
117.00	502.0
117.90	333.0
118.90	507.0
128.00	268.0
129.00	203.0
129.90	499.0
135.00	168.0
141.10	965.0
141.80	179.0
142.80	842.0
145.10	207.0
158.90	191.0
170.40	232.0
170.90	190.0
172.00	660.0
173.10	722.0
174.00	55304.0
175.00	4307.0
176.00	52264.0
177.00	3118.0
191.00	222.0
192.90	230.0
207.10	154.0
265.10	181.0
281.10	1173.0
282.10	401.0
283.10	472.0

Instrument :
MSVOA_D
ClientSampleId :
BFB198

m/z	Abundance
36.10	821.0
37.10	3515.0
38.10	3100.0
39.10	1412.0
40.00	1123.0
43.00	262.0
44.10	923.0
45.20	477.0
47.00	822.0
48.20	298.0
49.10	2449.0
50.10	11274.0
51.10	3772.0
52.20	234.0
54.20	162.0
56.10	972.0
57.10	2472.0
57.90	178.0
60.20	632.0
61.10	3189.0
62.10	3050.0
63.10	2581.0
64.00	254.0
64.20	250.0
65.00	283.0
68.10	7091.0
69.00	6558.0
70.10	511.0
72.20	398.0
73.00	3147.0
74.10	10350.0
75.10	27504.0
76.10	2445.0
76.80	369.0
78.20	231.0
79.10	2789.0
80.00	659.0
80.90	3493.0
81.90	454.0
87.00	3221.0
88.00	3582.0
90.80	336.0
92.10	1889.0
93.10	2984.0
94.10	7477.0
95.10	55080.0
96.10	3897.0
104.10	312.0
105.90	326.0
106.90	182.0
112.90	185.0
115.80	209.0
116.10	228.0
116.80	583.0
118.10	330.0
118.90	485.0
128.00	592.0
130.00	380.0
133.20	229.0
141.00	594.0
143.00	1021.0
147.80	151.0
155.10	220.0
172.10	346.0
172.90	451.0
174.00	45592.0
175.00	3411.0
176.00	44952.0
177.00	2518.0
191.00	204.0
193.00	199.0
207.00	152.0
281.20	1229.0

Instrument :
MSVOA_D
ClientSampleId :
BFB198