
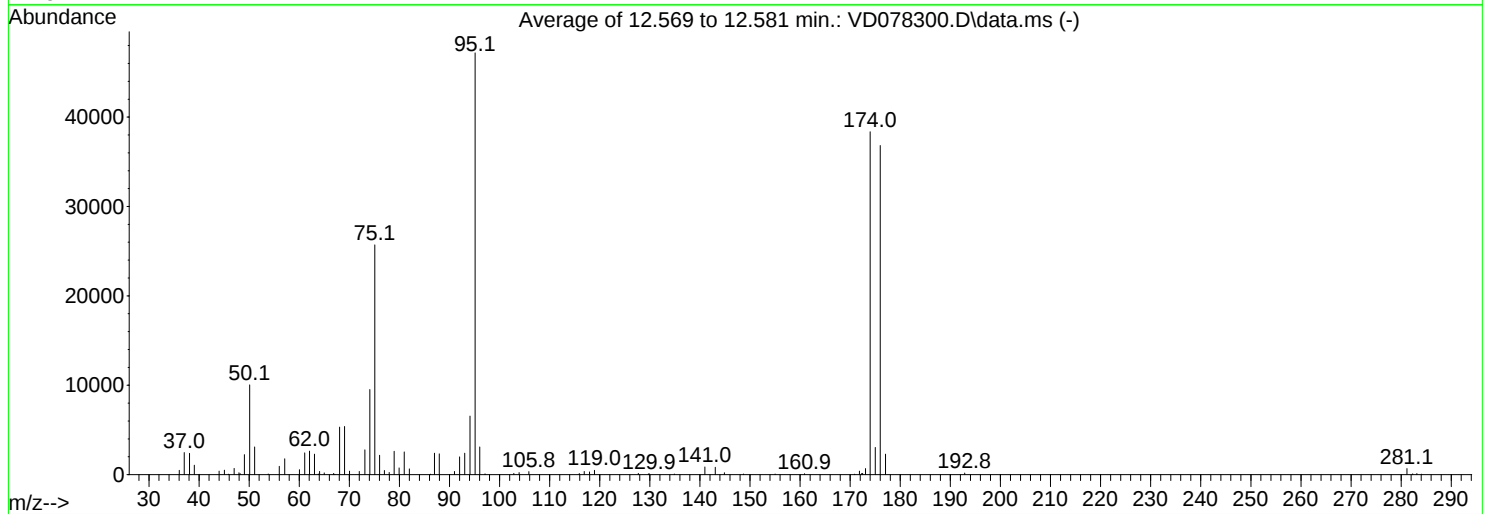


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020124\
Data File : VD078300.D
Acq On : 01 Feb 2024 10:51
Operator : RP/MD
Sample : BFB199
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB199

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Title : SFAM01.0
Last Update : Tue Feb 06 00:51:05 2024

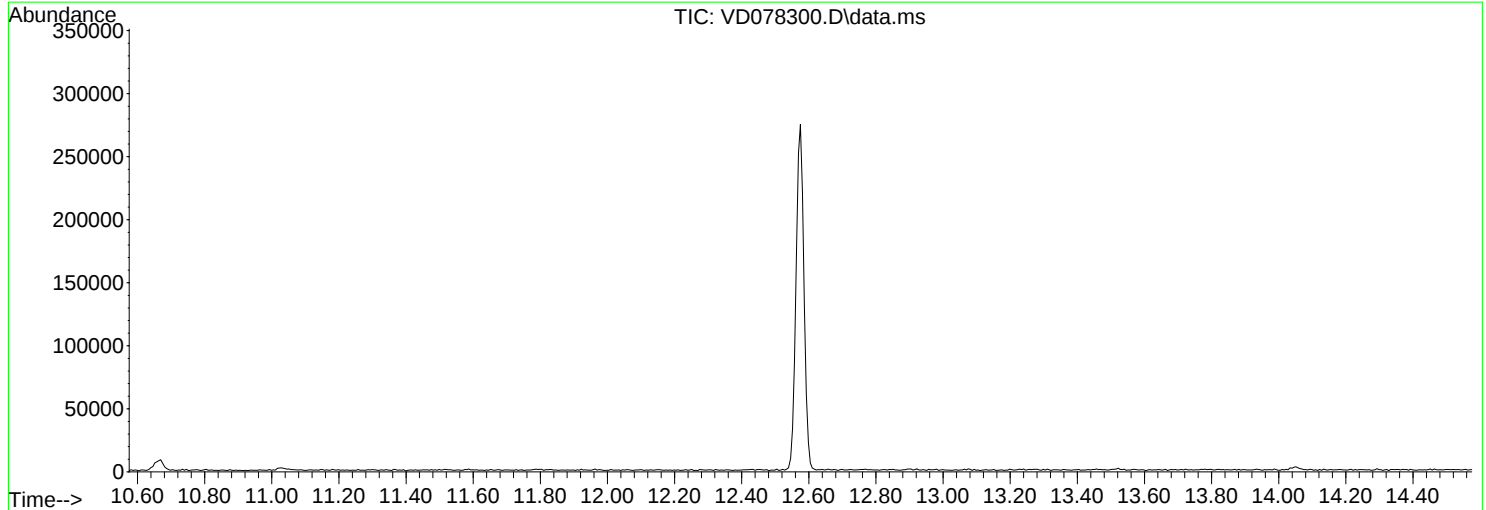

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.3	10034	PASS
75	95	30	80	54.5	25699	PASS
95	95	100	100	100.0	47187	PASS
96	95	5	9	6.6	3098	PASS
173	174	0.00	2	1.8	687	PASS
174	95	50	120	81.3	38363	PASS
175	174	5	9	7.9	3048	PASS
176	174	95	105	96.0	36827	PASS
177	176	5	10	6.2	2299	PASS

m/z	Abundance
40.00	839.0
44.00	595.0

Instrument :
MSVOA_D
ClientSampleId :
BFB199

m/z	Abundance
36.00	365.0
37.00	2418.0
38.10	3374.0
39.10	1051.0
40.00	699.0
44.10	827.0
45.00	665.0
45.90	186.0
47.00	637.0
48.20	398.0
49.10	2309.0
50.10	9984.0
51.10	3020.0
53.80	192.0
56.00	1136.0
57.10	1863.0
60.10	464.0
61.10	2651.0
62.10	2757.0
63.00	2533.0
63.80	197.0
64.20	194.0
65.00	171.0
66.80	178.0
68.10	5716.0
69.10	6118.0
70.10	387.0
72.10	293.0
73.10	3259.0
74.10	9900.0
75.10	27336.0
76.10	2043.0
77.10	684.0
78.00	300.0
79.00	2054.0
79.90	705.0
81.00	2755.0
82.00	706.0
87.00	2667.0
88.00	2246.0
91.00	241.0
92.00	2100.0
93.10	2605.0
94.10	7101.0
95.10	45776.0
96.10	3635.0
102.80	196.0
103.90	255.0
105.80	424.0
116.00	233.0
116.90	267.0
117.90	328.0
119.00	425.0
127.70	225.0
129.70	252.0
141.00	914.0
143.00	920.0
144.80	236.0
160.90	172.0
171.80	353.0
172.30	353.0
173.00	747.0
174.00	37904.0
175.00	2910.0
176.00	35352.0
177.00	2339.0
193.00	209.0
281.20	638.0

Instrument :
MSVOA_D
ClientSampleId :
BFB199

m/z	Abundance
36.10	666.0
37.10	2664.0
38.10	2411.0
39.00	1302.0
39.90	1141.0
44.00	1109.0
45.10	443.0
47.10	640.0
47.90	371.0
49.00	2583.0
50.10	11705.0
51.10	3925.0
56.00	1056.0
57.10	2004.0
60.00	832.0
61.00	3004.0
62.10	2276.0
63.10	2229.0
64.00	437.0
64.90	257.0
66.90	191.0
68.00	5760.0
69.10	5452.0
70.00	397.0
71.90	249.0
73.10	2948.0
74.10	9233.0
75.10	28152.0
76.00	2311.0
76.90	466.0
77.80	200.0
78.90	3060.0
80.00	908.0
81.00	2646.0
81.90	664.0
86.20	168.0
87.00	2534.0
87.90	2482.0
91.00	370.0
92.00	2179.0
93.00	2525.0
94.10	6658.0
95.10	53592.0
96.00	3227.0
97.10	262.0
102.90	233.0
104.00	263.0
105.90	228.0
115.80	152.0
116.90	487.0
118.00	361.0
118.90	681.0
127.70	216.0
129.90	270.0
141.00	965.0
143.10	1094.0
144.90	198.0
148.70	191.0
155.00	238.0
160.90	179.0
170.90	185.0
171.80	286.0
172.50	418.0
173.10	739.0
174.00	42232.0
175.00	2961.0
176.00	42008.0
177.10	2380.0
192.80	153.0
281.10	580.0
283.20	158.0

Instrument :
MSVOA_D
ClientSampleId :
BFB199

m/z	Abundance
36.10	432.0
37.10	2353.0
38.00	1389.0
39.10	801.0
40.10	767.0
44.00	1037.0
45.10	383.0
46.90	828.0
48.00	281.0
49.10	1813.0
50.10	8414.0
51.10	2365.0
55.90	624.0
57.10	1433.0
60.00	348.0
61.20	1628.0
62.00	2871.0
63.00	2123.0
64.00	431.0
65.10	154.0
67.10	165.0
68.00	4484.0
69.00	4589.0
70.10	393.0
72.00	518.0
73.10	2126.0
74.10	9414.0
75.10	21608.0
76.00	2129.0
76.90	273.0
78.00	237.0
79.00	2756.0
79.90	653.0
80.90	2244.0
82.10	555.0
87.00	1980.0
88.00	2278.0
91.00	442.0
92.00	1691.0
93.10	2067.0
94.10	5883.0
95.10	42192.0
96.10	2432.0
103.80	185.0
105.80	350.0
116.90	346.0
117.90	239.0
119.00	350.0
134.90	201.0
141.00	698.0
143.10	440.0
145.00	201.0
171.90	520.0
173.00	575.0
174.00	34952.0
175.00	3272.0
176.00	33120.0
177.00	2177.0
192.80	194.0
281.10	825.0
282.30	296.0
283.10	226.0
284.10	162.0

Instrument :
MSVOA_D
ClientSampleId :
BFB199