




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020224\
Data File : VD078330.D
Acq On : 02 Feb 2024 17:00
Operator : RP/MD
Sample : P1329-16
Misc : 5.32G/10ml/MSVOA_D/SOIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0FR7

Manual IntegrationsAPPROVED

Quant Time: Feb 03 00:23:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Feb 03 00:20:19 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/06/2024
Supervised By :Mahesh Dadoda 02/06/2024

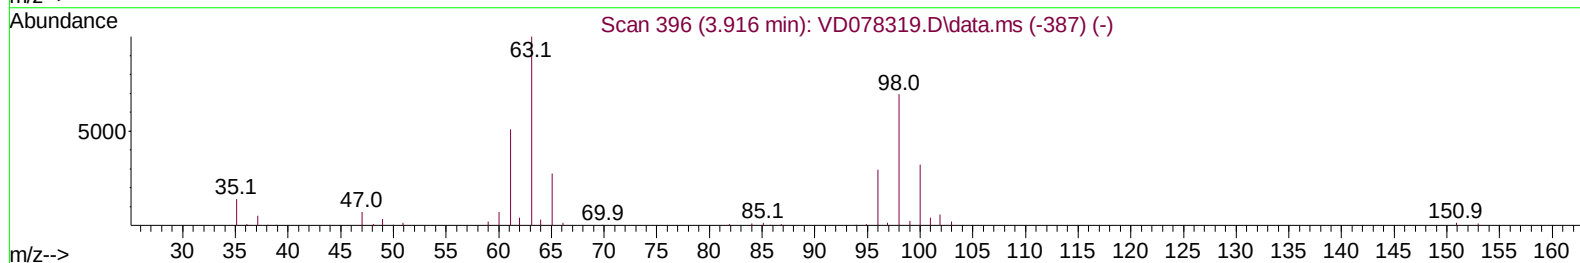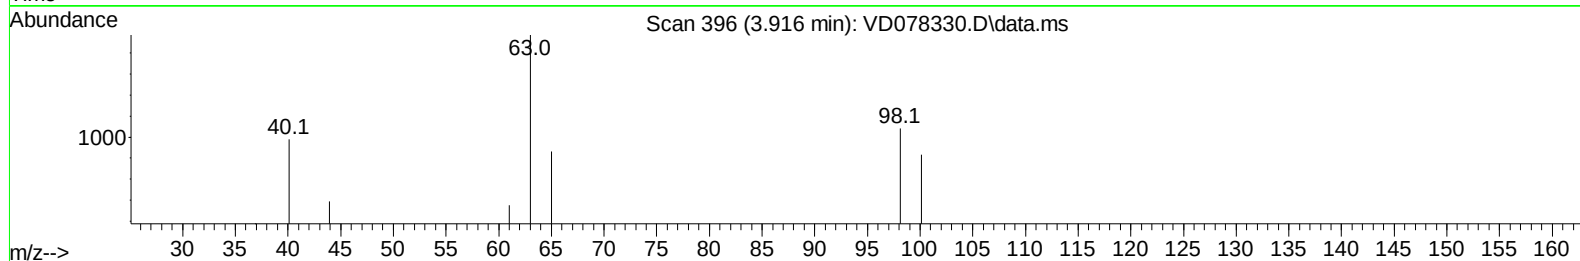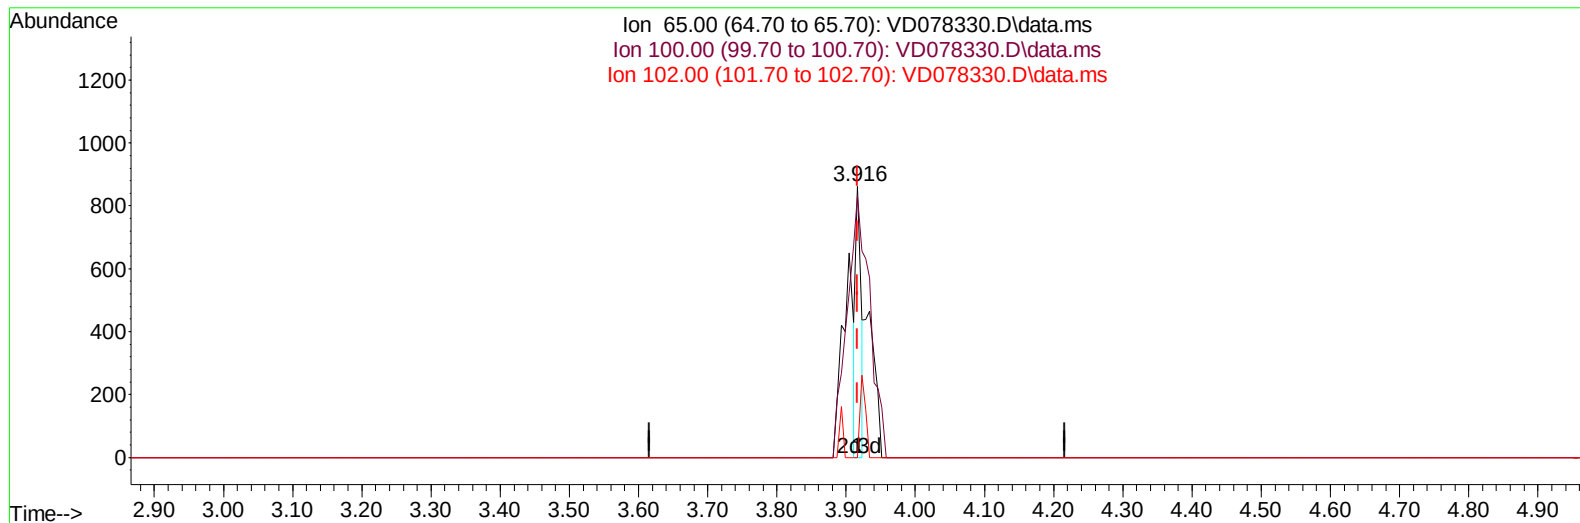

TIC: VD078330.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.916min (+ 0.000) 5.84 ug/L

response 459

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	151.80	412.42#
102.00	22.70	31.81#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020224\
Data File : VD078330.D
Acq On : 02 Feb 2024 17:00
Operator : RP/MD
Sample : P1329-16
Misc : 5.32G/10ml/MSVOA_D/SOIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0FR7

Manual IntegrationsAPPROVED

Quant Time: Feb 03 00:23:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Feb 03 00:20:19 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/06/2024
Supervised By :Mahesh Dadoda 02/06/2024

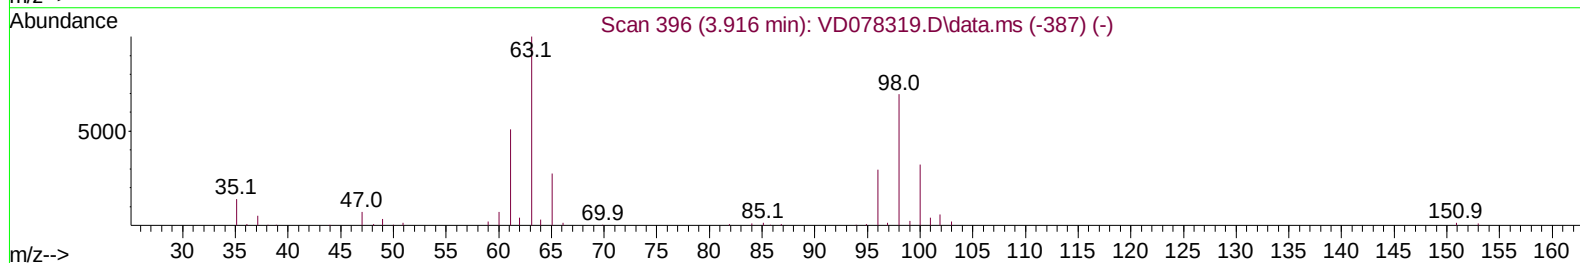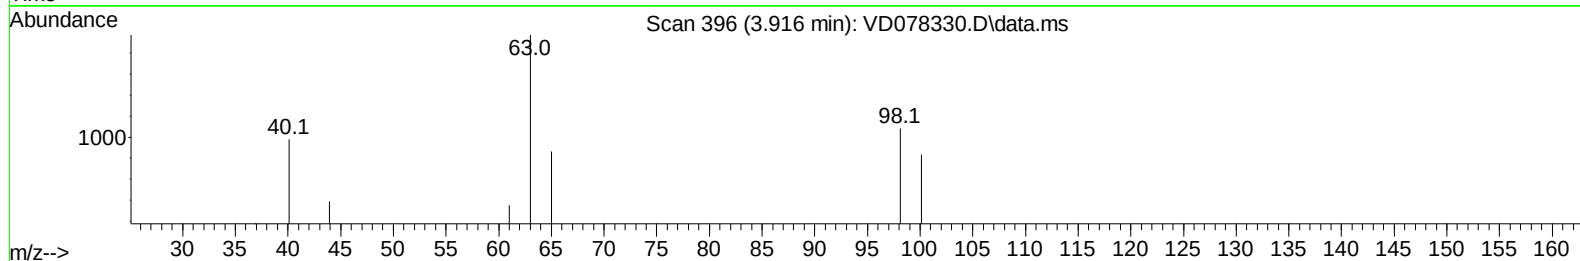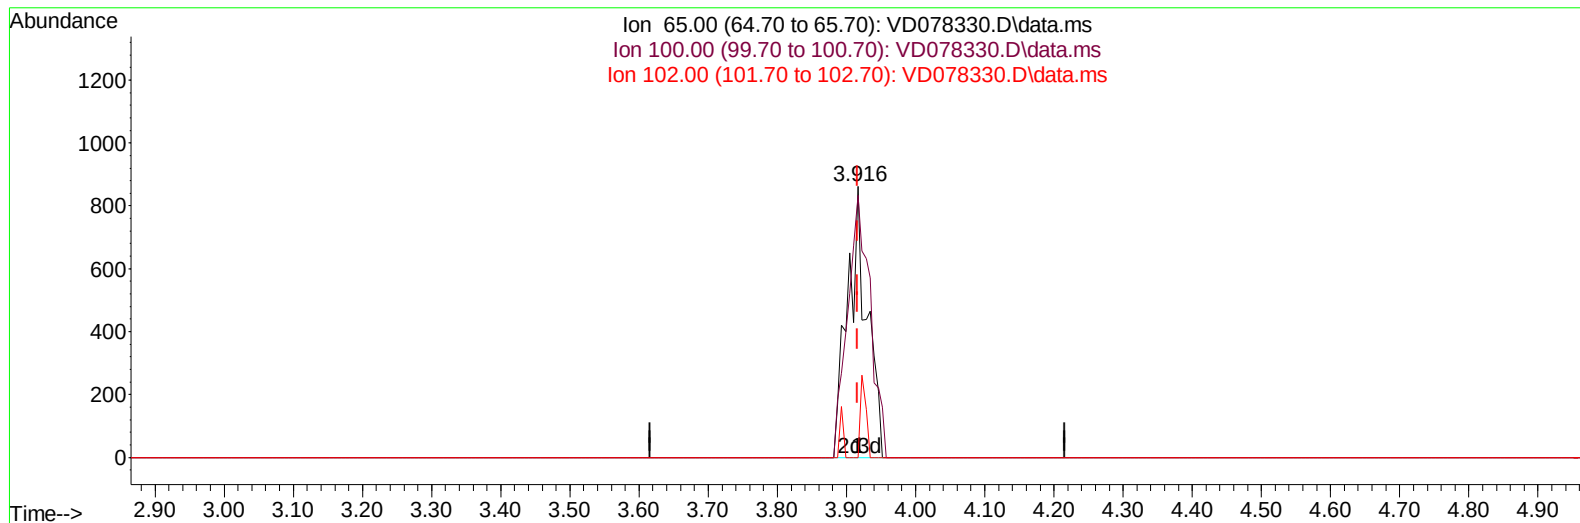

TIC: VD078330.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.916min (+ 0.000) 21.61 ug/L m

response 1697

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	151.80	111.55
102.00	22.70	8.60#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020224\
 Data File : VD078330.D
 Acq On : 02 Feb 2024 17:00
 Operator : RP/MD
 Sample : P1329-16
 Misc : 5.32G/10ml/MSVOA_D/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0FR7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/06/2024
 Supervised By :Mahesh Dadoda 02/06/2024

Quant Time: Feb 03 00:23:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Feb 03 00:20:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	12822	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	13877	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	5379	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	8305	22.830	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	91.320%	
7) Chloroethane-d5	2.799	69	7243	23.686	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	94.760%	
11) 1,1-Dichloroethene-d2	3.916	65	1697m	21.605	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	86.440%	
21) 2-Butanone-d5	6.993	46	6709	125.260	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	250.520%#	
24) Chloroform-d	7.569	84	10287	28.139	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	112.560%	
26) 1,2-Dichloroethane-d4	8.234	65	7615	38.598	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	154.400%#	
32) Benzene-d6	8.199	84	17345	21.376	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	85.520%	
36) 1,2-Dichloropropane-d6	9.210	67	6542	26.189	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	104.760%	
41) Toluene-d8	10.269	98	13679	18.769	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.080%	
43) trans-1,3-Dichloroprop...	10.528	79	2992	26.824	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	107.280%	
47) 2-Hexanone-d5	10.875	63	4017	79.258	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	158.520%#	
56) 1,1,2,2-Tetrachloroeth...	12.651	84	10629	45.790	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	183.160%#	
66) 1,2-Dichlorobenzene-d4	13.816	152	4305	22.356	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	89.440%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020224\
Data File : VD078330.D
Acq On : 02 Feb 2024 17:00
Operator : RP/MD
Sample : P1329-16
Misc : 5.32G/10ml/MSVOA_D/SOIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0FR7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/06/2024
Supervised By :Mahesh Dadoda 02/06/2024

Quant Time: Feb 03 00:23:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Feb 03 00:20:19 2024
Response via : Initial Calibration

