

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020224\
 Data File : VD078335.D
 Acq On : 02 Feb 2024 19:18
 Operator : RP/MD
 Sample : P1329-21
 Misc : 4.23G/10ml/MSVOA_D/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 COFM6

Quant Time: Feb 03 00:24:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Feb 03 00:20:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	166697	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.580	117	160640	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	63797	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	113941	24.092	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	96.360%		
7) Chloroethane-d5	2.799	69	94952	23.884	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	95.520%		
11) 1,1-Dichloroethene-d2	3.916	65	22671	22.201	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	88.800%		
21) 2-Butanone-d5	6.992	46	25924	37.229	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	74.460%		
24) Chloroform-d	7.569	84	104360	21.957	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.840%		
26) 1,2-Dichloroethane-d4	8.228	65	56991	22.219	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	88.880%		
32) Benzene-d6	8.204	84	212160	22.587	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	90.360%		
36) 1,2-Dichloropropane-d6	9.210	67	68891	23.824	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.280%		
41) Toluene-d8	10.269	98	187511	22.225	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	88.920%		
43) trans-1,3-Dichloroprop...	10.528	79	28022	21.702	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	86.800%		
47) 2-Hexanone-d5	10.875	63	20478	34.904	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	69.800%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	53653	19.967	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	79.880%		
66) 1,2-Dichlorobenzene-d4	13.816	152	54022	23.653	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	94.600%		
Target Compounds						Qvalue
16) Methylene chloride	4.804	84	9884	3.023	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020224\
Data File : VD078335.D
Acq On : 02 Feb 2024 19:18
Operator : RP/MD
Sample : P1329-21
Misc : 4.23G/10ml/MSVOA_D/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0FM6


Quant Time: Feb 03 00:24:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Feb 03 00:20:19 2024
Response via : Initial Calibration

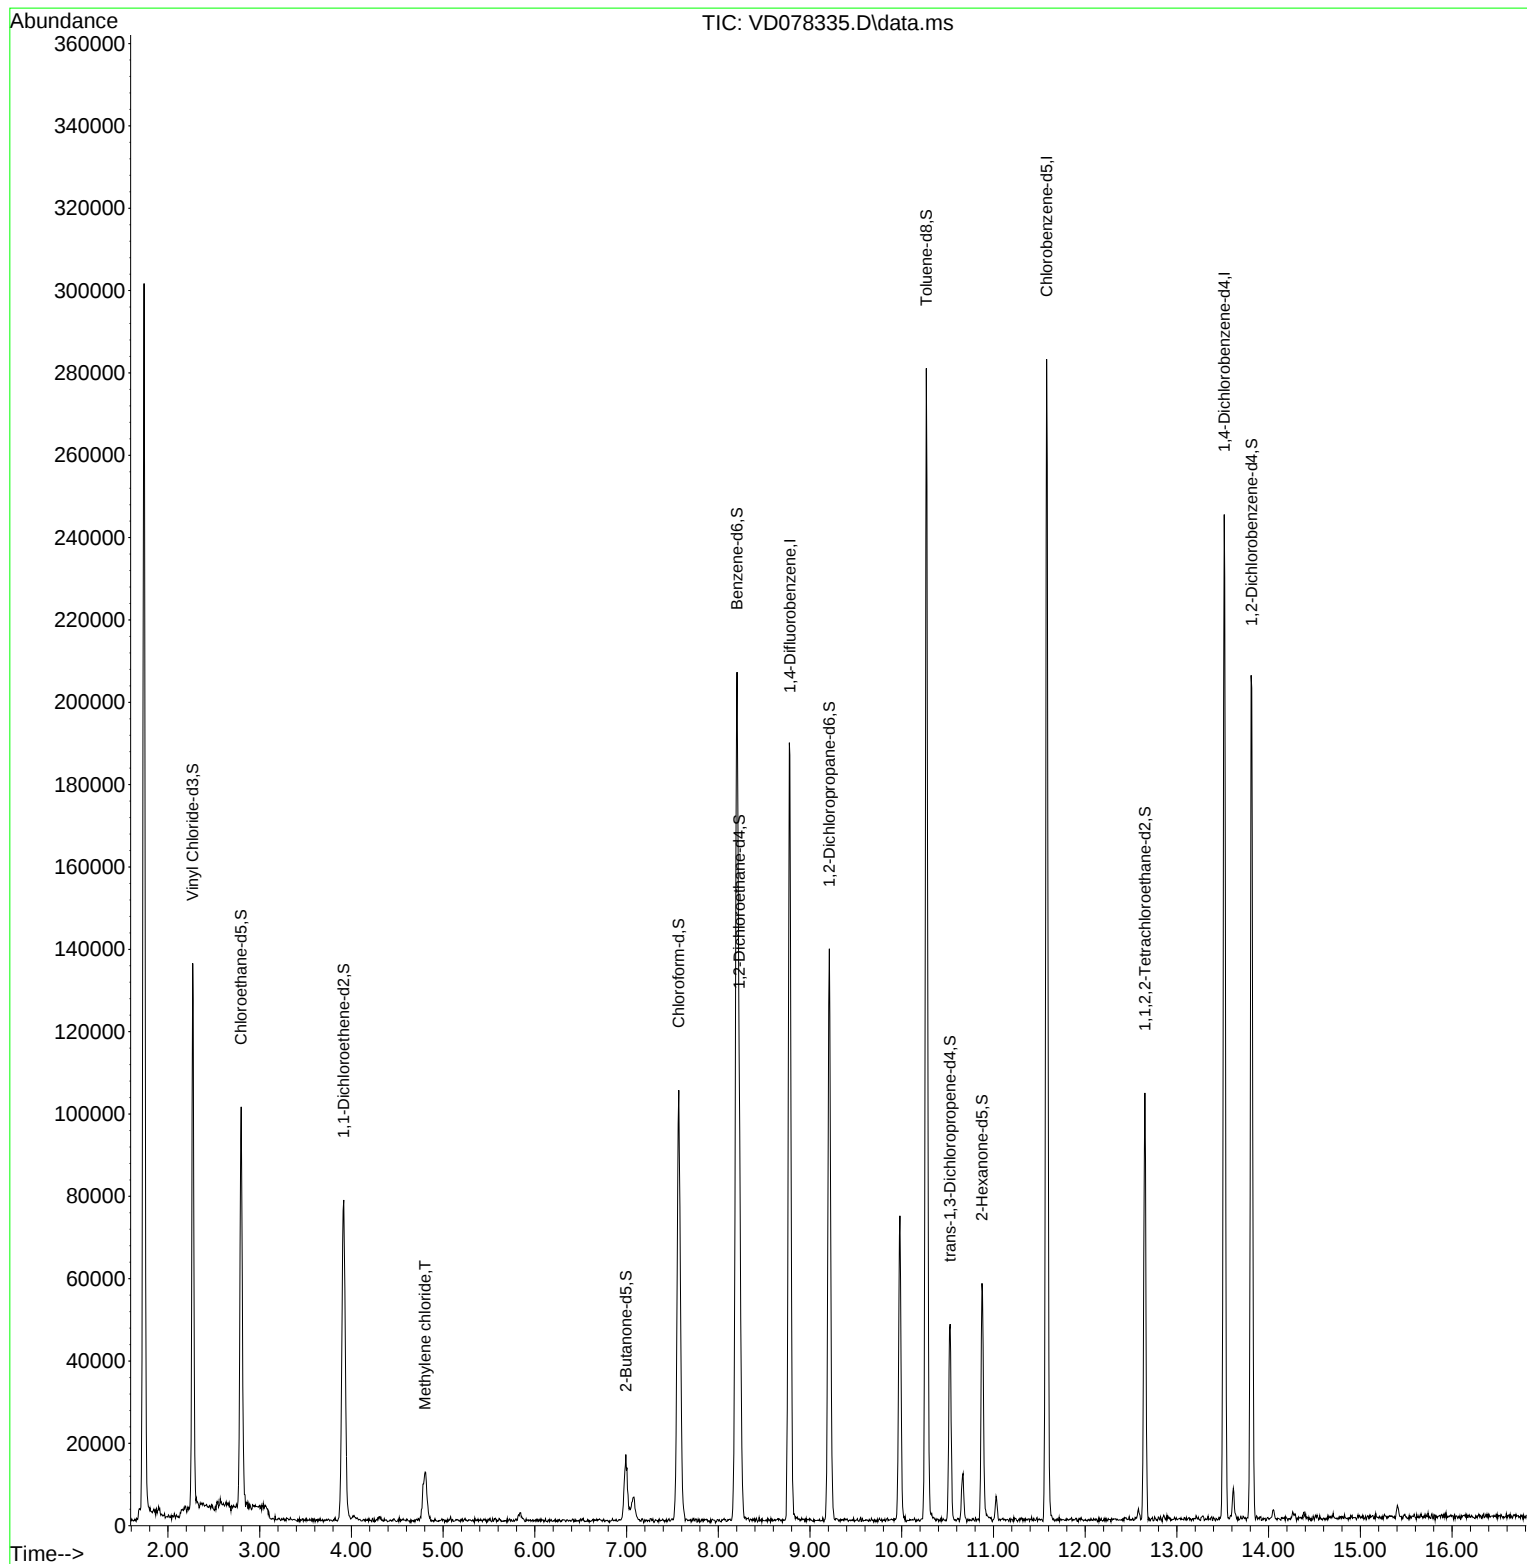

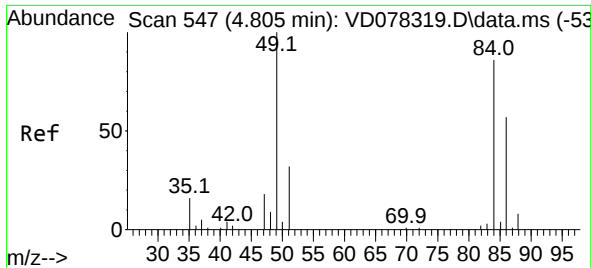

#16
Methylene chloride
Concen: 3.023 ug/L
RT: 4.804 min Scan# 54
Delta R.T. -0.000 min
Lab File: VD078335.D
Acq: 02 Feb 2024 19:18

Instrument :
MSVOA_D
ClientSampleId :
C0FM6

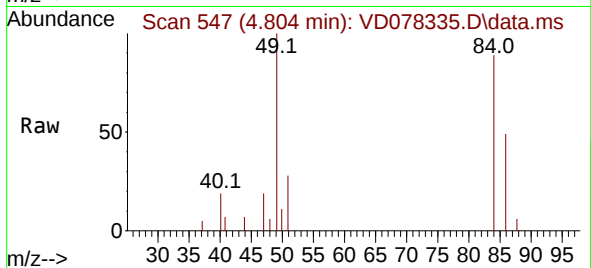

Tgt Ion:	84	Resp:	9884
Ion	Ratio	Lower	Upper
84	100		
86	55.5	45.4	84.2
49	112.8	77.3	143.7

