
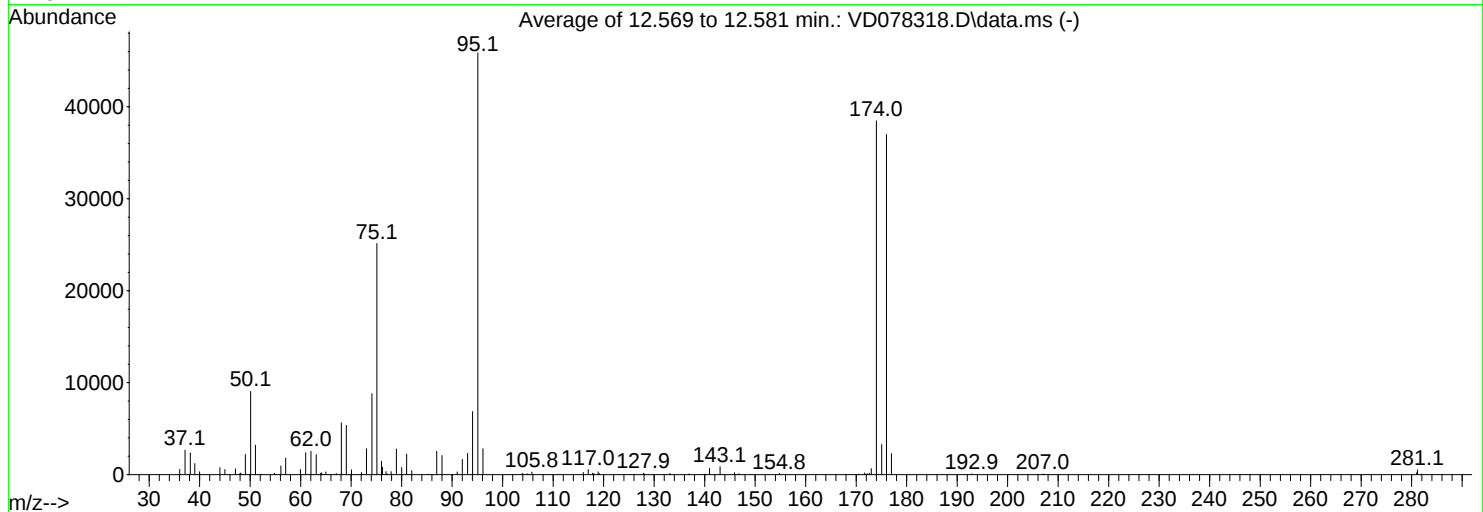


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020224\
Data File : VD078318.D
Acq On : 02 Feb 2024 10:02
Operator : RP/MD
Sample : BFB200
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB200

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM020124SMA.M
Title : SFAM01.0
Last Update : Tue Feb 06 00:51:05 2024

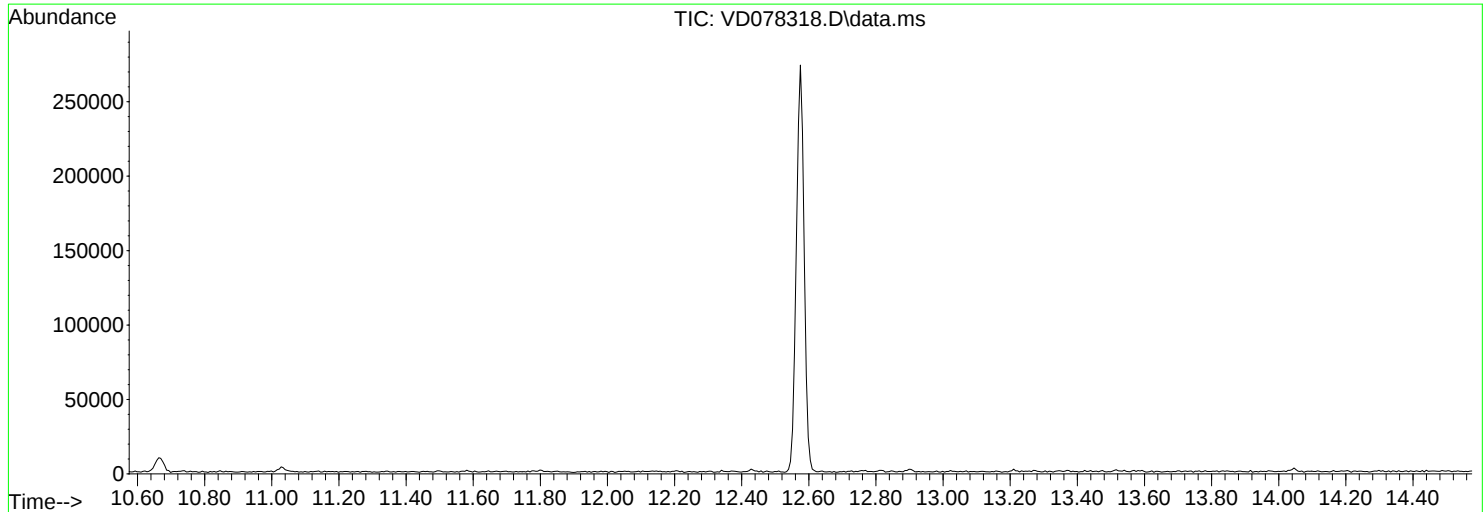

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	9051	PASS
75	95	30	80	54.8	25139	PASS
95	95	100	100	100.0	45869	PASS
96	95	5	9	6.2	2824	PASS
173	174	0.00	2	1.7	660	PASS
174	95	50	120	83.9	38467	PASS
175	174	5	9	8.5	3271	PASS
176	174	95	105	96.2	37000	PASS
177	176	5	10	6.2	2303	PASS

Scan 1860 (12.528 min): VD078318.D\data.ms
BFB200

m/z	Abundance
40.00	731.0
44.00	310.0

Instrument :
MSVOA_D
ClientSampleId :
BFB200

m/z	Abundance
36.00	497.0
37.10	2583.0
38.10	2252.0
39.10	1184.0
40.10	987.0
44.00	1121.0
45.00	604.0
47.10	858.0
48.00	490.0
49.10	2022.0
50.10	8414.0
51.10	3127.0
52.20	193.0
56.10	793.0
57.00	1723.0
59.90	476.0
61.00	2189.0
62.10	2535.0
63.10	2419.0
64.10	373.0
65.00	330.0
67.00	184.0
68.00	5105.0
69.10	5102.0
70.10	780.0
72.10	258.0
73.00	2826.0
74.10	8000.0
75.10	24808.0
76.00	2059.0
77.20	263.0
78.00	403.0
78.90	2669.0
80.00	710.0
81.00	2438.0
82.10	423.0
87.00	2663.0
88.00	2041.0
90.90	316.0
92.00	1602.0
93.10	1983.0
94.00	6621.0
95.10	45064.0
96.10	2737.0
103.80	196.0
104.80	251.0
105.80	310.0
116.10	184.0
116.90	379.0
117.90	209.0
118.90	572.0
127.90	204.0
136.80	171.0
141.00	741.0
143.00	671.0
145.90	157.0
154.80	217.0
171.70	340.0
173.00	642.0
174.00	35864.0
175.00	3157.0
176.00	33808.0
177.00	2248.0
207.00	204.0
281.00	615.0

Instrument :
MSVOA_D
ClientSampleId :
BFB200

m/z	Abundance
36.10	576.0
37.10	3313.0
38.20	2589.0
39.00	1112.0
40.00	1053.0
44.10	1076.0
45.00	516.0
47.20	509.0
48.20	242.0
49.00	2319.0
50.10	10340.0
51.10	3815.0
54.80	239.0
56.20	1123.0
57.10	1929.0
60.00	589.0
61.00	2345.0
62.00	2779.0
63.10	2291.0
64.20	279.0
65.00	290.0
67.10	180.0
68.10	6484.0
69.00	6203.0
70.00	583.0
72.00	172.0
73.00	3407.0
74.10	9908.0
75.10	26600.0
76.20	2395.0
76.90	473.0
77.80	410.0
78.90	3003.0
80.00	895.0
81.00	2475.0
82.00	548.0
87.00	2957.0
88.00	2603.0
91.00	337.0
92.00	1572.0
93.00	2856.0
94.10	7910.0
95.10	50984.0
96.10	2653.0
104.00	411.0
105.00	211.0
105.80	314.0
111.10	173.0
115.90	338.0
117.00	533.0
117.70	254.0
119.10	395.0
128.10	210.0
133.10	166.0
137.00	164.0
139.90	170.0
140.90	742.0
143.10	904.0
146.00	159.0
172.20	384.0
172.90	627.0
174.00	43696.0
175.10	3970.0
176.00	42384.0
177.00	2666.0
281.20	820.0

Instrument :
MSVOA_D
ClientSampleId :
BFB200

m/z	Abundance
36.00	637.0
37.10	2114.0
38.20	2255.0
39.10	1301.0
40.00	1075.0
44.10	1038.0
45.00	568.0
47.00	499.0
48.10	293.0
49.00	2216.0
50.10	8399.0
51.00	2663.0
54.90	213.0
56.00	907.0
57.00	1744.0
60.00	624.0
61.00	2609.0
62.00	2328.0
63.10	1829.0
63.90	404.0
65.00	245.0
68.00	5334.0
69.10	4796.0
70.10	179.0
72.10	271.0
73.10	2211.0
74.10	8529.0
75.10	24008.0
76.00	2346.0
76.90	519.0
77.90	196.0
79.00	2660.0
80.00	713.0
81.00	1772.0
81.90	352.0
85.30	153.0
86.90	2016.0
88.00	1612.0
91.10	222.0
92.00	1783.0
93.10	2095.0
94.10	6024.0
95.10	41560.0
96.10	3081.0
105.80	214.0
115.90	204.0
117.00	777.0
118.10	343.0
118.90	342.0
127.90	260.0
129.90	162.0
133.20	231.0
140.90	575.0
143.00	1014.0
145.80	298.0
146.80	299.0
154.80	184.0
170.50	183.0
171.70	228.0
172.60	485.0
173.10	711.0
174.00	35840.0
175.00	2686.0
176.00	34808.0
177.00	1995.0
192.90	260.0
207.20	165.0
281.10	760.0
281.90	235.0

Instrument :
MSVOA_D
ClientSampleId :
BFB200