

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020822\
 Data File : VD071920.D
 Acq On : 08 Feb 2022 16:17
 Operator : VA/SY
 Sample : VIBLK
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VIBLK

Quant Time: Feb 09 03:52:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 27 06:04:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	585483	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	1069121	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.637	117	1014295	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	467334	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	354033	47.841	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	95.680%
35) Dibromofluoromethane	7.914	113	347656	49.470	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	98.940%
50) Toluene-d8	10.332	98	1362089	51.897	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	103.800%
62) 4-Bromofluorobenzene	12.626	95	486378	53.067	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	106.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020822\
Data File : VD071920.D
Acq On : 08 Feb 2022 16:17
Operator : VA/SY
Sample : VIBLK
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VIBLK

Quant Time: Feb 09 03:52:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
Quant Title : SW846 8260
QLast Update : Thu Jan 27 06:04:38 2022
Response via : Initial Calibration




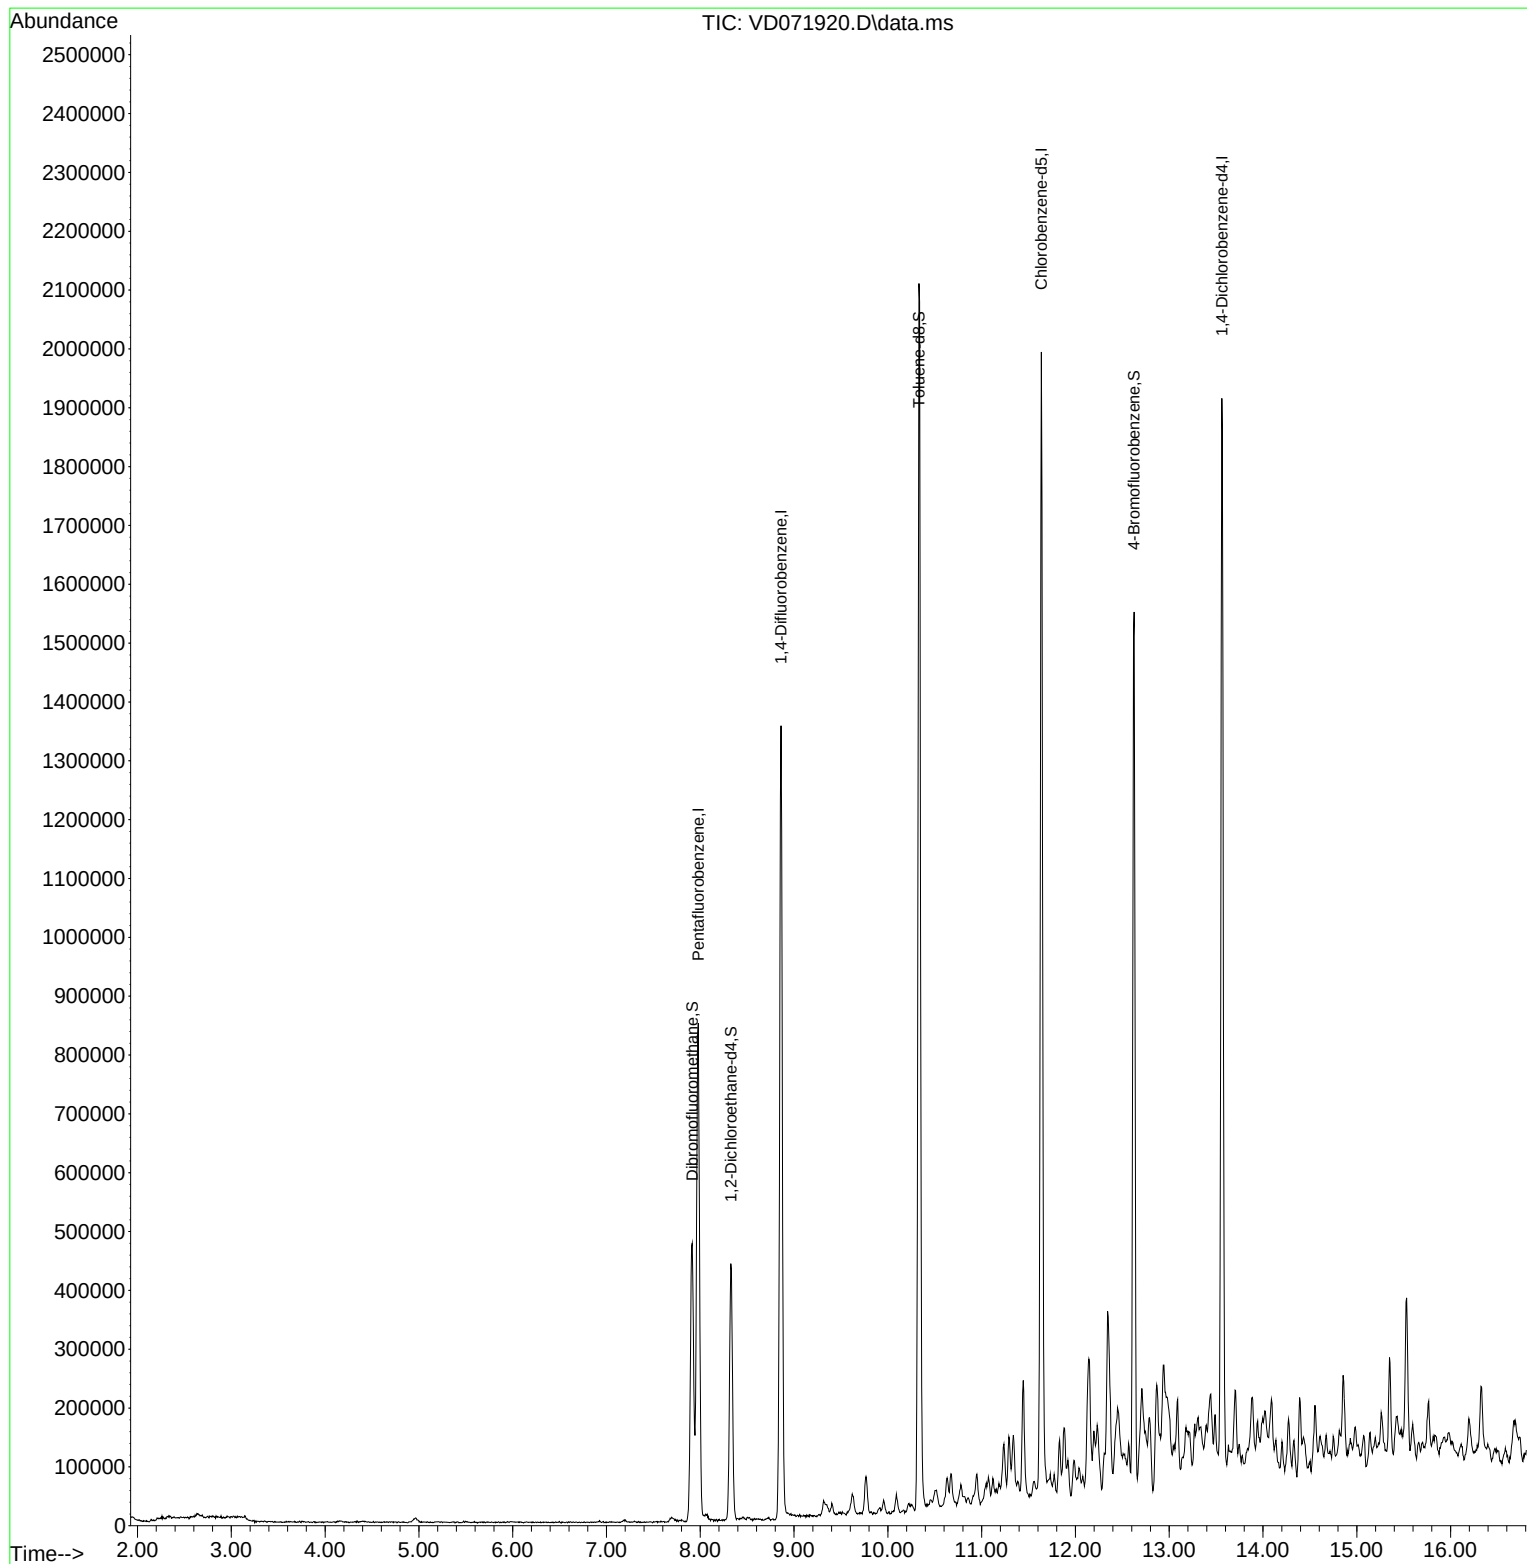


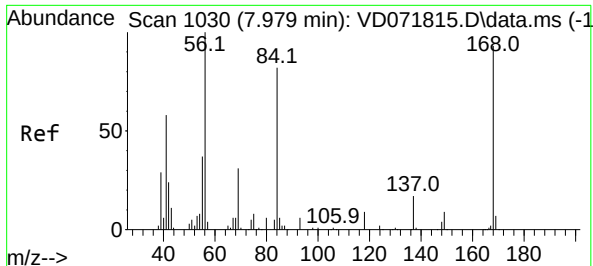

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.000 min
Lab File: VD071920.D
Acq: 08 Feb 2022 16:17




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 585483
Ion Ratio Lower Upper
168 100
99 65.6 49.8 74.6

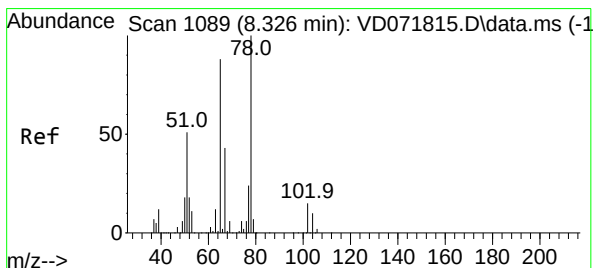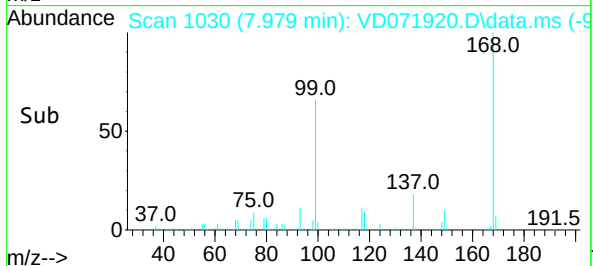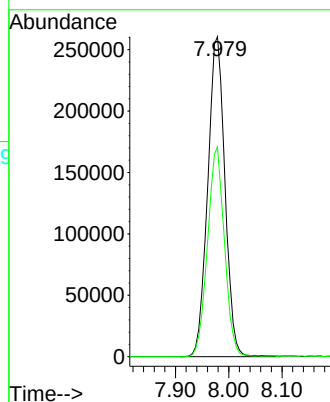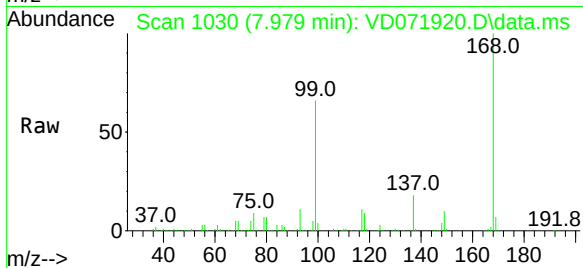

#33
1,2-Dichloroethane-d4
Concen: 47.841 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD071920.D
Acq: 08 Feb 2022 16:17

Tgt Ion: 65 Resp: 354033
Ion Ratio Lower Upper
65 100
67 52.5 0.0 101.4

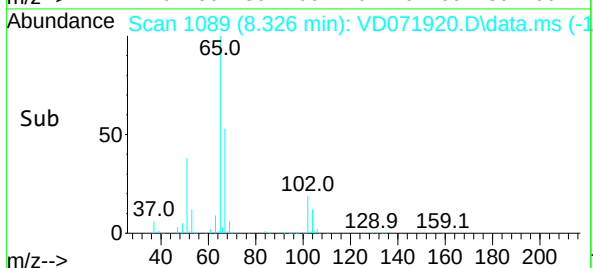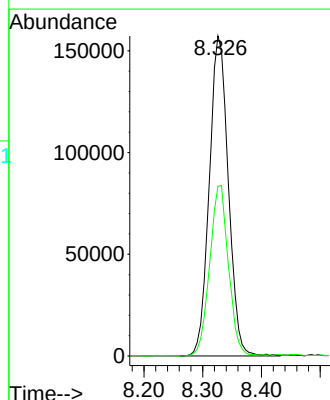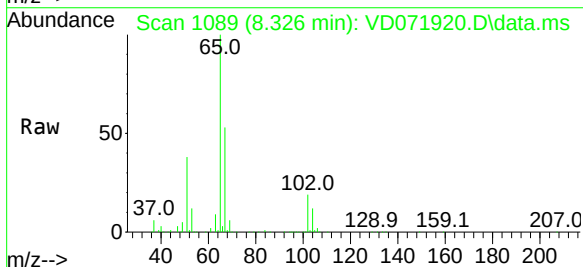

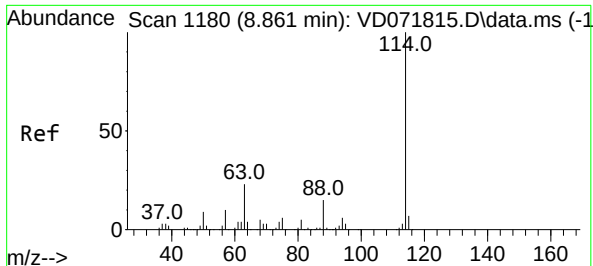

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. -0.000 min

Lab File: VD071920.D

Acq: 08 Feb 2022 16:17

Instrument :

MSVOA_D

ClientSampleId :

VIBLK





Tgt Ion:114 Resp: 1069121

Ion Ratio Lower Upper

114 100

63 22.7 0.0 46.6

88 15.9 0.0 33.2

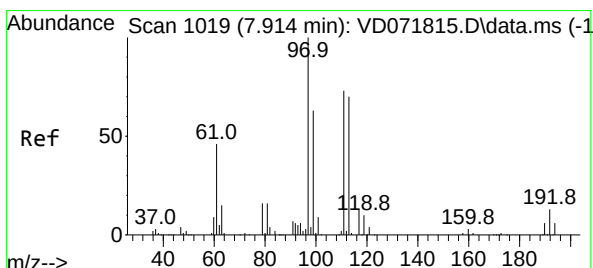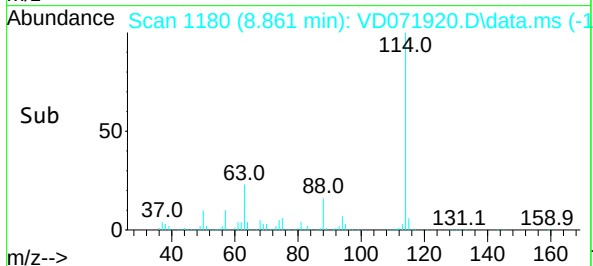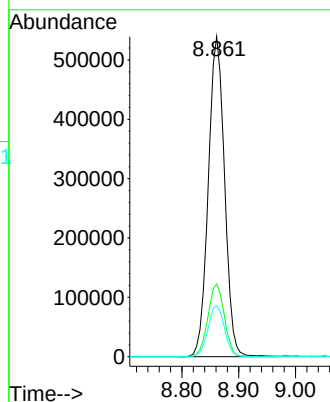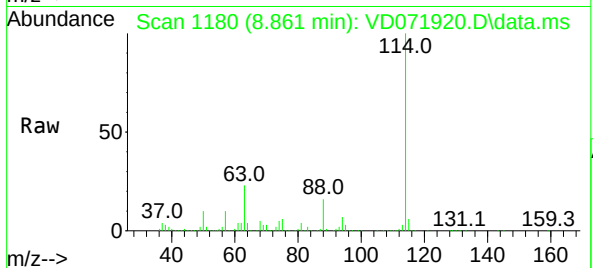

#35

Dibromofluoromethane

Concen: 49.470 ug/l

RT: 7.914 min Scan# 1019

Delta R.T. -0.000 min

Lab File: VD071920.D

Acq: 08 Feb 2022 16:17




Tgt Ion:113 Resp: 347656


Ion Ratio Lower Upper

113 100

111 102.7 83.8 125.6

192 17.6 14.6 21.8


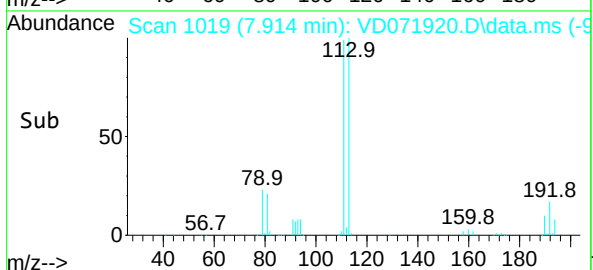
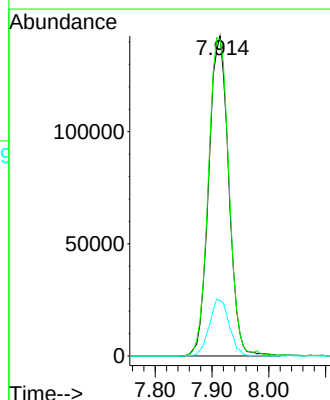
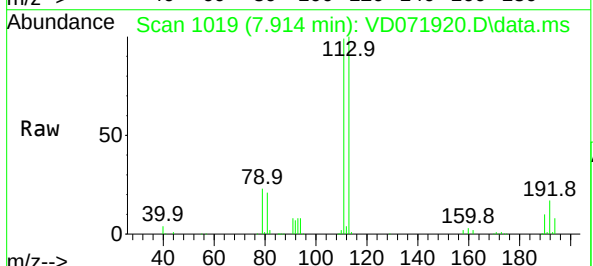


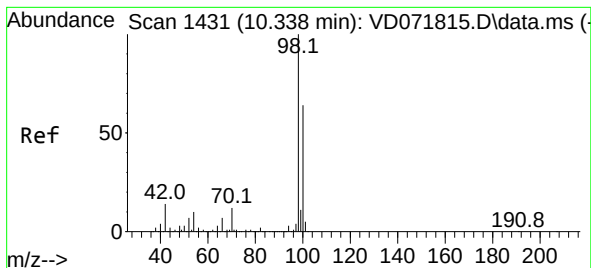

#50
Toluene-d8
Concen: 51.897 ug/l
RT: 10.332 min Scan# 1431
Delta R.T. -0.006 min
Lab File: VD071920.D
Acq: 08 Feb 2022 16:17




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 1362089
Ion Ratio Lower Upper
98 100
100 65.6 52.4 78.6

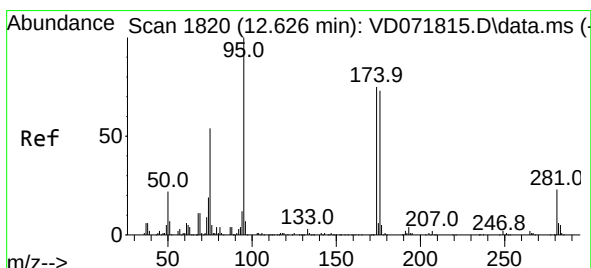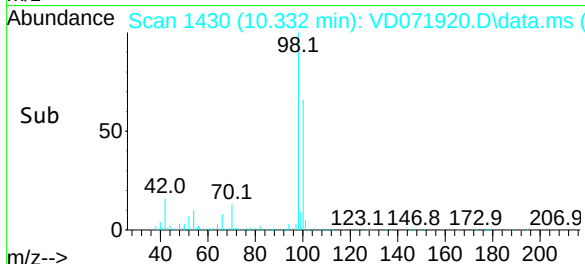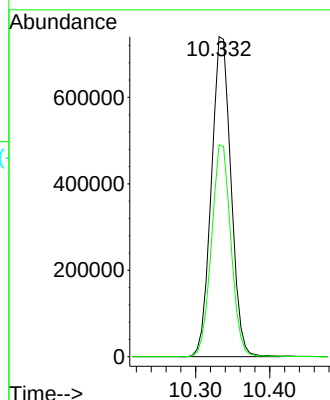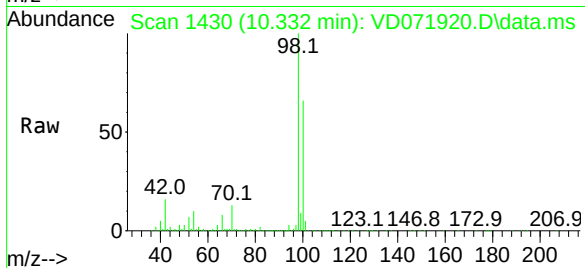

#62
4-Bromofluorobenzene
Concen: 53.067 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD071920.D
Acq: 08 Feb 2022 16:17

Tgt Ion: 95 Resp: 486378
Ion Ratio Lower Upper
95 100
174 74.0 0.0 152.8
176 70.2 0.0 145.4


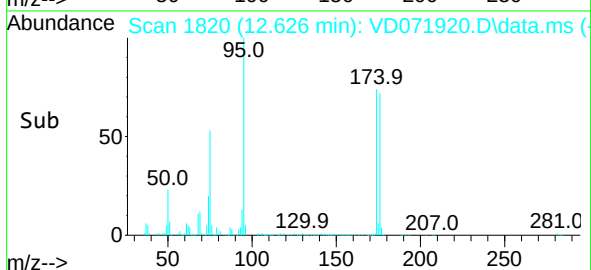
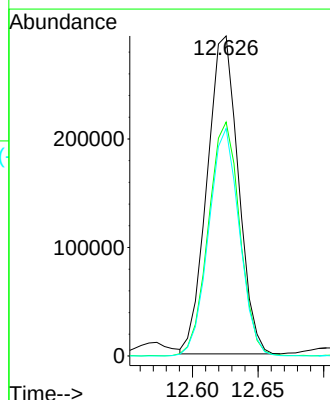
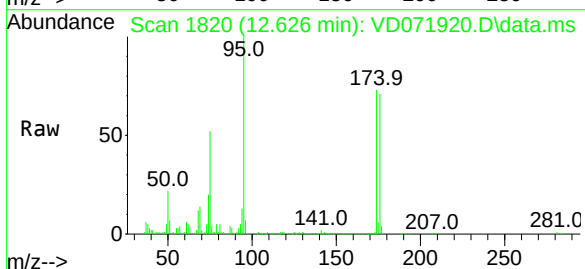


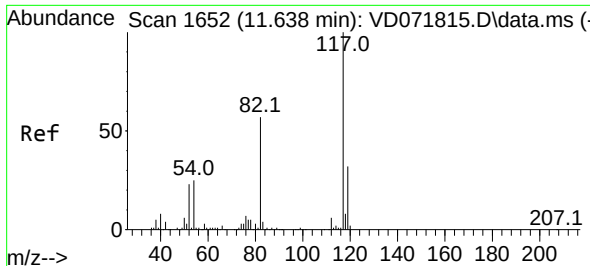

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.637 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD071920.D
Acq: 08 Feb 2022 16:17

Instrument :
MSVOA_D
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 1014295
Ion Ratio Lower Upper
117 100
82 58.2 45.3 67.9
119 31.4 26.6 40.0

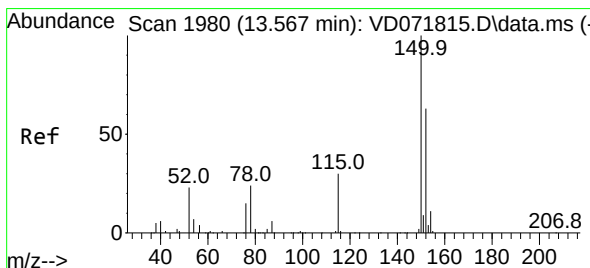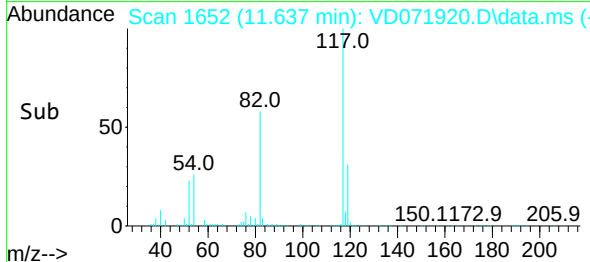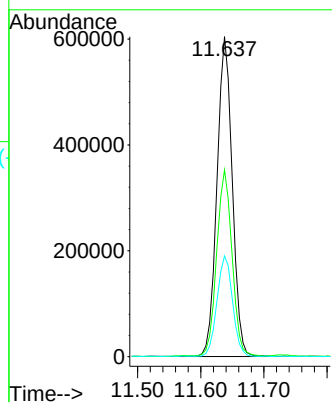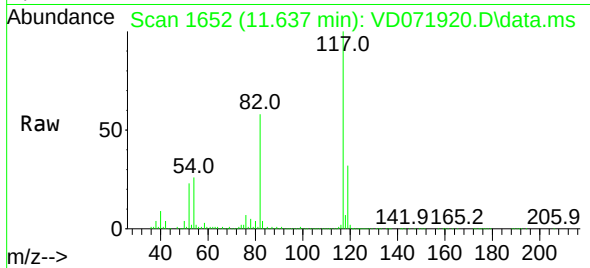

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. -0.006 min
Lab File: VD071920.D
Acq: 08 Feb 2022 16:17

Tgt Ion:152 Resp: 467334
Ion Ratio Lower Upper
152 100
115 61.0 31.3 93.8
150 154.6 0.0 348.6

