

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020822\
 Data File : VD071921.D
 Acq On : 08 Feb 2022 16:46
 Operator : VA/SY
 Sample : VIBLK
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VIBLK

Quant Time: Feb 09 04:00:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 27 06:04:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	534900	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	999648	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.637	117	983280	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	450407	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	375698	55.570	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	111.140%
35) Dibromofluoromethane	7.908	113	331892	50.509	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.020%
50) Toluene-d8	10.332	98	1284035	52.323	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.640%
62) 4-Bromofluorobenzene	12.626	95	478628	55.850	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	111.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020822\
Data File : VD071921.D
Acq On : 08 Feb 2022 16:46
Operator : VA/SY
Sample : VIBLK
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VIBLK

Quant Time: Feb 09 04:00:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
Quant Title : SW846 8260
QLast Update : Thu Jan 27 06:04:38 2022
Response via : Initial Calibration




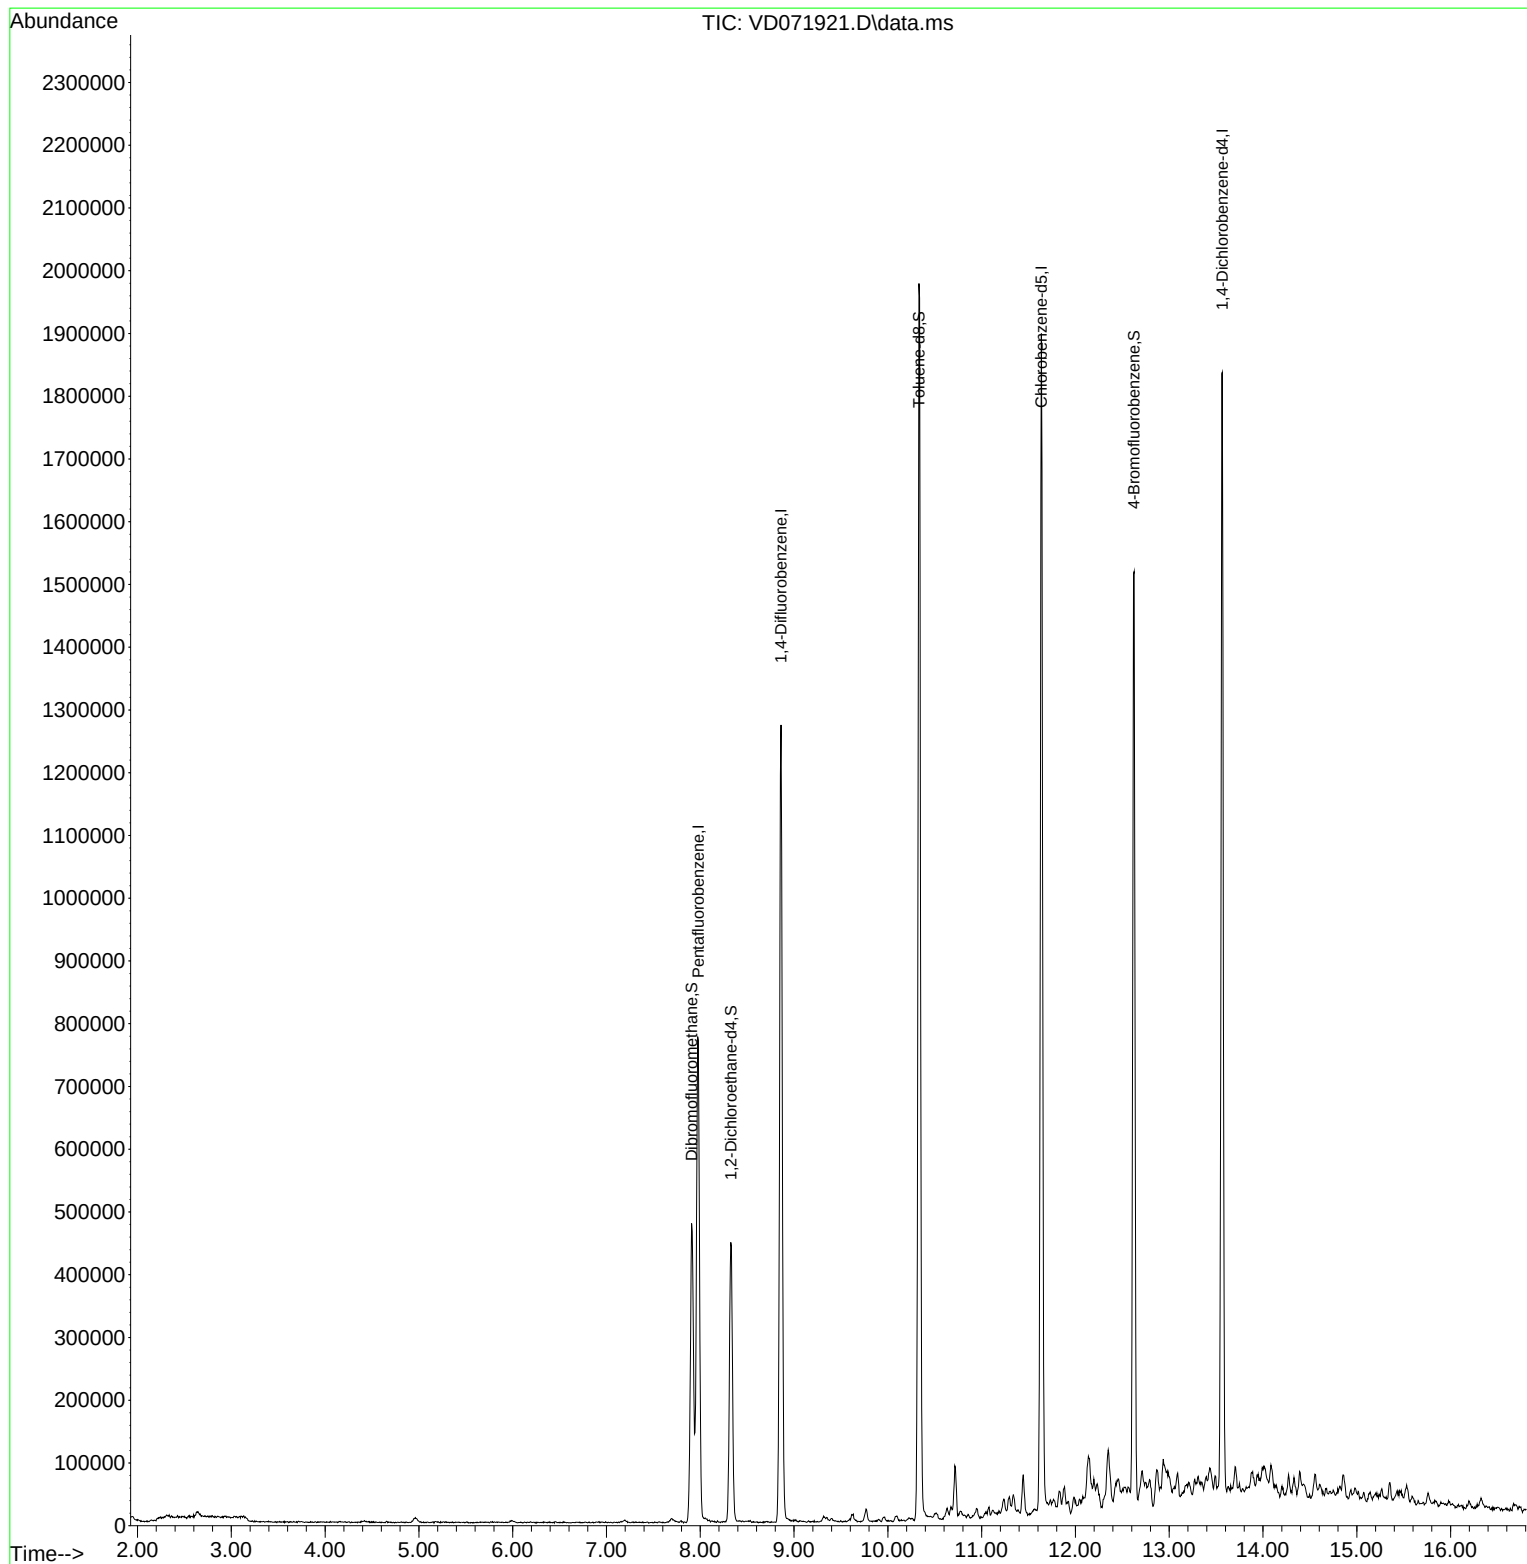


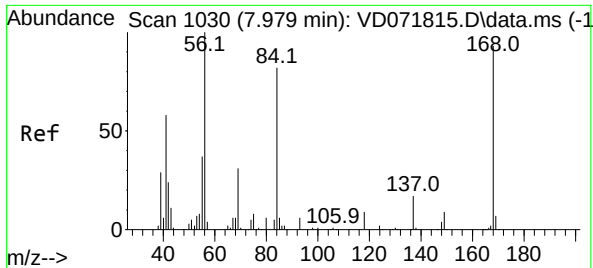

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.000 min
Lab File: VD071921.D
Acq: 08 Feb 2022 16:46




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 534900
Ion Ratio Lower Upper
168 100
99 65.0 49.8 74.6

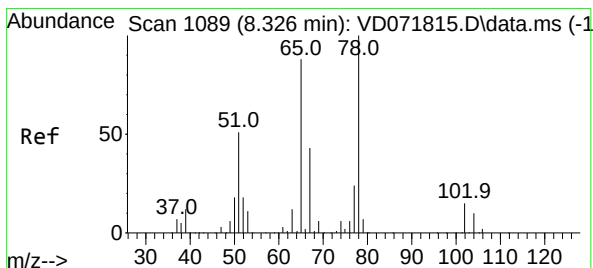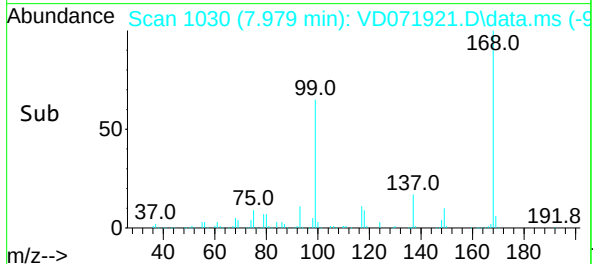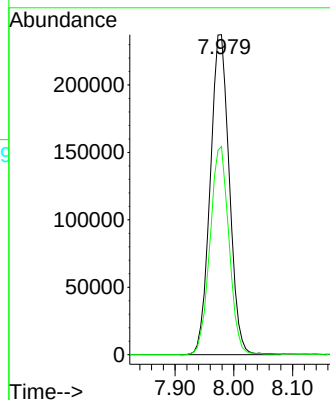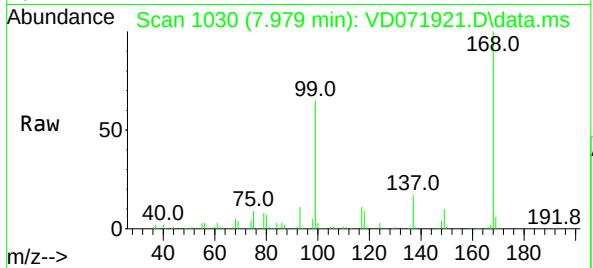

#33
1,2-Dichloroethane-d4
Concen: 55.570 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD071921.D
Acq: 08 Feb 2022 16:46

Tgt Ion: 65 Resp: 375698
Ion Ratio Lower Upper
65 100
67 49.7 0.0 101.4

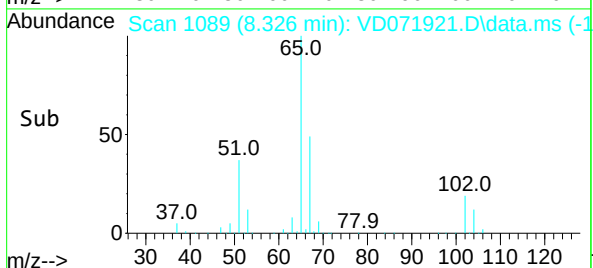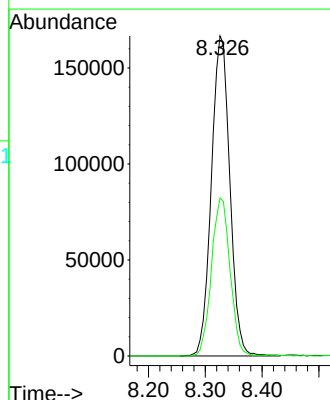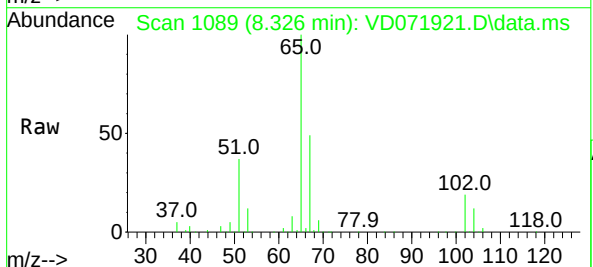

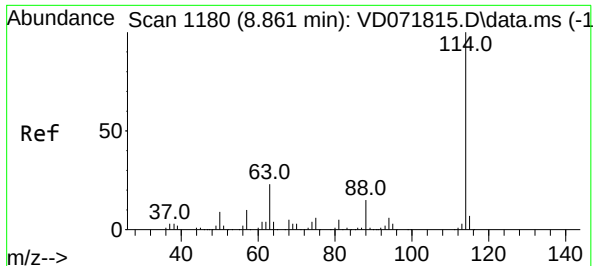

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. -0.000 min

Lab File: VD071921.D

Acq: 08 Feb 2022 16:46

Instrument :

MSVOA_D

ClientSampleId :

VIBLK





Tgt Ion:114 Resp: 999648

Ion Ratio Lower Upper

114 100

63 23.4 0.0 46.6

88 16.2 0.0 33.2

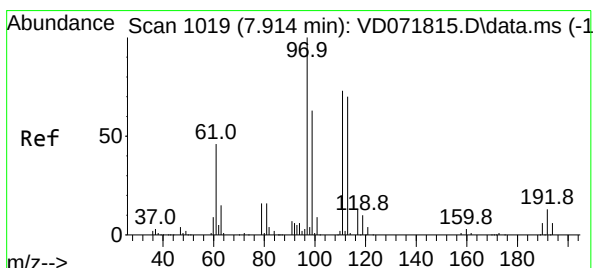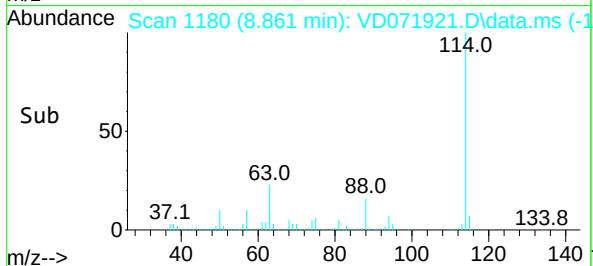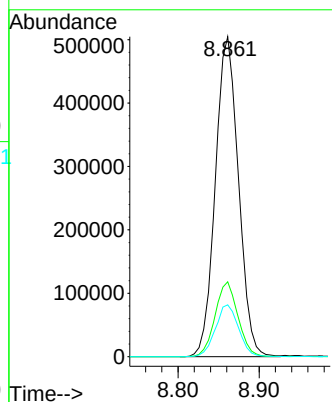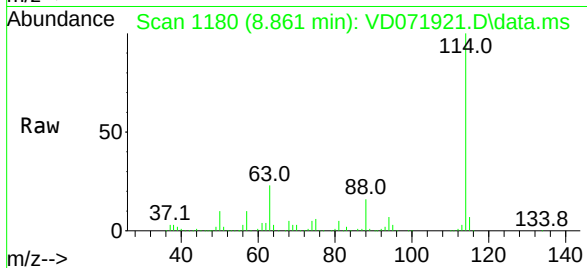

#35

Dibromofluoromethane

Concen: 50.509 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. -0.006 min

Lab File: VD071921.D

Acq: 08 Feb 2022 16:46




Tgt Ion:113 Resp: 331892


Ion Ratio Lower Upper

113 100

111 103.9 83.8 125.6

192 17.8 14.6 21.8


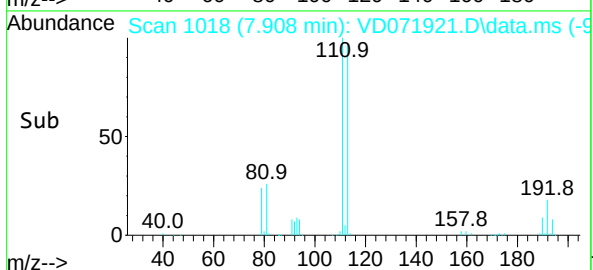
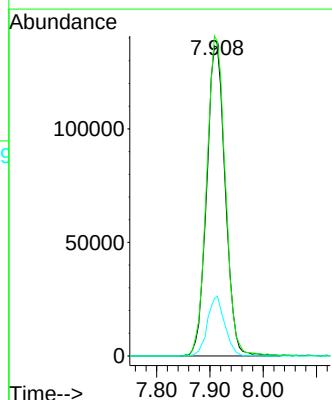
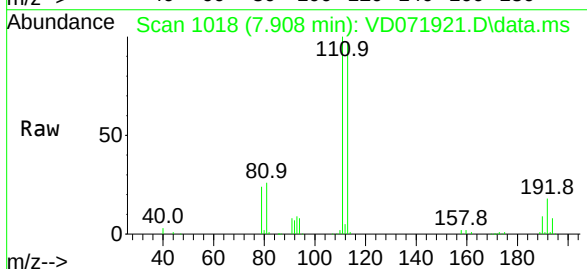


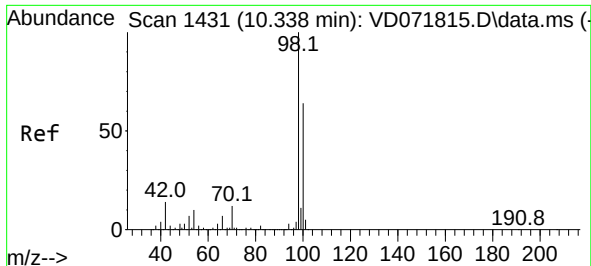

#50
Toluene-d8
Concen: 52.323 ug/l
RT: 10.332 min Scan# 1431
Delta R.T. -0.006 min
Lab File: VD071921.D
Acq: 08 Feb 2022 16:46




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 1284035
Ion Ratio Lower Upper
98 100
100 64.8 52.4 78.6

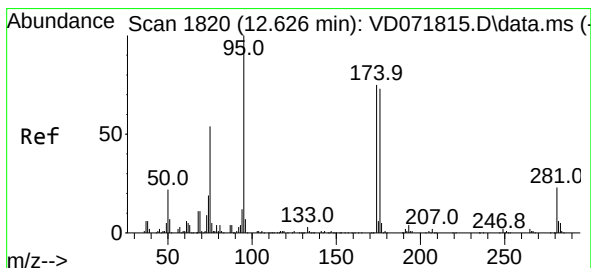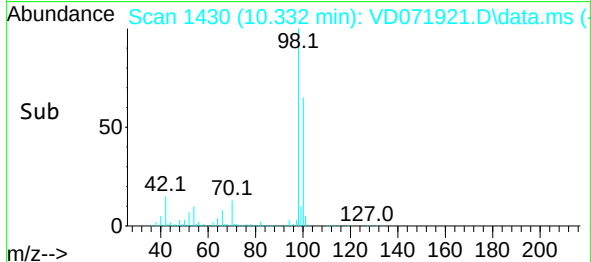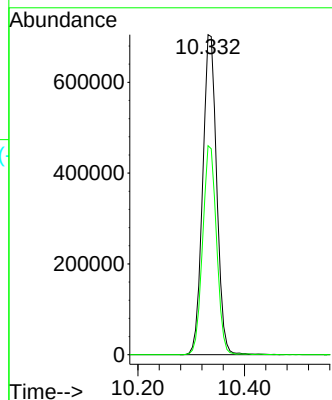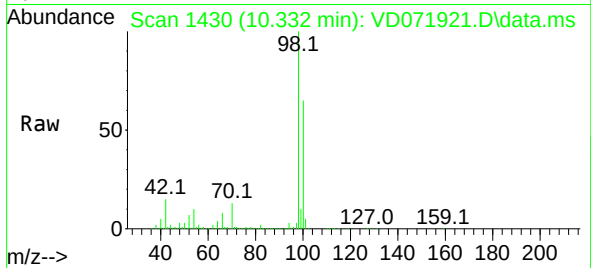

#62
4-Bromofluorobenzene
Concen: 55.850 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD071921.D
Acq: 08 Feb 2022 16:46

Tgt Ion: 95 Resp: 478628
Ion Ratio Lower Upper
95 100
174 73.5 0.0 152.8
176 71.1 0.0 145.4


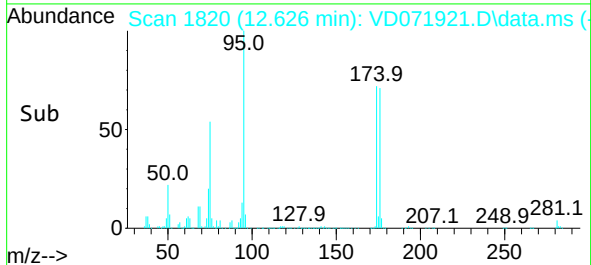
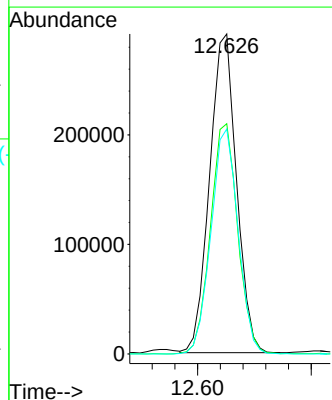
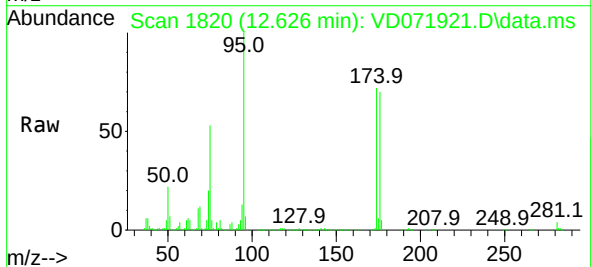


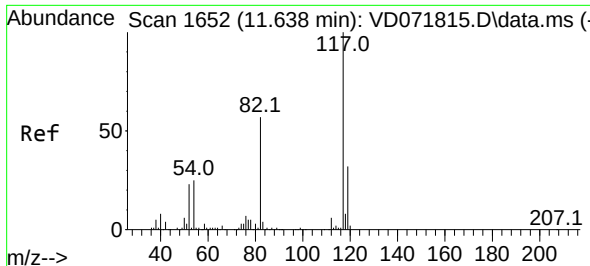

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.637 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD071921.D
Acq: 08 Feb 2022 16:46

Instrument :
MSVOA_D
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 983280
Ion Ratio Lower Upper
117 100
82 57.2 45.3 67.9
119 31.8 26.6 40.0

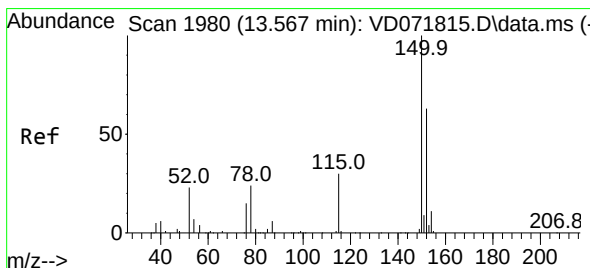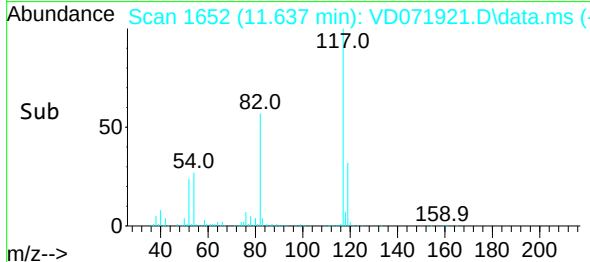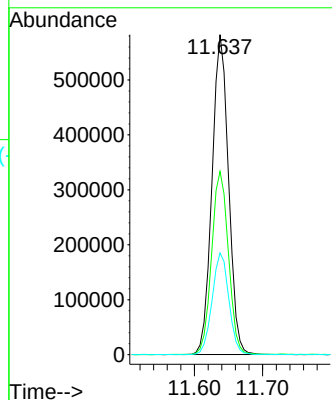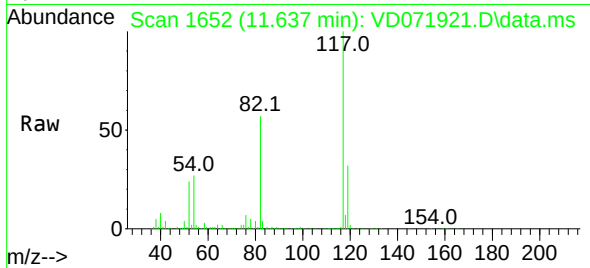

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD071921.D
Acq: 08 Feb 2022 16:46

Tgt Ion:152 Resp: 450407
Ion Ratio Lower Upper
152 100
115 62.2 31.3 93.8
150 155.6 0.0 348.6

