

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020822\
 Data File : VD071912.D
 Acq On : 08 Feb 2022 12:29
 Operator : VA/SY
 Sample : N1423-02
 Misc : 5.01G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP-21

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
 Title : SW846 8260

Signal : TIC: VD071912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.068	22	25	28	rVB2	1526	1939	1.35%	0.195%
2	2.138	35	37	41	rBV2	1514	2034	1.42%	0.205%
3	2.203	46	48	49	rBV2	4194	2937	2.05%	0.296%
4	2.450	89	90	93	rBV3	2966	3279	2.29%	0.330%
5	2.932	171	172	174	rVB2	3447	1576	1.10%	0.159%
6	3.332	237	240	243	rVB2	1954	2126	1.48%	0.214%
7	3.362	243	245	248	rVB	1676	1555	1.08%	0.157%
8	3.450	257	260	264	rVB	1697	2698	1.88%	0.272%
9	3.491	264	267	269	rBV3	1859	2086	1.46%	0.210%
10	3.626	287	290	293	rBV2	2401	2837	1.98%	0.286%
11	4.156	377	380	382	rBV2	1912	2354	1.64%	0.237%
12	4.297	401	404	407	rBV3	1501	2123	1.48%	0.214%
13	4.791	485	488	491	rBV2	1376	1814	1.27%	0.183%
14	4.873	500	502	505	rBV	2144	2071	1.44%	0.208%
15	4.932	509	512	515	rBV2	2608	2770	1.93%	0.279%
16	4.973	515	519	523	rVV2	1395	2137	1.49%	0.215%
17	5.162	548	551	552	rBV2	1773	1571	1.10%	0.158%
18	5.220	558	561	564	rBV2	1570	1611	1.12%	0.162%
19	5.491	606	607	611	rBV2	1542	1871	1.31%	0.188%
20	5.685	634	640	641	rBV2	1430	1739	1.21%	0.175%
21	5.750	648	651	654	rVB2	1424	1863	1.30%	0.188%
22	6.056	698	703	704	rBV2	1203	1645	1.15%	0.166%
23	6.232	730	733	737	rVB2	1321	2124	1.48%	0.214%
24	6.885	842	844	849	rBV2	1293	1730	1.21%	0.174%
25	7.191	895	896	899	rBV2	1560	1709	1.19%	0.172%
26	7.567	958	960	963	rBV2	1466	1759	1.23%	0.177%
27	7.667	975	977	979	rBV2	1962	2177	1.52%	0.219%
28	7.744	989	990	993	rBV	2725	2312	1.61%	0.233%
29	7.773	993	995	998	rVB2	2043	1601	1.12%	0.161%
30	7.908	1010	1018	1024	rBV2	23499	59246	41.33%	5.964%
31	7.973	1024	1029	1037	rVB2	37006	74940	52.28%	7.544%
32	8.120	1051	1054	1058	rBV	1401	1841	1.28%	0.185%
33	8.326	1081	1089	1097	rVB3	28757	70967	49.50%	7.144%
34	8.861	1171	1180	1187	rBV2	55539	113319	79.05%	11.408%
35	9.108	1220	1222	1225	rBV2	1471	1608	1.12%	0.162%
36	9.167	1231	1232	1236	rBV	1468	1560	1.09%	0.157%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020822\
 Data File : VD071912.D
 Acq On : 08 Feb 2022 12:29
 Operator : VA/SY
 Sample : N1423-02
 Misc : 5.01G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP-21

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
 Title : SW846 8260

37	9.267	1245	1249	1254	rVB	2792	3569	2.49%	0.359%
38	9.314	1254	1257	1260	rBV2	1033	1635	1.14%	0.165%
39	9.344	1260	1262	1266	rVB2	1949	2375	1.66%	0.239%
40	9.579	1299	1302	1307	rVB2	1156	1722	1.20%	0.173%
41	9.661	1312	1316	1319	rBV2	1245	1971	1.37%	0.198%
42	9.832	1339	1345	1346	rBV2	1537	2417	1.69%	0.243%
43	10.150	1398	1399	1403	rVB2	1626	1597	1.11%	0.161%
44	10.332	1424	1430	1438	rBV	78874	143354	100.00%	14.431%
45	10.444	1448	1449	1453	rBV2	1680	1555	1.08%	0.157%
46	10.538	1461	1465	1466	rBV2	1818	1914	1.34%	0.193%
47	10.791	1504	1508	1511	rBV2	1674	2115	1.48%	0.213%
48	11.638	1644	1652	1660	rBV	79794	141218	98.51%	14.216%
49	11.838	1681	1686	1694	rVB4	2719	7322	5.11%	0.737%
50	12.073	1719	1726	1727	rBV2	1231	2556	1.78%	0.257%
51	12.173	1740	1743	1746	rBV2	1795	2903	2.03%	0.292%
52	12.455	1789	1791	1794	rBV2	1275	1736	1.21%	0.175%
53	12.538	1804	1805	1809	rBV2	1913	1738	1.21%	0.175%
54	12.620	1813	1819	1827	rBV	57518	98294	68.57%	9.895%
55	12.749	1838	1841	1843	rBV2	1615	2004	1.40%	0.202%
56	12.879	1859	1863	1864	rBV2	1280	1542	1.08%	0.155%
57	12.996	1880	1883	1885	rVB3	1297	1584	1.10%	0.159%
58	13.038	1888	1890	1893	rBV2	1561	1780	1.24%	0.179%
59	13.202	1916	1918	1923	rVB2	1703	2231	1.56%	0.225%
60	13.502	1964	1969	1973	rBV3	2812	4900	3.42%	0.493%
61	13.561	1973	1979	1988	rVB	76556	131579	91.79%	13.246%
62	14.055	2061	2063	2065	rBV2	1529	1753	1.22%	0.176%
63	14.079	2065	2067	2070	rVB2	1773	1936	1.35%	0.195%
64	14.314	2103	2107	2108	rBV4	1633	1601	1.12%	0.161%
65	14.438	2125	2128	2130	rBV2	1621	2025	1.41%	0.204%
66	14.573	2150	2151	2154	rBV2	1996	1600	1.12%	0.161%
67	14.726	2175	2177	2179	rVB2	2068	1594	1.11%	0.160%
68	14.743	2179	2180	2183	rBV2	1929	1827	1.27%	0.184%
69	14.808	2189	2191	2195	rVB4	2277	2299	1.60%	0.231%
70	14.955	2214	2216	2218	rBV2	2751	1814	1.27%	0.183%
71	15.185	2253	2255	2257	rVB2	1821	1637	1.14%	0.165%
72	15.202	2257	2258	2262	rBV3	1448	1725	1.20%	0.174%
73	15.373	2284	2287	2289	rBV4	2553	3283	2.29%	0.330%
74	15.579	2318	2322	2325	rBV5	1724	2841	1.98%	0.286%
75	15.655	2333	2335	2336	rBV	2269	1607	1.12%	0.162%
76	15.779	2355	2356	2359	rBV2	1972	2425	1.69%	0.244%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020822\
Data File : VD071912.D
Acq On : 08 Feb 2022 12:29
Operator : VA/SY
Sample : N1423-02
Misc : 5.01G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP-21

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M

Title : SW846 8260

77	16.014	2394	2396	2400	rBV3	1888	3111	2.17%	0.313%
78	16.049	2400	2402	2404	rVB2	2870	1751	1.22%	0.176%
79	16.214	2428	2430	2432	rBV	1884	1790	1.25%	0.180%
80	16.496	2476	2478	2480	rVB2	2144	1618	1.13%	0.163%
81	16.520	2480	2482	2485	rBV2	2239	2014	1.40%	0.203%
82	16.614	2496	2498	2501	rVB3	2426	2189	1.53%	0.220%
83	16.679	2507	2509	2511	rBV2	2179	1788	1.25%	0.180%




Sum of corrected areas: 993368

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD071912\
Data File : VD071912.D
Acq On : 08 Feb 2022 12:29
Operator : VA/SY
Sample : N1423-02
Misc : 5.01G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP-21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

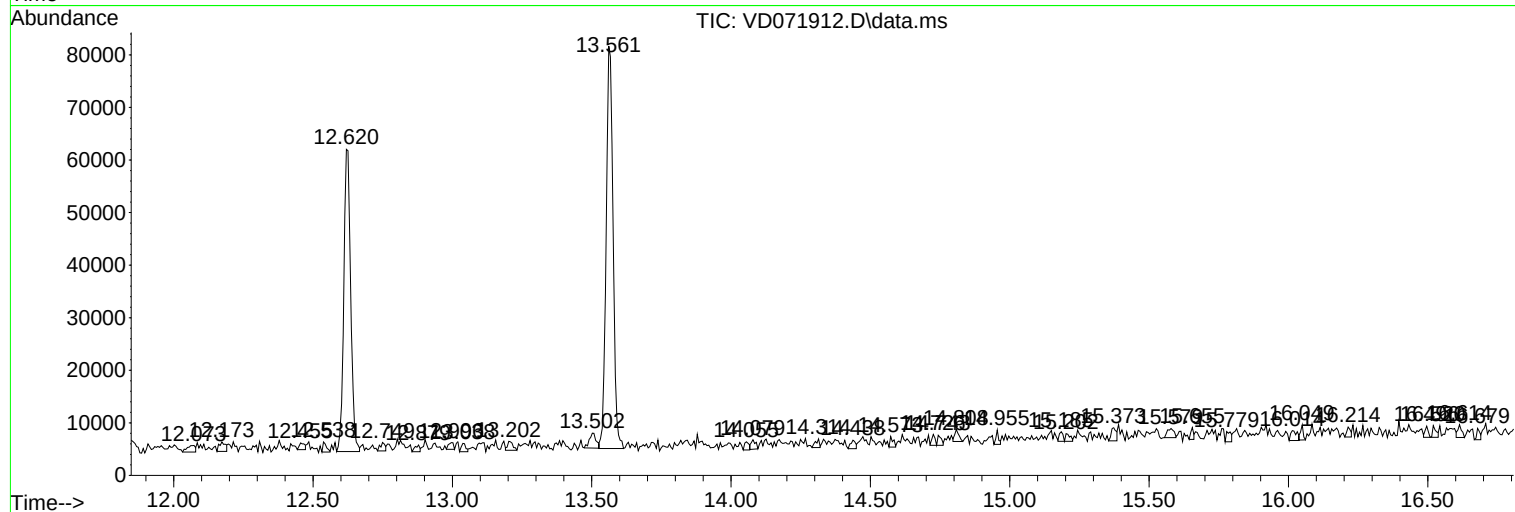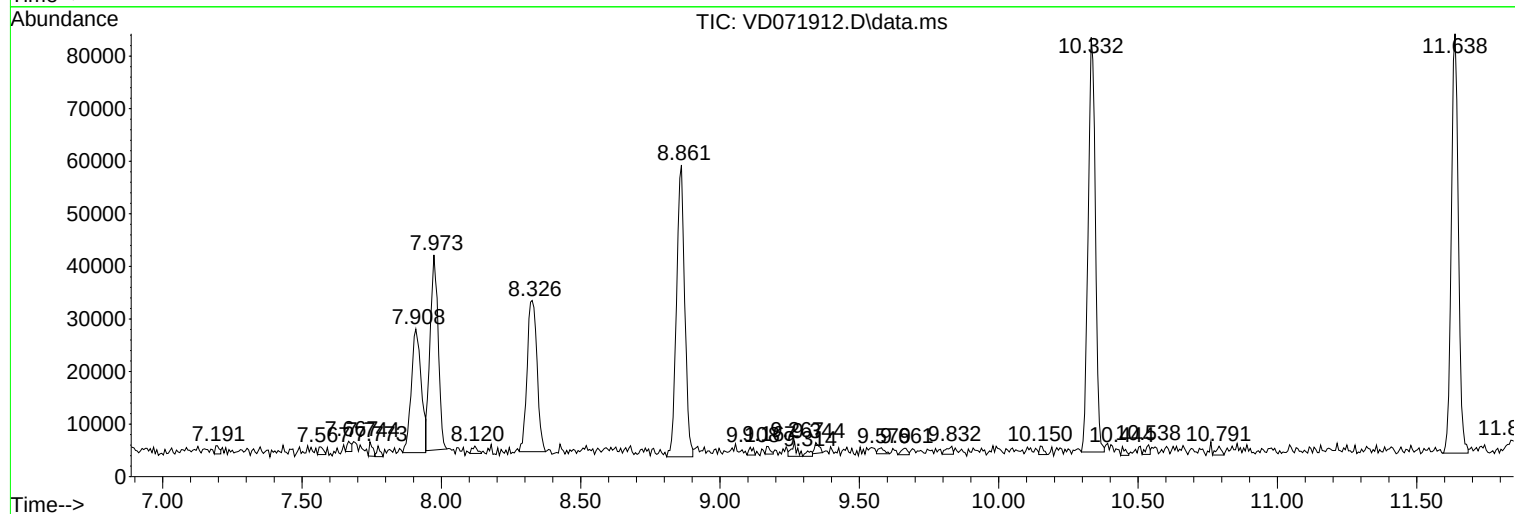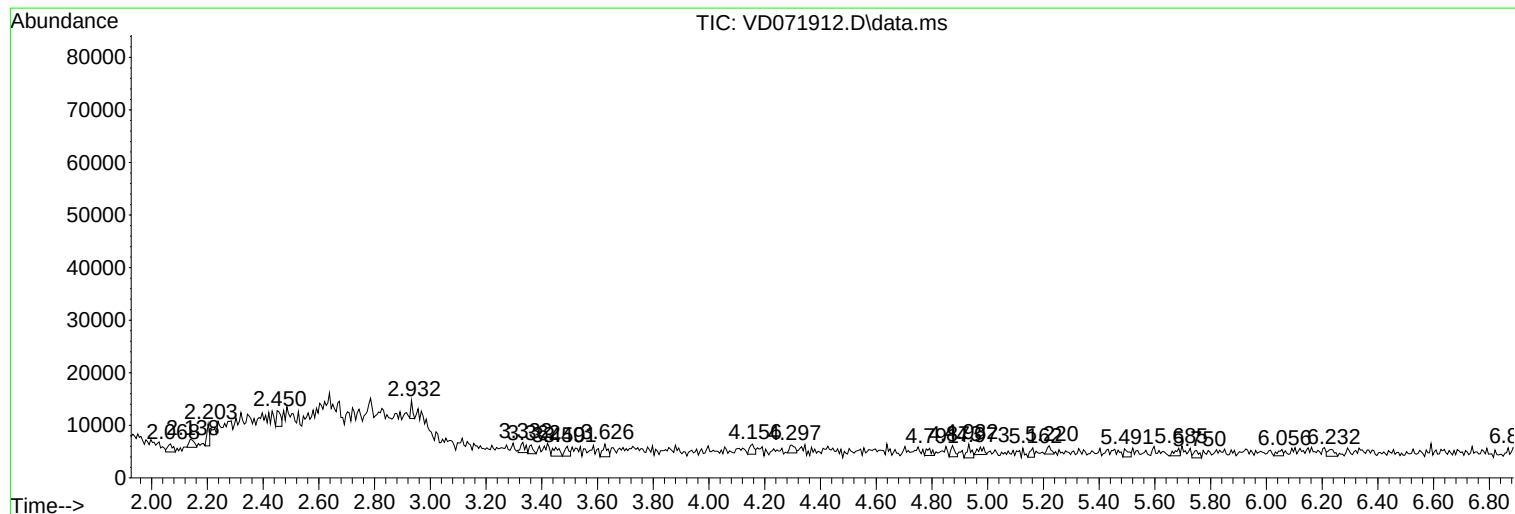

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020822\
Data File : VD071912.D
Acq On : 08 Feb 2022 12:29
Operator : VA/SY
Sample : N1423-02
Misc : 5.01G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP-21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020822\
Data File : VD071912.D
Acq On : 08 Feb 2022 12:29
Operator : VA/SY
Sample : N1423-02
Misc : 5.01G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP-21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------