
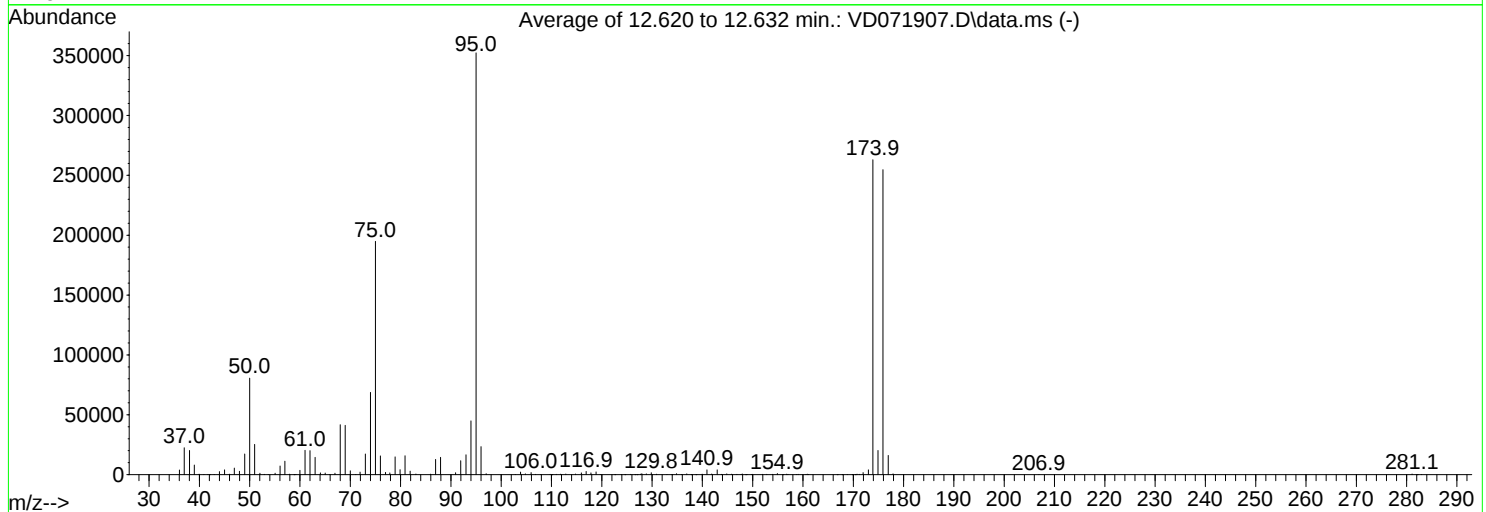


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020822\
Data File : VD071907.D
Acq On : 08 Feb 2022 08:48
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
Title : SW846 8260
Last Update : Thu Jan 27 06:04:38 2022

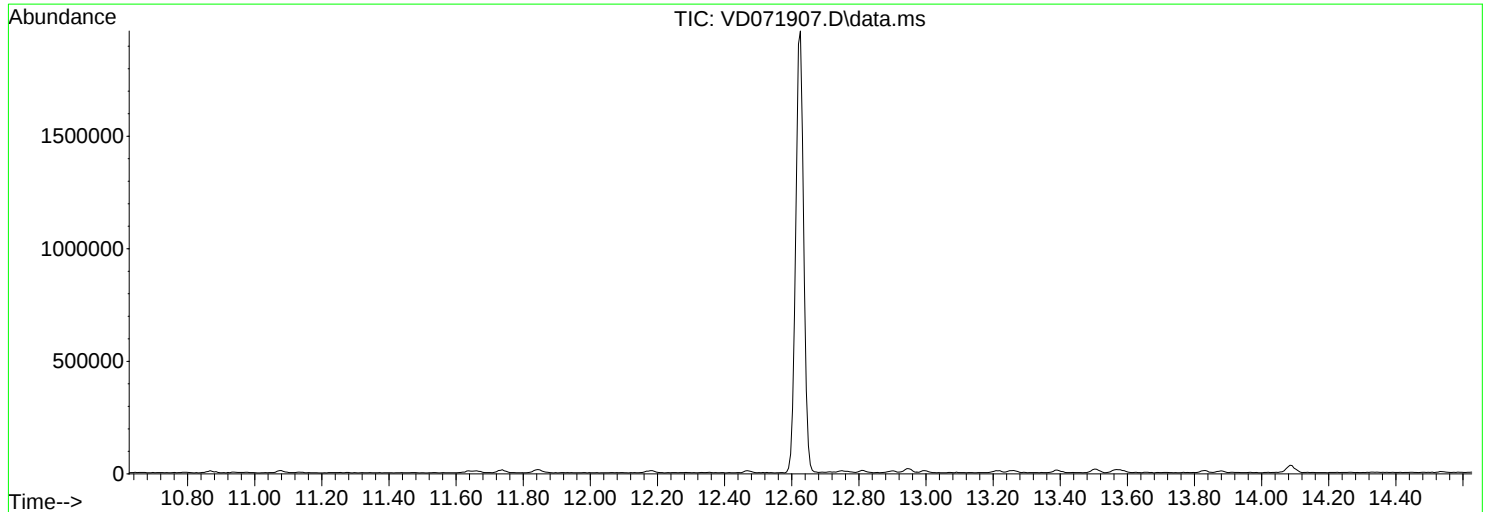

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.9	80632	PASS
75	95	30	60	55.3	194837	PASS
95	95	100	100	100.0	352320	PASS
96	95	5	9	6.6	23413	PASS
173	174	0.00	2	1.5	4067	PASS
174	95	50	100	74.7	263019	PASS
175	174	5	9	7.7	20191	PASS
176	174	95	101	96.9	254784	PASS
177	176	5	9	6.3	16086	PASS