
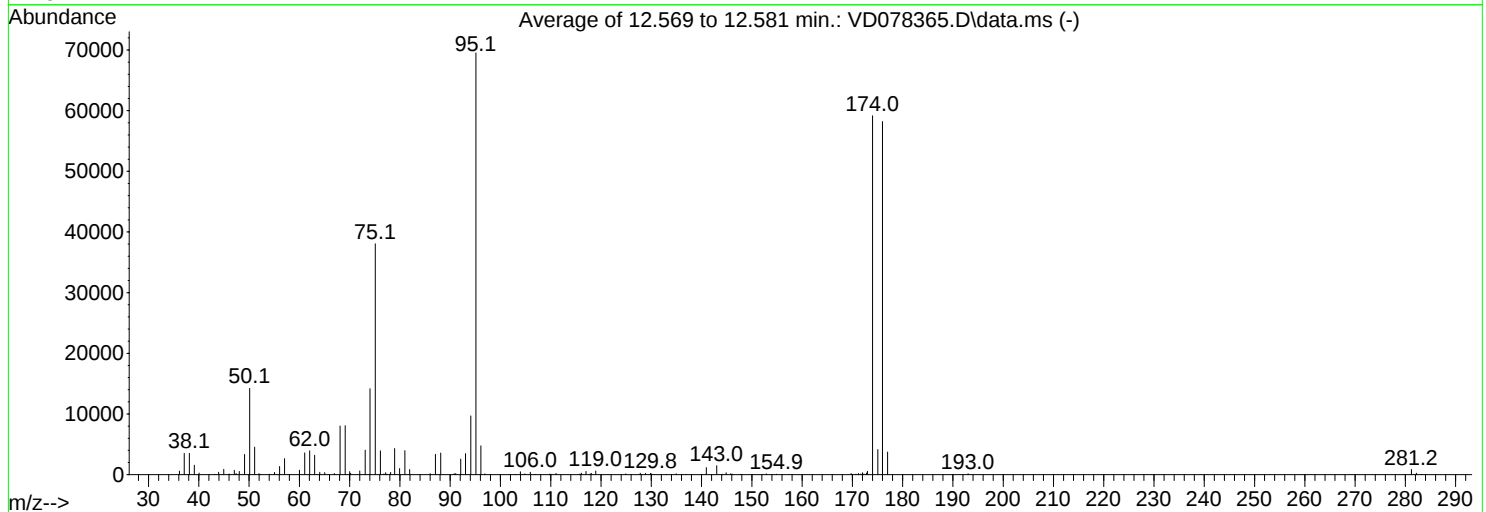


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD020824\
Data File : VD078365.D
Acq On : 08 Feb 2024 09:57
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D013024S.M
Title : SW846 8260
Last Update : Thu Feb 01 03:58:19 2024

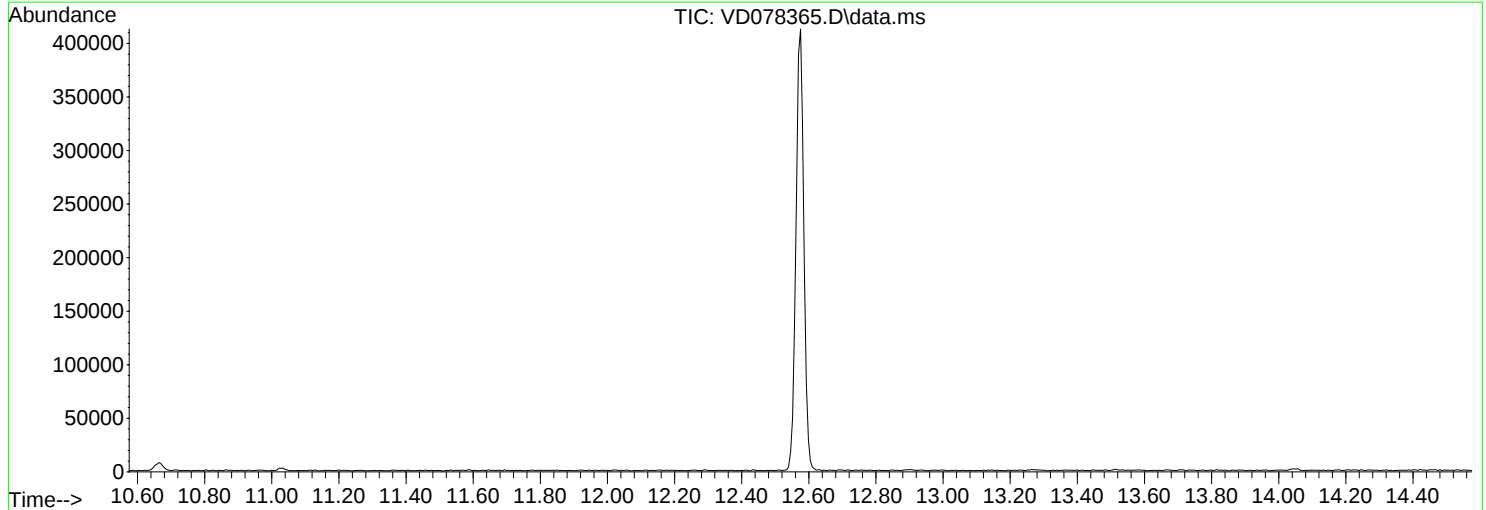

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	14222	PASS
75	95	30	60	54.7	38067	PASS
95	95	100	100	100.0	69533	PASS
96	95	5	9	6.8	4754	PASS
173	174	0.00	2	0.9	561	PASS
174	95	50	100	85.1	59163	PASS
175	174	5	9	7.0	4133	PASS
176	174	95	101	98.4	58227	PASS
177	176	5	9	6.4	3734	PASS