

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021422\
 Data File : VD071954.D
 Acq On : 14 Feb 2022 13:54
 Operator : VA/SY
 Sample : N1521-01
 Misc : 6.64G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP1-A

Quant Time: Feb 15 00:35:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 27 06:04:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	395159	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	764024	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	734056	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	313085	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	258392	51.734	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.460%
35) Dibromofluoromethane	7.914	113	252643	50.306	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.620%
50) Toluene-d8	10.338	98	995284	53.065	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	106.120%
62) 4-Bromofluorobenzene	12.626	95	321518	49.088	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	98.180%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021422\
Data File : VD071954.D
Acq On : 14 Feb 2022 13:54
Operator : VA/SY
Sample : N1521-01
Misc : 6.64G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP1-A

Quant Time: Feb 15 00:35:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012622S.M
Quant Title : SW846 8260
QLast Update : Thu Jan 27 06:04:38 2022
Response via : Initial Calibration




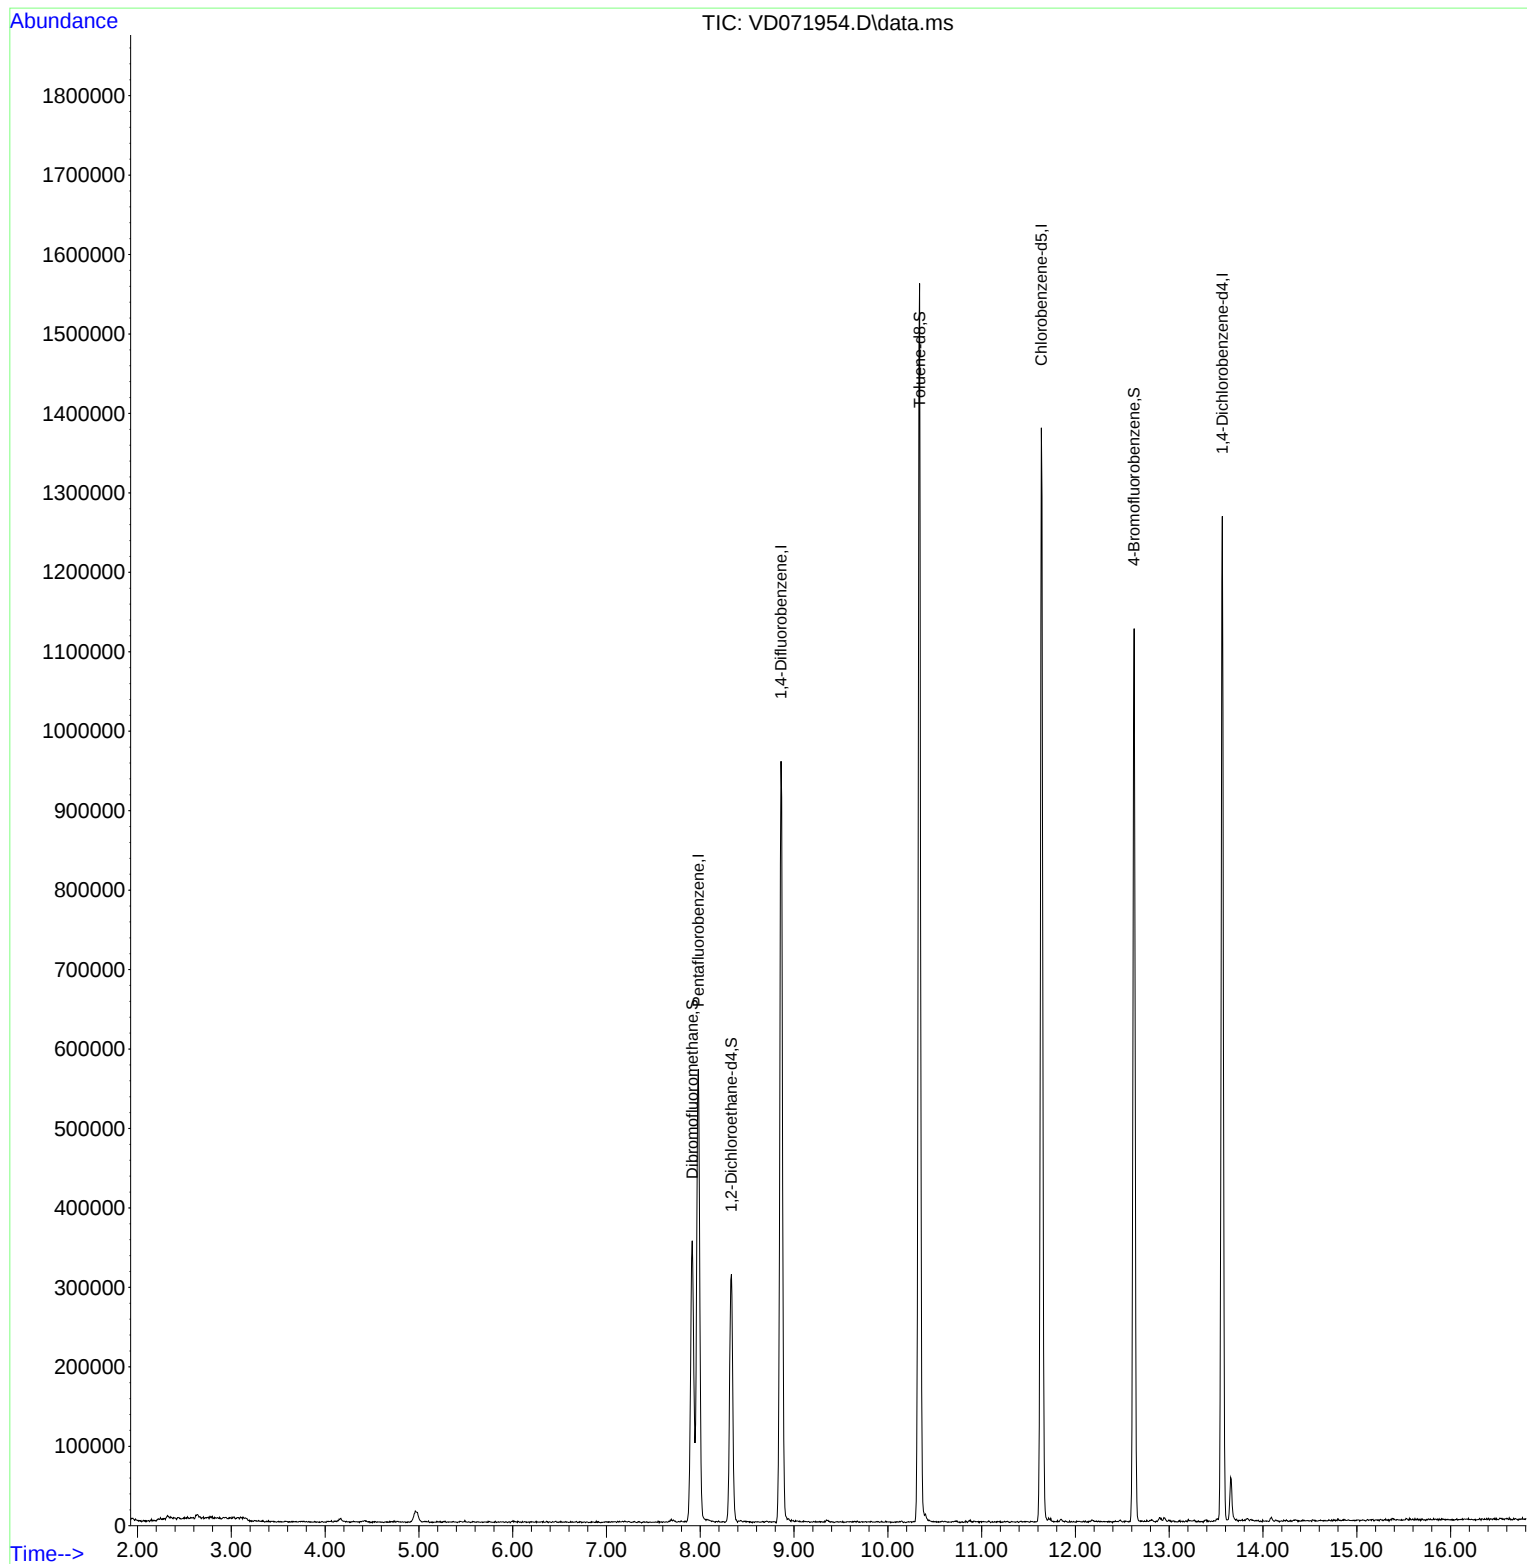


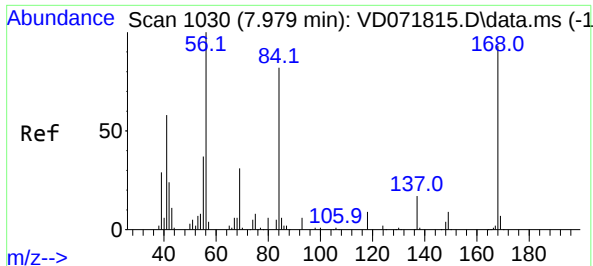

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD071954.D
Acq: 14 Feb 2022 13:54




Instrument :
MSVOA_D
ClientSampleId :
TP1-A


Tgt Ion:168 Resp: 395159
Ion Ratio Lower Upper
168 100
99 63.7 49.8 74.6

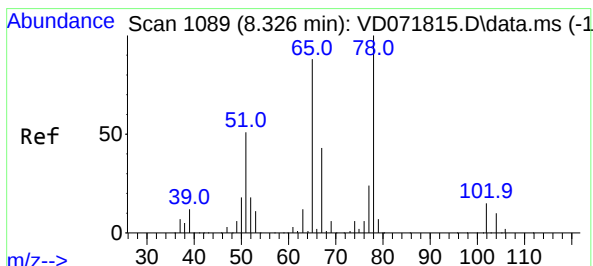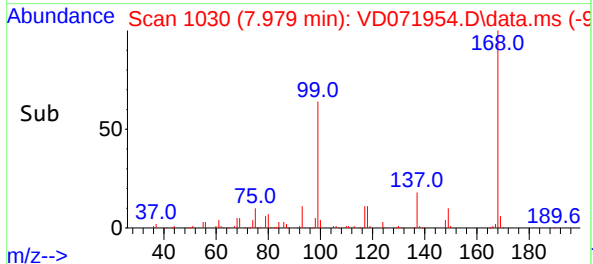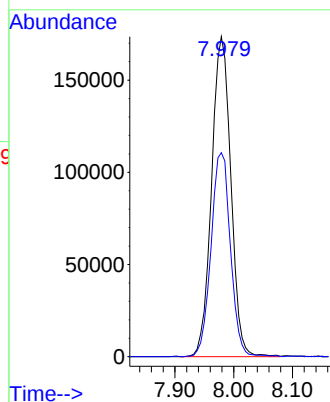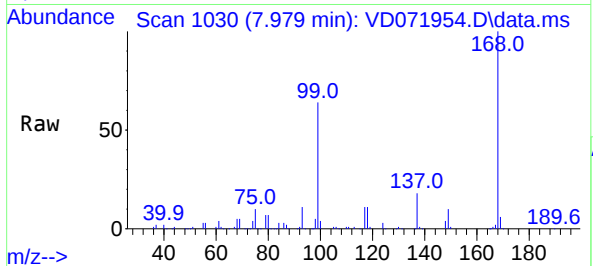

#33
1,2-Dichloroethane-d4
Concen: 51.734 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. 0.006 min
Lab File: VD071954.D
Acq: 14 Feb 2022 13:54

Tgt Ion: 65 Resp: 258392
Ion Ratio Lower Upper
65 100
67 51.6 0.0 101.4

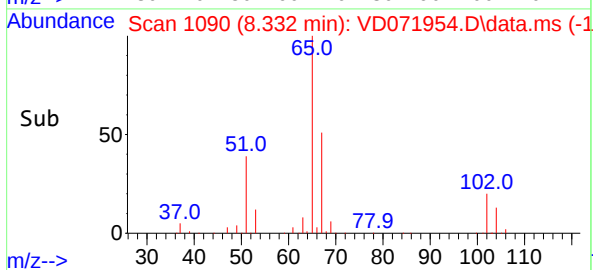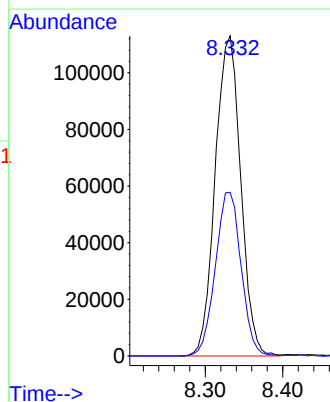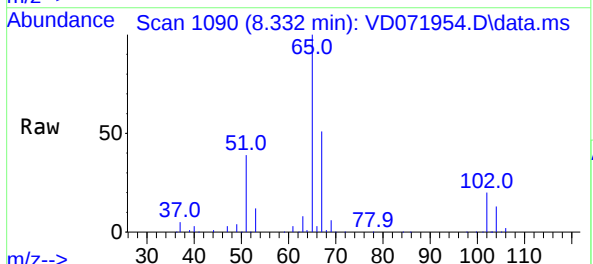




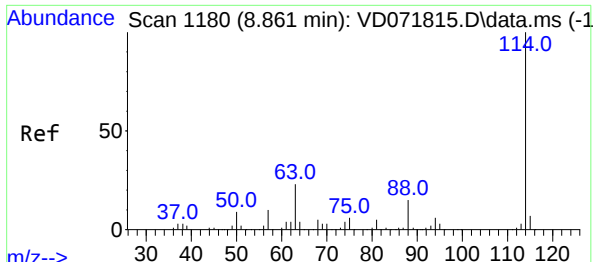


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.000 min
Lab File: VD071954.D
Acq: 14 Feb 2022 13:54

Instrument :
MSVOA_D
ClientSampleId :
TP1-A

Tgt Ion:114 Resp: 764024




Ion	Ratio	Lower	Upper
114	100		
63	22.1	0.0	46.6
88	16.0	0.0	33.2

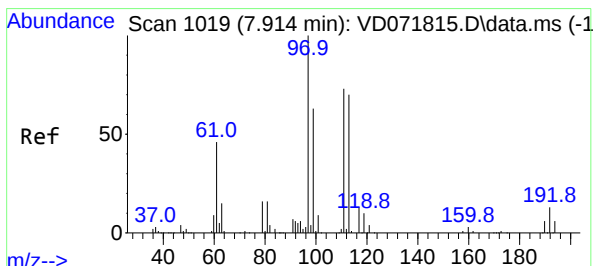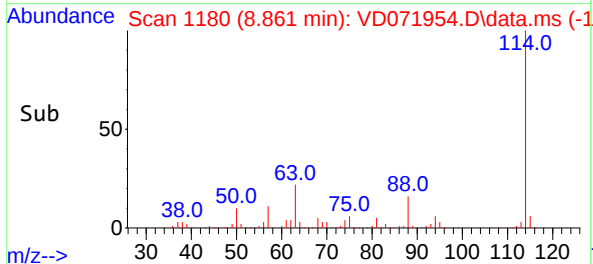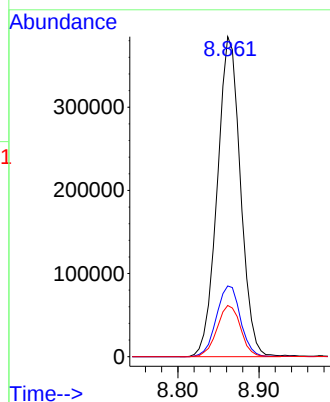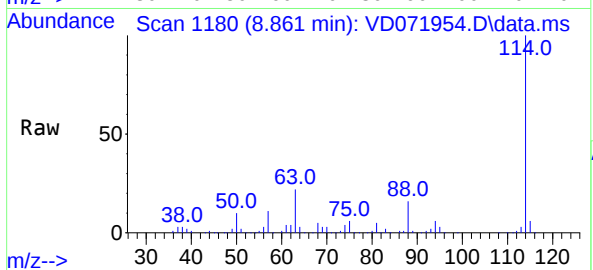


#35
Dibromofluoromethane
Concen: 50.306 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.000 min
Lab File: VD071954.D
Acq: 14 Feb 2022 13:54

Tgt Ion:113 Resp: 252643

Ion	Ratio	Lower	Upper
113	100		
111	101.6	83.8	125.6
192	17.2	14.6	21.8


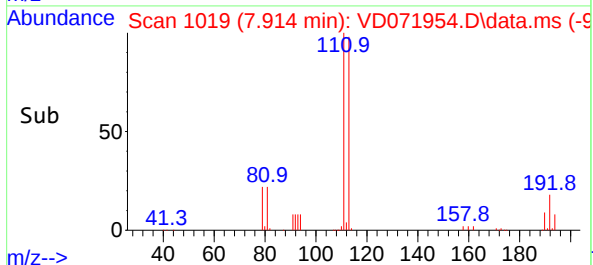
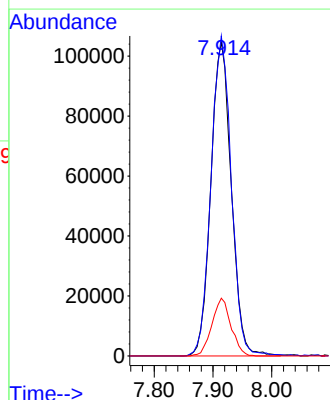
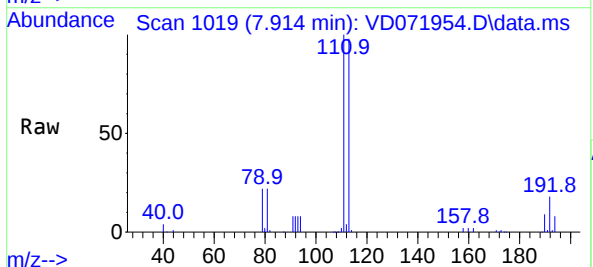


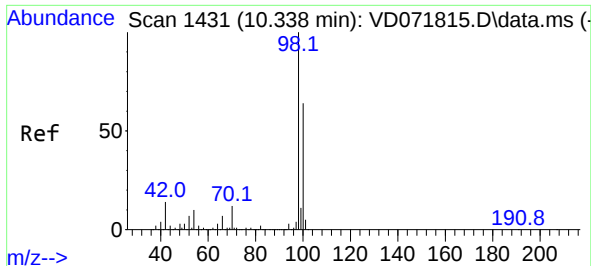

#50
Toluene-d8
Concen: 53.065 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD071954.D
Acq: 14 Feb 2022 13:54




Instrument :
MSVOA_D
ClientSampleId :
TP1-A


Tgt Ion: 98 Resp: 995284
Ion Ratio Lower Upper
98 100
100 64.5 52.4 78.6

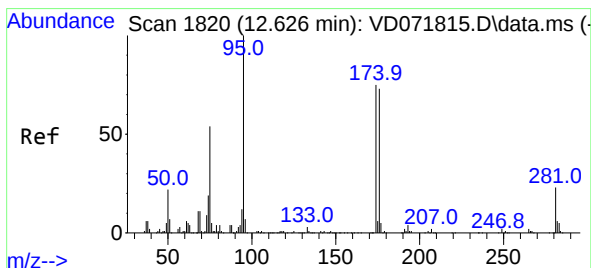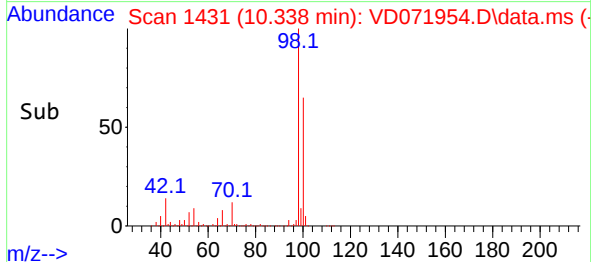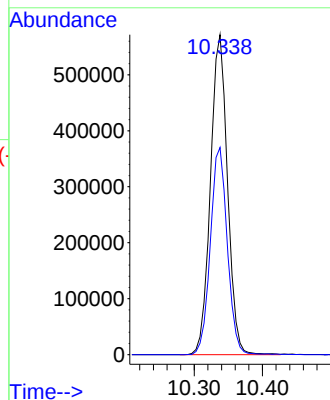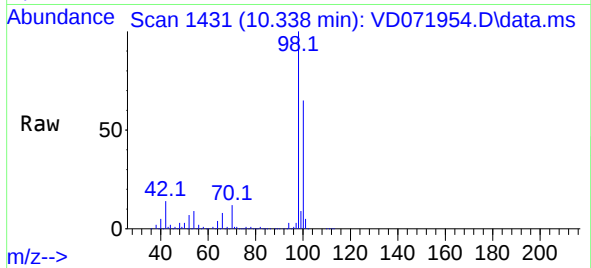

#62
4-Bromofluorobenzene
Concen: 49.088 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD071954.D
Acq: 14 Feb 2022 13:54

Tgt Ion: 95 Resp: 321518
Ion Ratio Lower Upper
95 100
174 75.7 0.0 152.8
176 71.9 0.0 145.4


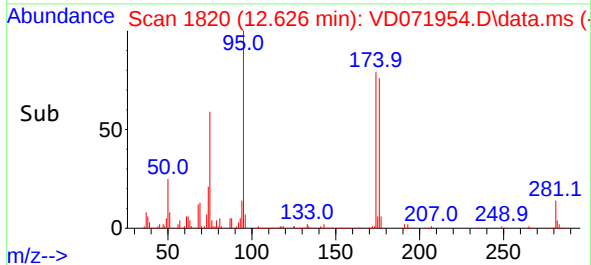
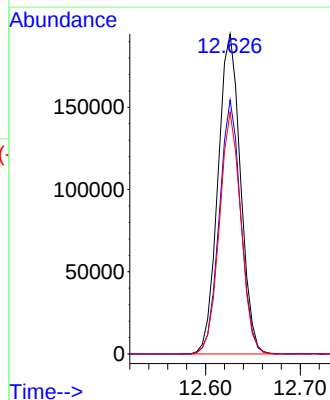
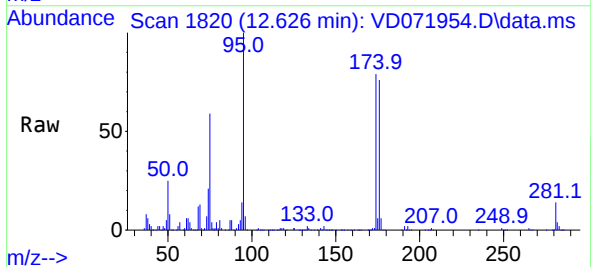


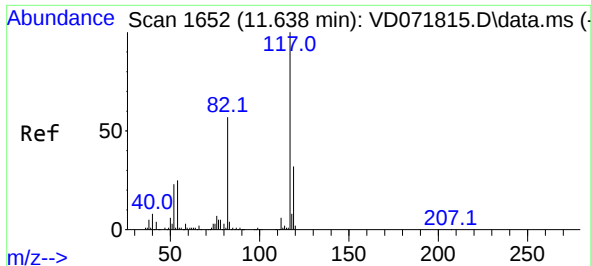

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VD071954.D
Acq: 14 Feb 2022 13:54

Instrument :
MSVOA_D
ClientSampleId :
TP1-A

Tgt Ion:117 Resp: 734056
Ion Ratio Lower Upper
117 100
82 59.8 45.3 67.9
119 32.0 26.6 40.0

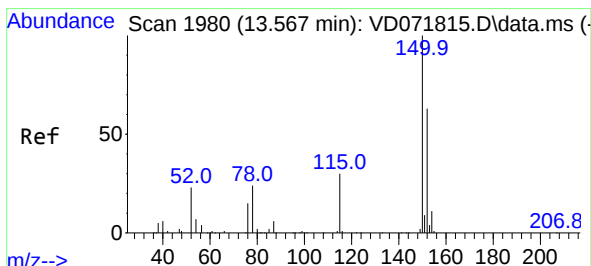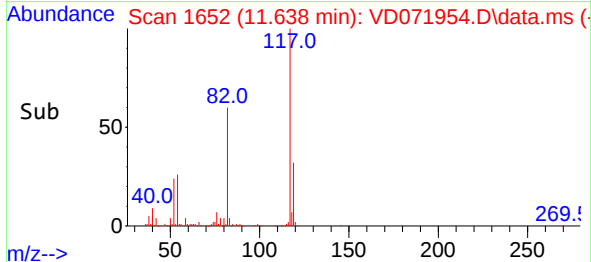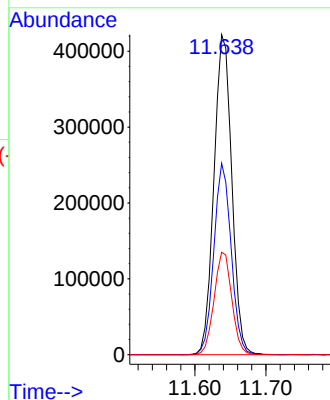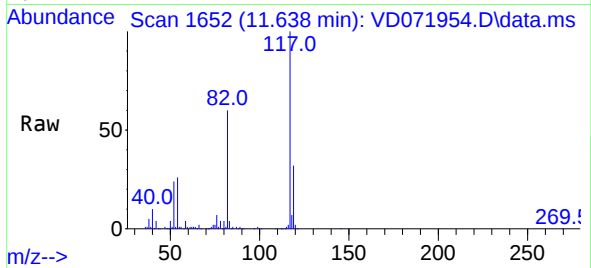

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD071954.D
Acq: 14 Feb 2022 13:54

Tgt Ion:152 Resp: 313085
Ion Ratio Lower Upper
152 100
115 60.6 31.3 93.8
150 157.3 0.0 348.6

