

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022122\
 Data File : VD072025.D
 Acq On : 21 Feb 2022 10:28
 Operator : VA/SY
 Sample : VD0221SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0221SBL01

Quant Time: Feb 22 00:32:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021822S.M
 Quant Title : SW846 8260
 QLast Update : Sat Feb 19 04:05:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	497329	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	836912	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	755933	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	338376	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	267245	51.804	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.600%
35) Dibromofluoromethane	7.914	113	259508	51.179	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.360%
50) Toluene-d8	10.338	98	988889	52.590	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	105.180%
62) 4-Bromofluorobenzene	12.626	95	323874	46.889	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	93.780%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022122\
Data File : VD072025.D
Acq On : 21 Feb 2022 10:28
Operator : VA/SY
Sample : VD0221SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0221SBL01

Quant Time: Feb 22 00:32:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021822S.M
Quant Title : SW846 8260
QLast Update : Sat Feb 19 04:05:38 2022
Response via : Initial Calibration

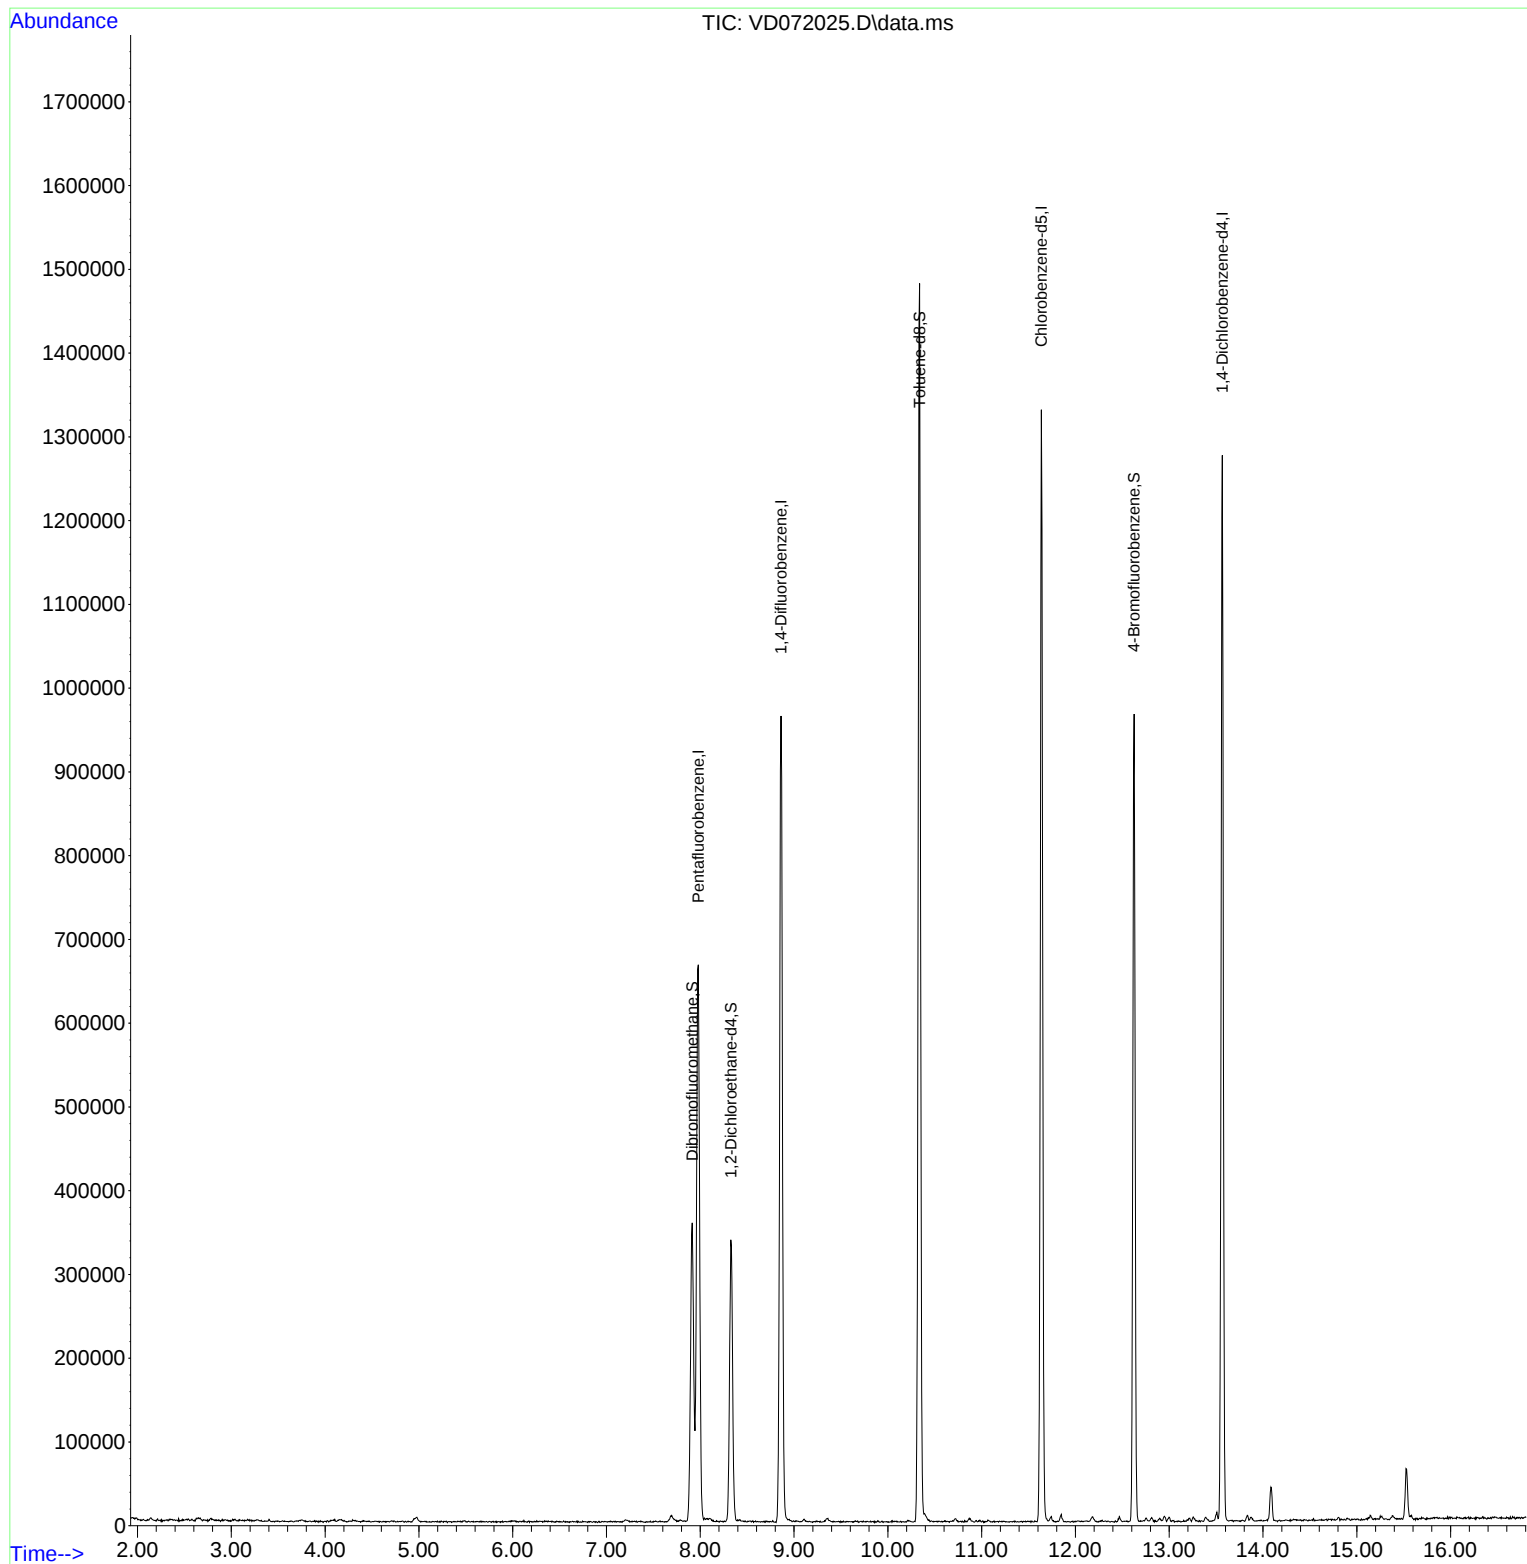

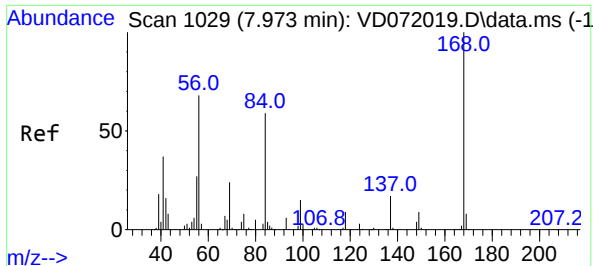

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.979 min Scan# 1029

Delta R.T. 0.006 min

Lab File: VD072025.D

Acq: 21 Feb 2022 10:28

Instrument :

MSVOA_D

ClientSampleId :





VD0221SBL01

Tgt Ion:168 Resp: 497329

Ion Ratio Lower Upper

168 100

99 57.8 47.1 70.7

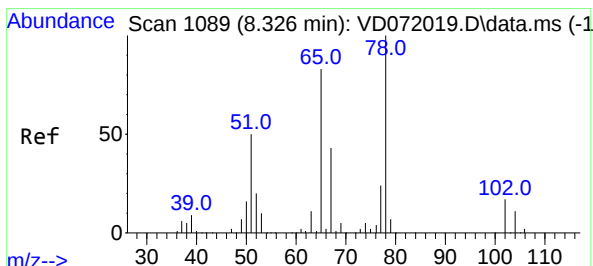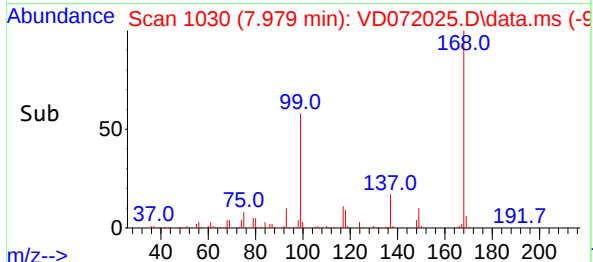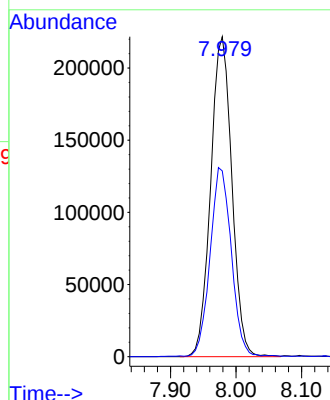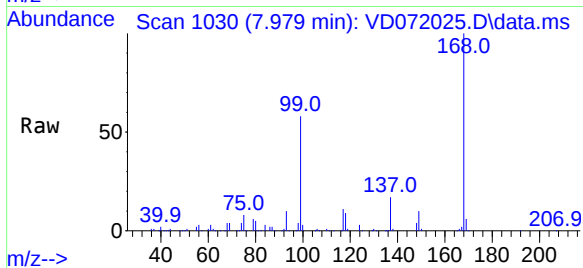

1,2-Dichloroethane-d4

Concen: 51.804 ug/l

RT: 8.326 min Scan# 1089

Delta R.T. 0.000 min

Lab File: VD072025.D




Acq: 21 Feb 2022 10:28


Tgt Ion: 65 Resp: 267245

Ion Ratio Lower Upper

65 100

67 52.3 0.0 105.6

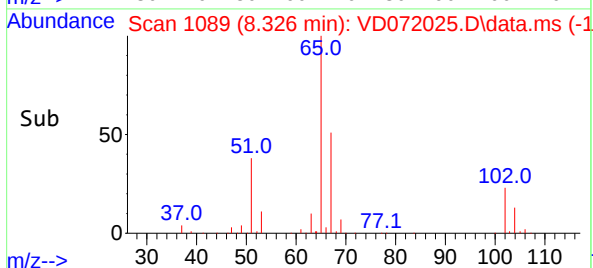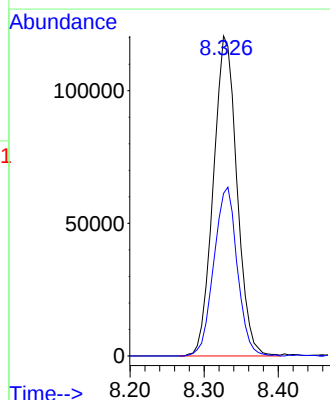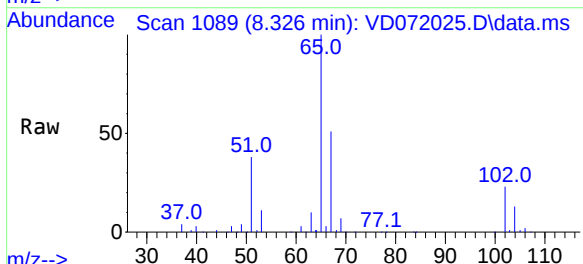




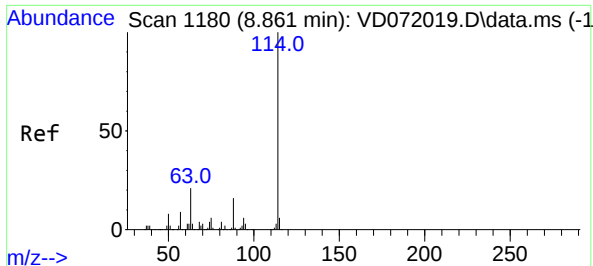


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD072025.D
Acq: 21 Feb 2022 10:28

Instrument :
MSVOA_D
ClientSampleId :
VD0221SBL01

Tgt Ion:114 Resp: 836912




Ion	Ratio	Lower	Upper
114	100		
63	21.1	0.0	42.2
88	16.3	0.0	31.2

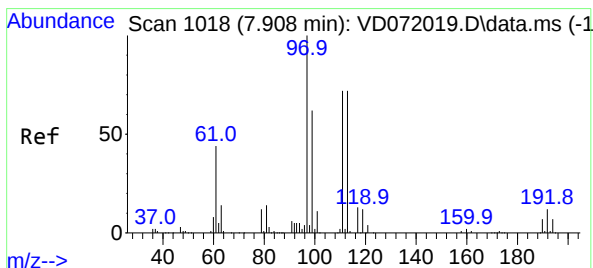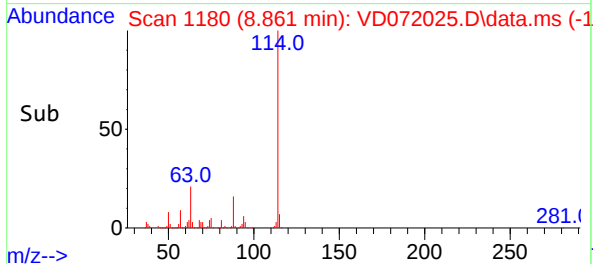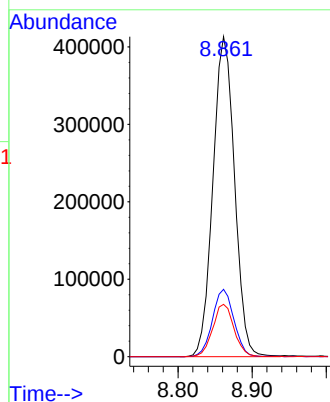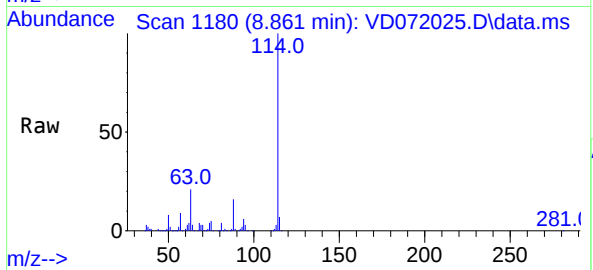


#35
Dibromofluoromethane
Concen: 51.179 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. 0.006 min
Lab File: VD072025.D
Acq: 21 Feb 2022 10:28

Tgt Ion:113 Resp: 259508

Ion	Ratio	Lower	Upper
113	100		
111	100.9	83.0	124.4
192	19.4	15.3	22.9


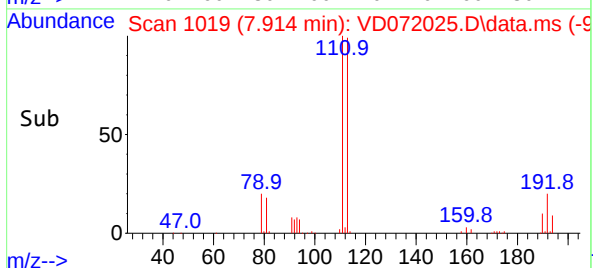
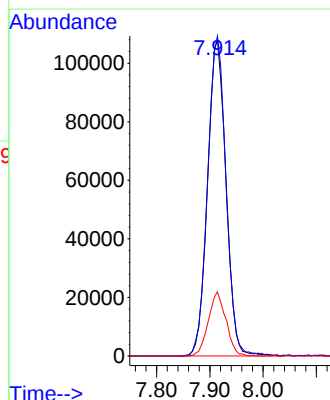
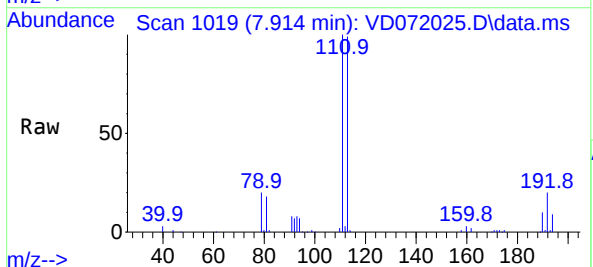


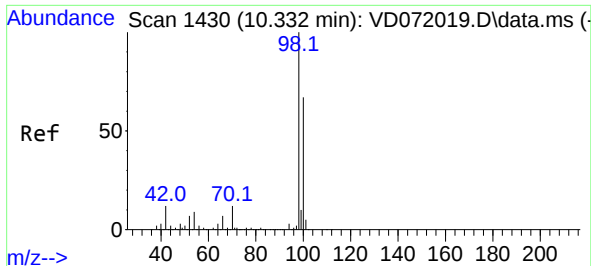

#50
Toluene-d8
Concen: 52.590 ug/l
RT: 10.338 min Scan# 1430
Delta R.T. 0.006 min
Lab File: VD072025.D
Acq: 21 Feb 2022 10:28




Instrument :
MSVOA_D
ClientSampleId :
VD0221SBL01


Tgt Ion: 98 Resp: 988889
Ion Ratio Lower Upper
98 100
100 67.2 53.8 80.6

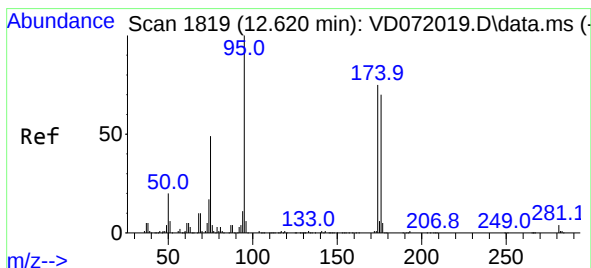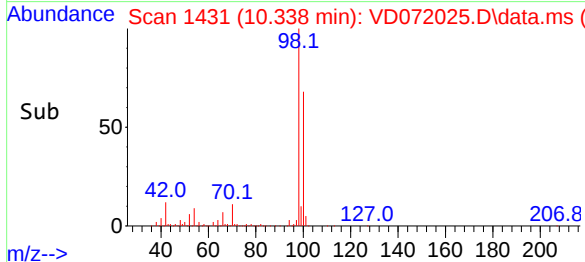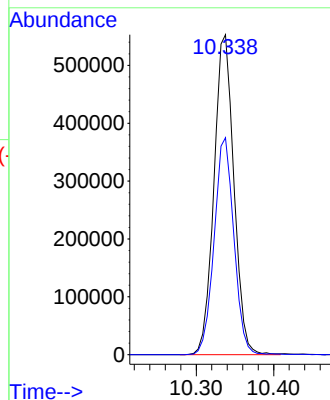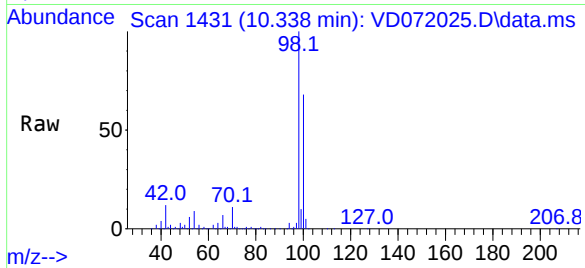

#62
4-Bromofluorobenzene
Concen: 46.889 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. 0.006 min
Lab File: VD072025.D
Acq: 21 Feb 2022 10:28

Tgt Ion: 95 Resp: 323874
Ion Ratio Lower Upper
95 100
174 80.8 0.0 155.0
176 77.0 0.0 148.8


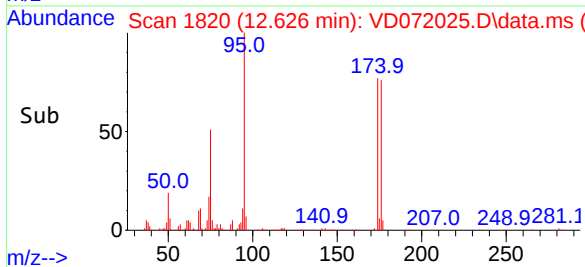
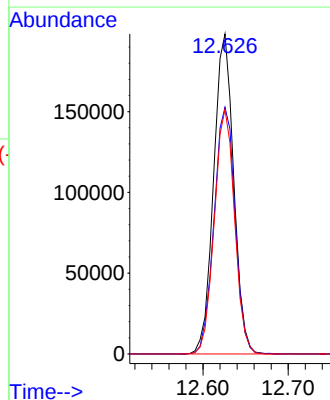
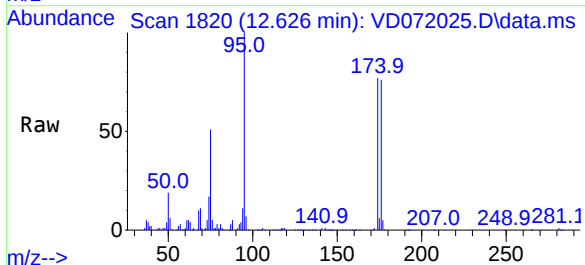


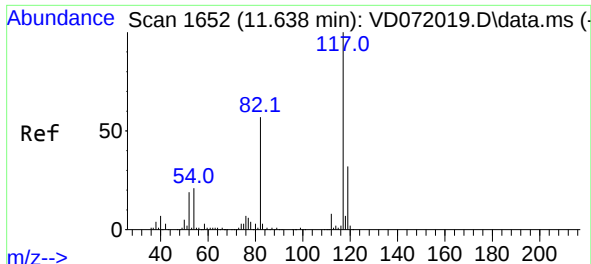

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VD072025.D
Acq: 21 Feb 2022 10:28

Instrument :
MSVOA_D
ClientSampleId :
VD0221SBL01

Tgt Ion:117 Resp: 755933
Ion Ratio Lower Upper
117 100
82 57.1 45.4 68.0
119 32.6 25.4 38.2

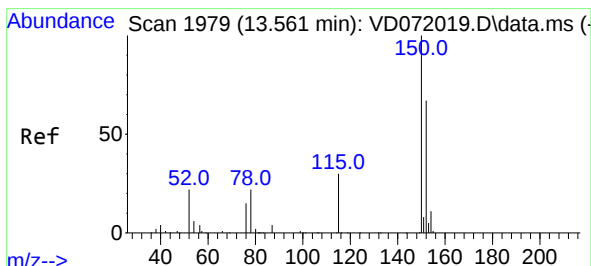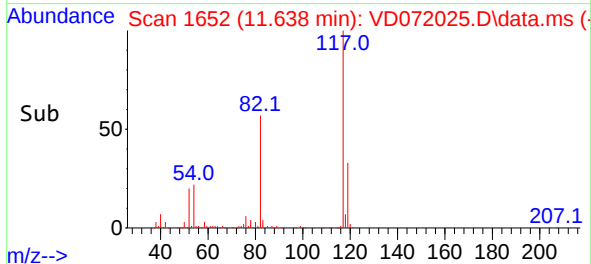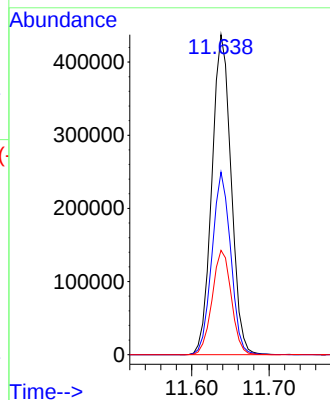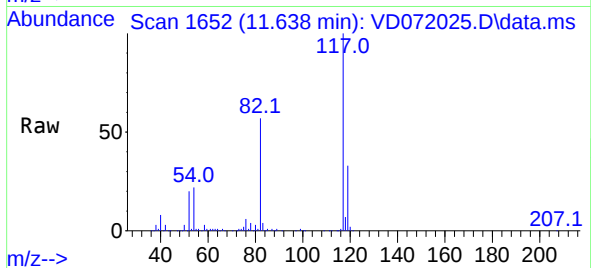

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. 0.006 min
Lab File: VD072025.D
Acq: 21 Feb 2022 10:28

Tgt Ion:152 Resp: 338376
Ion Ratio Lower Upper
152 100
115 59.2 29.9 89.7
150 158.8 0.0 347.6

