


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD022222\
Data File : VD072046.D
Acq On : 22 Feb 2022 08:58
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D021822S.M
Title : SW846 8260
Last Update : Sat Feb 19 04:05:38 2022

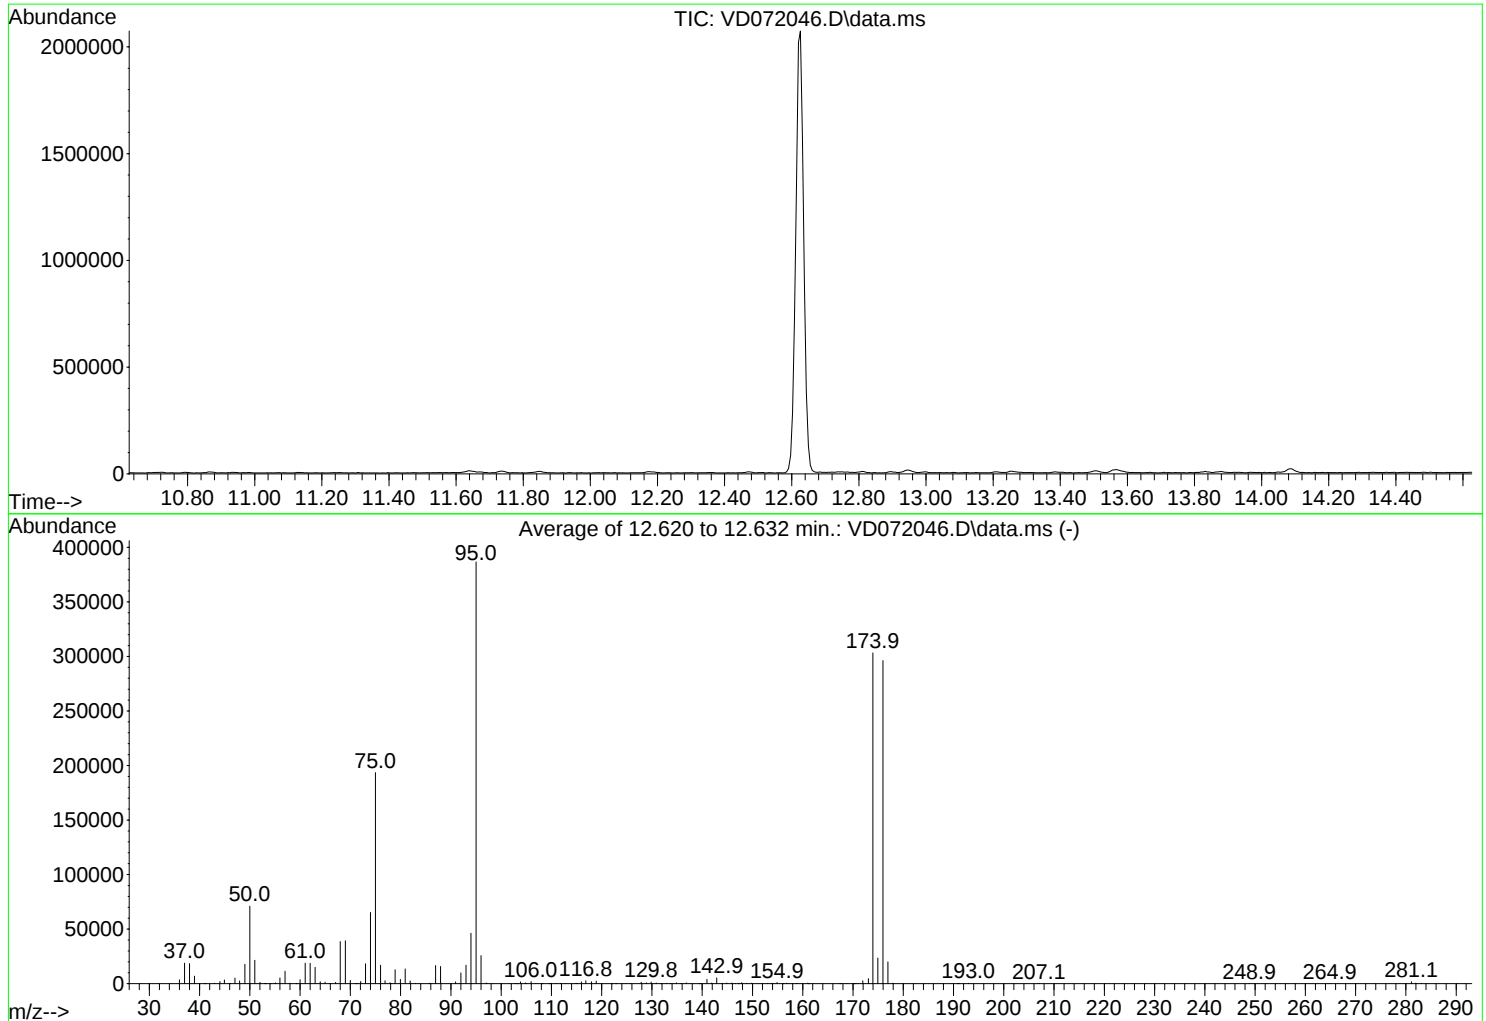

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1809

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	70944	PASS
75	95	30	60	50.0	193557	PASS
95	95	100	100	100.0	386731	PASS
96	95	5	9	6.6	25648	PASS
173	174	0.00	2	1.5	4521	PASS
174	95	50	100	78.4	303168	PASS
175	174	5	9	7.8	23501	PASS
176	174	95	101	97.7	296235	PASS
177	176	5	9	6.7	19907	PASS