
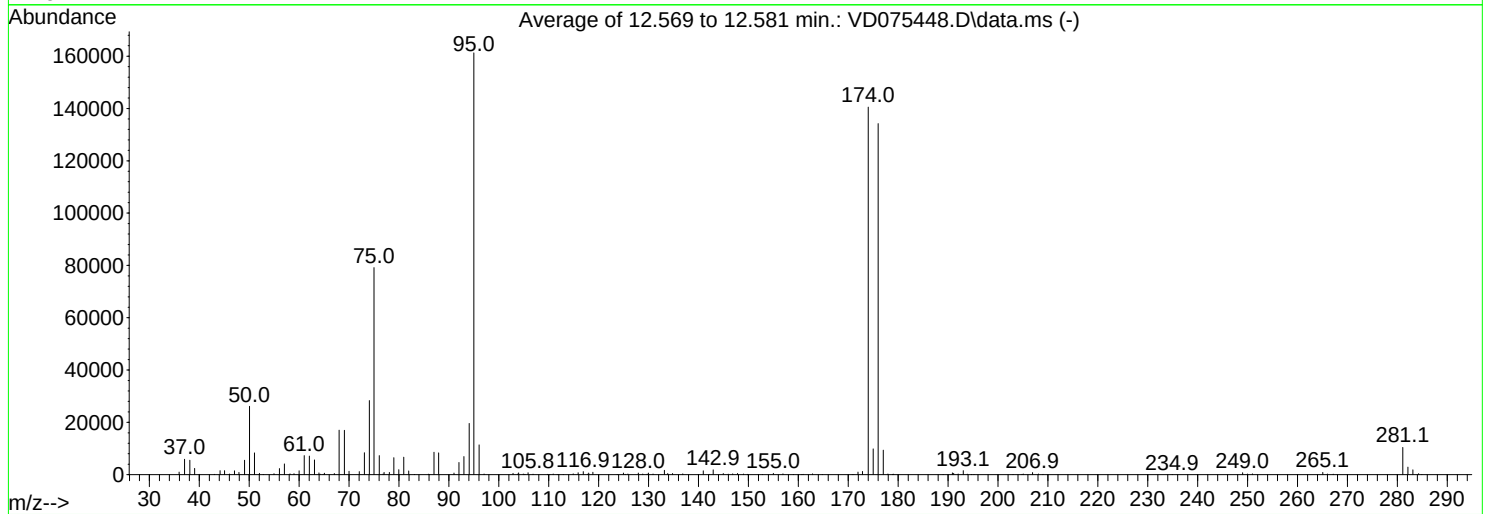


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030623\
Data File : VD075448.D
Acq On : 06 Mar 2023 08:54
Operator : KP/SY
Sample : BFB105
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB105

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM030123SMA.M
Title : SFAM01.0
Last Update : Fri Mar 03 23:23:38 2023

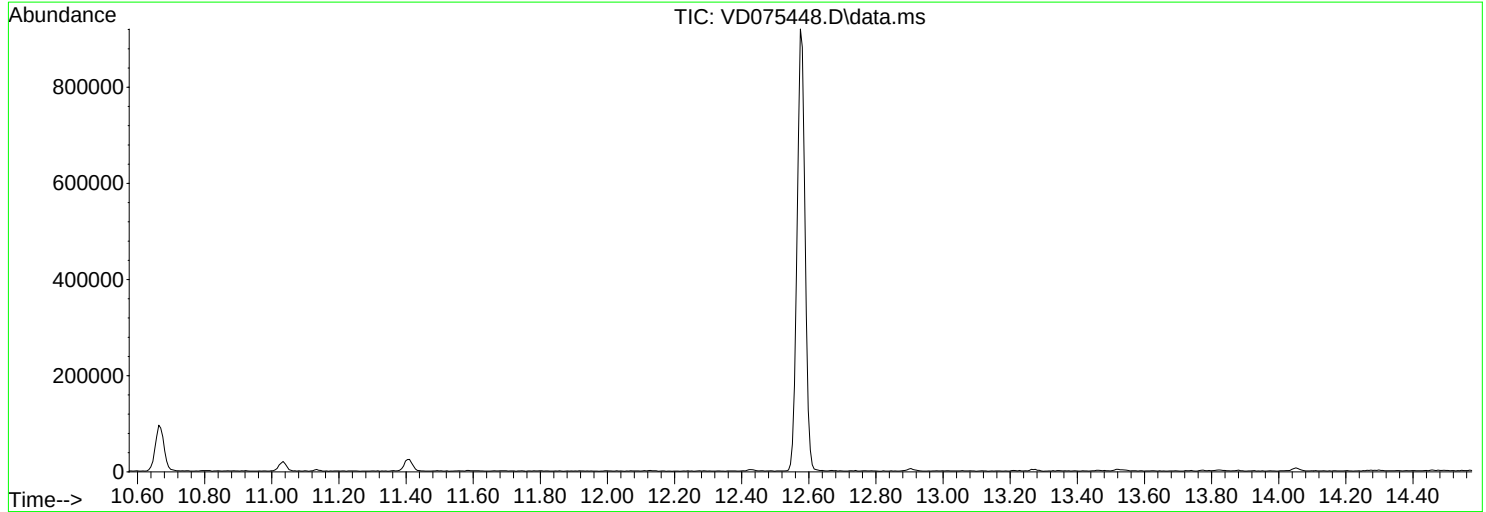

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	26109	PASS
75	95	30	80	49.1	79187	PASS
95	95	100	100	100.0	161280	PASS
96	95	5	9	7.1	11371	PASS
173	174	0.00	2	0.9	1261	PASS
174	95	50	120	87.1	140509	PASS
175	174	5	9	7.0	9868	PASS
176	174	95	105	95.5	134237	PASS
177	176	5	10	7.0	9338	PASS

Scan 1859 (12.522 min): VD075448.D\data.ms
BFB105

m/z	Abundance
40.00	1234.0
43.90	620.0
206.90	195.0

Instrument :
MSVOA_D
ClientSampleId :
BFB105

m/z	Abundance
36.00	736.0
37.00	5794.0
38.10	4855.0
39.00	2189.0
40.10	1531.0
44.20	1131.0
45.10	1555.0
47.10	1477.0
48.10	766.0
49.10	4323.0
50.10	23312.0
51.10	7343.0
52.10	411.0
52.80	267.0
55.00	199.0
56.00	1772.0
57.00	3635.0
58.10	277.0
59.10	326.0
60.00	1500.0
61.00	6794.0
62.10	5450.0
63.10	5271.0
63.90	846.0
65.00	769.0
67.00	402.0
68.00	14791.0
69.10	14508.0
70.00	1175.0
72.00	788.0
73.00	6804.0
74.00	24184.0
75.00	68984.0
76.10	6191.0
76.80	765.0
78.00	532.0
78.90	5787.0
80.10	1850.0
81.00	6324.0
82.00	1242.0
87.00	6888.0
87.90	6564.0
91.00	704.0
92.00	4575.0
93.00	6311.0
94.10	17984.0
95.00	134912.0
96.00	9395.0
97.10	167.0
102.90	467.0
103.80	698.0
105.00	279.0
105.90	432.0
106.90	289.0
114.90	187.0
115.80	590.0
116.90	1022.0
117.80	594.0
118.90	578.0
123.70	212.0
125.00	510.0
127.90	459.0
128.80	156.0
129.70	529.0
130.90	311.0
133.10	1650.0
133.80	375.0
134.70	321.0
136.80	289.0
141.10	935.0
143.00	1785.0
145.00	404.0
146.00	205.0
146.90	213.0
147.80	384.0
149.80	258.0
155.00	222.0
156.90	322.0
159.00	158.0
161.00	158.0
162.90	347.0
170.80	285.0
171.90	1066.0
172.90	1052.0
174.00	114008.0
175.00	8470.0
176.00	110360.0
177.00	8476.0
190.80	708.0
192.10	157.0
193.00	825.0
203.00	253.0

Instrument :
MSVOA_D
ClientSampleId :
BFB105

205.00	191.0
206.90	643.0
208.20	265.0
249.00	386.0
250.00	186.0
251.00	321.0
265.00	418.0
266.10	175.0
281.10	6616.0
282.10	1641.0
283.10	991.0
284.10	309.0

Instrument :
MSVOA_D
ClientSampleId :
BFB105

m/z	Abundance
36.00	1281.0
37.10	6163.0
38.10	5688.0
39.00	2941.0
40.00	1359.0
43.00	188.0
44.10	1769.0
45.00	1623.0
46.10	267.0
47.00	1406.0
47.90	753.0
49.00	6134.0
50.10	29200.0
51.10	8937.0
52.00	601.0
54.90	353.0
56.10	2881.0
57.10	4324.0
58.20	244.0
58.90	341.0
60.00	1596.0
61.00	8442.0
62.00	8227.0
63.00	5393.0
64.00	1167.0
65.10	640.0
67.10	459.0
68.00	18888.0
69.00	18128.0
70.00	1415.0
72.00	1477.0
73.00	9443.0
74.00	32528.0
75.00	88392.0
76.00	8236.0
77.00	1287.0
78.00	1001.0
79.00	6991.0
79.90	1927.0
80.90	6624.0
81.90	1675.0
83.10	249.0
85.90	574.0
87.00	10090.0
88.00	9090.0
90.90	679.0
92.00	4662.0
93.00	7793.0
94.00	21104.0
95.00	181376.0
96.10	12501.0
97.00	422.0
102.90	553.0
104.00	998.0
105.20	364.0
105.90	893.0
109.80	206.0
111.00	413.0
111.70	173.0
114.90	311.0
115.90	726.0
116.90	1352.0
118.00	861.0
118.90	1339.0
125.00	898.0
125.90	331.0
128.00	707.0
128.80	280.0
129.90	933.0
130.90	395.0
133.20	1752.0
133.90	332.0
134.80	361.0
136.90	254.0
140.90	1491.0
142.10	171.0
142.90	2035.0
144.90	616.0
145.90	208.0
146.90	269.0
147.80	496.0
149.00	358.0
149.80	204.0
155.10	645.0
156.90	392.0
160.70	217.0
162.70	168.0
164.80	167.0
171.10	247.0
172.00	1031.0
172.90	1382.0
174.00	152064.0

Instrument :
MSVOA_D
ClientSampleId :
BFB105

175.00	11151.0
176.00	149248.0
177.00	9632.0
177.90	408.0
178.90	364.0
190.90	1313.0
192.10	189.0
193.00	1937.0
194.00	206.0
205.10	261.0
207.00	936.0
208.00	232.0
209.00	176.0
234.90	274.0
248.90	682.0
250.00	226.0
250.90	289.0
265.10	1099.0
266.10	276.0
267.20	212.0
281.10	10479.0
282.10	3277.0
283.10	2267.0
284.20	197.0
284.90	157.0

Instrument :
MSVOA_D
ClientSampleId :
BFB105

m/z	Abundance
35.90	859.0
37.00	5626.0
38.10	6068.0
39.10	2081.0
40.00	1243.0
43.00	231.0
44.10	1663.0
45.00	1460.0
45.90	242.0
46.20	232.0
47.00	1588.0
47.90	1016.0
49.00	6046.0
50.00	25816.0
51.00	8764.0
52.10	390.0
55.00	528.0
56.00	2327.0
57.10	4391.0
58.10	327.0
58.90	387.0
60.00	1319.0
61.00	6712.0
62.10	7696.0
63.10	6312.0
64.20	654.0
64.80	339.0
65.20	261.0
67.00	457.0
68.00	17400.0
69.00	18160.0
70.00	1242.0
72.10	1184.0
73.10	8874.0
74.10	28352.0
75.00	80184.0
76.10	7497.0
77.00	1241.0
78.10	1088.0
79.00	6673.0
79.90	2016.0
80.90	7162.0
81.90	1328.0
86.10	219.0
87.00	8762.0
88.00	9281.0
91.10	532.0
92.00	4810.0
93.00	6748.0
94.00	19656.0
95.00	167552.0
96.00	12216.0
97.10	249.0
102.80	520.0
103.90	988.0
104.80	441.0
105.80	850.0
106.80	273.0
109.70	238.0
110.20	265.0
110.80	299.0
112.00	285.0
112.90	252.0
114.90	345.0
116.00	828.0
116.90	1094.0
118.00	1042.0
118.80	929.0
124.80	454.0
125.30	390.0
125.80	347.0
128.00	769.0
128.90	318.0
130.00	891.0
133.10	1574.0
133.90	585.0
134.90	527.0
136.90	334.0
140.00	156.0
140.90	1960.0
142.10	167.0
143.00	1774.0
145.00	347.0
145.90	162.0
146.80	511.0
147.80	353.0
149.00	328.0
152.00	156.0
152.80	240.0
154.90	633.0
156.80	183.0
160.90	219.0

Instrument :
MSVOA_D
ClientSampleId :
BFB105

162.90	337.0
171.90	932.0
172.80	1350.0
174.00	155456.0
175.00	9983.0
176.00	143104.0
177.00	9905.0
178.00	266.0
179.10	515.0
189.00	237.0
191.10	1494.0
191.90	427.0
193.10	1791.0
193.80	405.0
194.70	156.0
195.20	211.0
204.80	323.0
205.00	319.0
207.00	1327.0
208.10	314.0
209.00	201.0
249.00	1188.0
250.00	323.0
250.90	313.0
265.10	1149.0
265.90	351.0
267.10	329.0
281.10	14170.0
282.10	3638.0
283.10	2329.0
284.30	662.0

Instrument :
MSVOA_D
ClientSampleId :
BFB105