
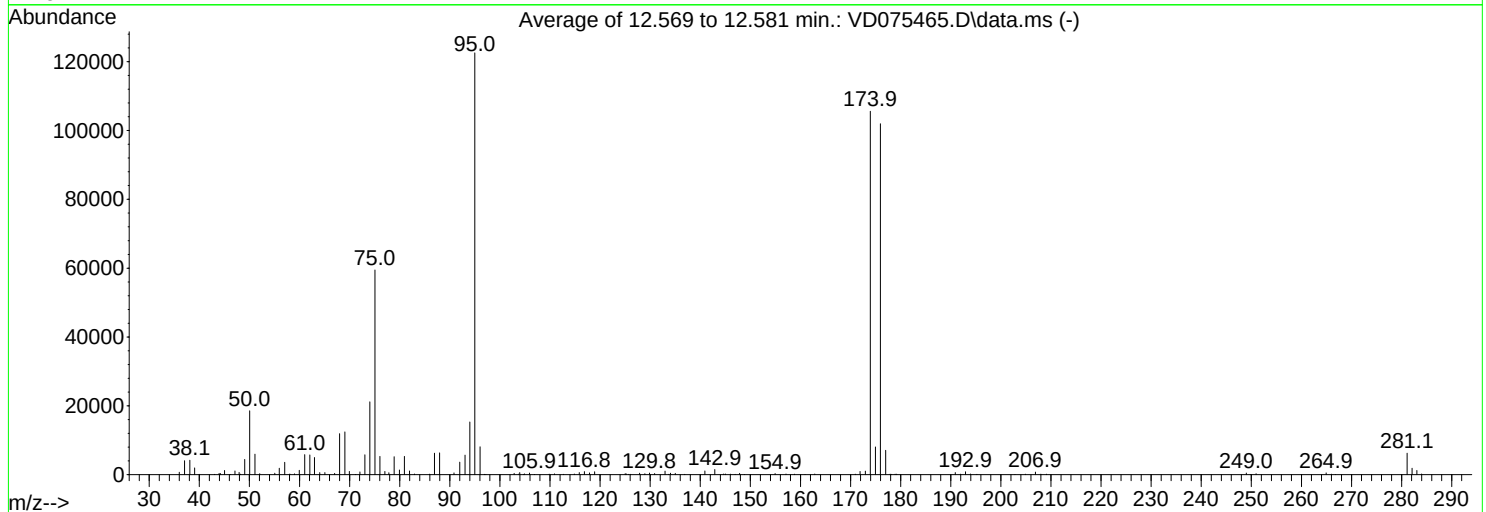


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030823\
Data File : VD075465.D
Acq On : 08 Mar 2023 10:42
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D030723S.M
Title : SW846 8260
Last Update : Wed Mar 08 12:19:57 2023

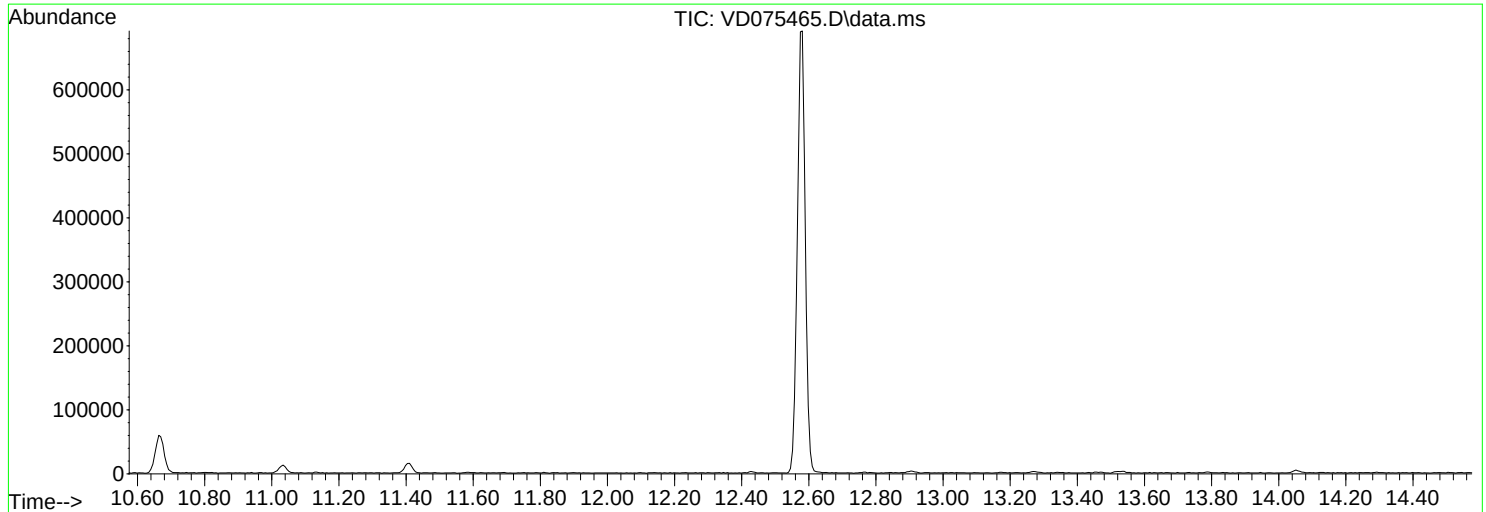

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	18573	PASS
75	95	30	60	48.5	59485	PASS
95	95	100	100	100.0	122573	PASS
96	95	5	9	6.6	8106	PASS
173	174	0.00	2	1.0	1027	PASS
174	95	50	100	86.2	105616	PASS
175	174	5	9	7.6	8024	PASS
176	174	95	101	96.5	101947	PASS
177	176	5	9	6.9	7080	PASS