

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD032019\
 Data File : VD061201.D
 Acq On : 20 Mar 2019 11:53
 Operator : VA/AP
 Sample : VD0320SBL01
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0320SBL01

Quant Time: Mar 22 01:57:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 08 02:35:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.04	168	704623	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.21	114	1174172	50.00	ug/l	0.00
63) Chlorobenzene-d5	12.36	117	930133	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.51	152	432892	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.45	65	287947	49.09	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	98.18%	
35) Dibromofluoromethane	6.91	113	451164	51.78	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	103.56%	
50) Toluene-d8	10.40	98	1040865	47.57	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	95.14%	
62) 4-Bromofluorobenzene	13.55	95	415058	48.88	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	97.76%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Methyl Iodide	3.33	142	4293	3.274	ug/l #	83
16) Acetone	3.23	43	1878	1.120	ug/l #	48
20) Methylene Chloride	3.81	84	27461	Below Cal	#	85
36) 1,1-Dichloropropene	7.03	75	51251	5.064	ug/l #	47
38) Carbon Tetrachloride	7.04	117	68599	6.153	ug/l #	15
43) Isopropyl Acetate	9.54	43	13572	2.063	ug/l #	43
81) trans-1,4-Dichloro-2-buten	13.55	75	155049	84.444	ug/l #	17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD032019\
Data File : VD061201.D
Acq On : 20 Mar 2019 11:53
Operator : VA/AP
Sample : VD0320SBL01
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleID :
VD0320SBL01

Quant Time: Mar 22 01:57:54 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 08 02:35:39 2019
Response via : Initial Calibration




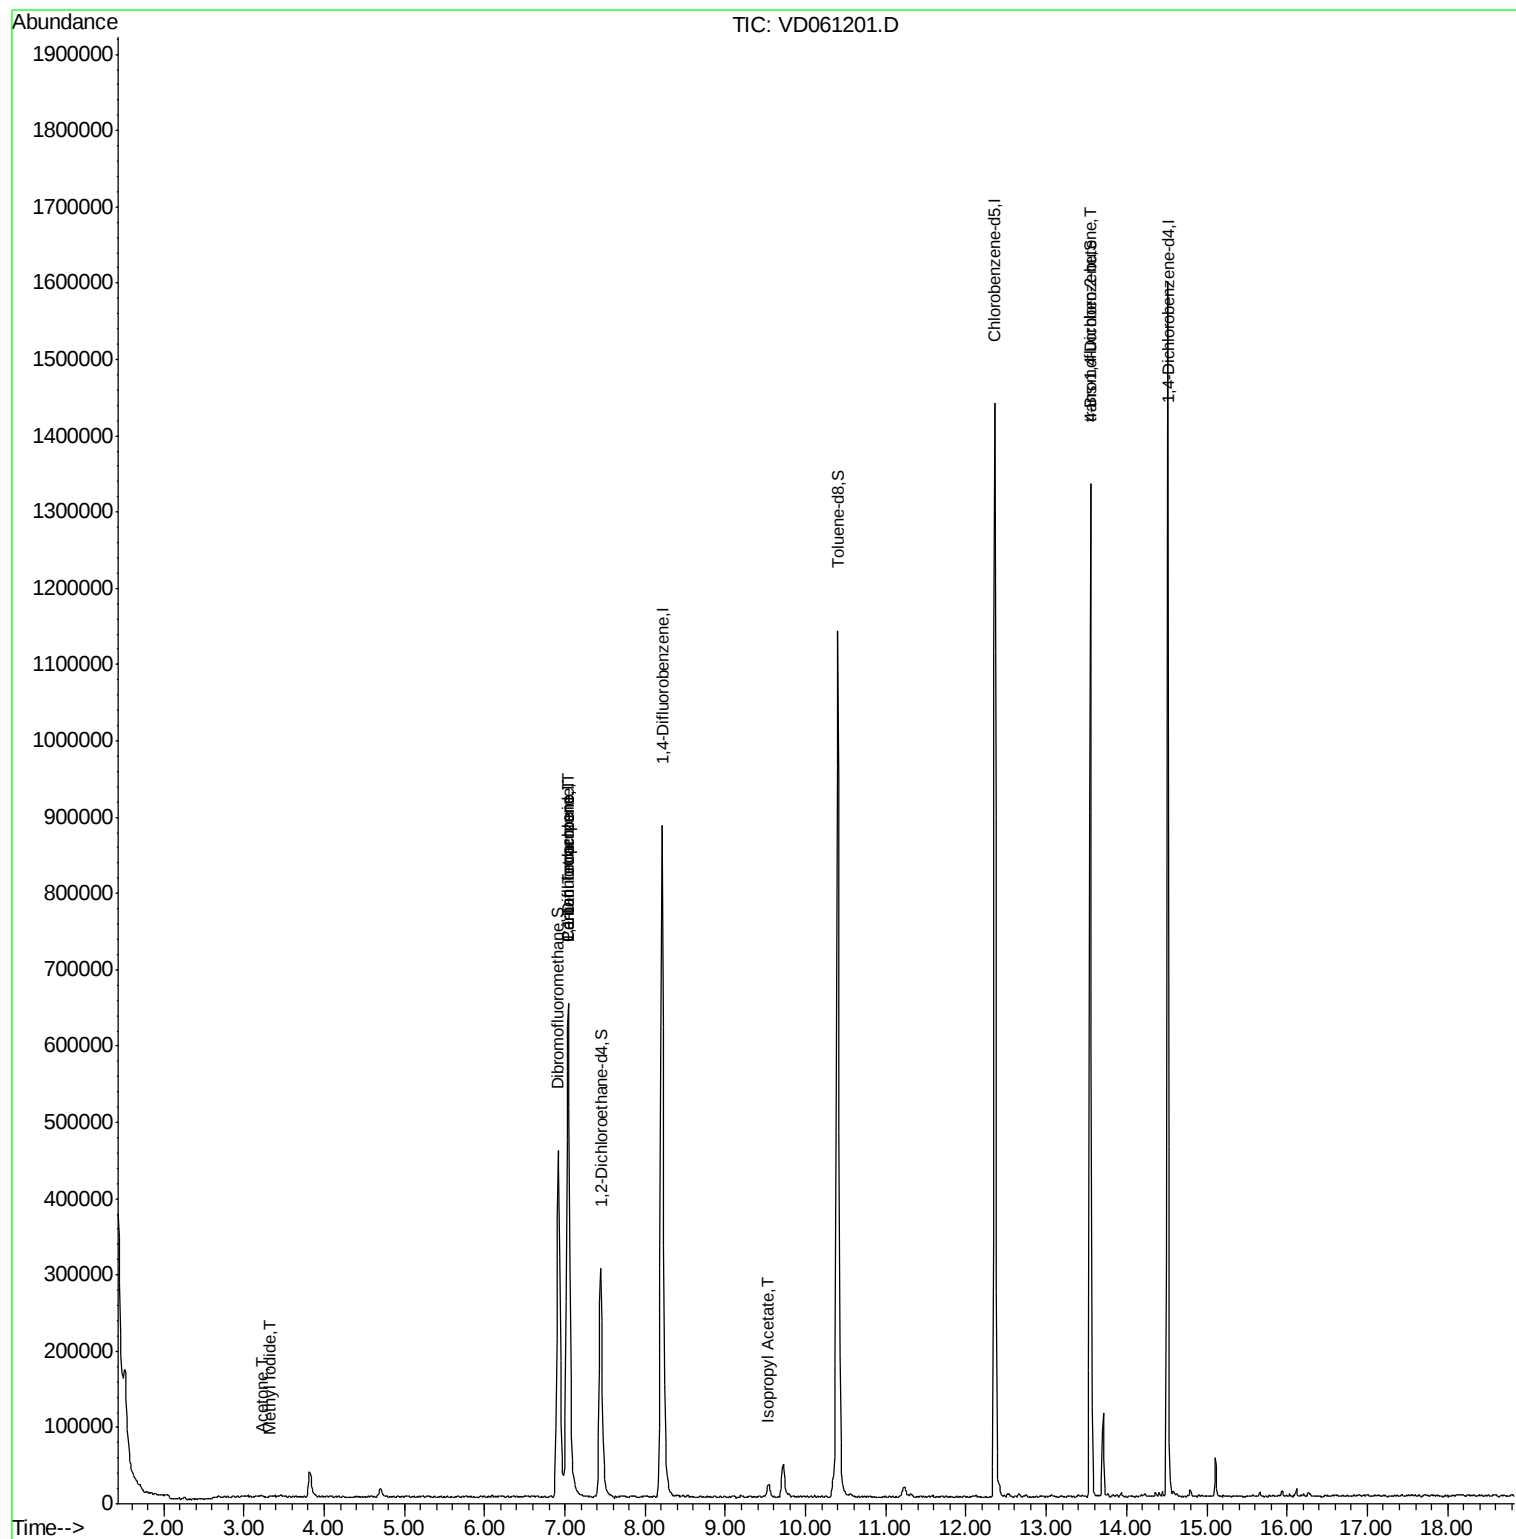




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.04 min Scan# 571
Delta R.T. -0.00 min
Lab File: VD061201.D
Acq: 20 Mar 2019 11:53




Instrument :
MSVOA_D
ClientSampleId :
VD0320SBL01


Tot Ion:168 Resp: 704623
Ion Ratio Lower Upper
168 100
99 57.4 47.3 70.9

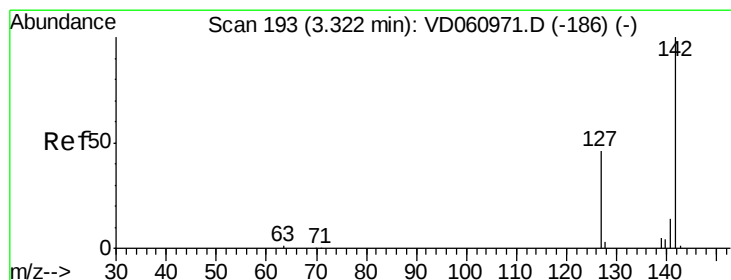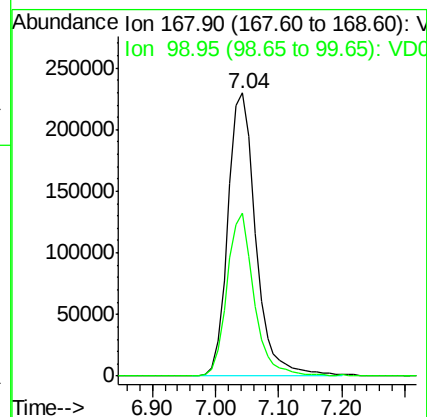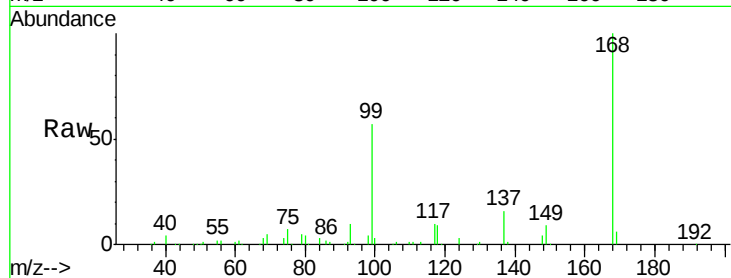

#10
Methyl Iodide
Concen: 3.274 ug/l
RT: 3.33 min Scan# 194
Delta R.T. 0.01 min
Lab File: VD061201.D
Acq: 20 Mar 2019 11:53

Tgt Ion:142 Resp: 4293
Ion Ratio Lower Upper
142 100
127 38.2 36.8 55.2
141 0.0 11.2 16.8#

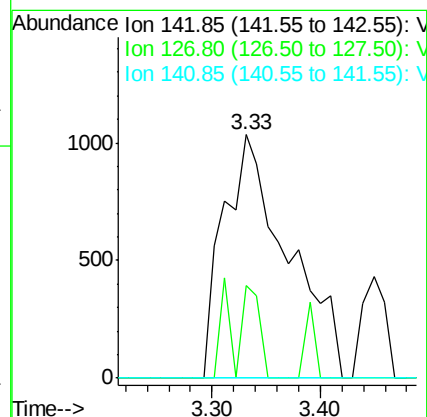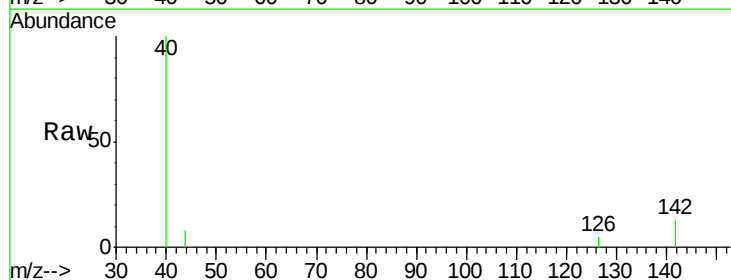



#16

Acetone

Concen: 1.120 ug/l

RT: 3.23 min Scan# 184

Delta R.T. 0.01 min

Lab File: VD061201.D

Acq: 20 Mar 2019 11:53

Instrument :

MSVOA_D

ClientSampleId :





VD0320SBL01

Tot Ion: 43 Resp: 1878

Ion Ratio Lower Upper

43 100

58 0.0 21.6 32.4#

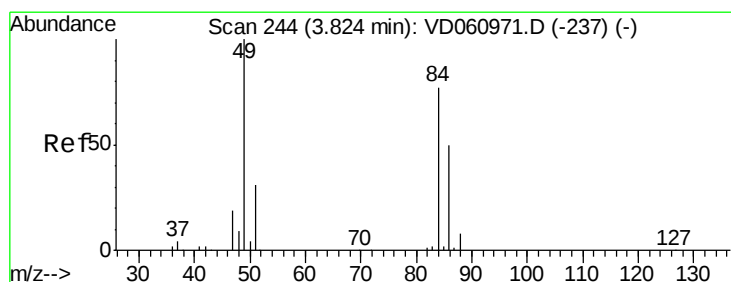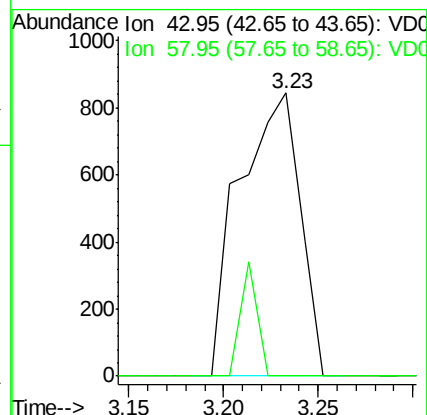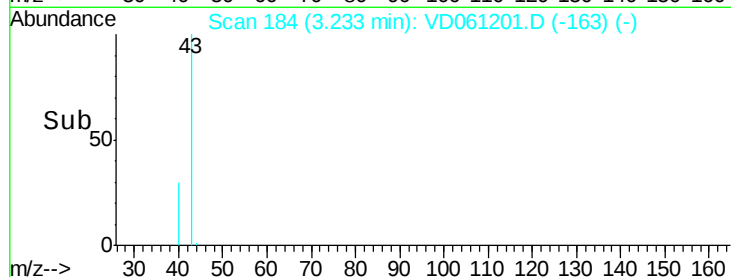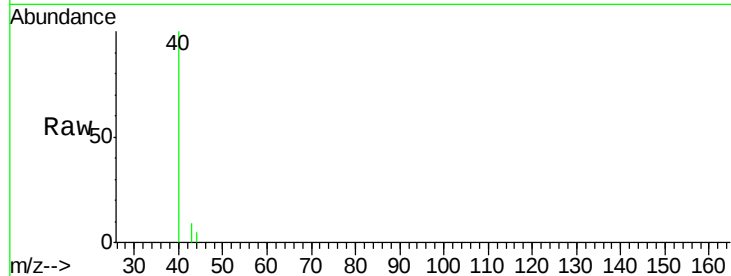

#20

Methylene Chloride

Concen: Below Cal

RT: 3.81 min Scan# 243

Delta R.T. -0.01 min

Lab File: VD061201.D

Acq: 20 Mar 2019 11:53

Tgt Ion: 84 Resp: 27461




Ion Ratio Lower Upper


84 100

49 113.0 104.2 156.2

51 25.9 32.3 48.5#

86 56.8 52.3 78.5

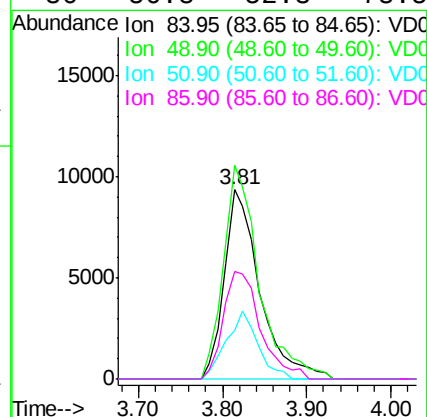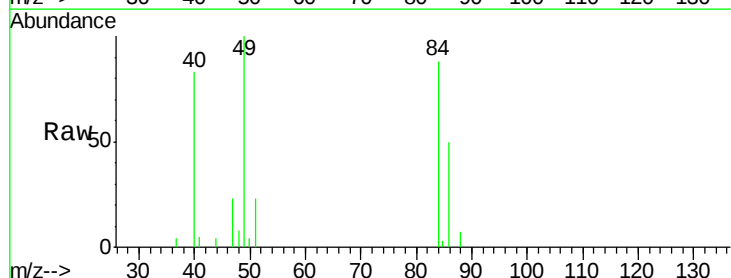



#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 7.45 min Scan# 612

Delta R.T. -0.00 min

Lab File: VD061201.D

Acq: 20 Mar 2019 11:53

Instrument :

MSVOA_D

ClientSampleId :


VD0320SBL01

Tot Ion: 65 Resp: 287947

Ion Ratio Lower Upper




65 100

67 50.3 0.0 105.2

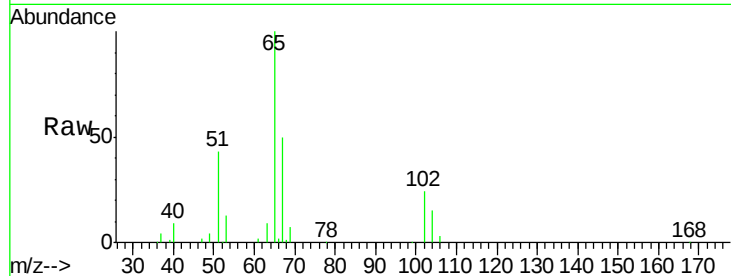

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

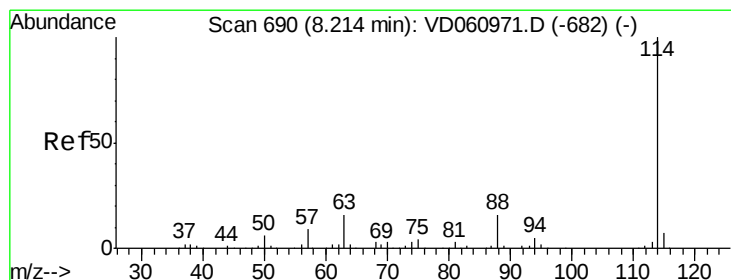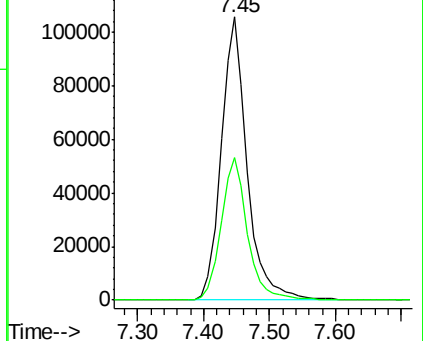

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.21 min Scan# 690

Delta R.T. -0.00 min

Lab File: VD061201.D

Acq: 20 Mar 2019 11:53


Tgt Ion: 114 Resp: 1174172

Ion Ratio Lower Upper

114 100

63 15.8 0.0 31.4



88 16.1 0.0 33.0

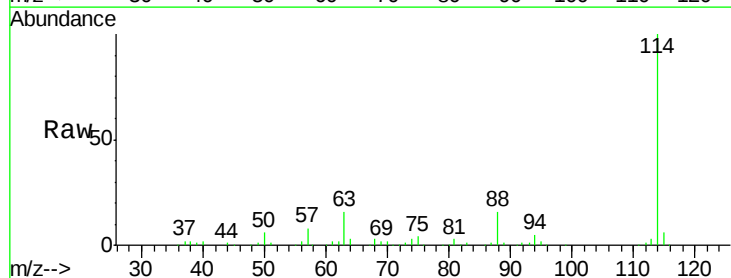


Abundance Ion 114.00 (113.70 to 114.70): V

Ion 62.95 (62.65 to 63.65): VDC

Ion 87.90 (87.60 to 88.60): VDC

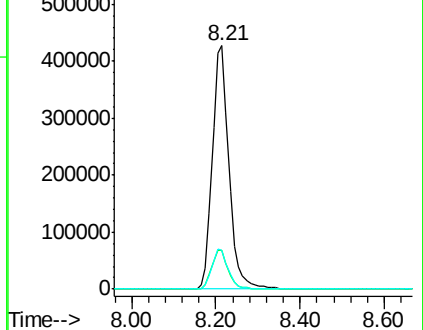


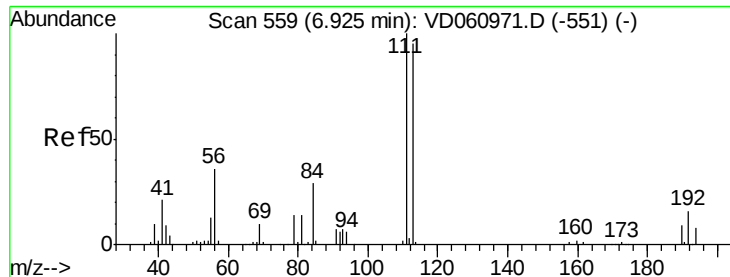




#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 6.91 min Scan# 558
 Delta R.T. -0.01 min
 Lab File: VD061201.D
 Acq: 20 Mar 2019 11:53

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0320SBL01

Tot Ion:113 Resp: 451164
 Ion Ratio Lower Upper
 113 100
 111 102.5 84.2 126.4
 192 17.4 13.1 19.7

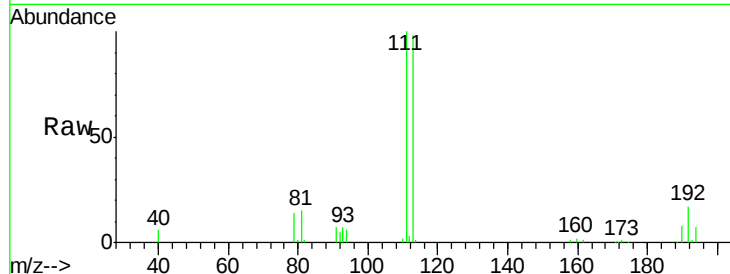


Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V

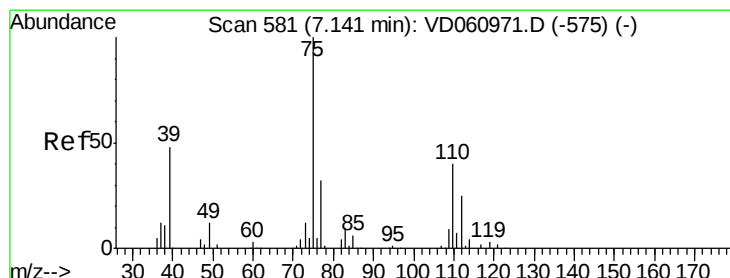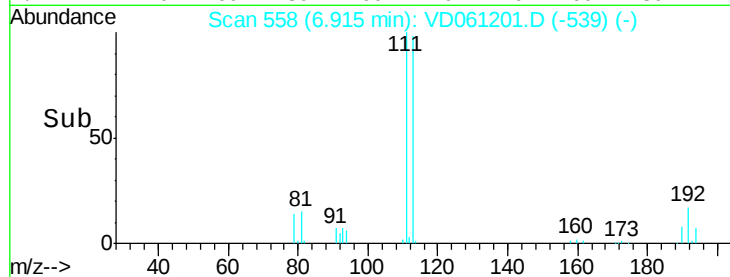
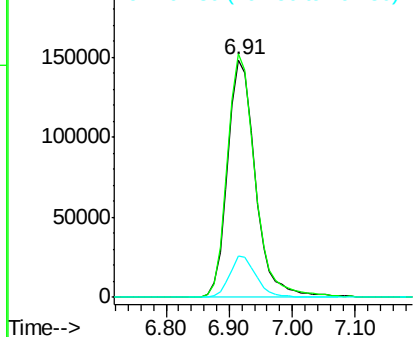



#36
 1,1-Dichloropropene
 Concen: 5.064 ug/l
 RT: 7.03 min Scan# 570
 Delta R.T. -0.11 min
 Lab File: VD061201.D
 Acq: 20 Mar 2019 11:53

Tgt Ion: 75 Resp: 51251
 Ion Ratio Lower Upper
 75 100
 110 8.3 19.7 59.1#
 77 0.0 24.7 37.1#

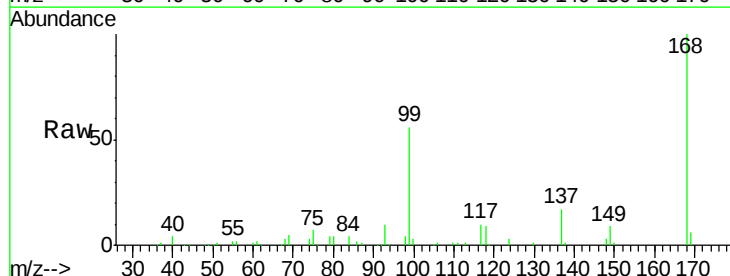

Abundance Ion 75.00 (74.70 to 75.70): VDC
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.95 (76.65 to 77.65): VDC



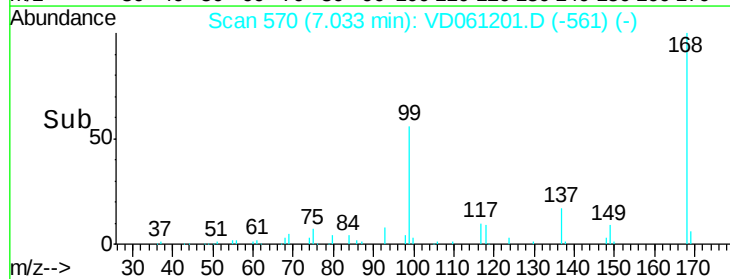
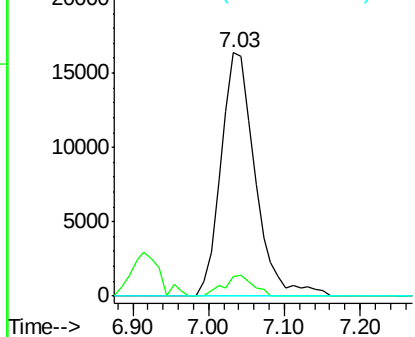




#38
Carbon Tetrachloride
Concen: 6.153 ug/l
RT: 7.04 min Scan# 571
Delta R.T. -0.07 min
Lab File: VD061201.D
Acq: 20 Mar 2019 11:53




Instrument :
MSVOA_D
ClientSampleId :
VD0320SBL01


Tot Ion:117 Resp: 68599
Ion Ratio Lower Upper
117 100
119 4.3 77.8 116.8#
121 0.0 25.3 37.9#

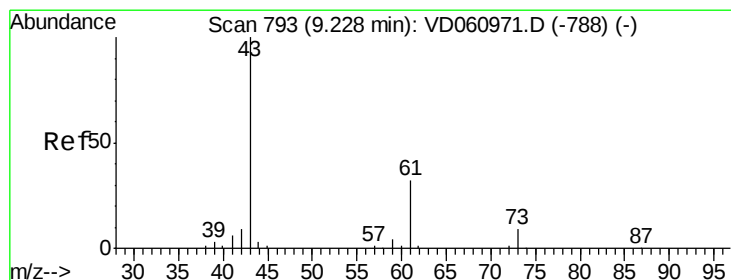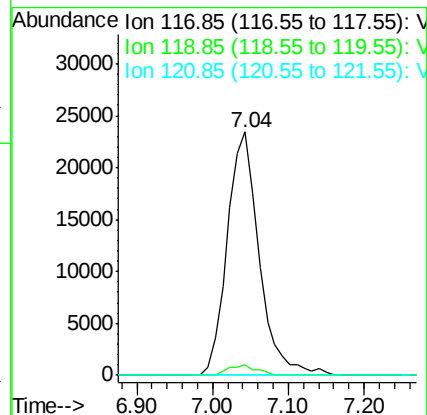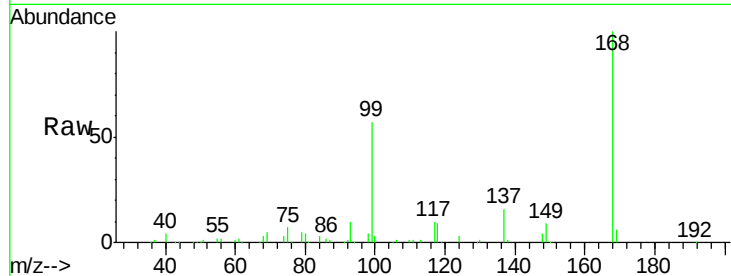

#43
Isopropyl Acetate
Concen: 2.063 ug/l
RT: 9.54 min Scan# 825
Delta R.T. 0.31 min
Lab File: VD061201.D
Acq: 20 Mar 2019 11:53

Tgt Ion: 43 Resp: 13572
Ion Ratio Lower Upper
43 100
61 0.0 25.6 38.4#
87 0.0 0.2 0.4#

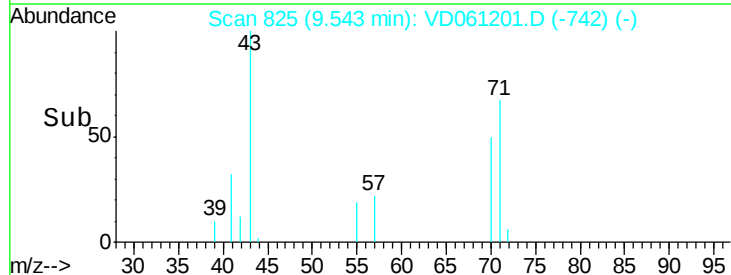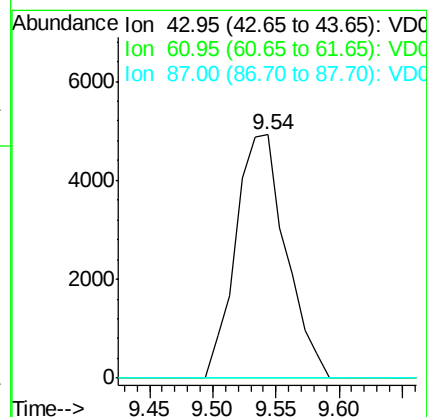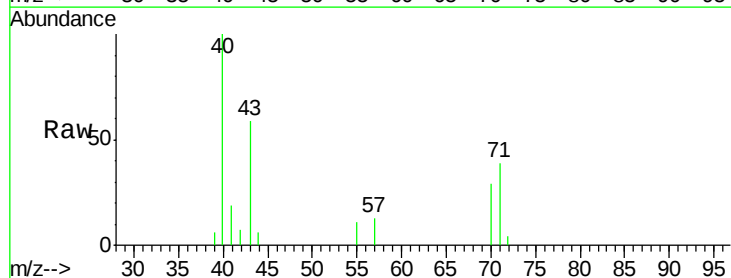

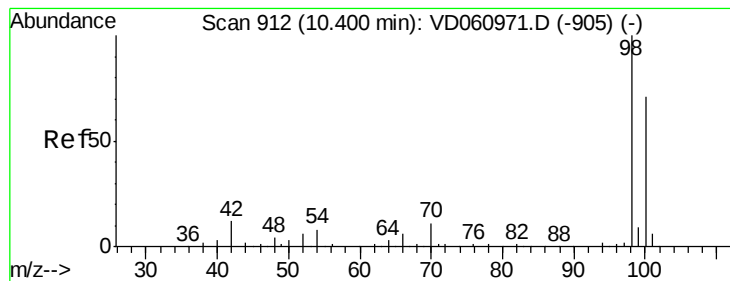

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.40 min Scan# 912

Delta R.T. -0.00 min

Lab File: VD061201.D

Acq: 20 Mar 2019 11:53


Instrument :
MSVOA_D
ClientSampleId :
VD0320SBL01

Tot Ion: 98 Resp: 1040865

Ion Ratio Lower Upper

98 100

100 69.8 57.4 86.2

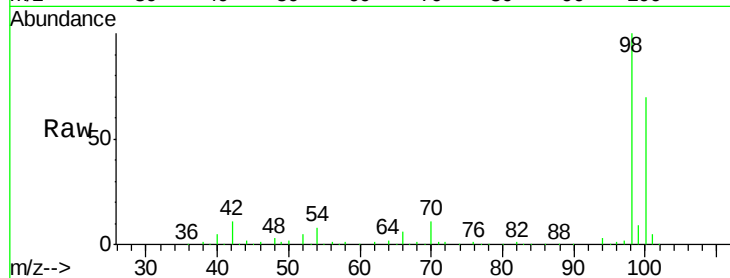

Abundance Ion 98.05 (97.75 to 98.75): VD060971.D (-905) (-)

Ion 100.05 (99.75 to 100.75): VD060971.D (-905) (-)

10.40

400000



300000

200000

100000

0

Time-->

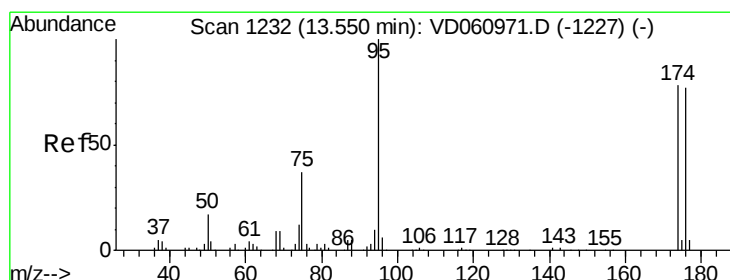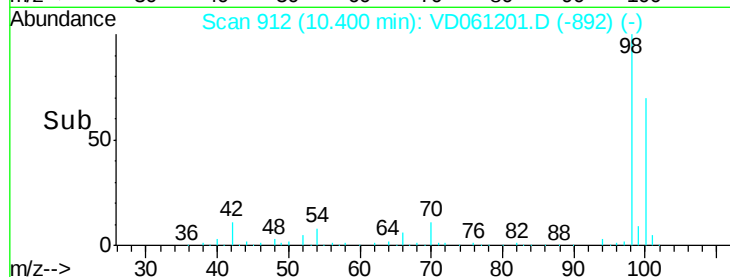

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 13.55 min Scan# 1232

Delta R.T. -0.00 min

Lab File: VD061201.D

Acq: 20 Mar 2019 11:53


Tgt Ion: 95 Resp: 415058

Ion Ratio Lower Upper

95 100

174 87.9 0.0 155.6

176 85.0 0.0 153.8

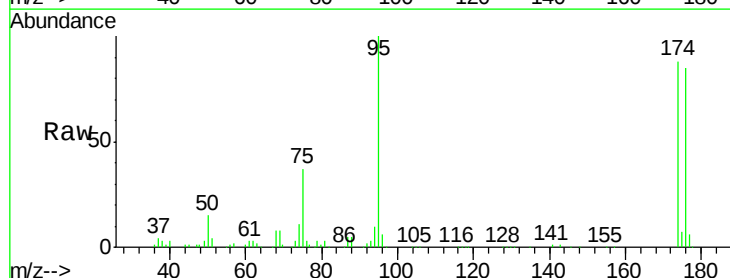

Abundance Ion 95.00 (94.70 to 95.70): VD060971.D (-1227) (-)

Ion 173.90 (173.60 to 174.60): VD060971.D (-1227) (-)

Ion 175.90 (175.60 to 176.60): VD060971.D (-1227) (-)

13.55

400000


300000


200000

100000

0

Time-->

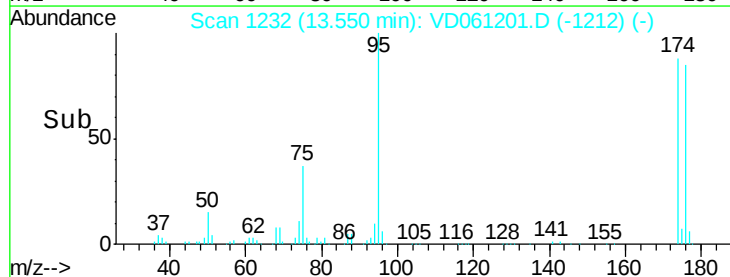


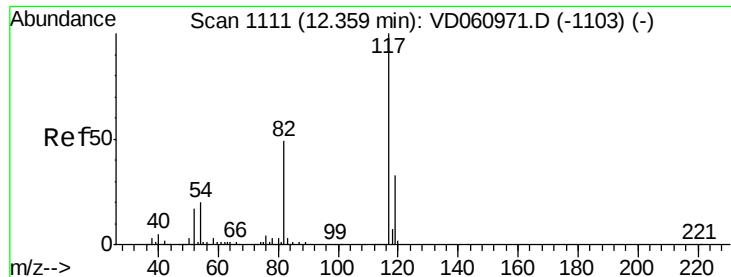




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.36 min Scan# 1111
Delta R.T. -0.00 min
Lab File: VD061201.D
Acq: 20 Mar 2019 11:53

Instrument :
MSVOA_D
ClientSampleId :
VD0320SBL01

Tot Ion:117 Resp: 930133
Ion Ratio Lower Upper
117 100
82 46.2 38.9 58.3
119 33.5 26.6 39.8

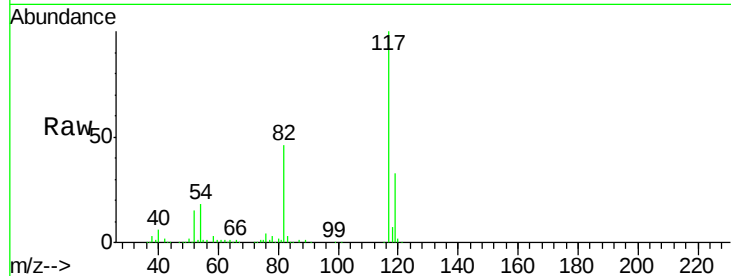


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V

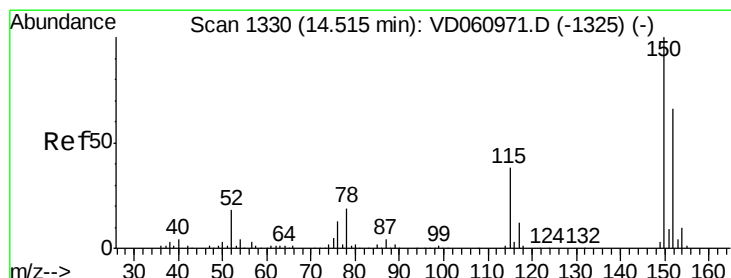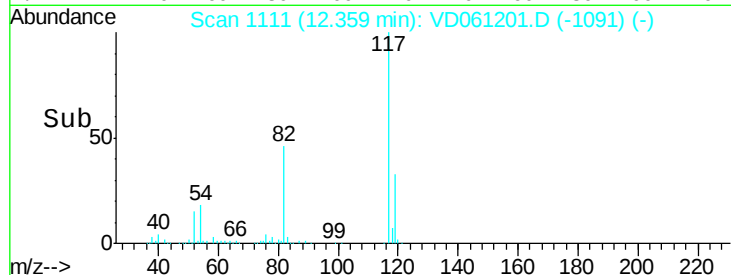
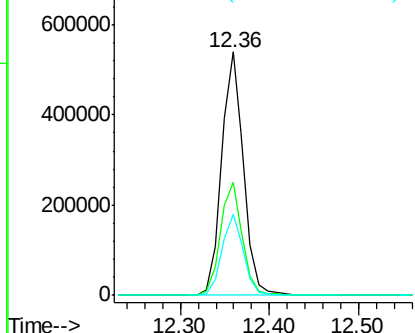



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 14.51 min Scan# 1330
Delta R.T. -0.00 min
Lab File: VD061201.D
Acq: 20 Mar 2019 11:53

Tgt Ion:152 Resp: 432892
Ion Ratio Lower Upper
152 100
115 51.6 28.6 85.9
150 154.0 0.0 310.6

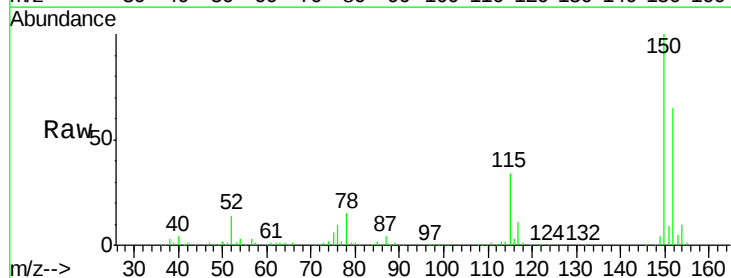

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

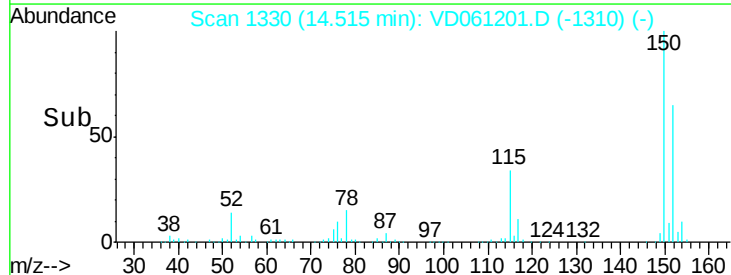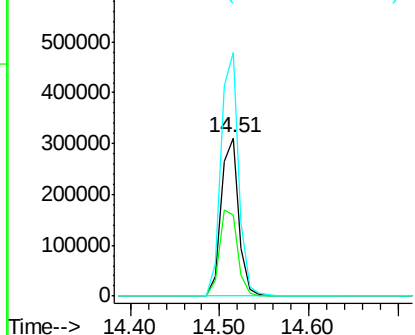



#81

trans-1,4-Dichloro-2-butene

Concen: 84.444 ug/l

RT: 13.55 min Scan# 1232

Delta R.T. 0.08 min

Lab File: VD061201.D

Acq: 20 Mar 2019 11:53

Instrument :

MSVOA_D

ClientSampleId :

VD0320SBL01


Tot Ion: 75 Resp: 155049

Ion Ratio Lower Upper

75 100

53 0.0 64.4 96.6#

89 0.0 34.8 52.2#

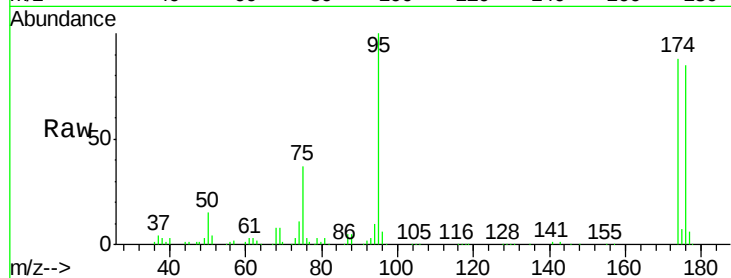

Abundance Ion 75.00 (74.70 to 75.70): VDC

Ion 53.00 (52.70 to 53.70): VDC

Ion 89.00 (88.70 to 89.70): VDC

