

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD032019\
 Data File : VD061208.D
 Acq On : 20 Mar 2019 15:18
 Operator : VA/AP
 Sample : K1987-05RE
 Misc : 5.10g/5ml/MSVOA D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 20190147-COMPOSITE-FRE

Quant Time: Mar 22 02:29:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 08 02:35:39 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.04	168	471361	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.21	114	829956	50.00	ug/l	0.00
63) Chlorobenzene-d5	12.36	117	517797	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.52	152	160097	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.45	65	205426	52.36	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.72%	
35) Dibromofluoromethane	6.93	113	318942	51.78	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.56%	
50) Toluene-d8	10.40	98	714702	46.21	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.42%	
62) 4-Bromofluorobenzene	13.55	95	195271	32.54	ug/l	0.00
Spiked Amount 50.000			Recovery	=	65.08%	
Target Compounds						
16) Acetone	3.22	43	42571	37.943	ug/l	92
20) Methylene Chloride	3.82	84	34486	2.291	ug/l	90
25) 2-Butanone	6.06	43	11407	8.960	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD032019\
Data File : VD061208.D
Acq On : 20 Mar 2019 15:18
Operator : VA/AP
Sample : K1987-05RE
Misc : 5.10g/5ml/MSVOA D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
20190147-COMPOSITE-FRE

Quant Time: Mar 22 02:29:09 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 08 02:35:39 2019
Response via : Initial Calibration

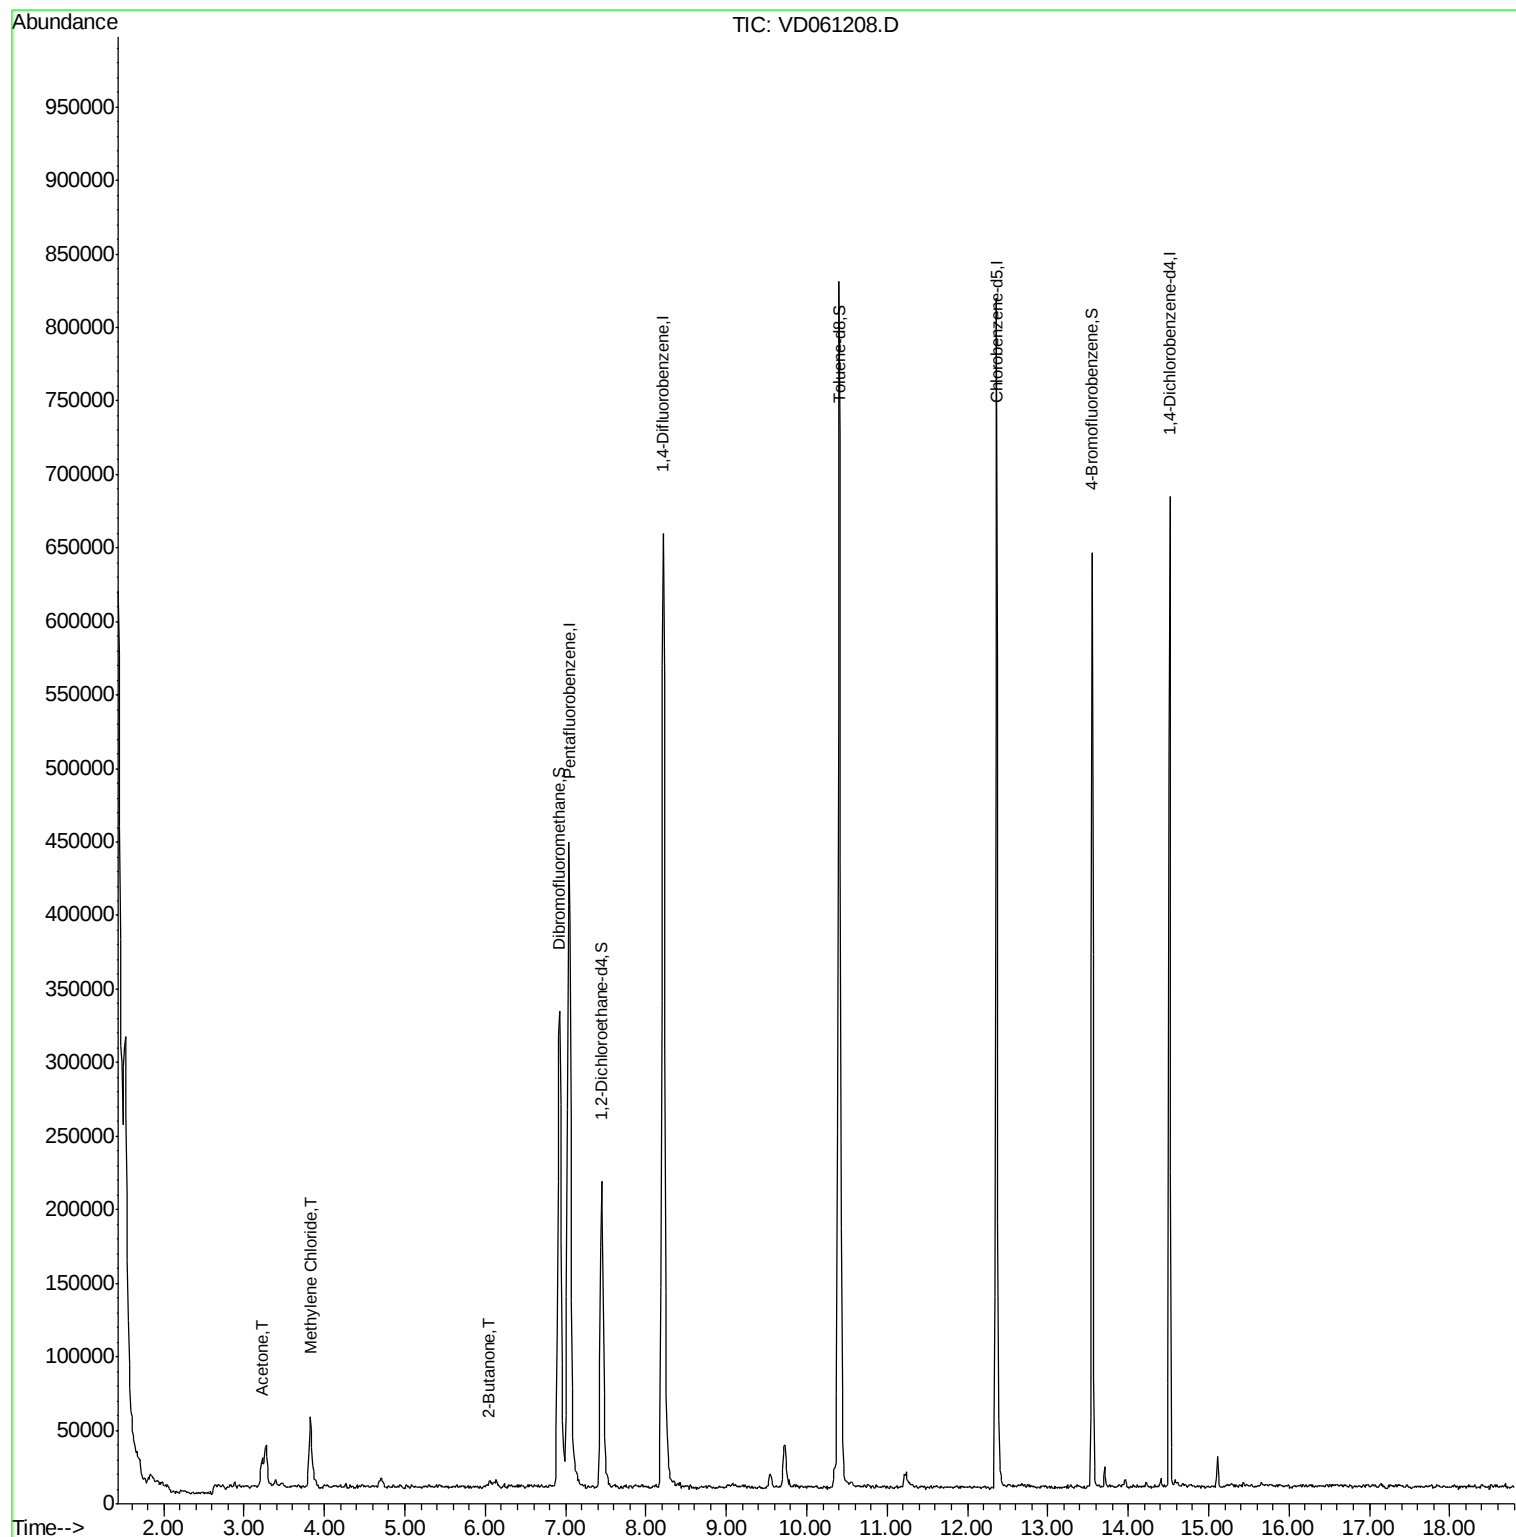



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.04 min Scan# 571

Delta R.T. 0.00 min

Lab File: VD061208.D

Acq: 20 Mar 2019 15:18

Instrument :

MSVOA_D

ClientSampleId :


20190147-COMPOSITE-FRE

Tot Ion:168 Resp: 471361

Ion Ratio Lower Upper




168 100

99 54.9 47.3 70.9

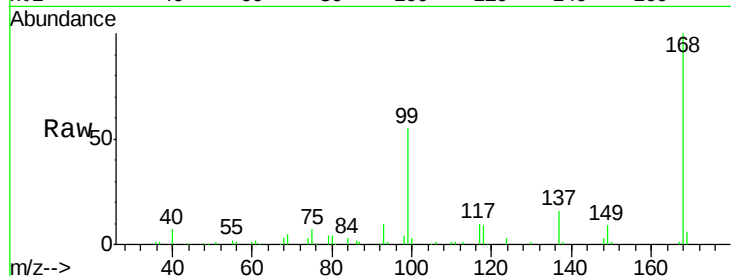

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

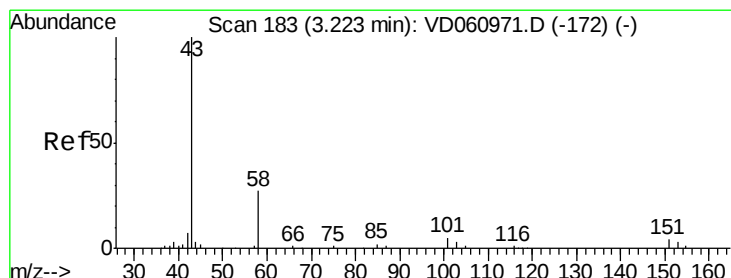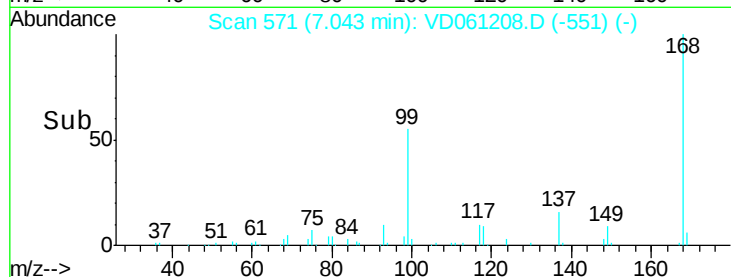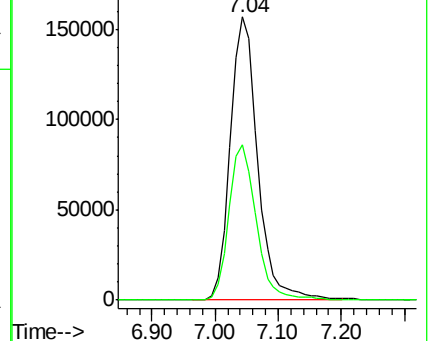

#16

Acetone

Concen: 37.943 ug/l

RT: 3.22 min Scan# 183

Delta R.T. 0.00 min

Lab File: VD061208.D


Acq: 20 Mar 2019 15:18

Tgt Ion: 43 Resp: 42571

Ion Ratio Lower Upper



43 100

58 23.1 21.6 32.4

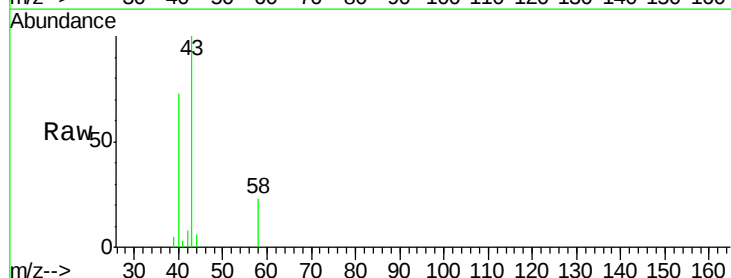

Abundance Ion 42.95 (42.65 to 43.65): VDC

Ion 57.95 (57.65 to 58.65): VDC



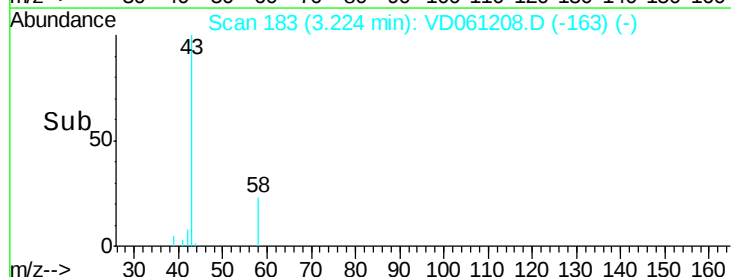
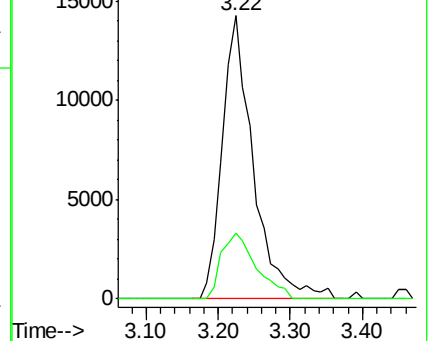




#20
Methylene Chloride
Concen: 2.291 ug/l
RT: 3.82 min Scan# 244
Delta R.T. 0.00 min
Lab File: VD061208.D
Acq: 20 Mar 2019 15:18




Instrument :
MSVOA_D
ClientSampleId :
20190147-COMPOSITE-FRE

Tot Ion: 84 Resp: 34486
Ion Ratio Lower Upper
84 100
49 116.0 104.2 156.2
51 35.7 32.3 48.5
86 71.0 52.3 78.5

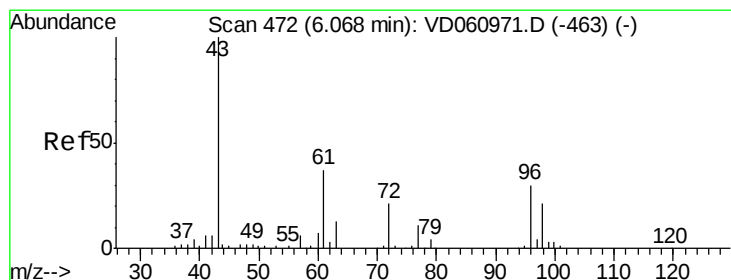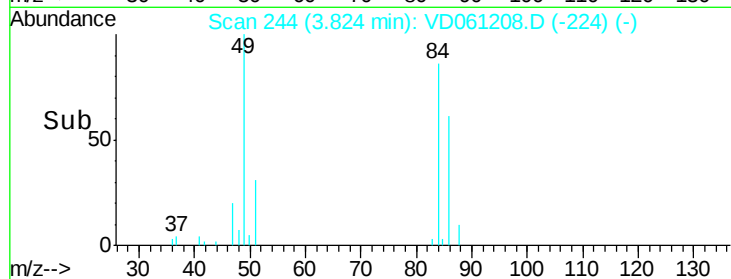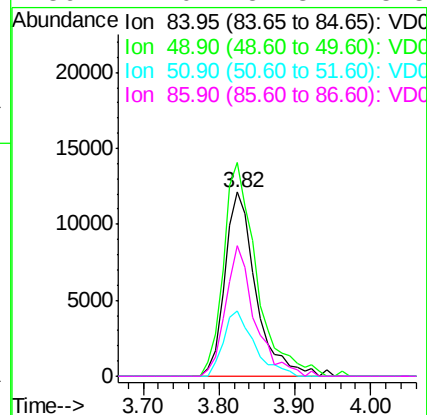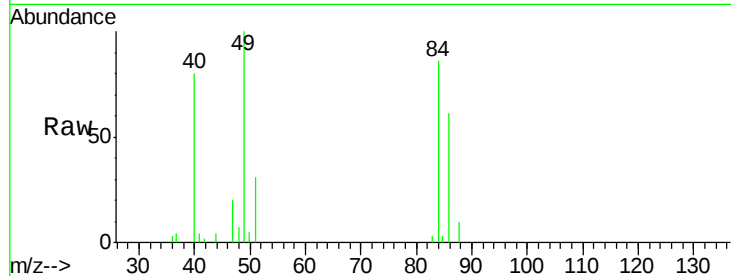

#25
2-Butanone
Concen: 8.960 ug/l
RT: 6.06 min Scan# 471
Delta R.T. -0.01 min
Lab File: VD061208.D
Acq: 20 Mar 2019 15:18

Tgt Ion: 43 Resp: 11407
Ion Ratio Lower Upper
43 100
72 19.8 16.7 25.1

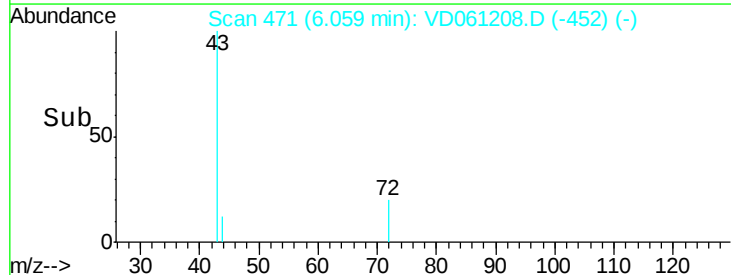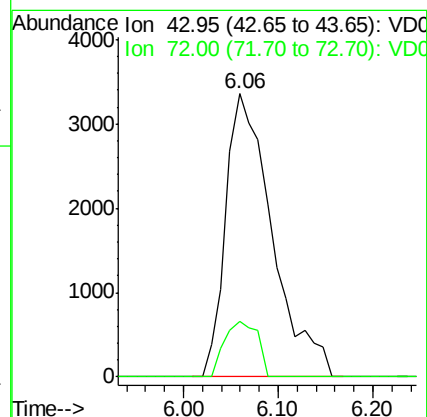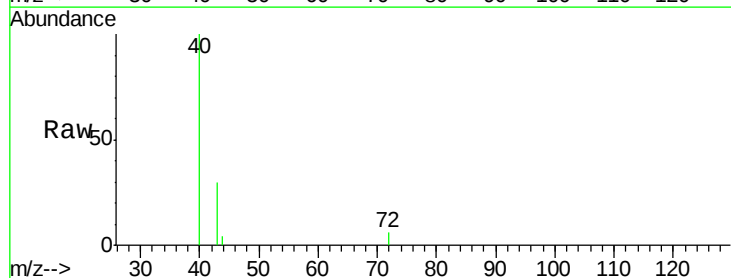



#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 7.45 min Scan# 612

Delta R.T. 0.00 min

Lab File: VD061208.D

Acq: 20 Mar 2019 15:18

Instrument :

MSVOA_D

ClientSampleId :


20190147-COMPOSITE-FRE

Tot Ion: 65 Resp: 205426

Ion Ratio Lower Upper




65 100

67 50.6 0.0 105.2

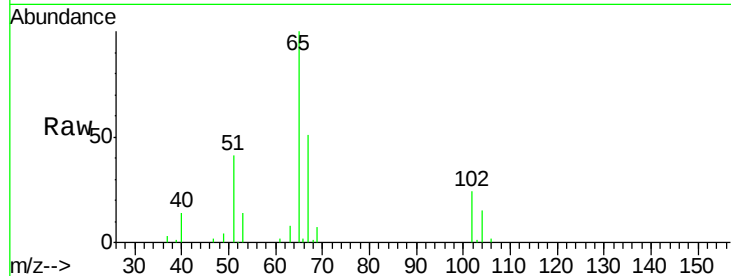

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

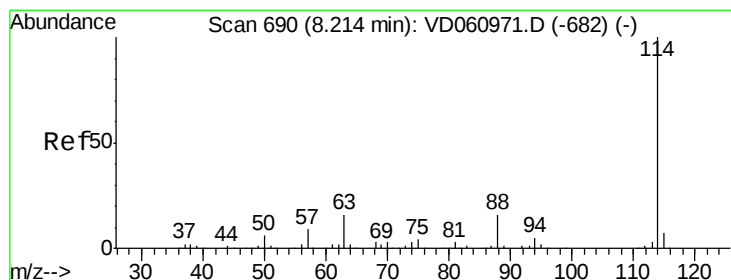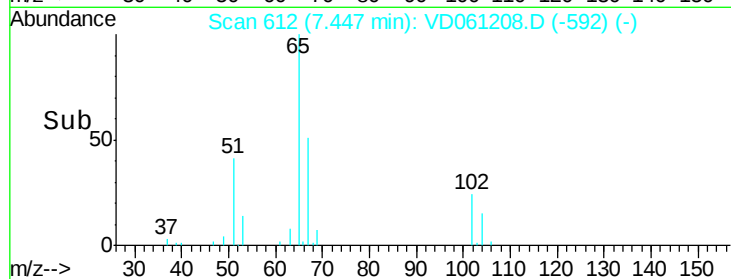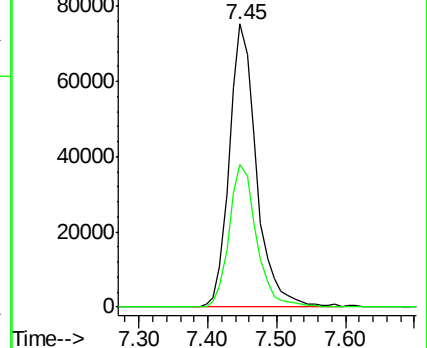

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.21 min Scan# 690

Delta R.T. 0.00 min

Lab File: VD061208.D

Acq: 20 Mar 2019 15:18


Tgt Ion: 114 Resp: 829956

Ion Ratio Lower Upper

114 100

63 15.2 0.0 31.4



88 15.9 0.0 33.0

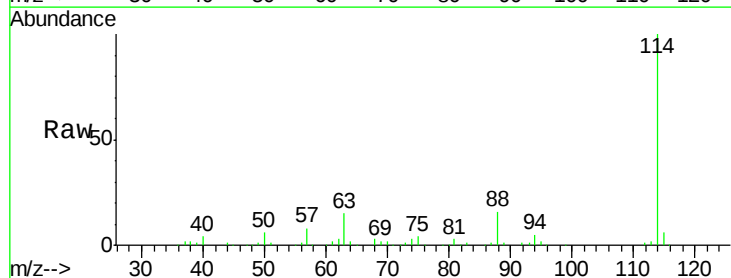

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 62.95 (62.65 to 63.65): VDC

Ion 87.90 (87.60 to 88.60): VDC

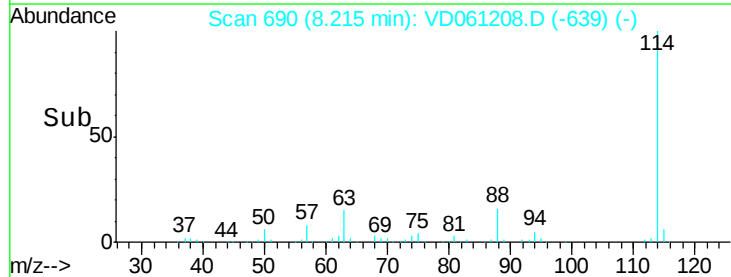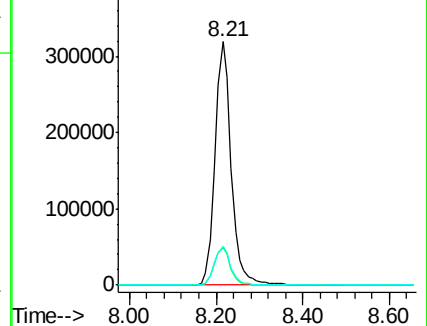







#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 6.93 min Scan# 559
 Delta R.T. 0.00 min
 Lab File: VD061208.D
 Acq: 20 Mar 2019 15:18

Instrument :
 MSVOA_D
 ClientSampleId :
 20190147-COMPOSITE-FRE

Tot Ion	Ratio	Lower	Upper
113	100		
111	101.1	84.2	126.4
192	16.7	13.1	19.7

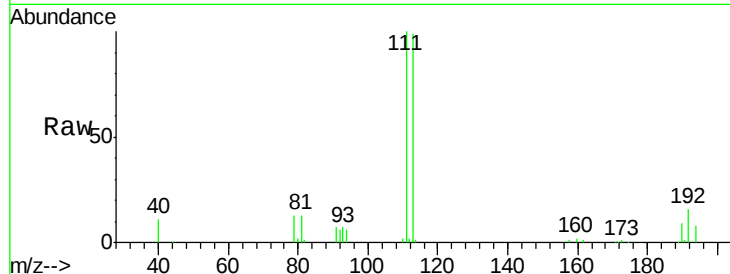


Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V

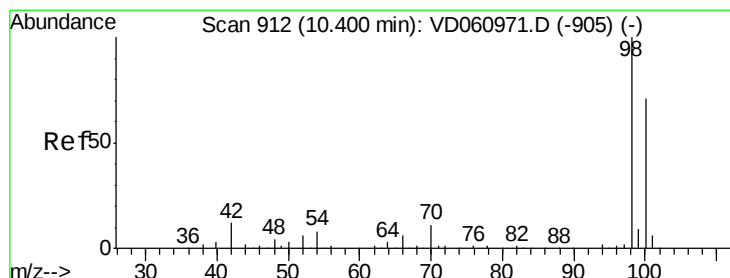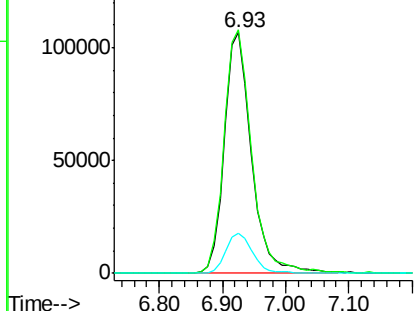
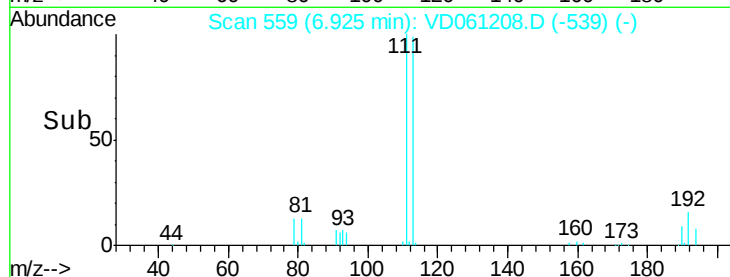



#50
 Toluene-d8
 Concen: N.D. ug/l
 RT: 10.40 min Scan# 912
 Delta R.T. 0.00 min
 Lab File: VD061208.D
 Acq: 20 Mar 2019 15:18

Tgt Ion	Ratio	Lower	Upper
98	100		
100	68.4	57.4	86.2

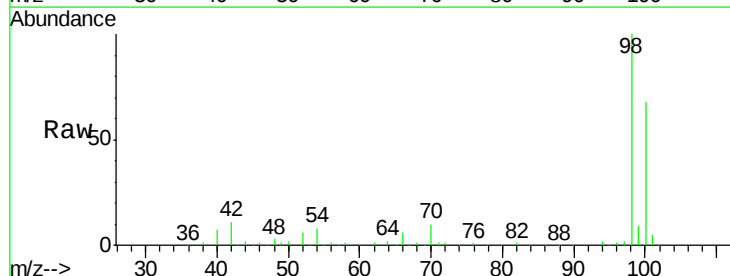

Abundance Ion 98.05 (97.75 to 98.75): VDC
 Ion 100.05 (99.75 to 100.75): VDC



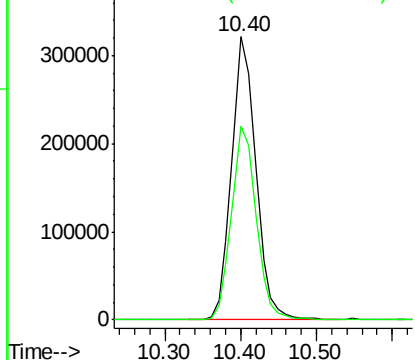
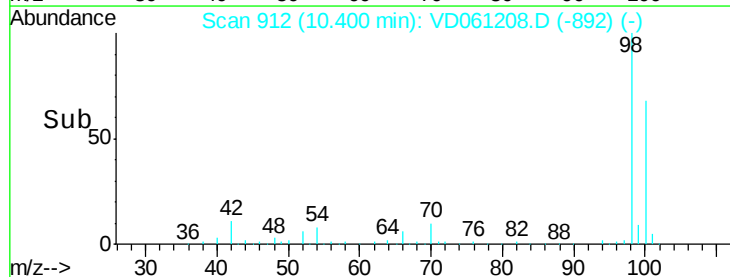


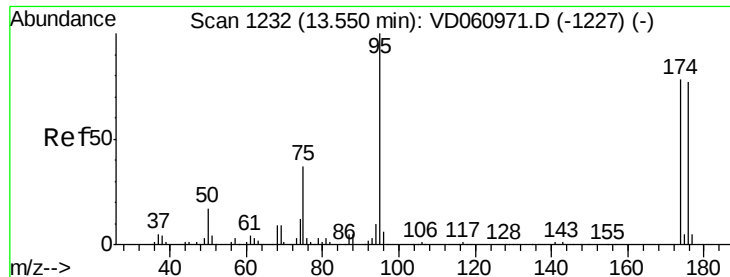

#62
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 13.55 min Scan# 1232
Delta R.T. 0.00 min
Lab File: VD061208.D
Acq: 20 Mar 2019 15:18




Instrument :
MSVOA_D
ClientSampleId :
20190147-COMPOSITE-FRE


Tot Ion: 95 Resp: 195271
Ion Ratio Lower Upper
95 100
174 85.9 0.0 155.6
176 81.4 0.0 153.8

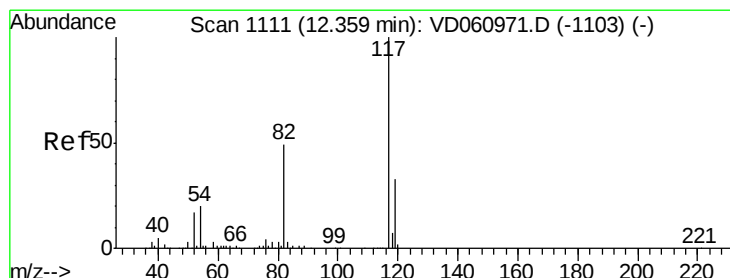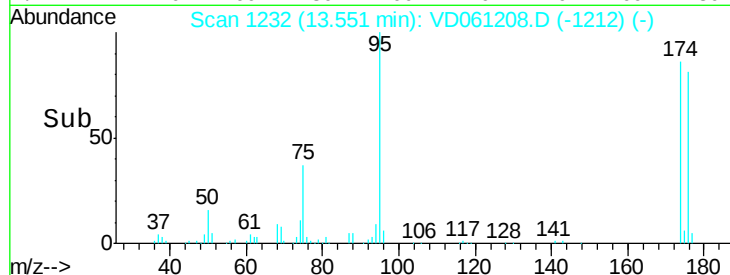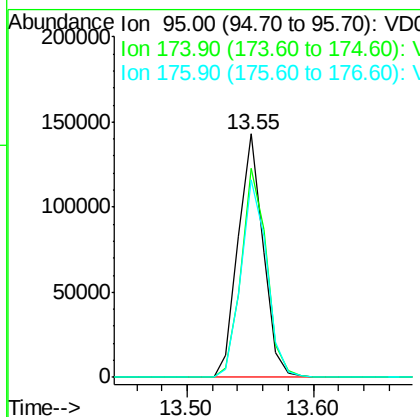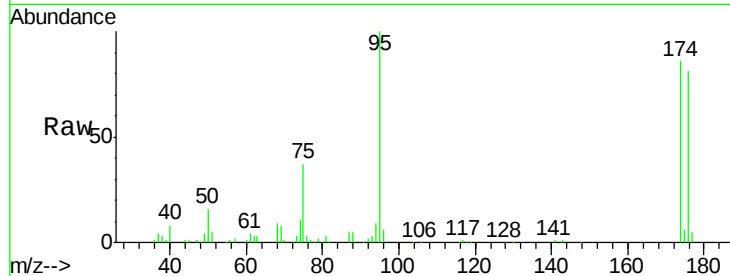

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.36 min Scan# 1111
Delta R.T. 0.00 min
Lab File: VD061208.D
Acq: 20 Mar 2019 15:18

Tgt Ion: 117 Resp: 517797
Ion Ratio Lower Upper
117 100
82 45.0 38.9 58.3
119 33.1 26.6 39.8

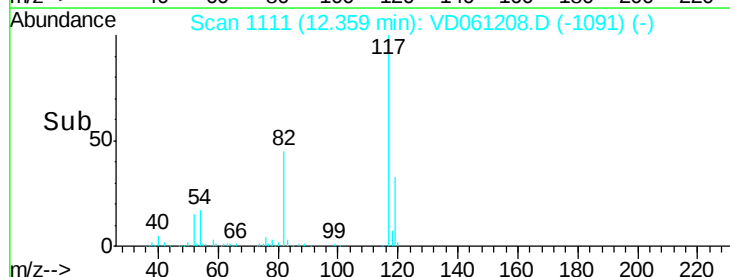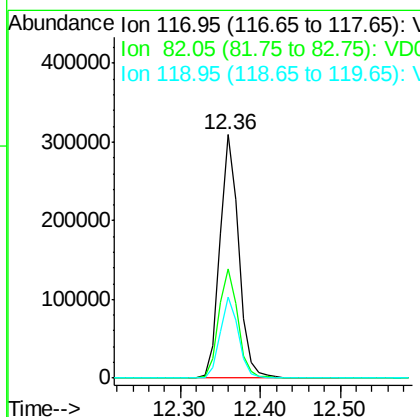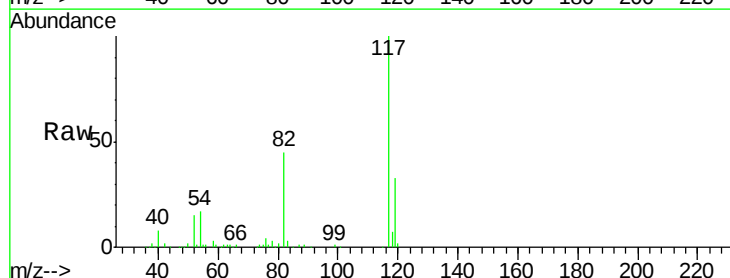

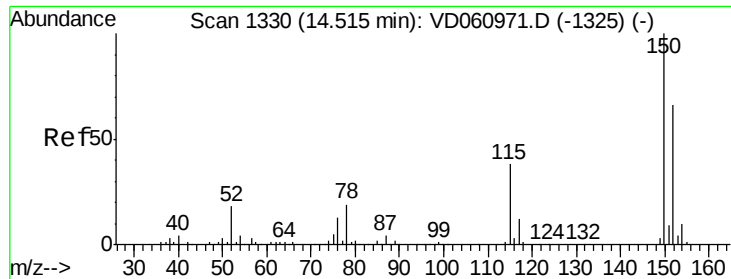

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 14.52 min Scan# 1330
 Delta R.T. 0.00 min
 Lab File: VD061208.D
 Acq: 20 Mar 2019 15:18

Instrument :
 MSVOA_D
 ClientSampleId :
 20190147-COMPOSITE-FRE

Tot Ion	Ratio	Lower	Upper
152	100		
115	52.2	28.6	85.9
150	152.2	0.0	310.6

