

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD032019\
 Data File : VD061210.D
 Acq On : 20 Mar 2019 16:13
 Operator : VA/AP
 Sample : K1943-10RE
 Misc : 4.55g/5ml/MSVOA D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 20190133-LOC-10RE

Quant Time: Mar 22 02:33:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 08 02:35:39 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.04	168	466889	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.21	114	776057	50.00	ug/l	0.00
63) Chlorobenzene-d5	12.36	117	494926	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.51	152	133446	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.45	65	243884	62.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	125.52%	
35) Dibromofluoromethane	6.91	113	371725	64.54	ug/l	-0.01
Spiked Amount 50.000			Recovery	=	129.08%	
50) Toluene-d8	10.40	98	766831	53.02	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.04%	
62) 4-Bromofluorobenzene	13.55	95	213412	38.03	ug/l	0.00
Spiked Amount 50.000			Recovery	=	76.06%	
Target Compounds						
16) Acetone	3.21	43	202090	181.846	ug/l	98
17) Carbon Disulfide	3.38	76	33662	2.129	ug/l #	93
20) Methylene Chloride	3.81	84	32465	1.922	ug/l #	94
25) 2-Butanone	6.05	43	70395	55.823	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD032019\
Data File : VD061210.D
Acq On : 20 Mar 2019 16:13
Operator : VA/AP
Sample : K1943-10RE
Misc : 4.55q/5ml/MSVOA D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
20190133-LOC-10RE

Quant Time: Mar 22 02:33:06 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 08 02:35:39 2019
Response via : Initial Calibration

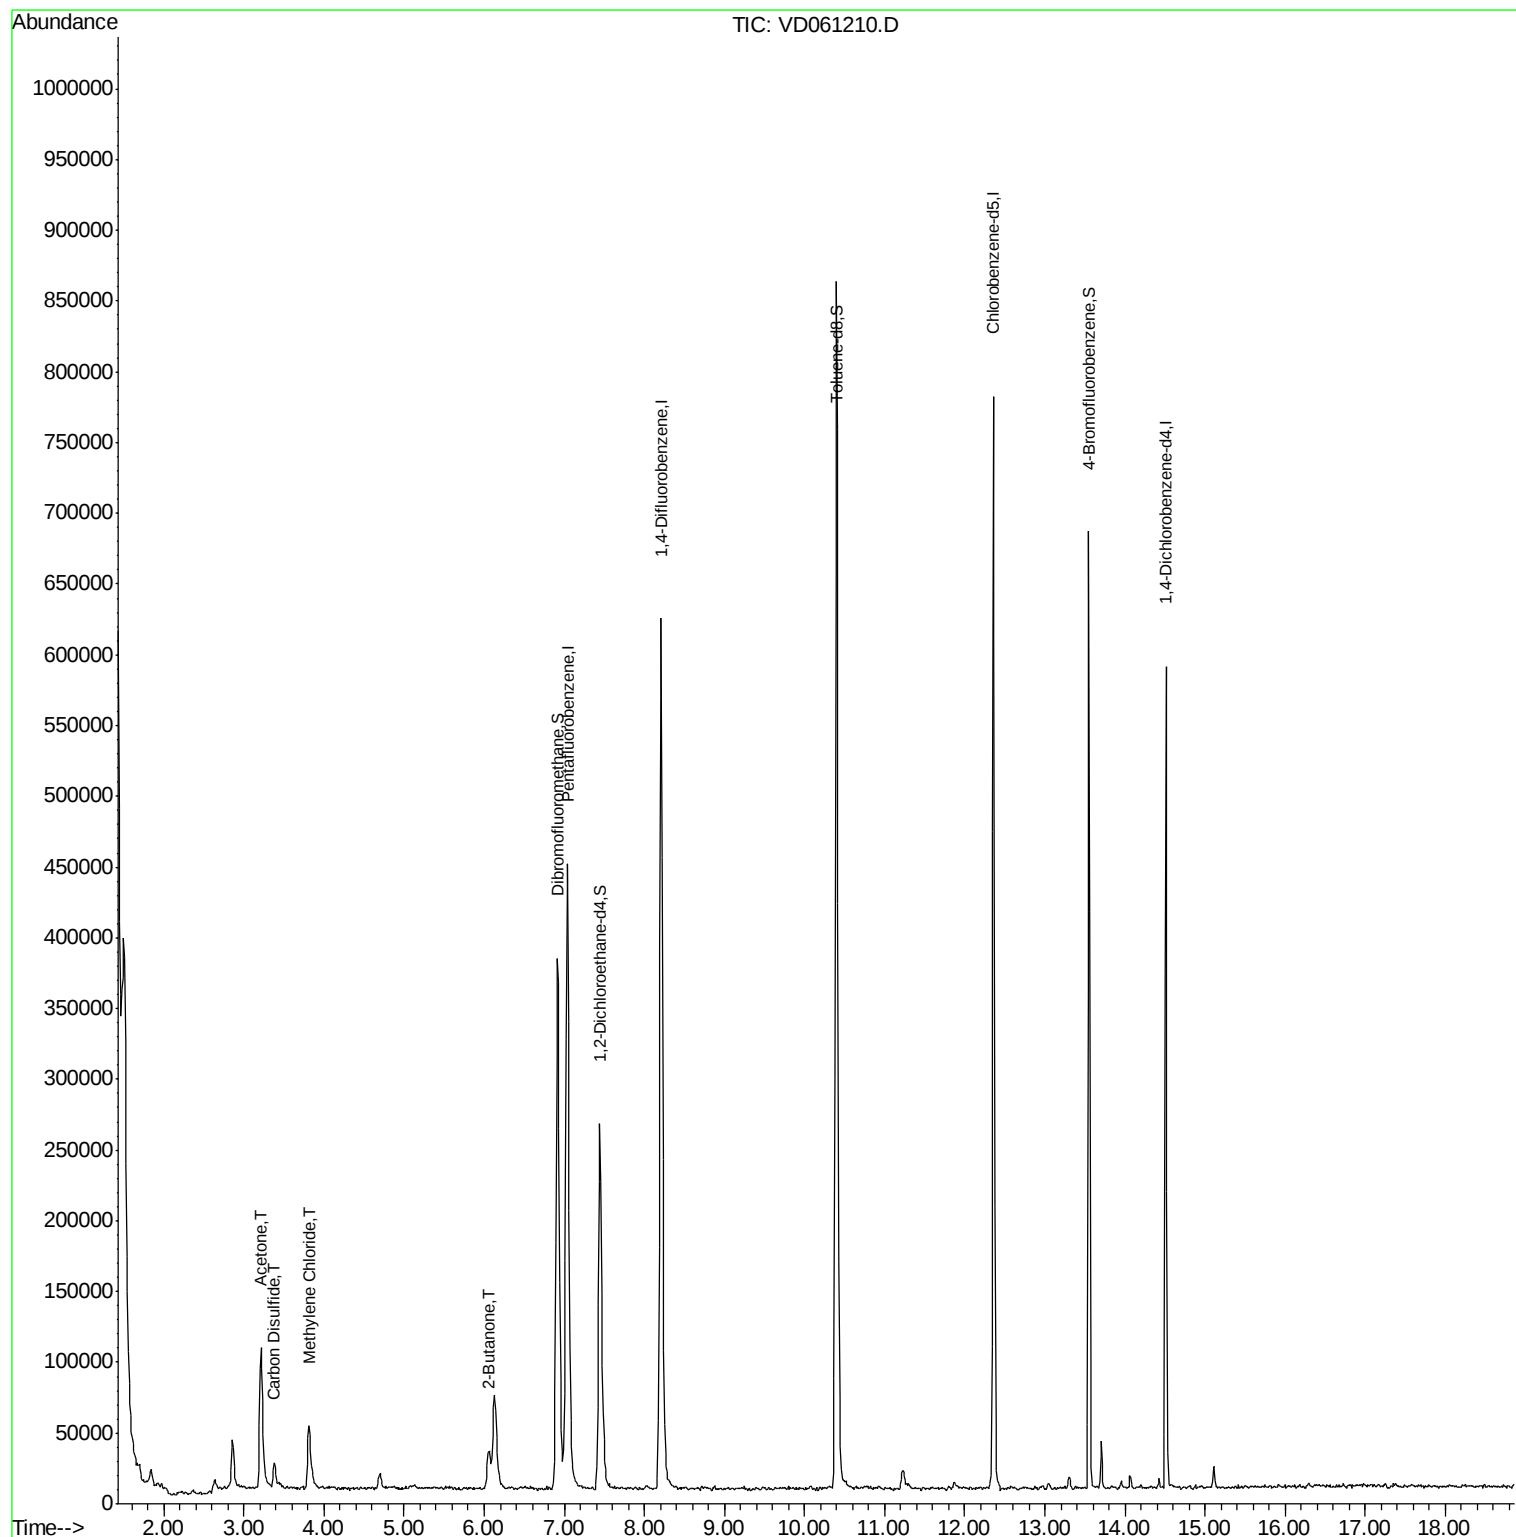



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.04 min Scan# 571

Delta R.T. -0.00 min

Lab File: VD061210.D

Acq: 20 Mar 2019 16:13

Instrument :

MSVOA_D

ClientSampleId :


20190133-LOC-10RE

Tot Ion:168 Resp: 466889

Ion Ratio Lower Upper




168 100

99 54.4 47.3 70.9

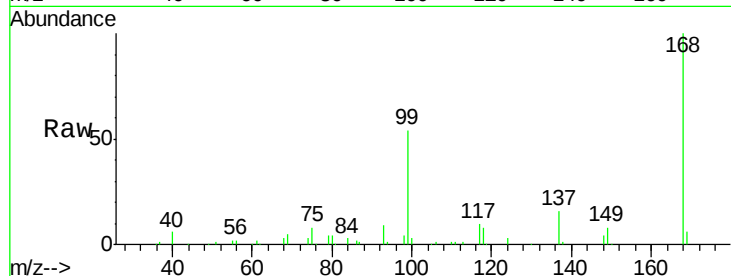

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

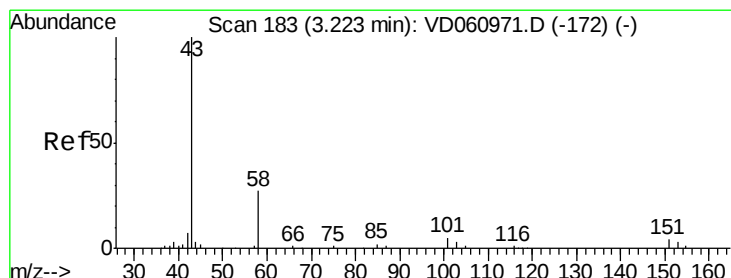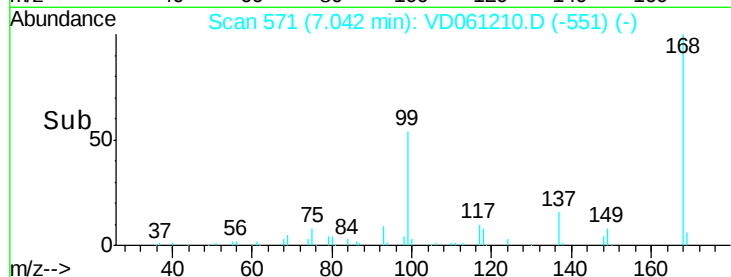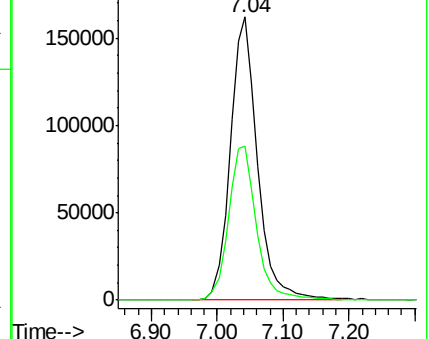

#16

Acetone

Concen: 181.846 ug/l

RT: 3.21 min Scan# 182

Delta R.T. -0.01 min

Lab File: VD061210.D


Acq: 20 Mar 2019 16:13

Tgt Ion: 43 Resp: 202090

Ion Ratio Lower Upper



43 100


58 27.9 21.6 32.4

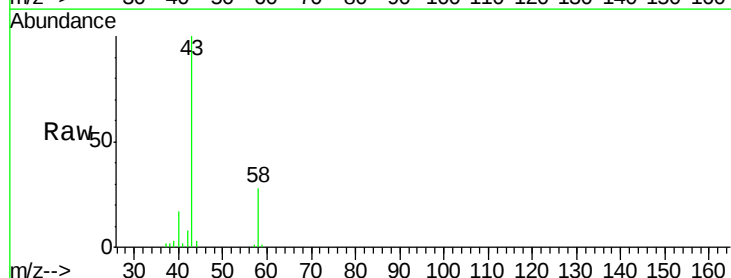

Abundance Ion 42.95 (42.65 to 43.65): VDC

Ion 57.95 (57.65 to 58.65): VDC

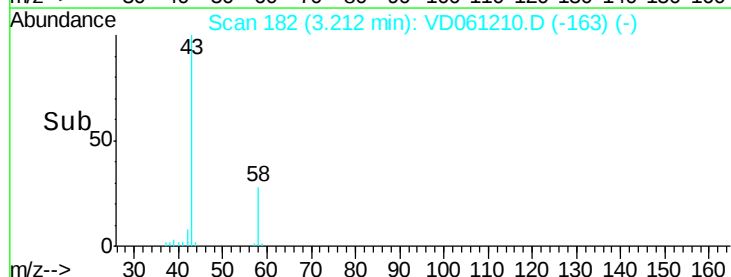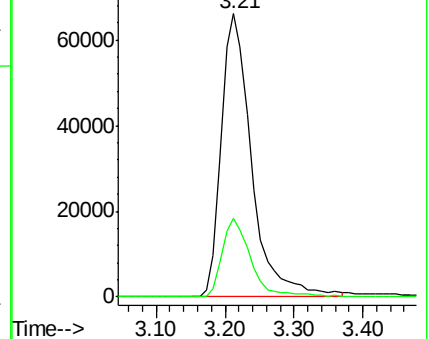

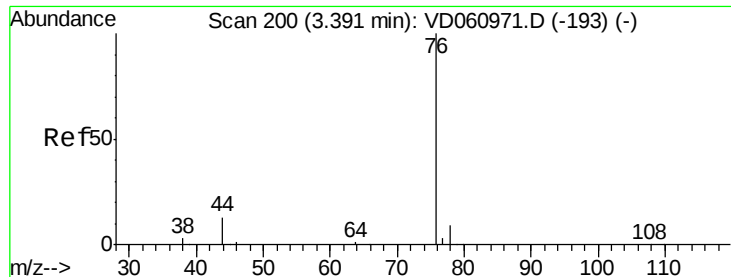

#17

Carbon Disulfide

Concen: 2.129 ug/l

RT: 3.38 min Scan# 199

Delta R.T. -0.01 min

Lab File: VD061210.D

Acq: 20 Mar 2019 16:13

Instrument :

MSVOA_D

ClientSampleId :


20190133-LOC-10RE

Tot Ion: 76 Resp: 33662

Ion Ratio Lower Upper

76 100

78 6.7 7.4 11.2#

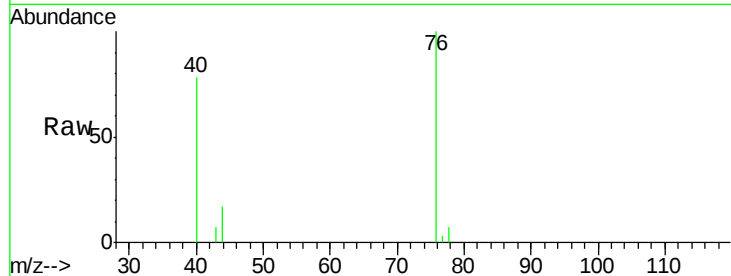

Abundance Ion 75.85 (75.55 to 76.55): VDC

Ion 77.85 (77.55 to 78.55): VDC



15000

10000

5000

0

Time-->

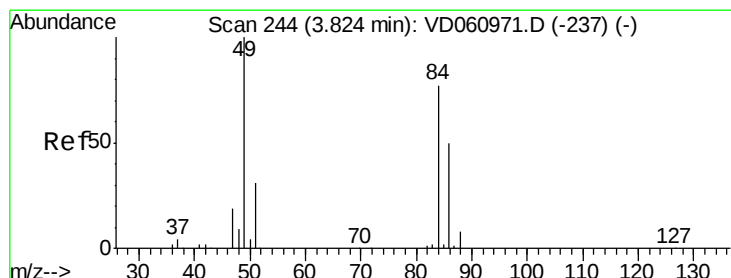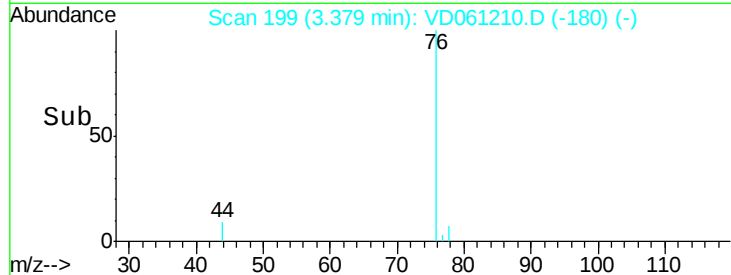

#20

Methylene Chloride

Concen: 1.922 ug/l

RT: 3.81 min Scan# 243

Delta R.T. -0.01 min

Lab File: VD061210.D

Acq: 20 Mar 2019 16:13

Tgt Ion: 84 Resp: 32465


Ion Ratio Lower Upper

84 100

49 126.2 104.2 156.2

51 30.8 32.3 48.5#

86 60.9 52.3 78.5

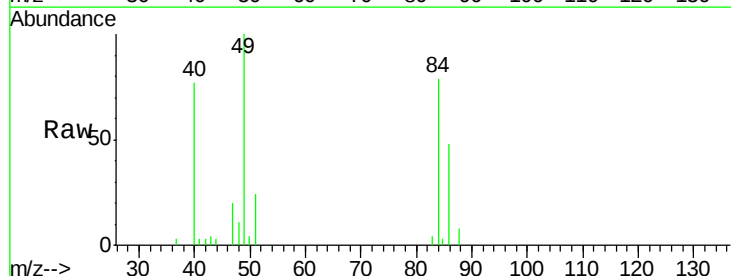

Abundance Ion 83.95 (83.65 to 84.65): VDC

Ion 48.90 (48.60 to 49.60): VDC

Ion 50.90 (50.60 to 51.60): VDC

Ion 85.90 (85.60 to 86.60): VDC

20000


15000

10000

5000

0

Time-->

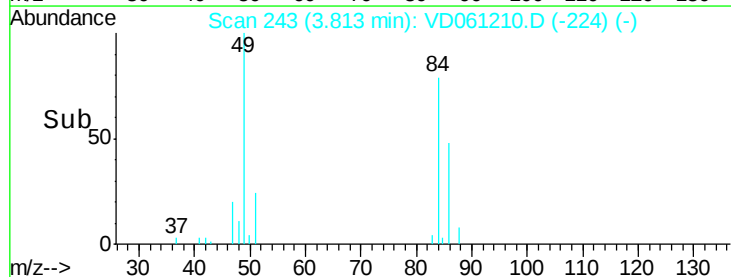



#25

2-Butanone

Concen: 55.823 ug/l

RT: 6.05 min Scan# 470

Delta R.T. -0.02 min

Lab File: VD061210.D

Acq: 20 Mar 2019 16:13

Instrument :

MSVOA_D

ClientSampleId :


20190133-LOC-10RE

Tot Ion: 43 Resp: 70395

Ion Ratio Lower Upper




43 100

72 20.6 16.7 25.1

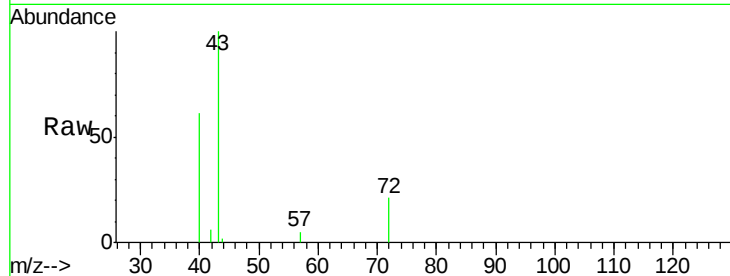

Abundance Ion 42.95 (42.65 to 43.65): VDC

Ion 72.00 (71.70 to 72.70): VDC

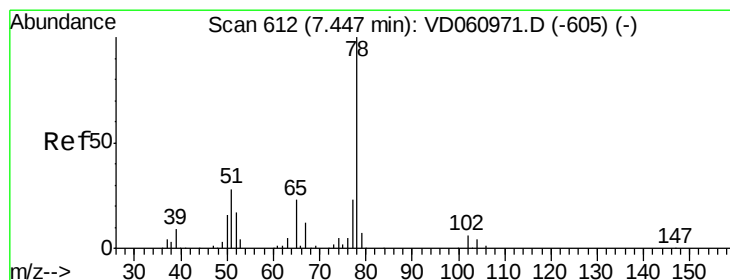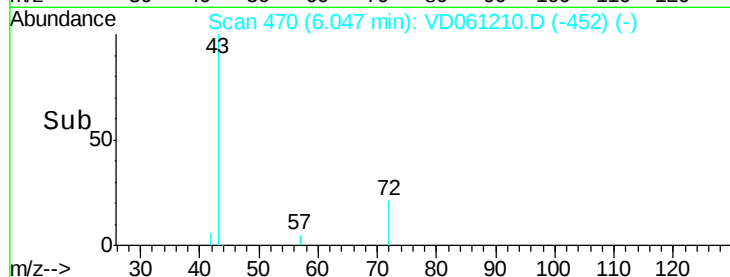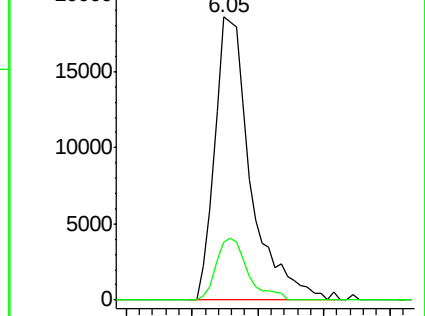

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 7.45 min Scan# 612

Delta R.T. -0.00 min

Lab File: VD061210.D


Acq: 20 Mar 2019 16:13

Tgt Ion: 65 Resp: 243884

Ion Ratio Lower Upper



65 100


67 52.3 0.0 105.2

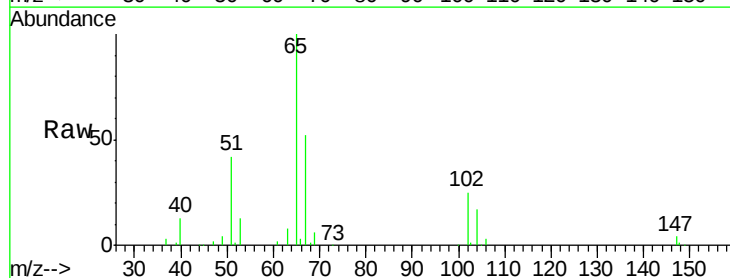

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

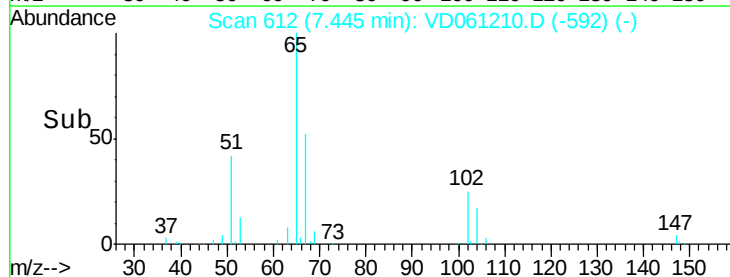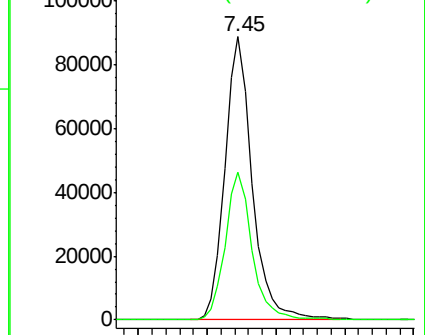

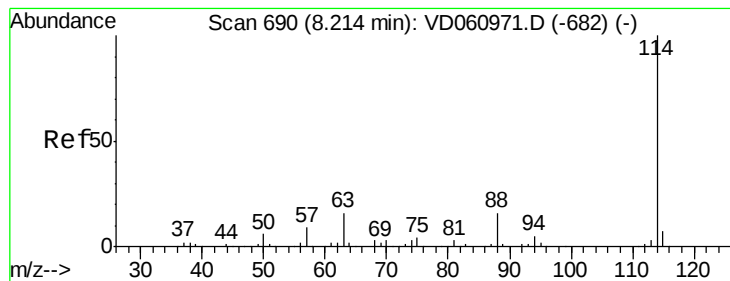

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.21 min Scan# 690

Delta R.T. -0.00 min

Lab File: VD061210.D

Acq: 20 Mar 2019 16:13

Instrument :

MSVOA_D

ClientSampleId :

20190133-LOC-10RE


Tot Ion:114 Resp: 776057

Ion Ratio Lower Upper

114 100

63 15.7 0.0 31.4




88 16.2 0.0 33.0

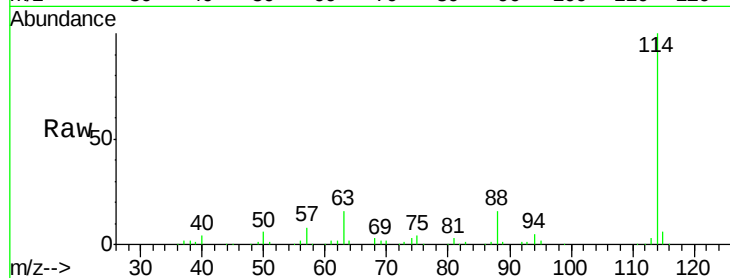

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 62.95 (62.65 to 63.65): V

Ion 87.90 (87.60 to 88.60): V

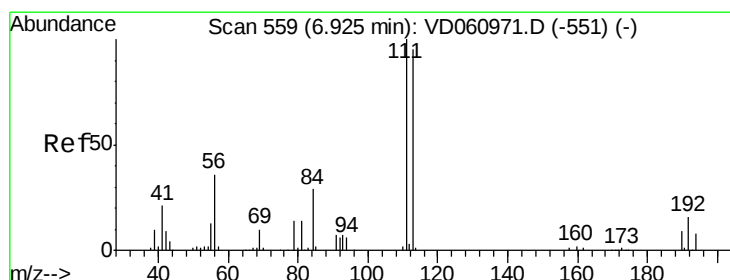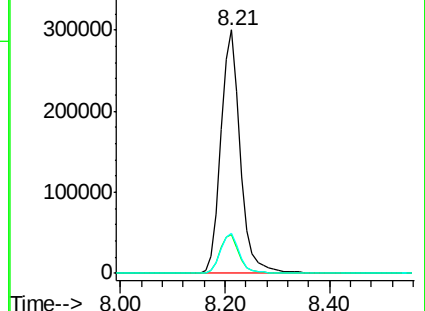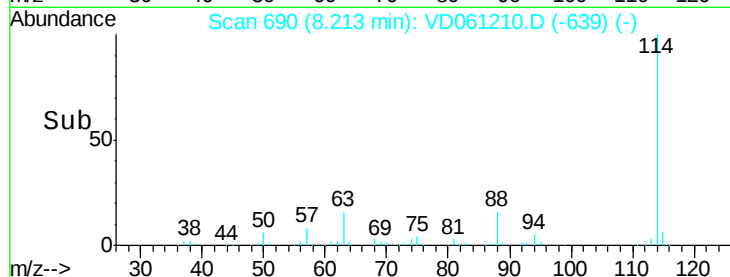

#35

Dibromofluoromethane

Concen: 50.000 ug/l

RT: 6.91 min Scan# 558

Delta R.T. -0.01 min

Lab File: VD061210.D

Acq: 20 Mar 2019 16:13


Tgt Ion:113 Resp: 371725

Ion Ratio Lower Upper

113 100

111 98.2 84.2 126.4



192 17.0 13.1 19.7

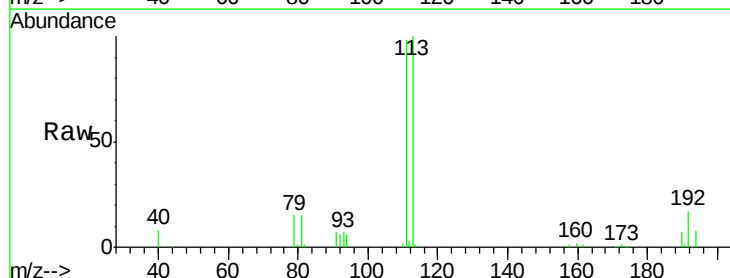


Abundance Ion 112.90 (112.60 to 113.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 191.80 (191.50 to 192.50): V

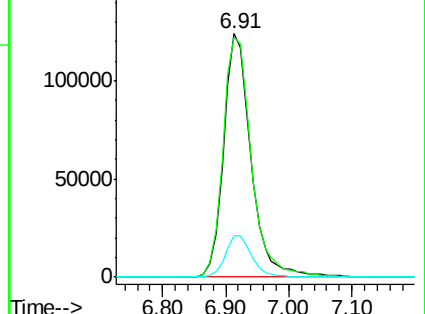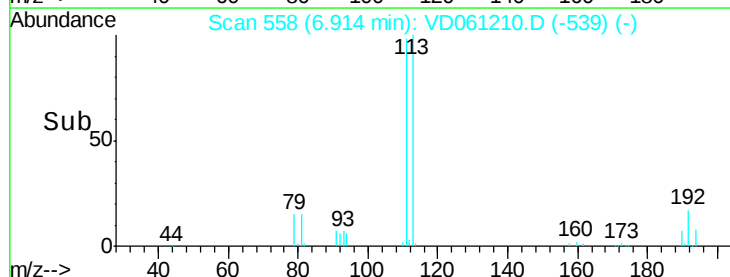

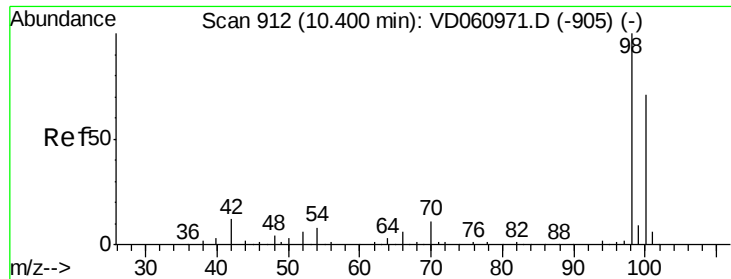

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.40 min Scan# 912

Delta R.T. -0.00 min

Lab File: VD061210.D

Acq: 20 Mar 2019 16:13

Instrument :

MSVOA_D

ClientSampleId :


20190133-LOC-10RE

Tot Ion: 98 Resp: 766831

Ion Ratio Lower Upper




98 100

100 70.2 57.4 86.2

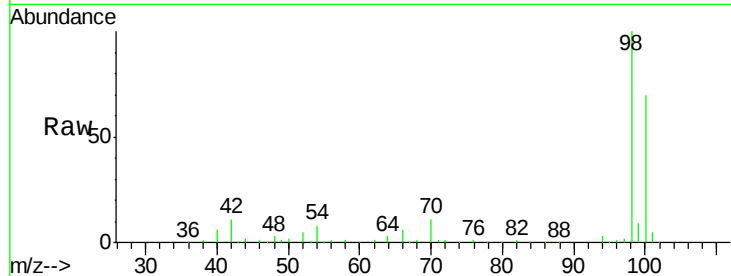

Abundance Ion 98.05 (97.75 to 98.75): VD060971.D (-905) (-)

Ion 100.05 (99.75 to 100.75): VD060971.D (-905) (-)

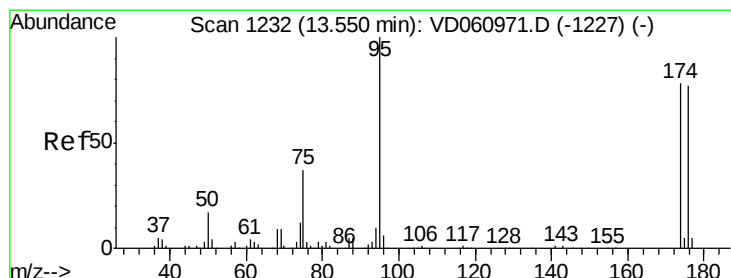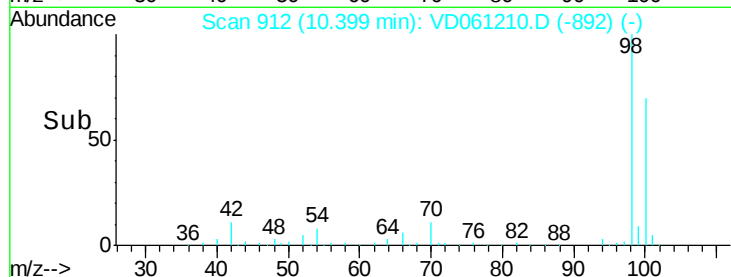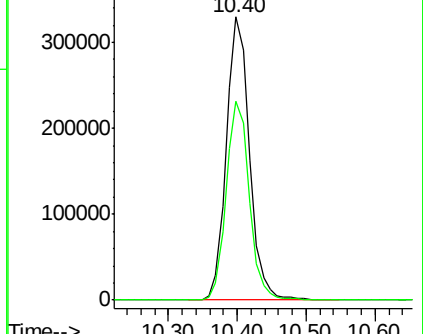

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 13.55 min Scan# 1232

Delta R.T. -0.00 min

Lab File: VD061210.D

Acq: 20 Mar 2019 16:13


Tgt Ion: 95 Resp: 213412

Ion Ratio Lower Upper

95 100

174 79.9 0.0 155.6



176 77.5 0.0 153.8

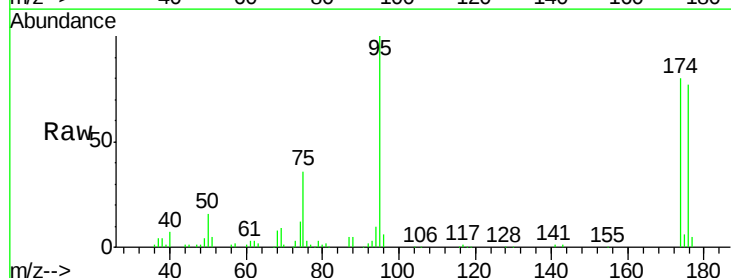


Abundance Ion 95.00 (94.70 to 95.70): VD060971.D (-1227) (-)

Ion 173.90 (173.60 to 174.60): VD060971.D (-1227) (-)

Ion 175.90 (175.60 to 176.60): VD060971.D (-1227) (-)



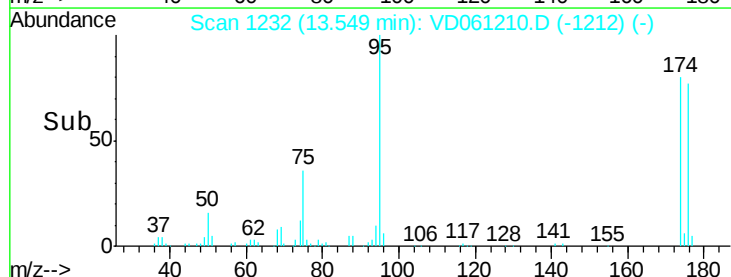
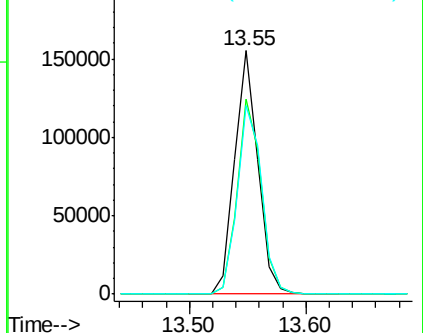


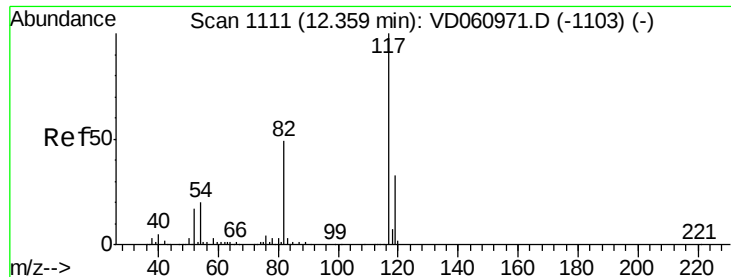

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.36 min Scan# 1111
Delta R.T. -0.00 min
Lab File: VD061210.D
Acq: 20 Mar 2019 16:13

Instrument :
MSVOA_D
ClientSampleId :
20190133-LOC-10RE

Tot Ion:117 Resp: 494926
Ion Ratio Lower Upper
117 100
82 45.9 38.9 58.3
119 32.8 26.6 39.8

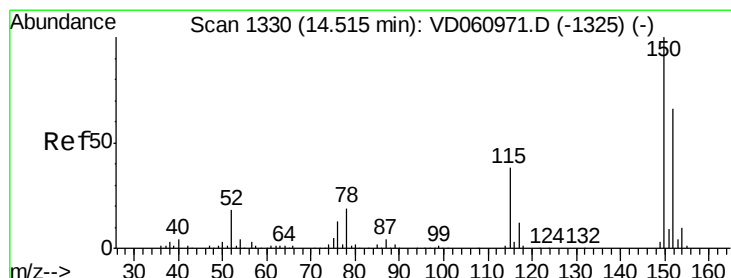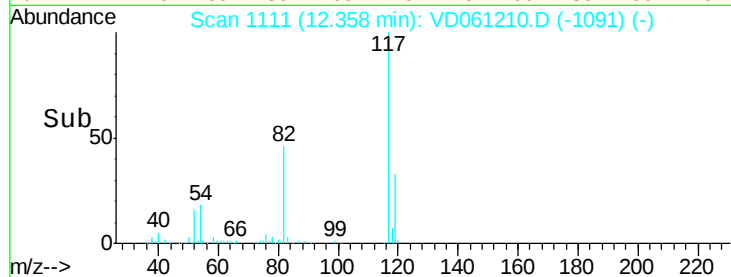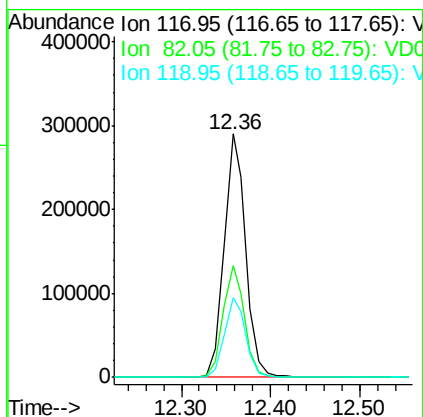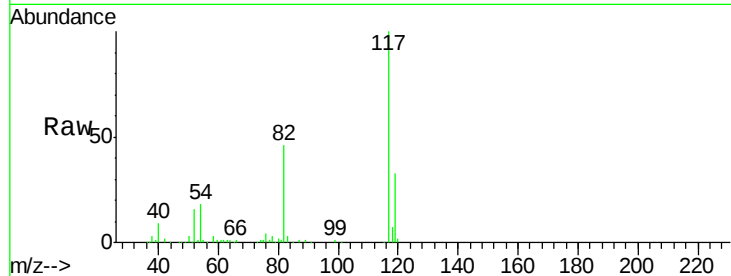

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 14.51 min Scan# 1330
Delta R.T. -0.00 min
Lab File: VD061210.D
Acq: 20 Mar 2019 16:13

Tgt Ion:152 Resp: 133446
Ion Ratio Lower Upper
152 100
115 55.0 28.6 85.9
150 156.6 0.0 310.6

