


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD032019\
Data File : VD061199.D
Acq On : 20 Mar 2019 9:56
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030719S.M
Title : SW846 8260
Last Update : Fri Mar 08 02:35:39 2019

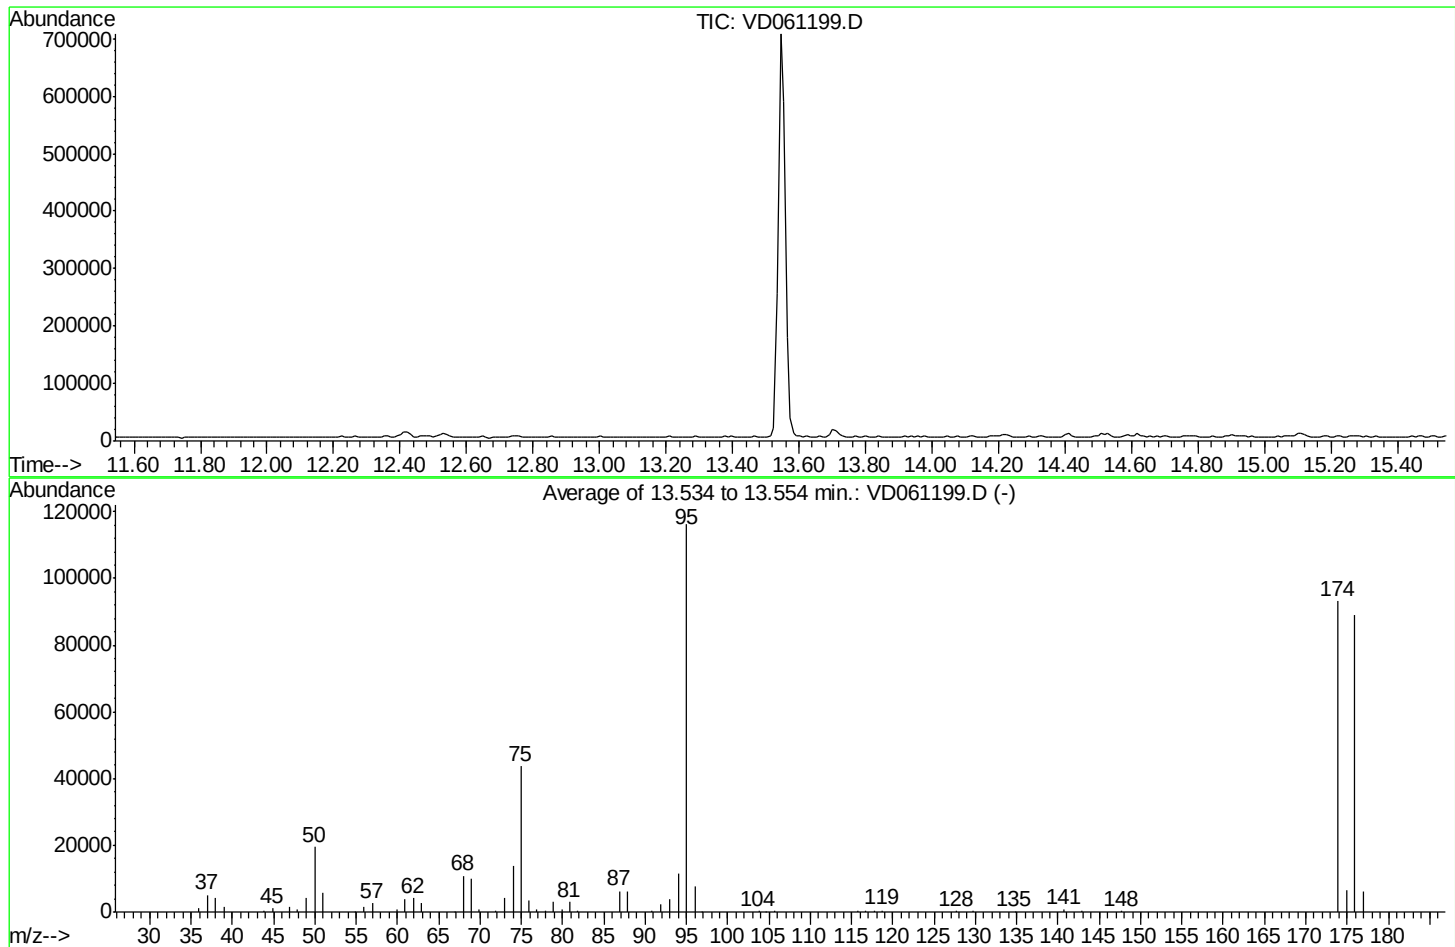

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	19479	PASS
75	95	30	60	37.6	43706	PASS
95	95	100	100	100.0	116205	PASS
96	95	5	9	6.5	7608	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.2	93216	PASS
175	174	5	9	7.1	6625	PASS
176	174	95	101	95.5	89010	PASS
177	176	5	9	6.9	6137	PASS