

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032924\
 Data File : VD078797.D
 Acq On : 29 Mar 2024 17:44
 Operator : RP/MD
 Sample : P1927-03
 Misc : 2.48G/5ml/MSVOA_D/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 72-11998

Quant Time: Mar 30 00:09:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031424S.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 15 05:38:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	163995	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	312757	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	300767	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	133009	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	98423	64.040	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	128.080%
35) Dibromofluoromethane	7.810	113	103807	51.551	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.100%
50) Toluene-d8	10.269	98	378853	51.157	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	102.320%
62) 4-Bromofluorobenzene	12.575	95	103657	47.844	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	95.680%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032924\
Data File : VD078797.D
Acq On : 29 Mar 2024 17:44
Operator : RP/MD
Sample : P1927-03
Misc : 2.48G/5ml/MSVOA_D/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
72-11998

Quant Time: Mar 30 00:09:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031424S.M
Quant Title : SW846 8260
QLast Update : Fri Mar 15 05:38:03 2024
Response via : Initial Calibration




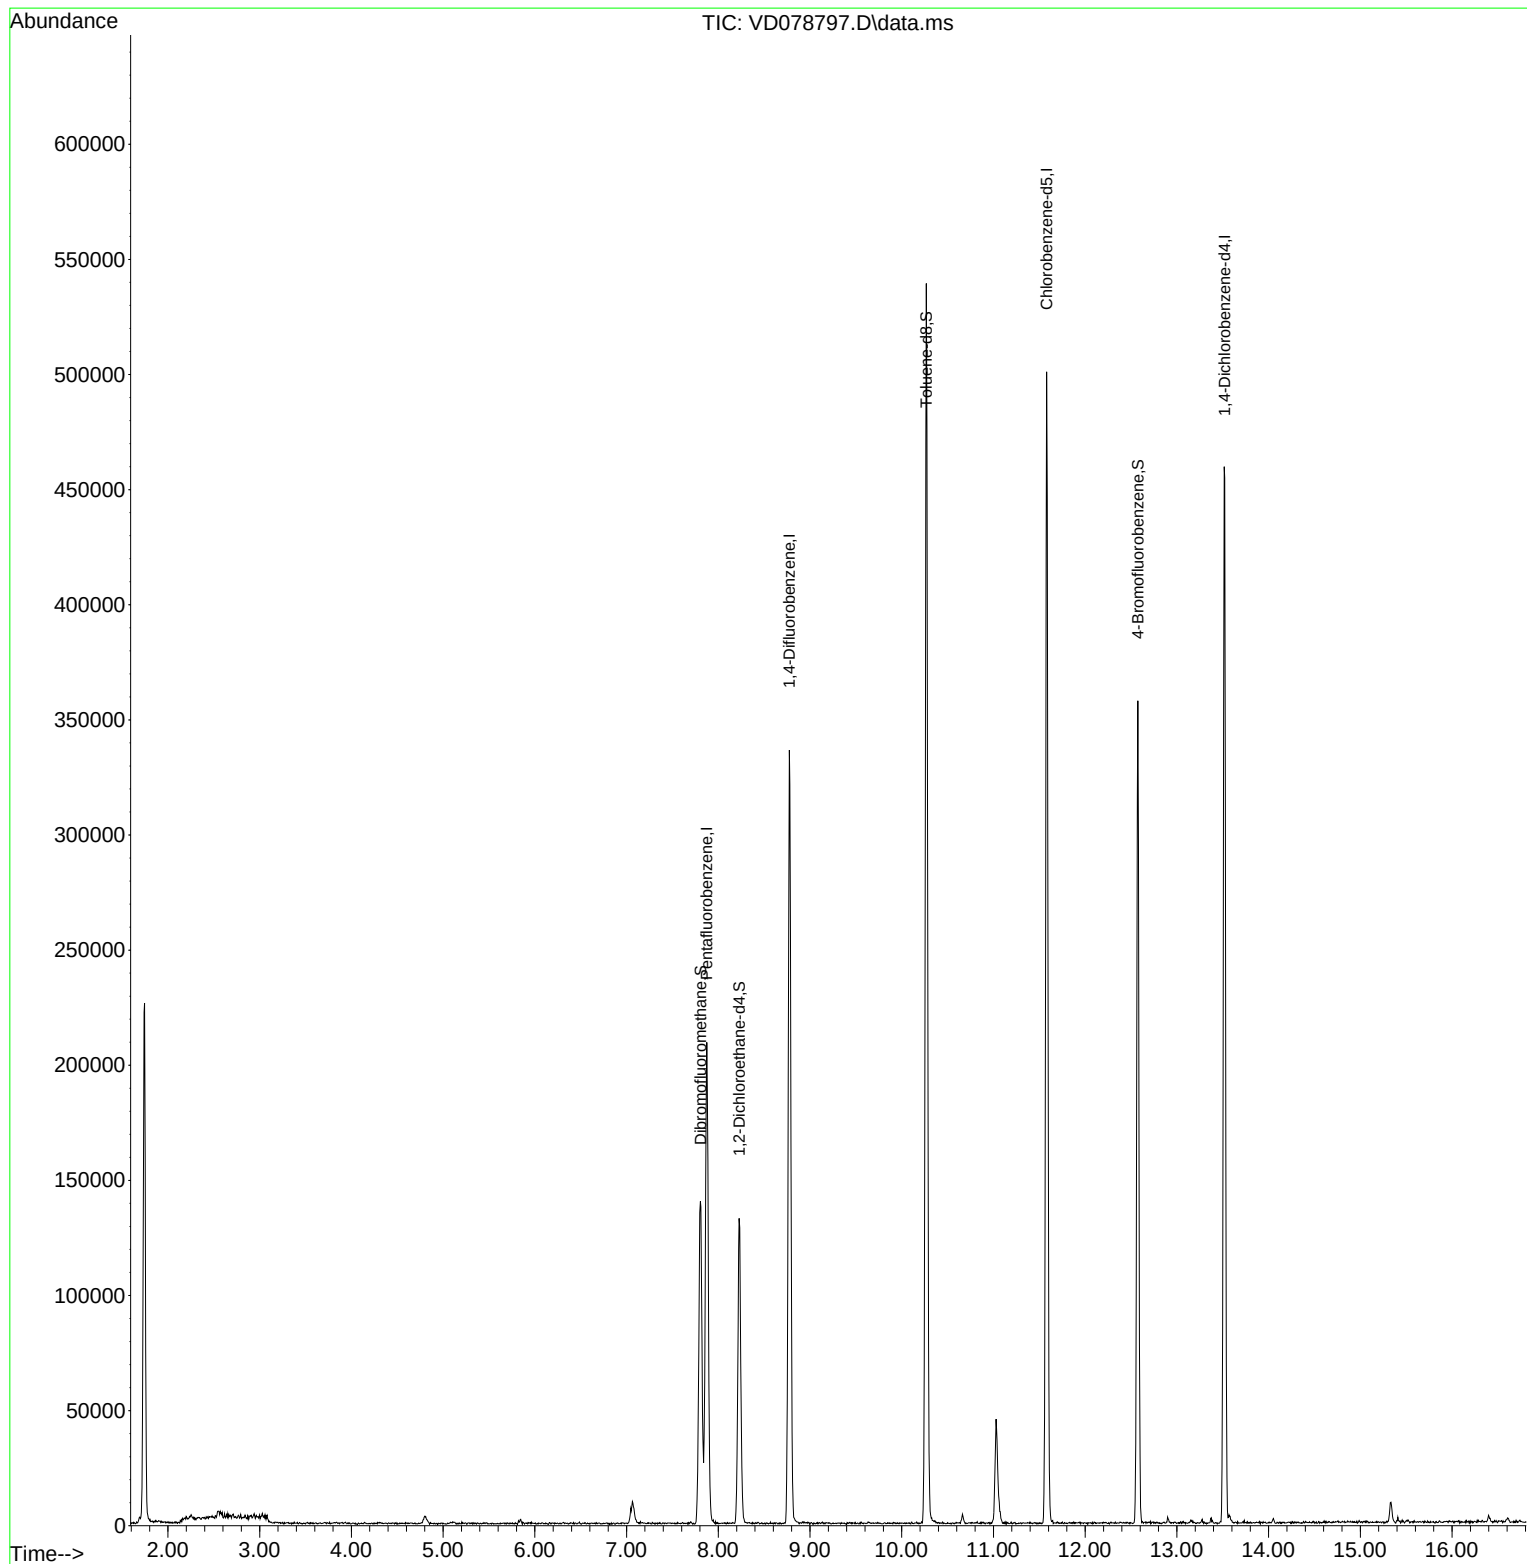


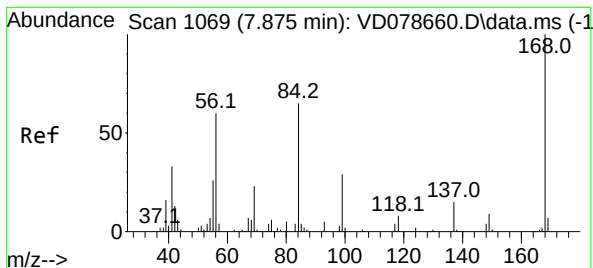

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1129
Delta R.T. 0.000 min
Lab File: VD078797.D
Acq: 29 Mar 2024 17:44




Instrument :
MSVOA_D
ClientSampleId :
72-11998


Tgt Ion:168 Resp: 163995
Ion Ratio Lower Upper
168 100
99 52.6 38.8 58.2

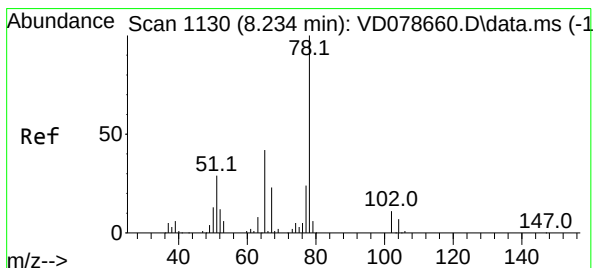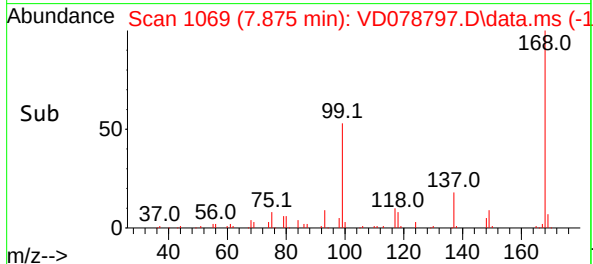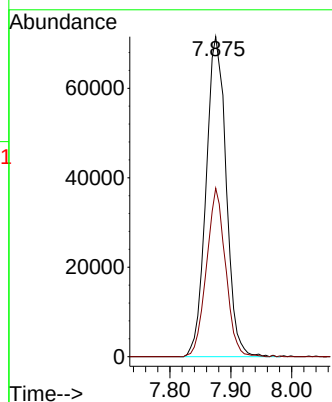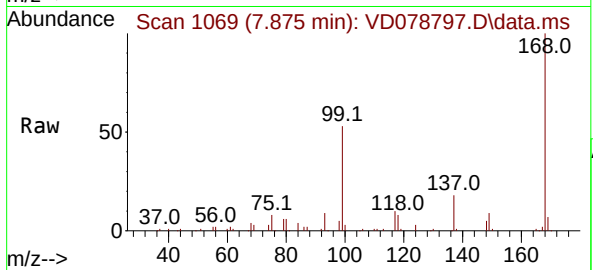

#33
1,2-Dichloroethane-d4
Concen: 64.040 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.006 min
Lab File: VD078797.D
Acq: 29 Mar 2024 17:44

Tgt Ion: 65 Resp: 98423
Ion Ratio Lower Upper
65 100
67 53.6 0.0 110.2

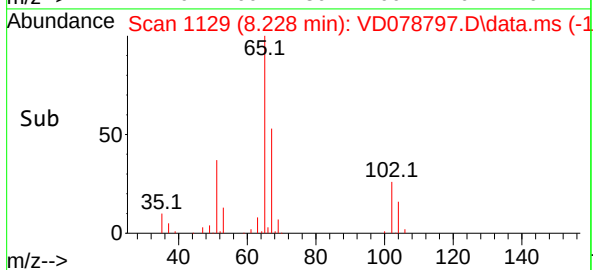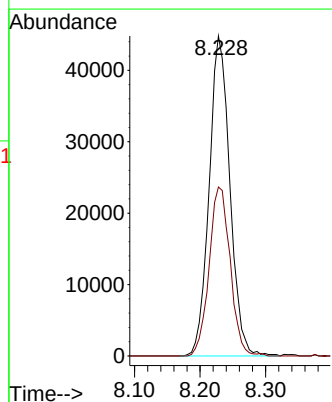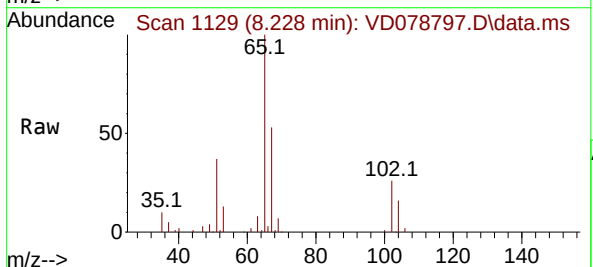

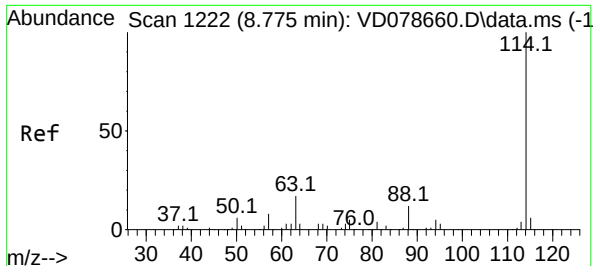

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 11

Delta R.T. -0.000 min

Lab File: VD078797.D

Acq: 29 Mar 2024 17:44

Instrument :

MSVOA_D

ClientSampleId :

72-11998





Tgt Ion:114 Resp: 312757

Ion Ratio Lower Upper

114 100

63 17.2 0.0 33.4

88 13.0 0.0 24.6

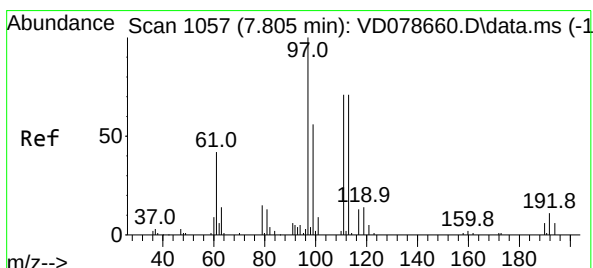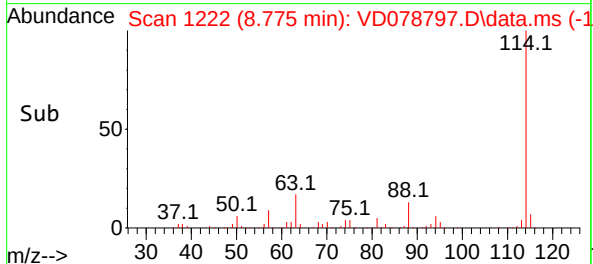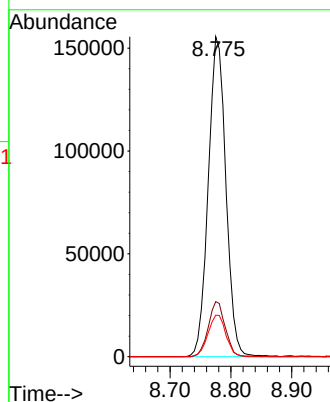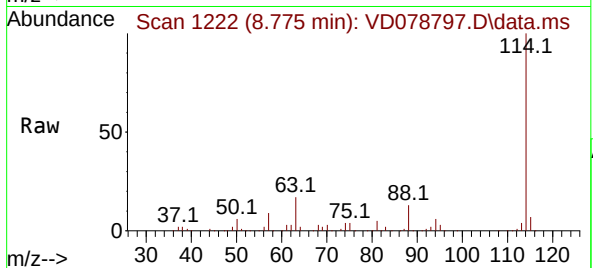

#35

Dibromofluoromethane

Concen: 51.551 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD078797.D

Acq: 29 Mar 2024 17:44




Tgt Ion:113 Resp: 103807


Ion Ratio Lower Upper

113 100

111 101.5 81.9 122.9

192 18.8 15.4 23.0


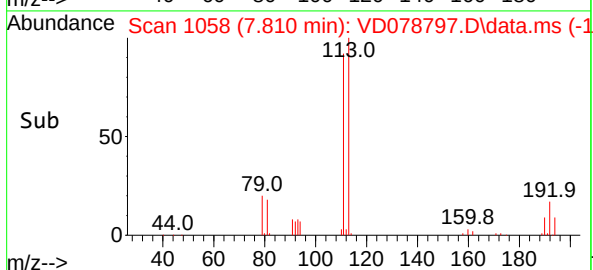
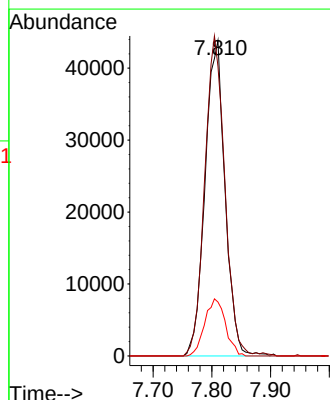
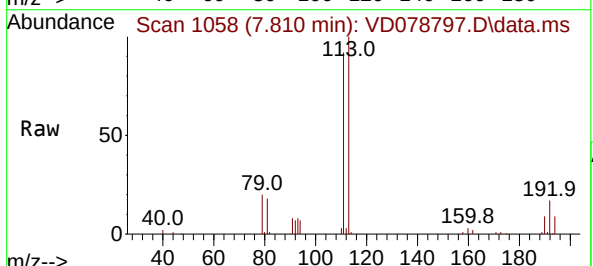


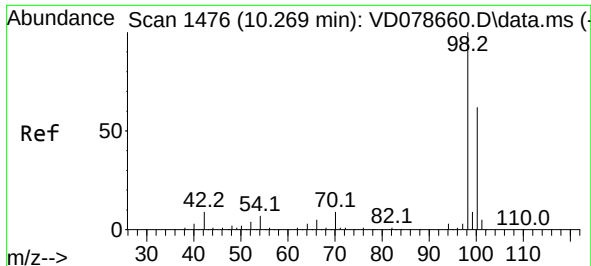

#50
Toluene-d8
Concen: 51.157 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD078797.D
Acq: 29 Mar 2024 17:44




Instrument :
MSVOA_D
ClientSampleId :
72-11998


Tgt Ion: 98 Resp: 378853
Ion Ratio Lower Upper
98 100
100 64.1 50.5 75.7

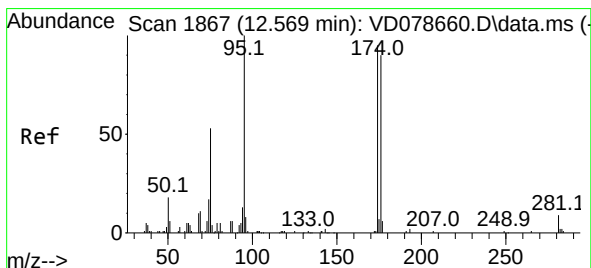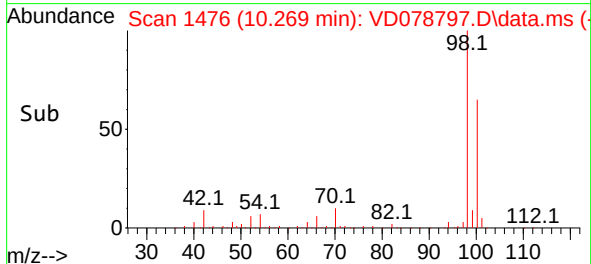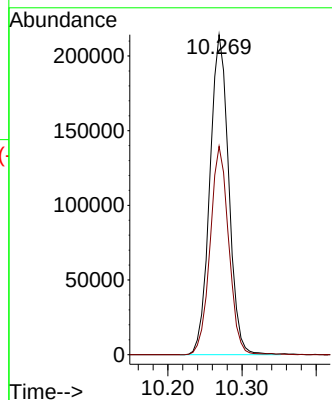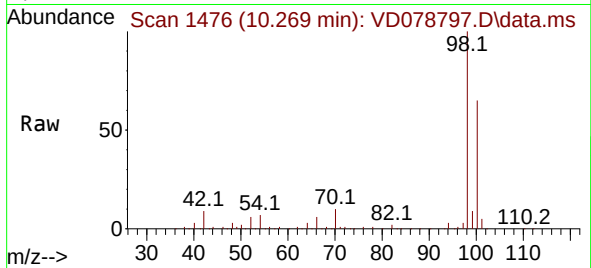

#62
4-Bromofluorobenzene
Concen: 47.844 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. 0.006 min
Lab File: VD078797.D
Acq: 29 Mar 2024 17:44

Tgt Ion: 95 Resp: 103657
Ion Ratio Lower Upper
95 100
174 96.9 0.0 195.2
176 93.5 0.0 188.2

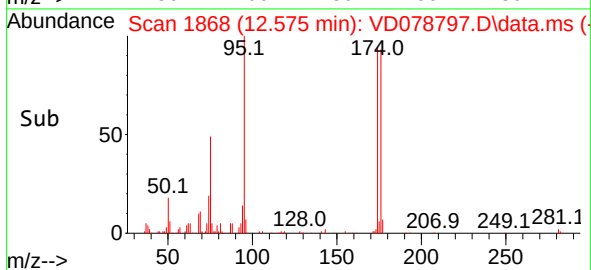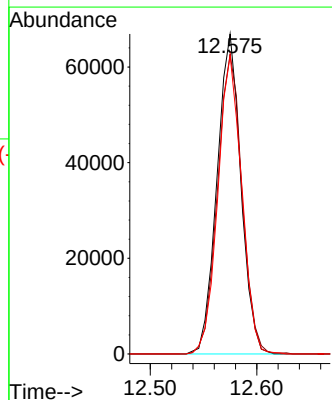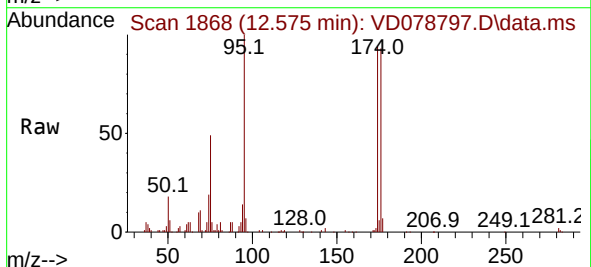

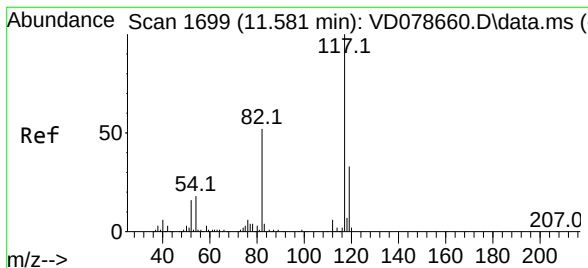

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.581 min Scan# 1

Delta R.T. -0.000 min

Lab File: VD078797.D

Acq: 29 Mar 2024 17:44

Instrument :

MSVOA_D

ClientSampleId :

72-11998





Tgt Ion:117 Resp: 300767

Ion Ratio Lower Upper

117 100

82 51.0 41.4 62.2

119 30.8 26.5 39.7

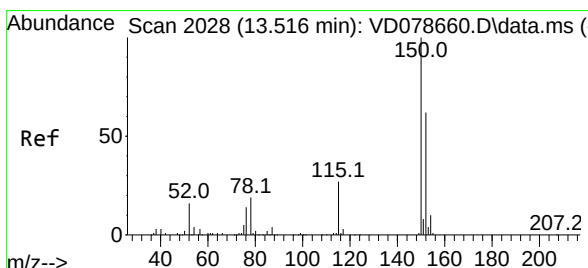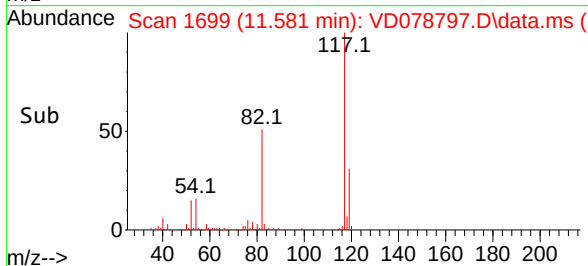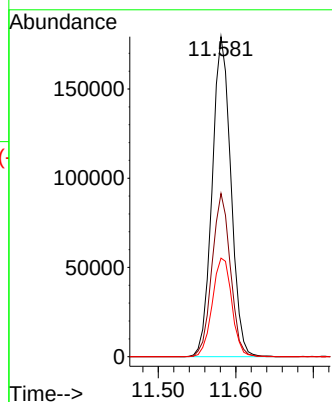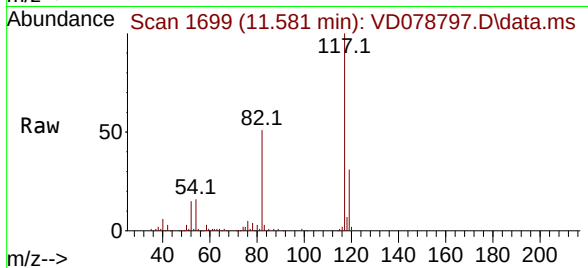

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.522 min Scan# 2029

Delta R.T. 0.006 min

Lab File: VD078797.D

Acq: 29 Mar 2024 17:44

Tgt Ion:152 Resp: 133009

Ion Ratio Lower Upper

152 100

115 52.7 27.1 81.2

150 155.3 0.0 350.2

